

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE112219\
 Data File : BE100765.D
 Acq On : 22 Nov 2019 19:36
 Operator : JU
 Sample : K5969-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 HF-702U

Quant Time: Nov 23 04:25:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE112119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 06:40:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	5954	0.40	ng	0.00
7) Naphthalene-d8	10.55	136	26857	0.40	ng	0.00
13) Acenaphthene-d10	14.40	164	16043	0.40	ng	0.00
19) Phenanthrene-d10	17.13	188	39435	0.40	ng	0.00
27) Chrysene-d12	21.32	240	41671	0.40	ng	0.00
34) Perylene-d12	23.77	264	46138	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.38	112	502	0.03	ng	0.00
5) Phenol-d6	6.93	99	576	0.02	ng	0.00
8) Nitrobenzene-d5	8.90	82	3408	0.40	ng	0.00
11) 2-Methylnaphthalene-d10	12.14	152	7522	0.19	ng	0.00
14) 2,4,6-Tribromophenol	15.88	330	349	0.15	ng	0.00
15) 2-Fluorobiphenyl	13.03	172	11729	0.19	ng	0.00
25) Fluoranthene-d10	19.18	212	99881	0.21	ng	0.02
29) Terphenyl-d14	19.77	244	19644	0.20	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.34	88	723	0.065	ng	# 20
22) Pentachlorophenol	16.79	266	51	0.070	ng	# 80
32) Bis(2-ethylhexyl)phthalate	21.26	149	28264	0.108	ng	99
33) Indeno(1,2,3-cd)pyrene	26.34	276	522	0.040	ng	# 67
39) Benzo(g,h,i)perylene	27.14	276	565	0.026	ng	# 9

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE112219\
Data File : BE100765.D
Acq On : 22 Nov 2019 19:36
Operator : JU
Sample : K5969-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
HF-702U

Quant Time: Nov 23 04:25:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE112119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 06:40:44 2019
Response via : Initial Calibration

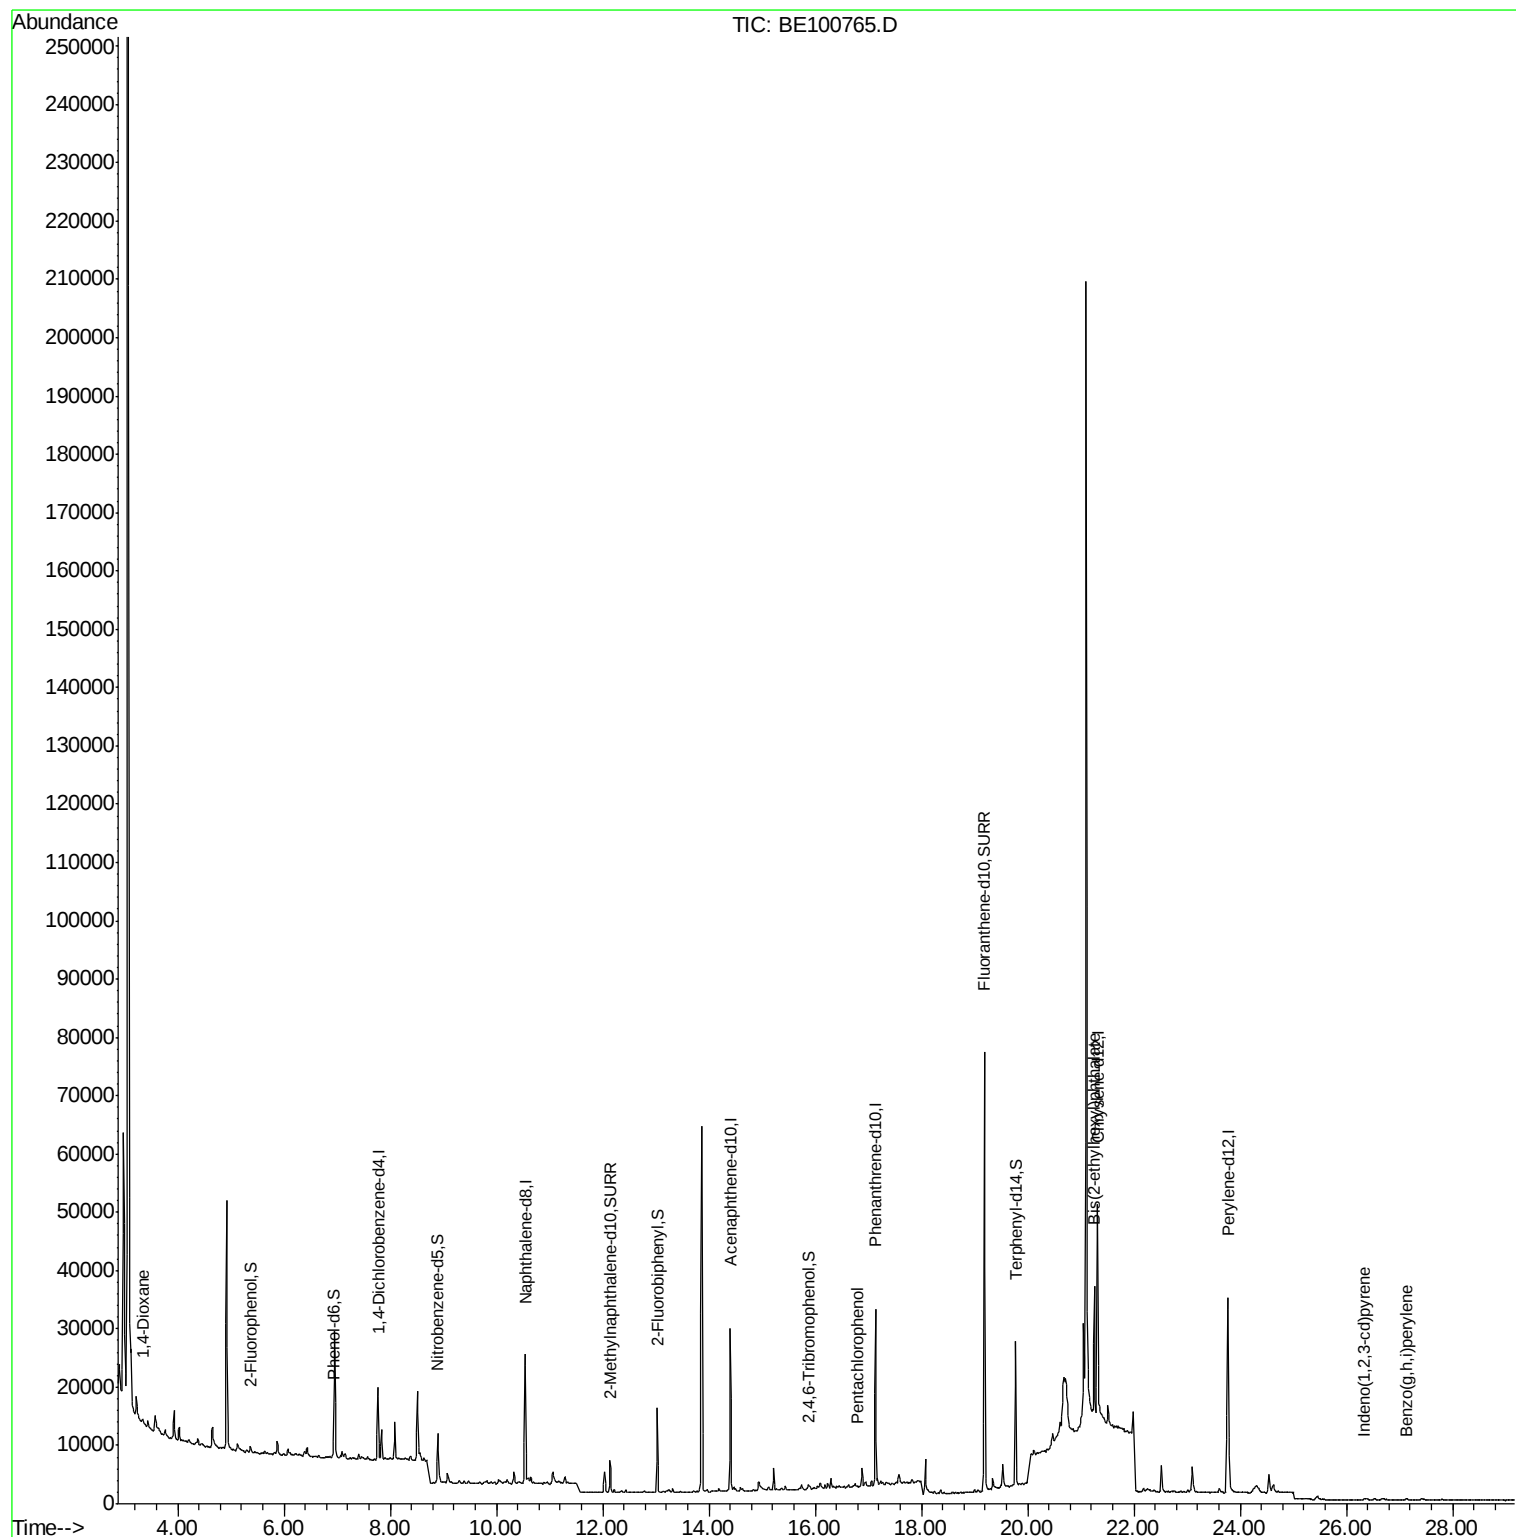



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.77 min Scan# 426

Delta R.T. 0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36

Instrument :

BNA_E

ClientSampleId :

HF-702U


Tot Ion:152 Resp: 5954

Ion Ratio Lower Upper

152 100

150 150.3 127.1 190.7




115 59.6 53.0 79.4

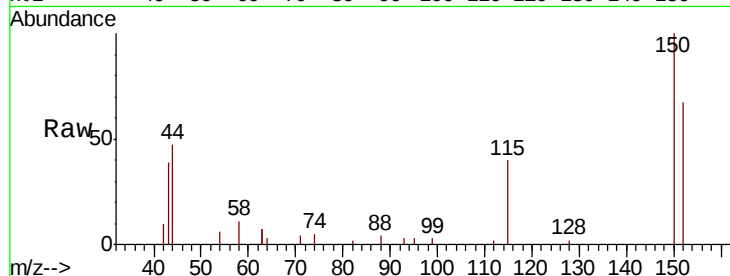

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

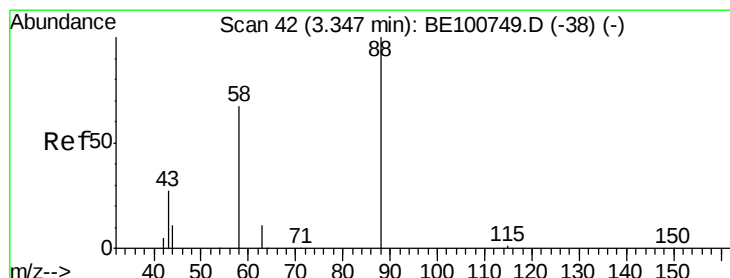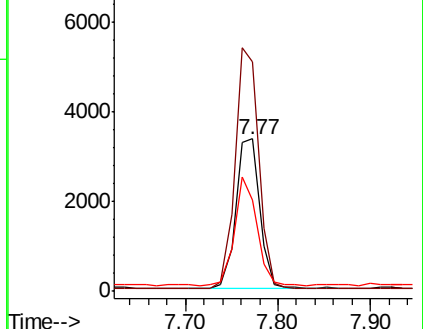

#2

1,4-Dioxane

Concen: 0.065 ng

RT: 3.34 min Scan# 41

Delta R.T. -0.01 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36


Tgt Ion: 88 Resp: 723

Ion Ratio Lower Upper

88 100

58 0.0 60.7 91.1#



43 0.0 27.4 41.2#




Abundance Ion 88.00 (87.70 to 88.70): BE1

Ion 58.00 (57.70 to 58.70): BE1

Ion 43.00 (42.70 to 43.70): BE1

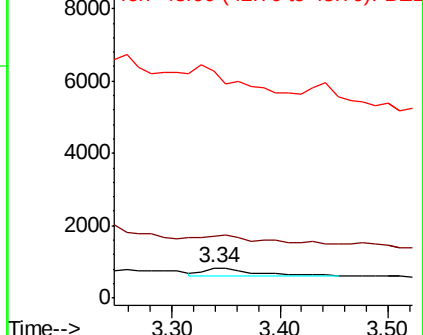



#4

2-Fluorophenol

Concen: 0.031 ng

RT: 5.38 min Scan# 218

Delta R.T. 0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36

Instrument :

BNA_E

ClientSampleId :

HF-702U


Tot Ion:112 Resp: 502

Ion Ratio Lower Upper

112 100

64 89.4 54.3 81.5#


63 198.0 114.0 171.0#

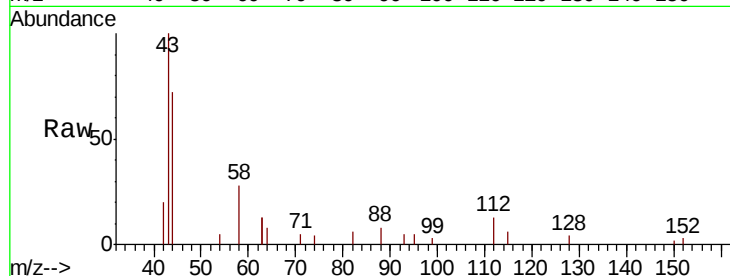



Abundance Ion 112.00 (111.70 to 112.70): BE1

Ion 64.00 (63.70 to 64.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

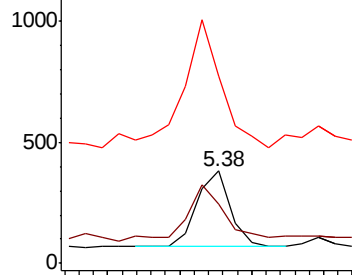

Time-->



#5

Phenol-d6

Concen: 0.025 ng

RT: 6.93 min Scan# 353

Delta R.T. 0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36


Tgt Ion: 99 Resp: 576

Ion Ratio Lower Upper

99 100

42 217.5 17.9 26.9#


71 51.2 29.3 43.9#




Abundance Ion 99.00 (98.70 to 99.70): BE1


Ion 42.00 (41.70 to 42.70): BE1

Ion 71.00 (70.70 to 71.70): BE1

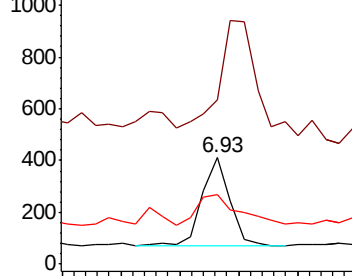

Time-->



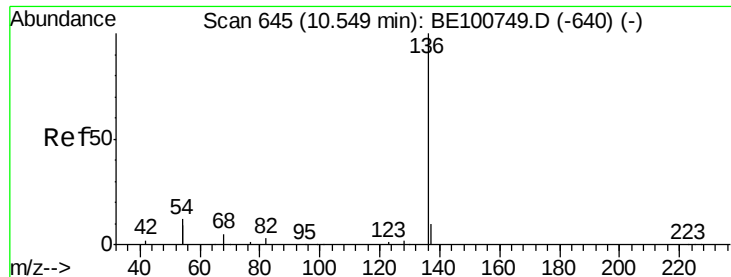

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.55 min Scan# 645

Delta R.T. -0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36

Instrument :

BNA_E

ClientSampleId :

HF-702U

Tot Ion:136 Resp: 26857


Ion Ratio Lower Upper

136 100

137 11.5 8.6 12.8

54 21.0 19.4 29.0

68 5.5 4.6 6.8



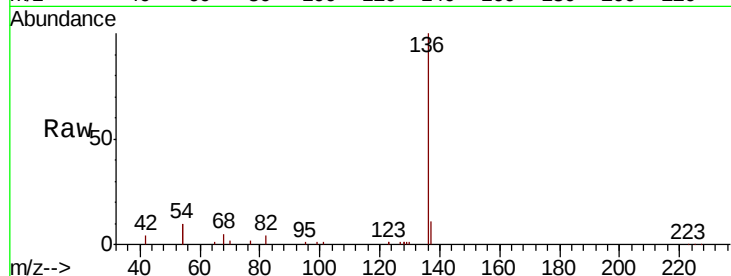


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE1

Ion 68.00 (67.70 to 68.70): BE1

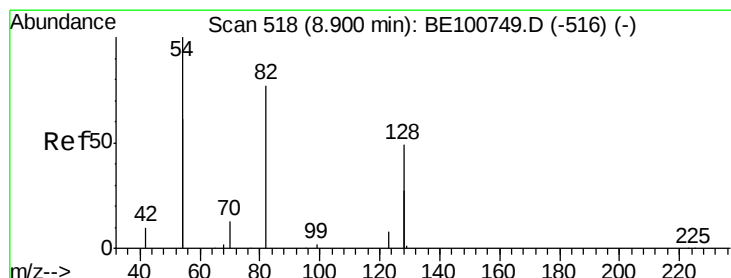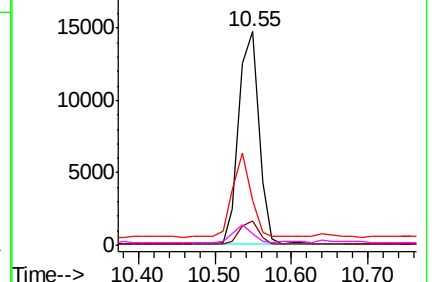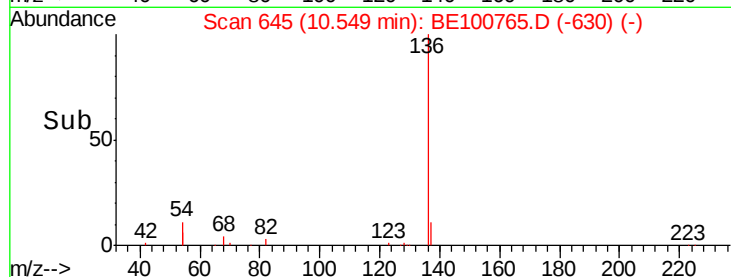

#8

Nitrobenzene-d5

Concen: 0.396 ng

RT: 8.90 min Scan# 518

Delta R.T. -0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36


Tgt Ion: 82 Resp: 3408

Ion Ratio Lower Upper

82 100

128 113.6 90.2 135.4



54 225.3 186.0 279.0

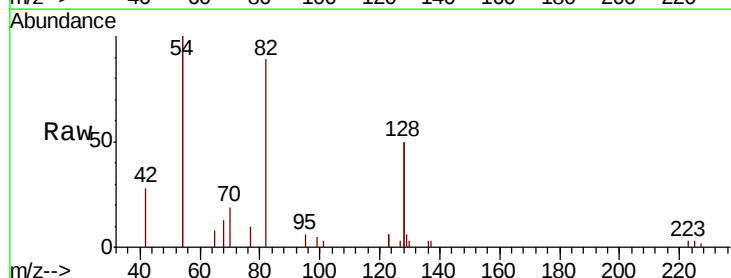


Abundance Ion 82.00 (81.70 to 82.70): BE1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE1



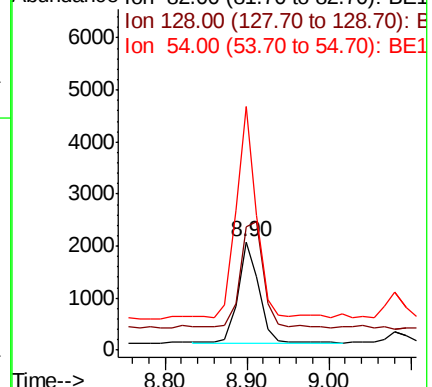
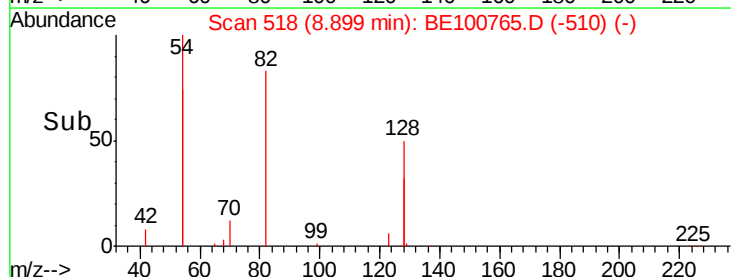


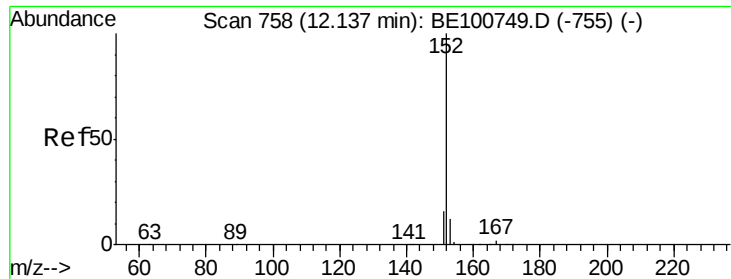

#11
2-Methylnaphthalene-d10
Concen: 0.191 ng
RT: 12.14 min Scan# 758
Delta R.T. -0.00 min
Lab File: BE100765.D
Acq: 22 Nov 2019 19:36




Instrument :
BNA_E
ClientSampleId :
HF-702U


Tot Ion:152 Resp: 7522
Ion Ratio Lower Upper
152 100
151 19.7 15.8 23.8

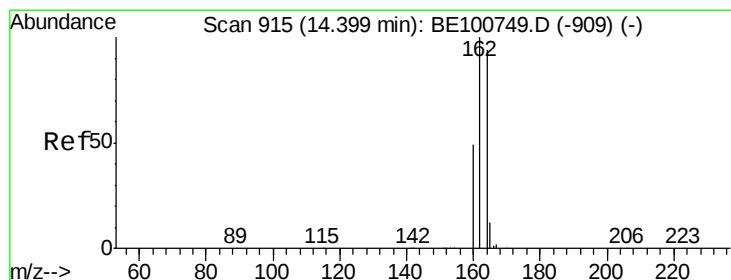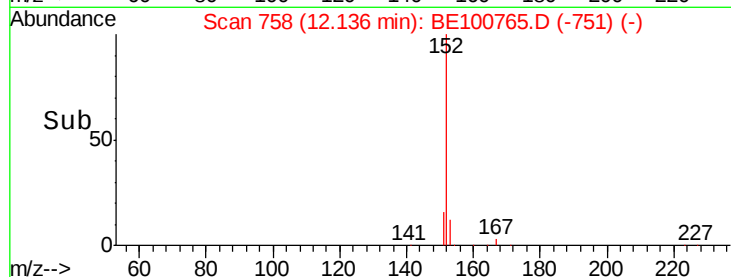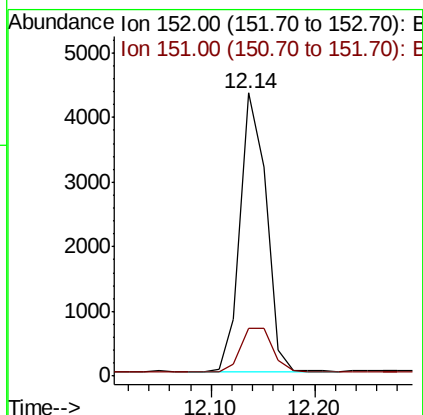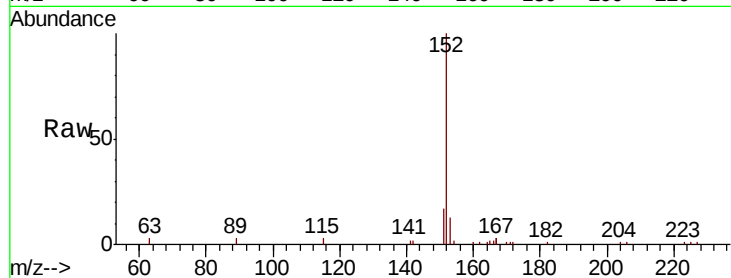

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.40 min Scan# 915
Delta R.T. -0.00 min
Lab File: BE100765.D
Acq: 22 Nov 2019 19:36

Tgt Ion:164 Resp: 16043
Ion Ratio Lower Upper
164 100
162 105.0 84.8 127.2
160 50.1 42.3 63.5

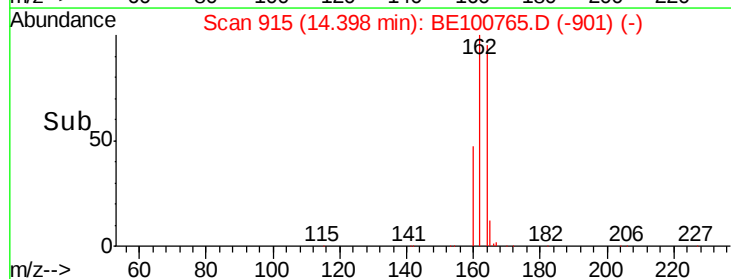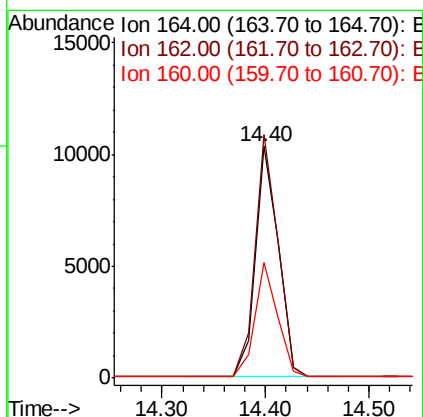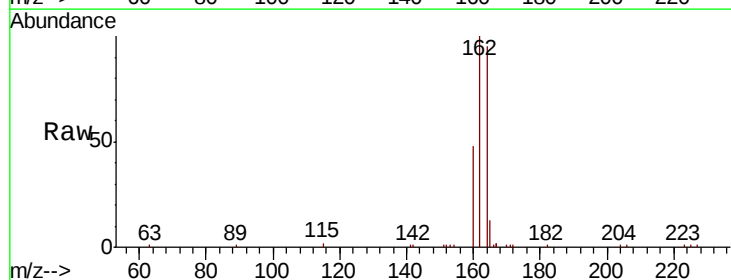



#14

2,4,6-Tribromophenol

Concen: 0.154 ng

RT: 15.88 min Scan# 1019

Delta R.T. -0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36

Instrument :

BNA_E

ClientSampleId :

HF-702U


Tot Ion:330 Resp: 349

Ion Ratio Lower Upper




330 100

332 107.7 79.3 118.9

141 98.3 43.8 65.6#

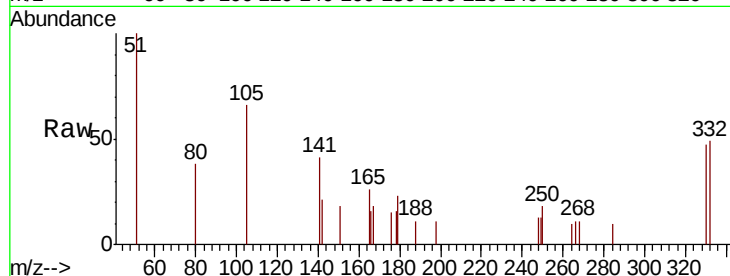

Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

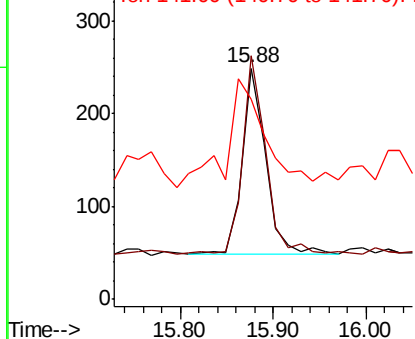

#15

2-Fluorobiphenyl

Concen: 0.188 ng

RT: 13.03 min Scan# 820

Delta R.T. -0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36


Tgt Ion:172 Resp: 11729

Ion Ratio Lower Upper



172 100


171 35.3 27.8 41.6

170 23.9 19.4 29.2



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

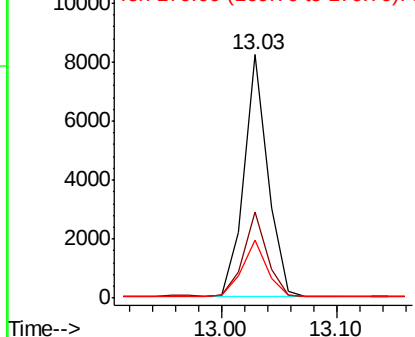

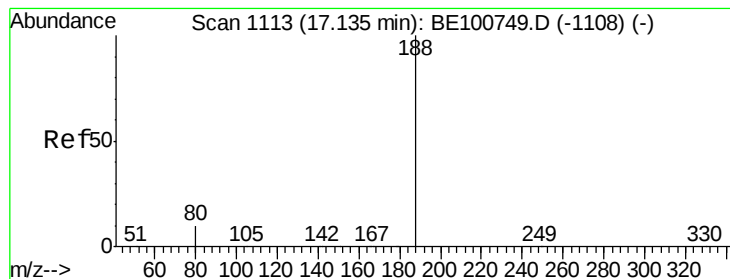

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.13 min Scan# 1113

Delta R.T. -0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36

Instrument :

BNA_E

ClientSampleId :

HF-702U


Tot Ion:188 Resp: 39435

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 9.4 8.2 12.2



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE1

Ion 80.00 (79.70 to 80.70): BE1

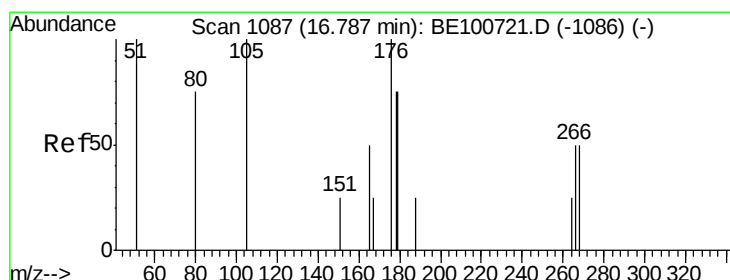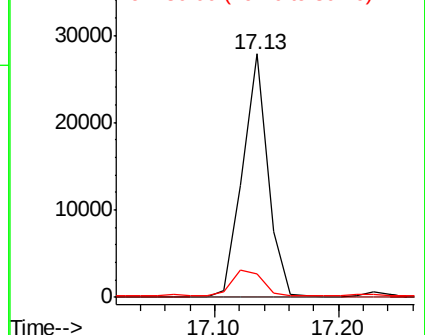

#22

Pentachlorophenol

Concen: 0.070 ng

RT: 16.79 min Scan# 1087

Delta R.T. -0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36


Tgt Ion:266 Resp: 51

Ion Ratio Lower Upper

266 100

264 80.0 54.6 82.0



268 86.3 52.6 78.8#




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

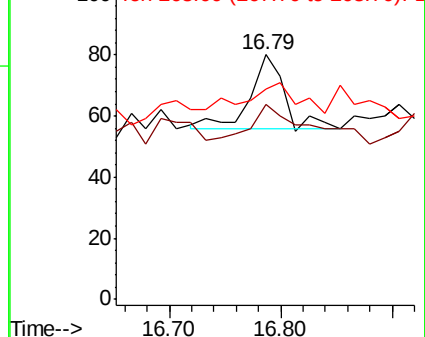


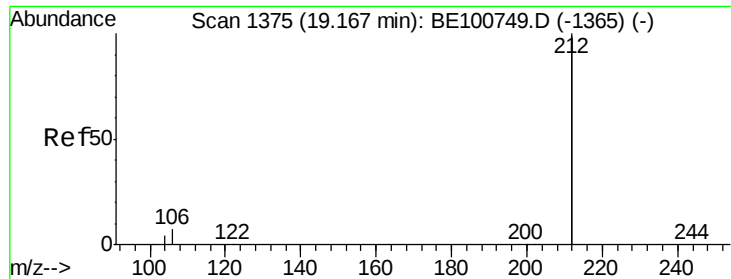




#25
 Fluoranthene-d10
 Concen: 0.207 ng
 RT: 19.18 min Scan# 1378
 Delta R.T. 0.02 min
 Lab File: BE100765.D
 Acq: 22 Nov 2019 19:36

Instrument :
 BNA_E
 ClientSampleId :
 HF-702U

Tot Ion:212 Resp: 99881
 Ion Ratio Lower Upper
 212 100
 106 3.4 2.6 4.0
 104 1.9 1.5 2.3

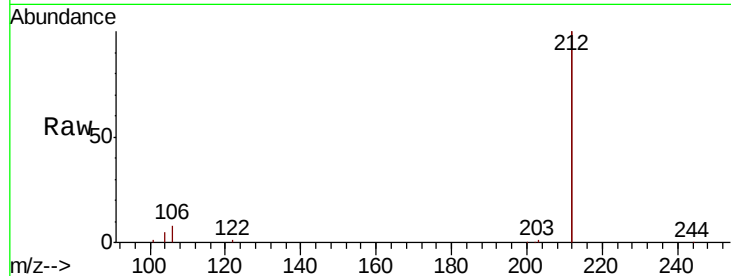


Abundance Ion 212.00 (211.70 to 212.70): E
 Ion 106.00 (105.70 to 106.70): E
 Ion 104.00 (103.70 to 104.70): E

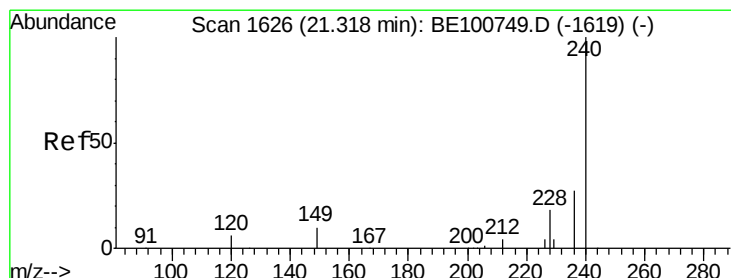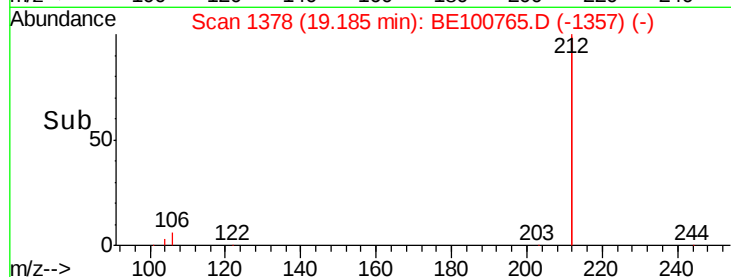
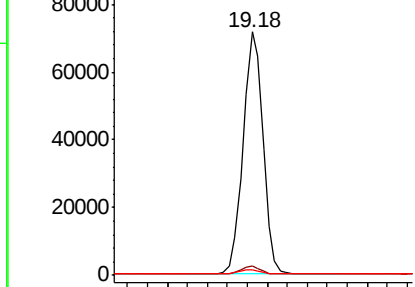



#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.32 min Scan# 1626
 Delta R.T. 0.00 min
 Lab File: BE100765.D
 Acq: 22 Nov 2019 19:36

Tgt Ion:240 Resp: 41671
 Ion Ratio Lower Upper
 240 100
 120 7.0 5.8 8.8
 236 27.1 21.9 32.9

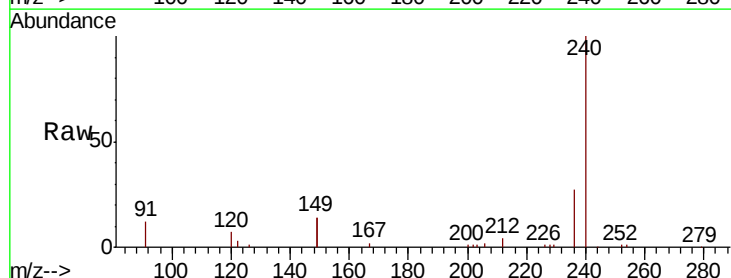

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

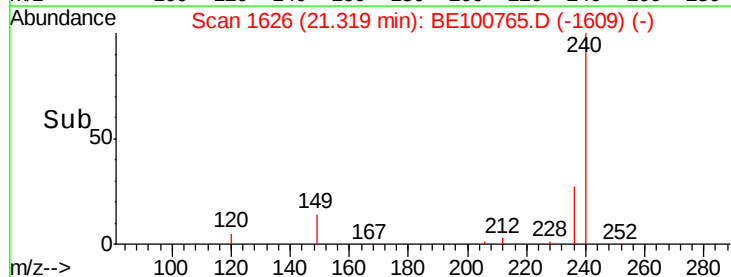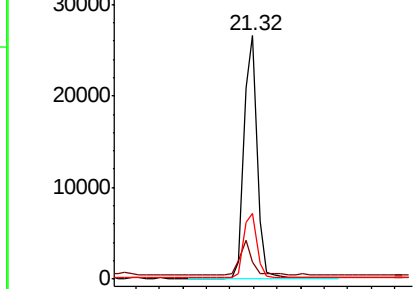



#29

Terphenyl-d14

Concen: 0.205 ng

RT: 19.77 min Scan# 1480

Delta R.T. -0.01 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36

Instrument :

BNA_E

ClientSampleId :

HF-702U


Tot Ion:244 Resp: 19644

Ion Ratio Lower Upper

244 100

212 33.4 25.2 37.8




122 15.0 9.8 14.6#

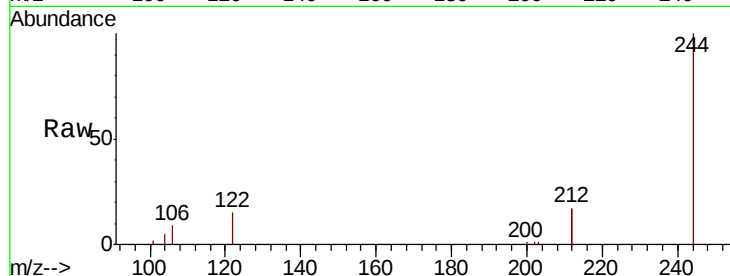

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

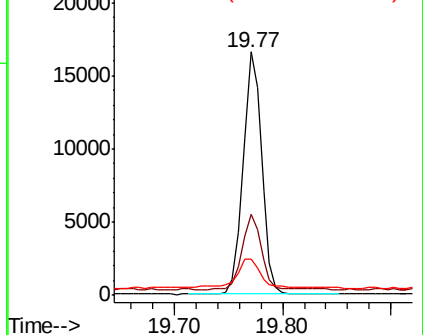

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.108 ng

RT: 21.26 min Scan# 1621

Delta R.T. 0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36


Tgt Ion:149 Resp: 28264

Ion Ratio Lower Upper

149 100

167 6.4 5.5 8.3



279 0.7 0.7 1.1




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

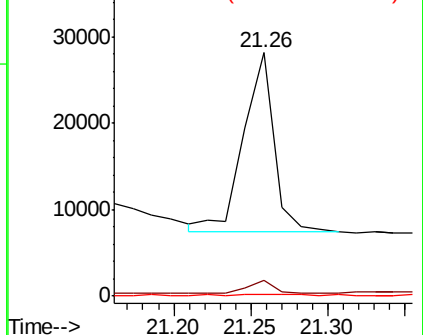

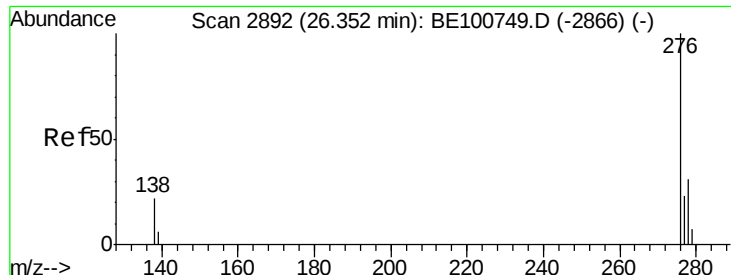

#33

Indeno(1,2,3-cd)pyrene

Concen: 0.040 ng

RT: 26.34 min Scan# 2889

Delta R.T. -0.01 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36

Instrument :

BNA_E

ClientSampleId :

HF-702U


Tot Ion:276 Resp: 522

Ion Ratio Lower Upper




276 100

138 6.3 19.8 29.6#

277 10.2 19.7 29.5#

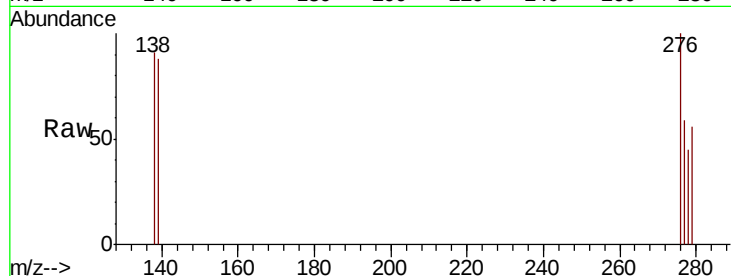

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

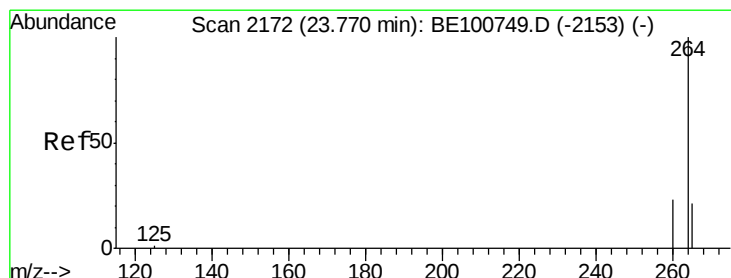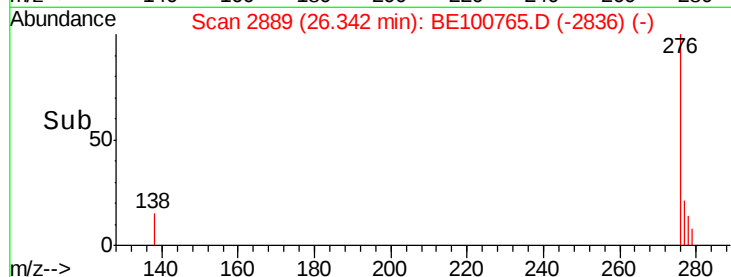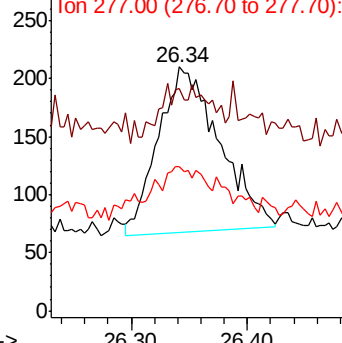

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.77 min Scan# 2171

Delta R.T. -0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36


Tgt Ion:264 Resp: 46138

Ion Ratio Lower Upper



264 100


260 24.0 18.7 28.1

265 25.1 22.4 33.6

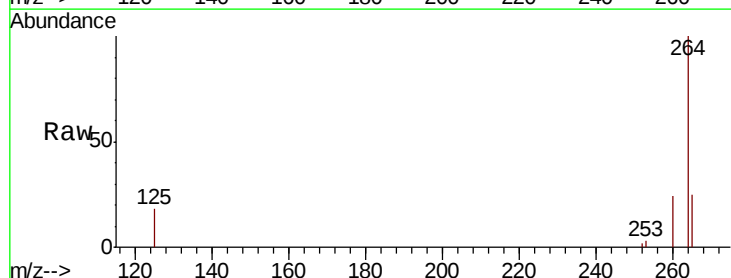

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

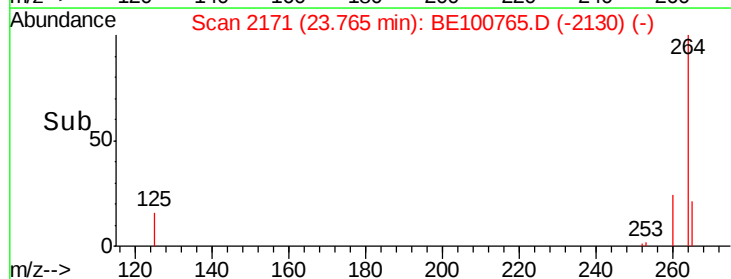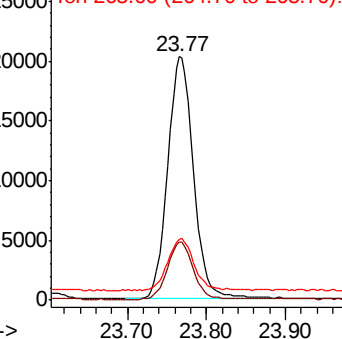

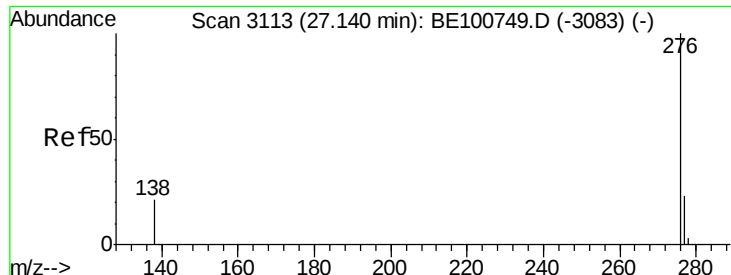

#39

Benzo(a,h,i)perylene

Concen: 0.026 ng

RT: 27.14 min Scan# 3112

Delta R.T. -0.00 min

Lab File: BE100765.D

Acq: 22 Nov 2019 19:36

Instrument :

BNA_E

ClientSampleId :

HF-702U

Tot Ion: 276 Resp: 565

Ion Ratio Lower Upper

276 100

277 52.0 18.9 28.3#

138 82.8 17.8 26.8#

