


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE112219\
 Data File : BE100755.D
 Acq On : 22 Nov 2019 12:26
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE112119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 22 06:40:44 2019

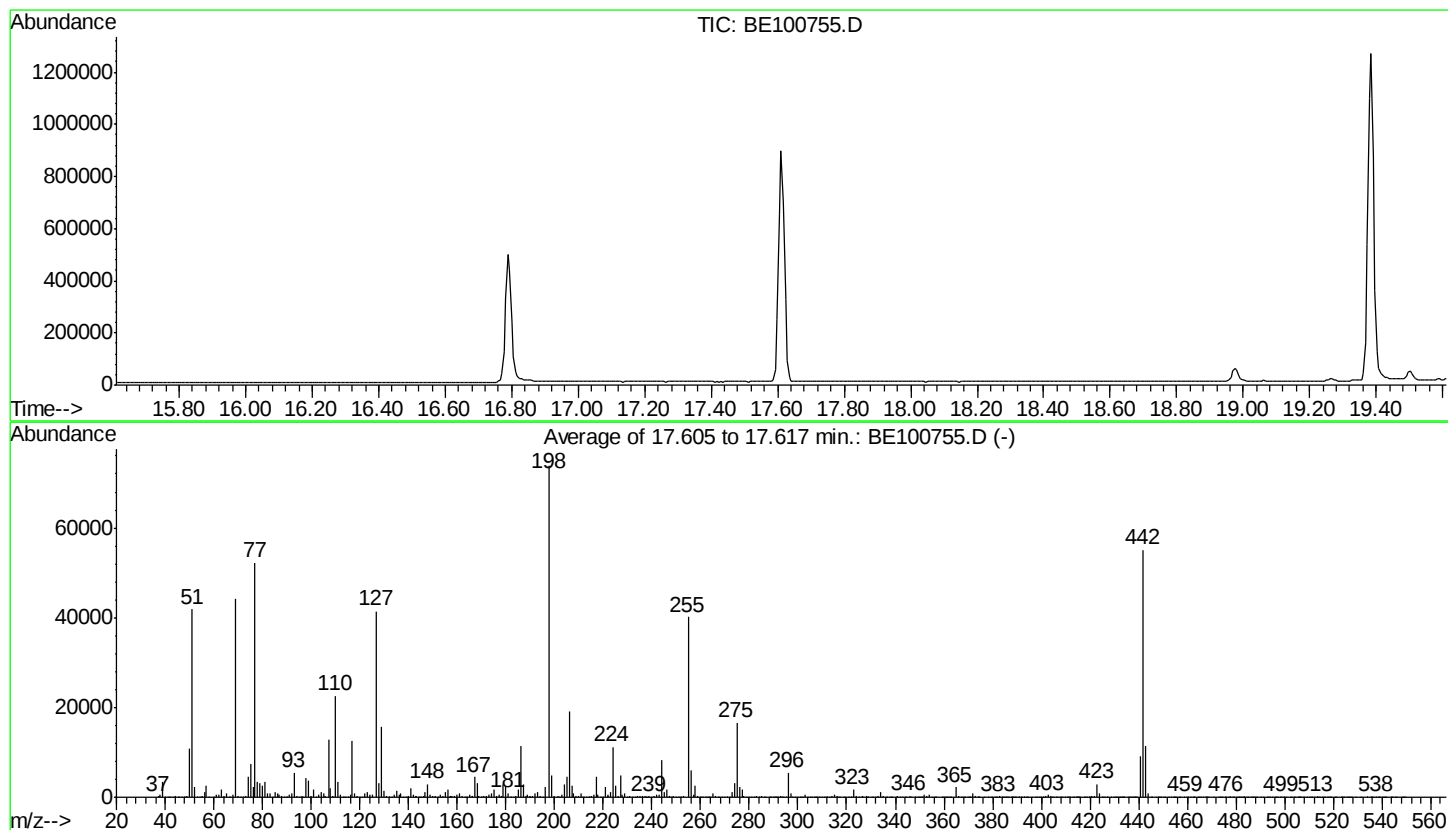

AutoFind: Scans 2556, 2557, 2558; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.6	41794	PASS
68	69	0.00	2	1.6	716	PASS
69	198	0.00	100	59.9	44207	PASS
70	69	0.00	2	0.4	180	PASS
127	198	10	80	56.0	41348	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73856	PASS
199	198	5	9	6.5	4809	PASS
275	198	10	60	22.5	16654	PASS
365	198	1	100	3.1	2281	PASS
441	198	0.01	100	12.5	9206	PASS
442	198	50	100	74.6	55088	PASS
443	442	15	24	20.7	11429	PASS