

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE112918\
 Data File : BE098278.D
 Acq On : 29 Nov 2018 17:41
 Operator : SJ/JU
 Sample : J6047-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 EP2-MW-102

Quant Time: Nov 30 01:46:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE112918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 29 13:50:43 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	1753	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	7230	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	4539	0.40	ng	0.00
19) Phenanthrene-d10	17.28	188	10743	0.40	ng	0.00
27) Chrysene-d12	21.46	240	10524	0.40	ng	0.00
34) Perylene-d12	24.01	264	10334	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.45	112	888	0.19	ng	0.01
5) Phenol-d6	7.04	99	764	0.12	ng	0.00
8) Nitrobenzene-d5	9.02	82	3451	0.47	ng	0.00
11) 2-Methylnaphthalene-d10	12.27	152	5197	0.44	ng	0.00
14) 2,4,6-Tribromophenol	16.02	330	1095	0.51	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	10408	0.55	ng	0.00
25) Fluoranthene-d10	19.31	212	59434	0.41	ng	0.00
29) Terphenyl-d14	19.91	244	11892	0.50	ng	0.00
Target Compounds						
32) Bis(2-ethylhexyl)phthalate	21.37	149	7176	0.097	ng	Qvalue # 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE112918\
Data File : BE098278.D
Acq On : 29 Nov 2018 17:41
Operator : SJ/JU
Sample : J6047-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EP2-MW-102

Quant Time: Nov 30 01:46:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE112918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 29 13:50:43 2018
Response via : Initial Calibration

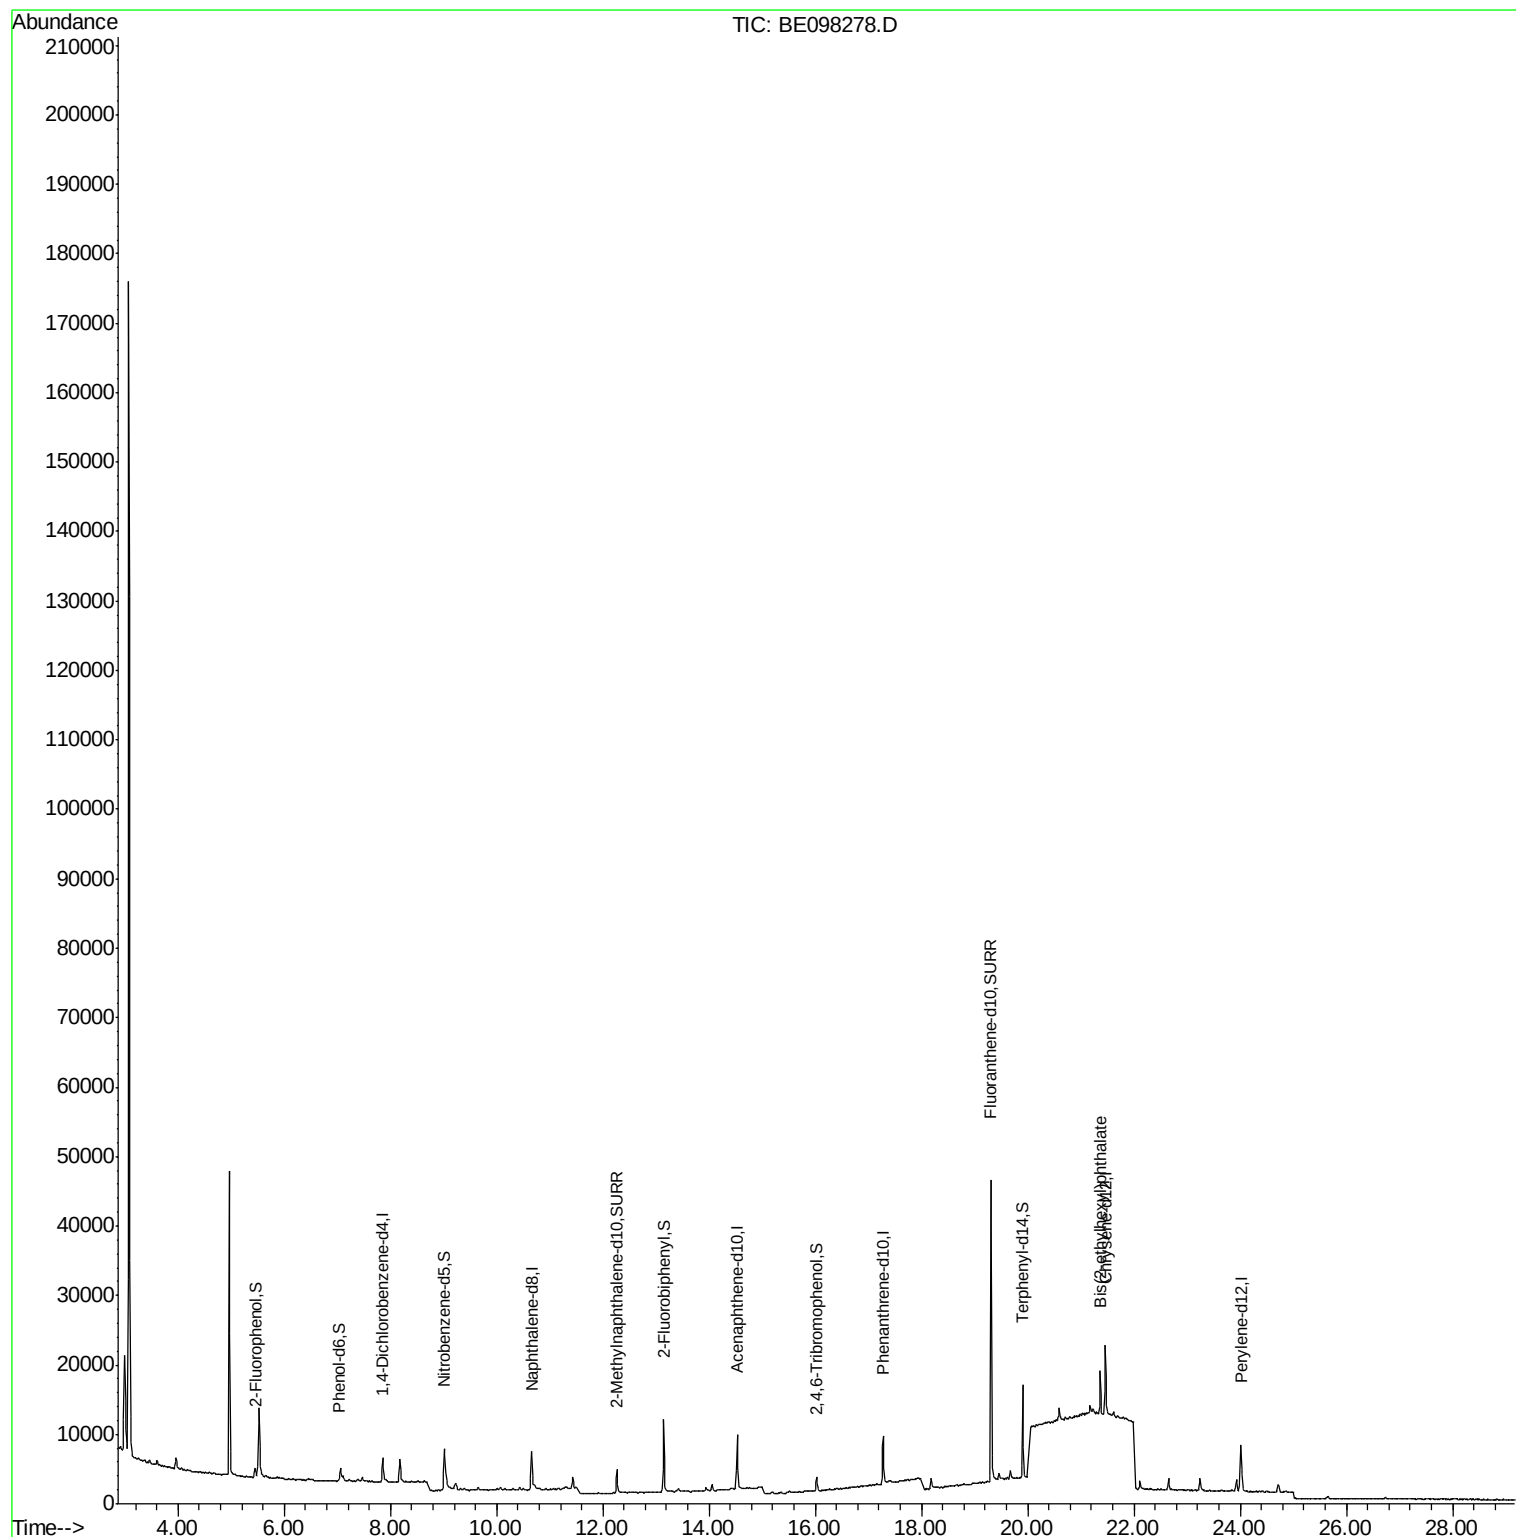

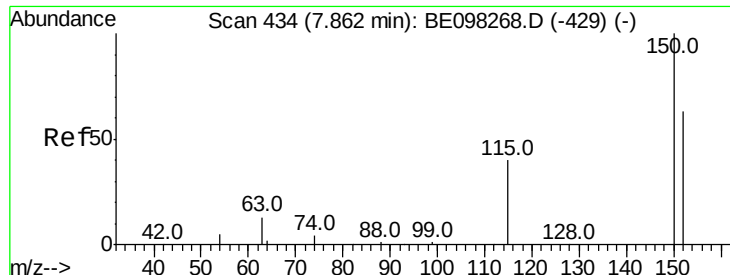

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.86 min Scan# 434

Delta R.T. -0.00 min

Lab File: BE098278.D

Acq: 29 Nov 2018 17:41

Instrument :

BNA_E

ClientSampleId :

EP2-MW-102


Tot Ion:152 Resp: 1753

Ion Ratio Lower Upper

152 100

150 151.2 124.2 186.4




115 61.7 53.9 80.9

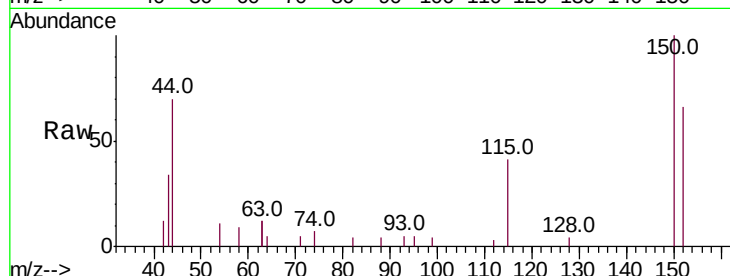

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

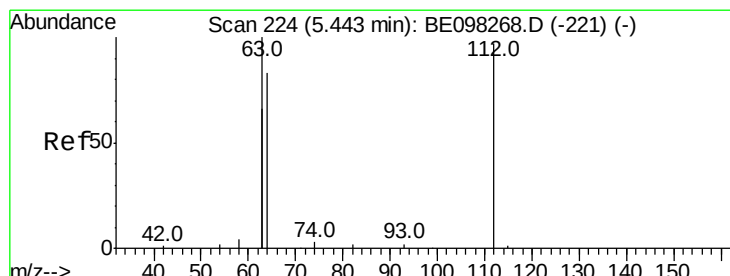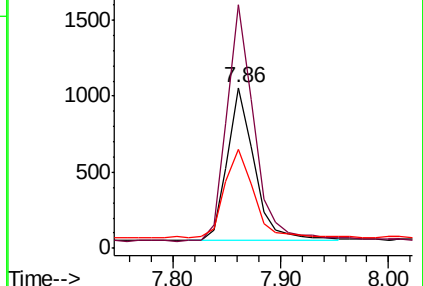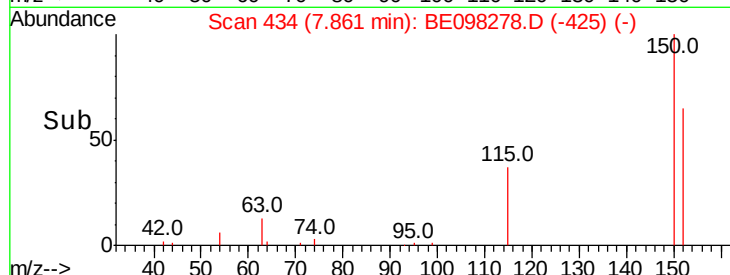

#4

2-Fluorophenol

Concen: 0.190 ng

RT: 5.45 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098278.D

Acq: 29 Nov 2018 17:41


Tgt Ion:112 Resp: 888

Ion Ratio Lower Upper

112 100

64 72.1 59.8 89.8



63 178.0 133.7 200.5

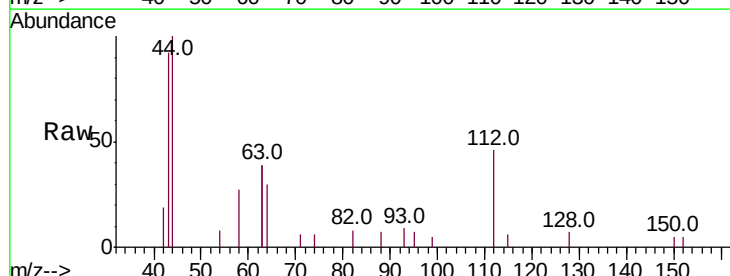


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

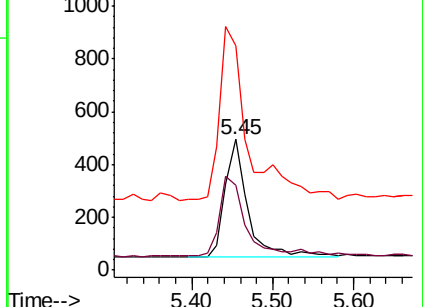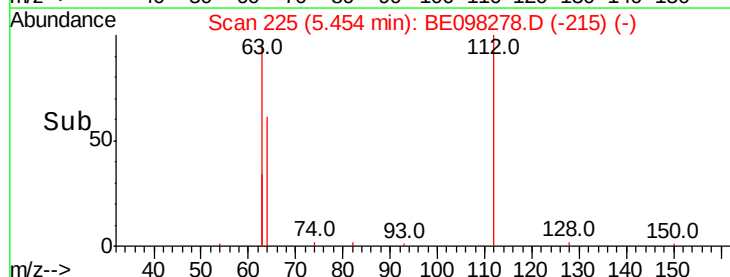

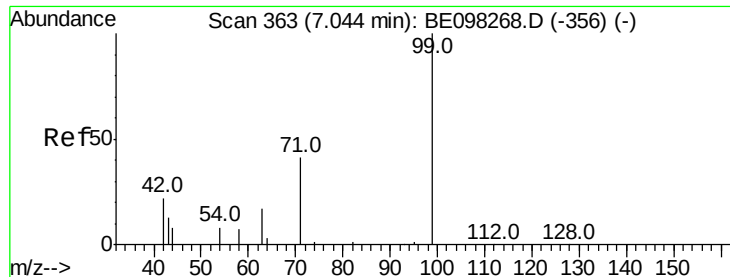

#5

Phenol-d6

Concen: 0.116 ng

RT: 7.04 min Scan# 363

Delta R.T. -0.00 min

Lab File: BE098278.D

Acq: 29 Nov 2018 17:41

Instrument :

BNA_E

ClientSampleId :

EP2-MW-102


Tot Ion: 99 Resp: 764

Ion Ratio Lower Upper

99 100

42 63.0 26.3 39.5#

71 52.4 33.6 50.4#



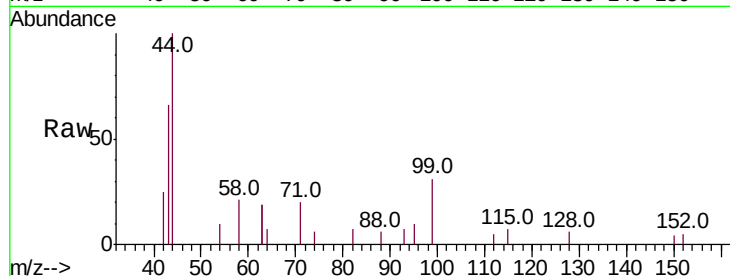


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

Time-->

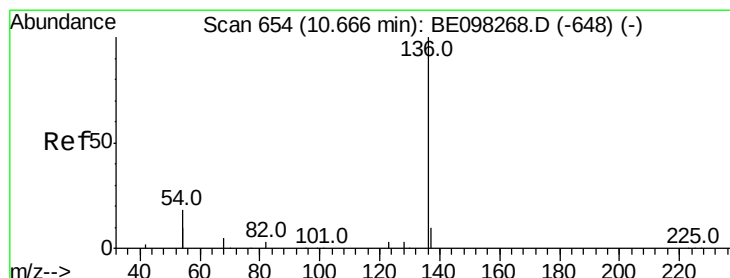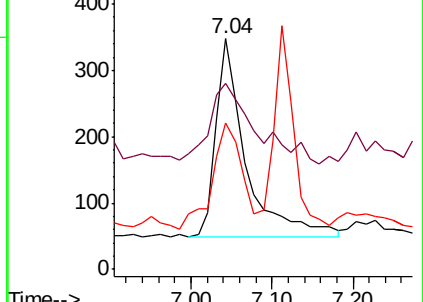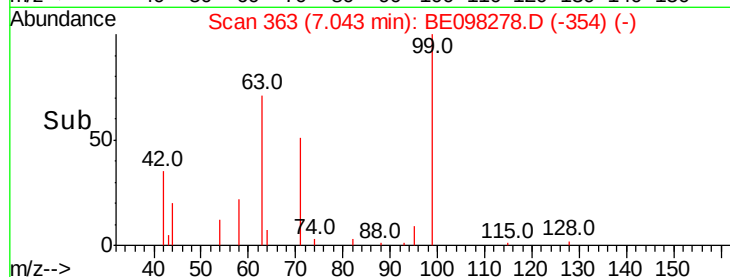

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. 0.00 min

Lab File: BE098278.D

Acq: 29 Nov 2018 17:41

Tgt Ion: 136 Resp: 7230


Ion Ratio Lower Upper

136 100

137 12.2 9.2 13.8

54 37.8 28.4 42.6

68 6.9 5.4 8.0

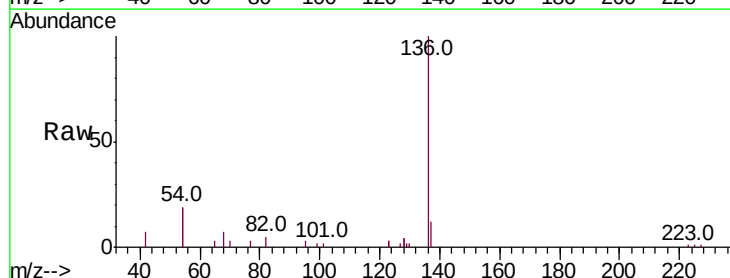



Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

Time-->

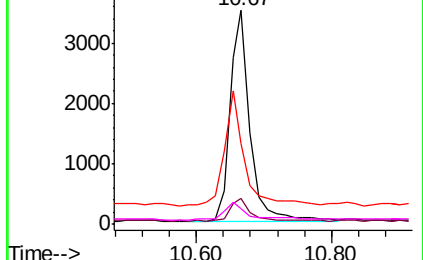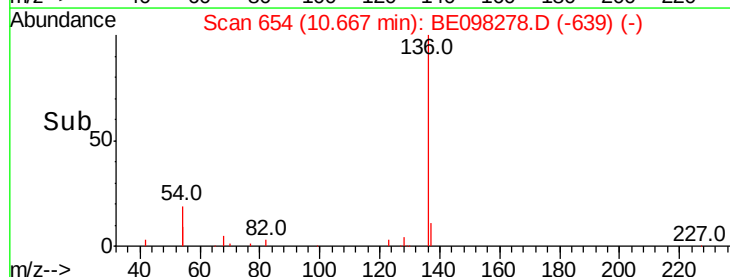



#8

Nitrobenzene-d5

Concen: 0.471 ng

RT: 9.02 min Scan# 527

Delta R.T. 0.00 min

Lab File: BE098278.D

Acq: 29 Nov 2018 17:41

Instrument :

BNA_E

ClientSampleId :

EP2-MW-102


Tot Ion: 82 Resp: 3451

Ion Ratio Lower Upper




82 100

128 127.4 102.4 153.6

54 276.4 221.8 332.8

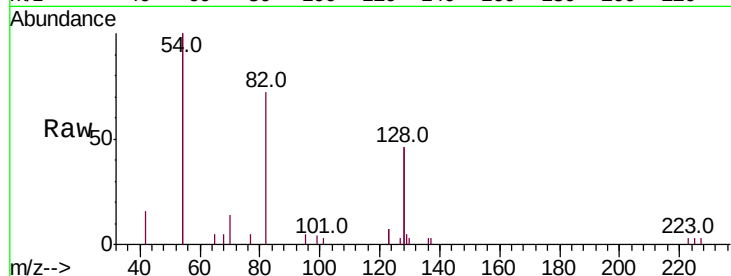

Abundance Ion 82.00 (81.70 to 82.70): BE0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BE0

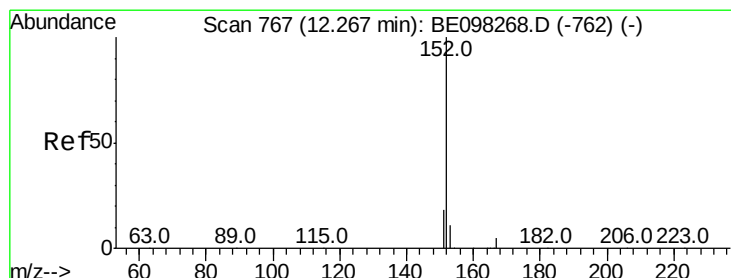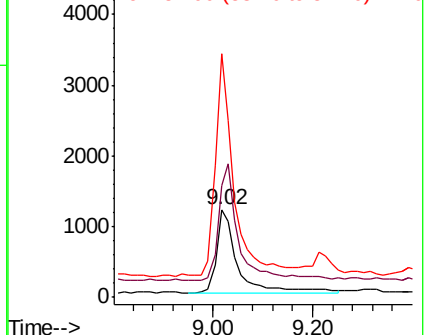

#11

2-Methylnaphthalene-d10

Concen: 0.443 ng

RT: 12.27 min Scan# 767

Delta R.T. -0.00 min

Lab File: BE098278.D


Acq: 29 Nov 2018 17:41

Tgt Ion: 152 Resp: 5197



Ion Ratio Lower Upper


152 100

151 19.8 16.2 24.4

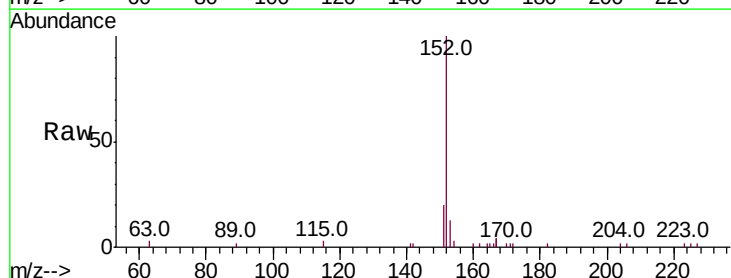

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E

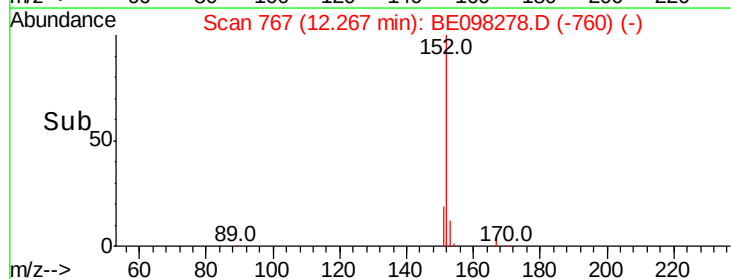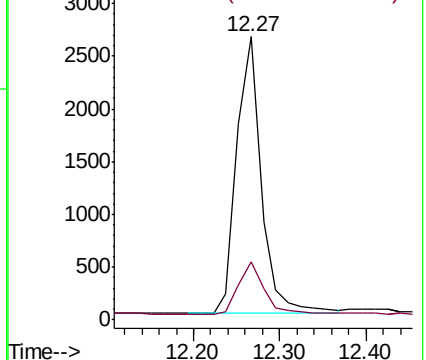

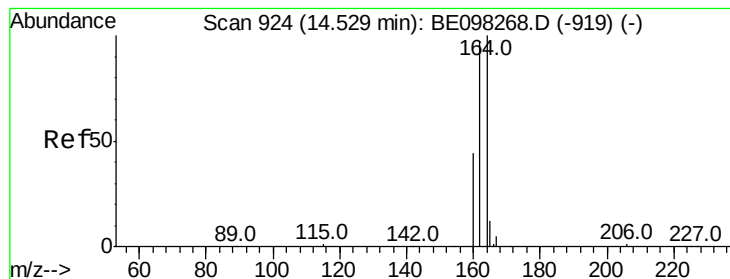

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.53 min Scan# 924

Delta R.T. -0.00 min

Lab File: BE098278.D

Acq: 29 Nov 2018 17:41

Instrument :

BNA_E

ClientSampleId :

EP2-MW-102


Tot Ion:164 Resp: 4539

Ion Ratio Lower Upper

164 100

162 99.4 77.6 116.4




160 47.9 36.0 54.0

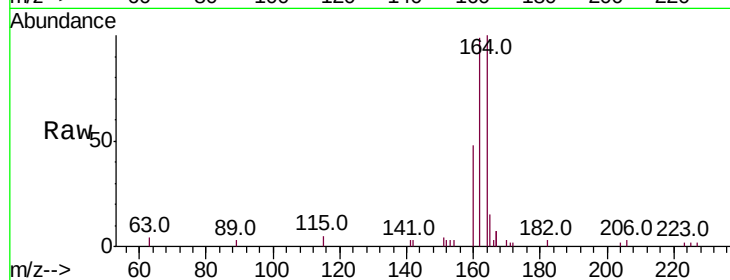

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

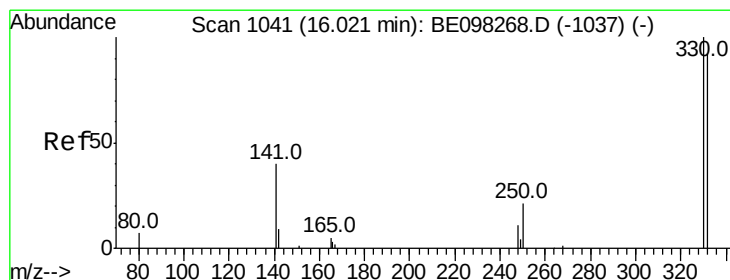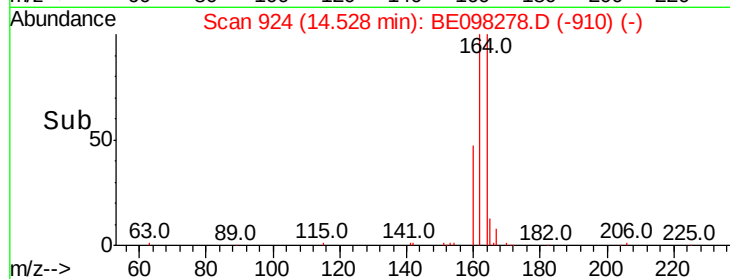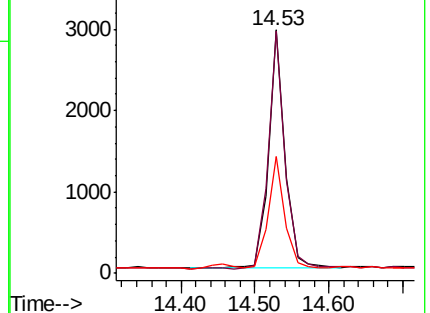

#14

2,4,6-Tribromophenol

Concen: 0.509 ng

RT: 16.02 min Scan# 1041

Delta R.T. 0.00 min

Lab File: BE098278.D

Acq: 29 Nov 2018 17:41


Tgt Ion:330 Resp: 1095

Ion Ratio Lower Upper

330 100

332 95.9 76.2 114.4



141 49.4 39.0 58.4

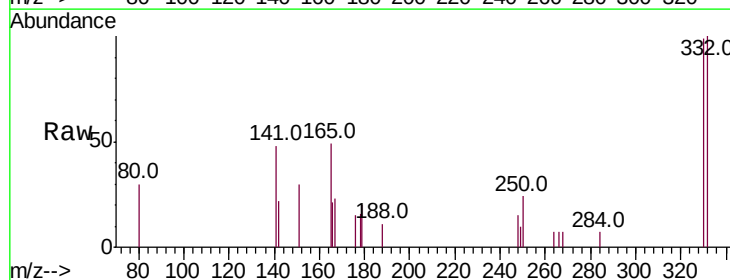


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

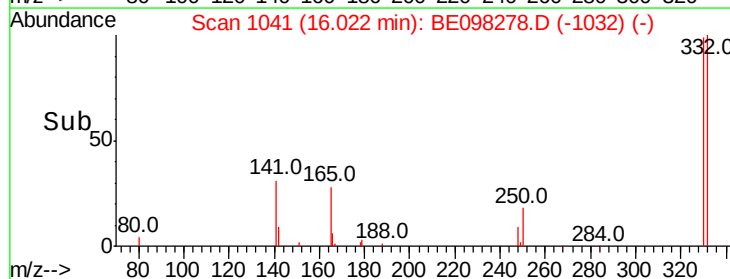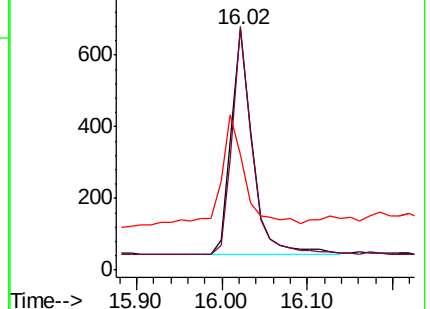







#15
2-Fluorobiphenyl
Concen: 0.554 ng
RT: 13.15 min Scan# 828
Delta R.T. -0.00 min
Lab File: BE098278.D
Acq: 29 Nov 2018 17:41

Instrument :
BNA_E
ClientSampleId :
EP2-MW-102

Tot Ion:172 Resp: 10408
Ion Ratio Lower Upper
172 100
171 32.5 27.5 41.3
170 23.0 19.6 29.4

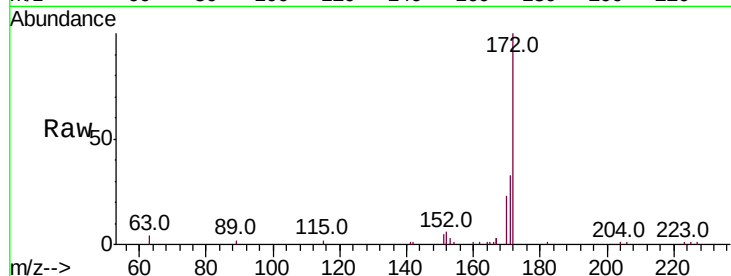


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

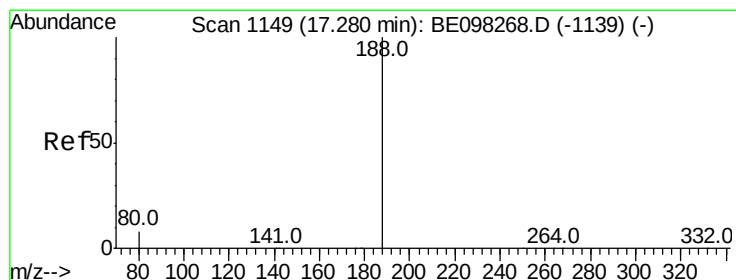
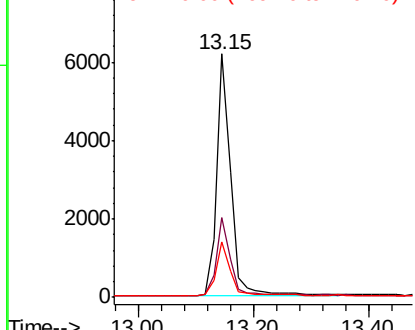



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.28 min Scan# 1149
Delta R.T. 0.00 min
Lab File: BE098278.D
Acq: 29 Nov 2018 17:41

Tgt Ion:188 Resp: 10743
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.3 7.2 10.8#

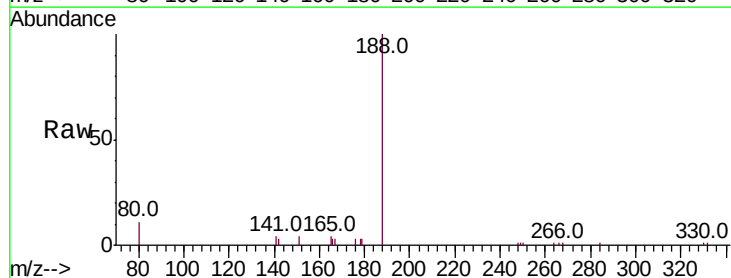

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0




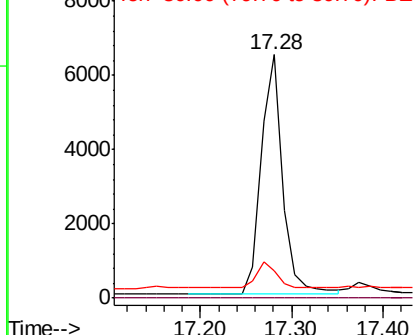




#25
Fluoranthene-d10
Concen: 0.410 ng
RT: 19.31 min Scan# 1433
Delta R.T. -0.00 min
Lab File: BE098278.D
Acq: 29 Nov 2018 17:41




Instrument :
BNA_E
ClientSampled :
EP2-MW-102


Tot Ion:212 Resp: 59434
Ion Ratio Lower Upper
212 100
106 2.8 2.2 3.2
104 1.6 1.3 1.9

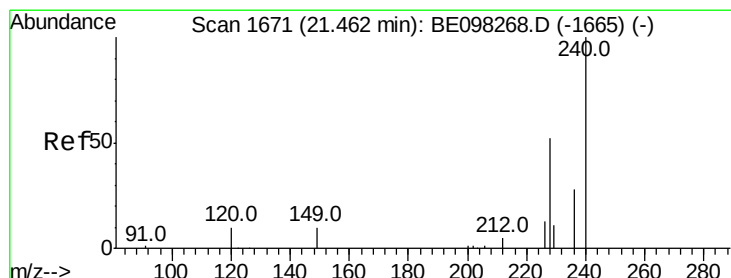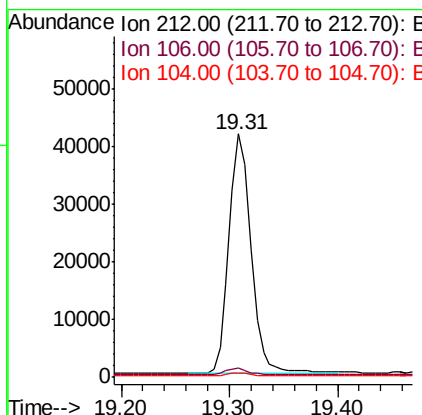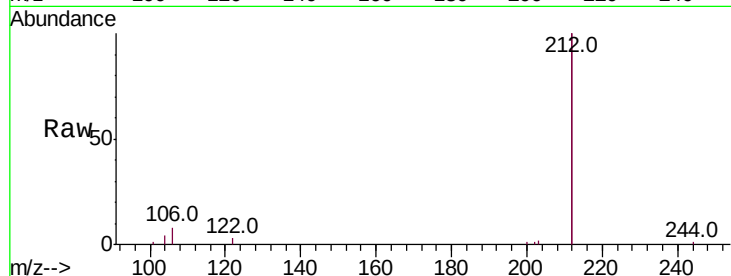

#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.46 min Scan# 1671
Delta R.T. 0.00 min
Lab File: BE098278.D
Acq: 29 Nov 2018 17:41

Tgt Ion:240 Resp: 10524
Ion Ratio Lower Upper
240 100
120 15.2 9.5 14.3#
236 28.7 22.7 34.1

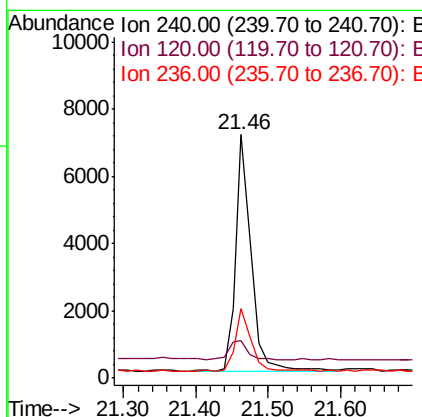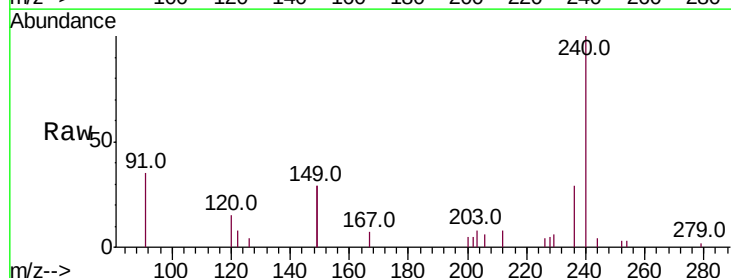

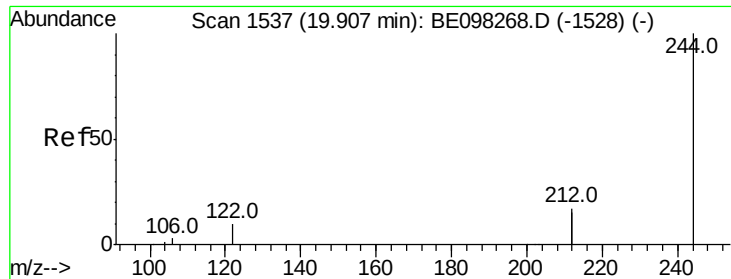

#29

Terphenyl-d14

Concen: 0.502 ng

RT: 19.91 min Scan# 1537

Delta R.T. -0.00 min

Lab File: BE098278.D

Acq: 29 Nov 2018 17:41

Instrument :

BNA_E

ClientSampleId :

EP2-MW-102


Tot Ion:244 Resp: 11892

Ion Ratio Lower Upper

244 100

212 39.7 27.4 41.0




122 14.3 8.3 12.5#

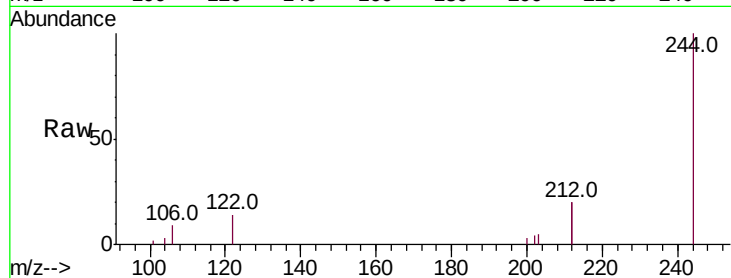

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

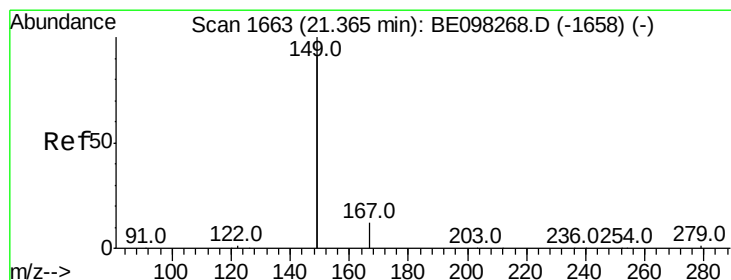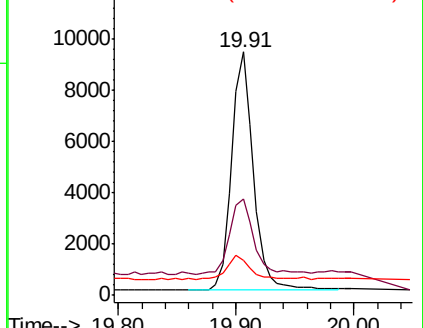

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.097 ng

RT: 21.37 min Scan# 1663

Delta R.T. 0.00 min

Lab File: BE098278.D

Acq: 29 Nov 2018 17:41


Tgt Ion:149 Resp: 7176

Ion Ratio Lower Upper

149 100

167 7.1 5.7 8.5



279 2.3 1.0 1.4#



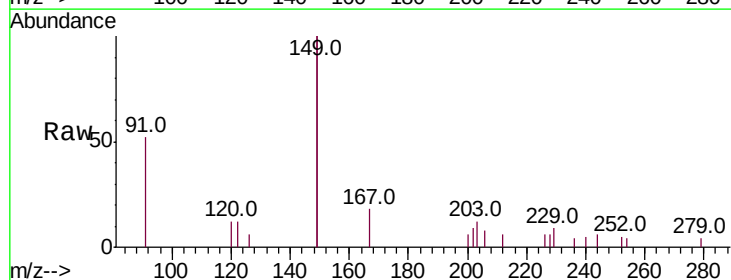


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

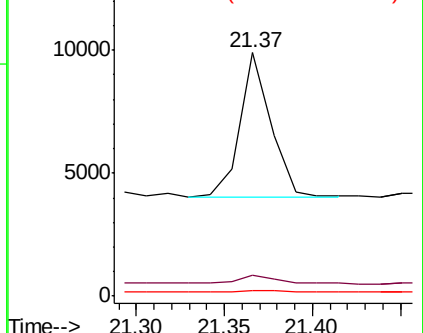

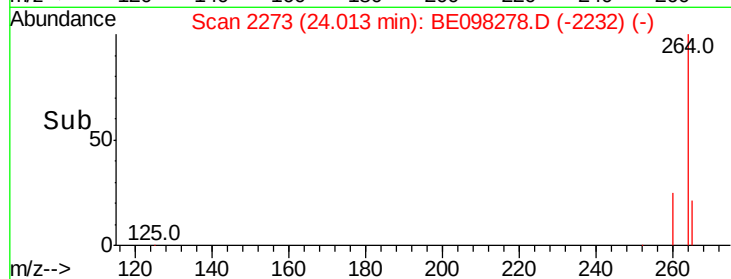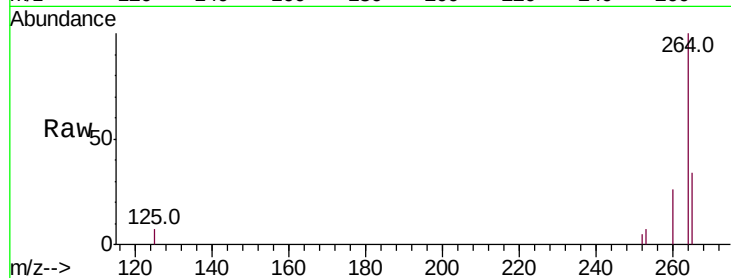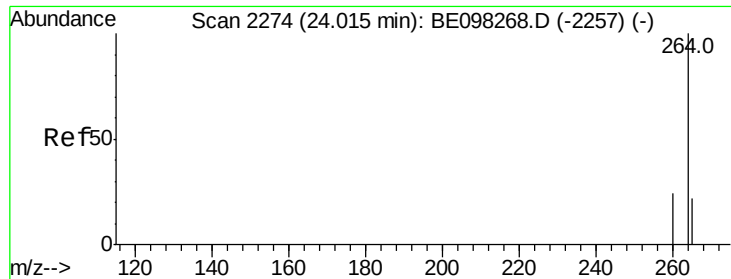

#34
Pervlene-d12
Concen: 0.400 ng
RT: 24.01 min Scan# 2273
Delta R.T. -0.00 min
Lab File: BE098278.D
Acq: 29 Nov 2018 17:41

Instrument :
BNA_E
ClientSampleId :
EP2-MW-102

Tot Ion:264 Resp: 10334
Ion Ratio Lower Upper
264 100
260 26.2 20.2 30.2
265 33.9 25.2 37.8

