


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE112918\
 Data File : BE098265.D
 Acq On : 29 Nov 2018 9:27
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE112918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 29 13:50:43 2018

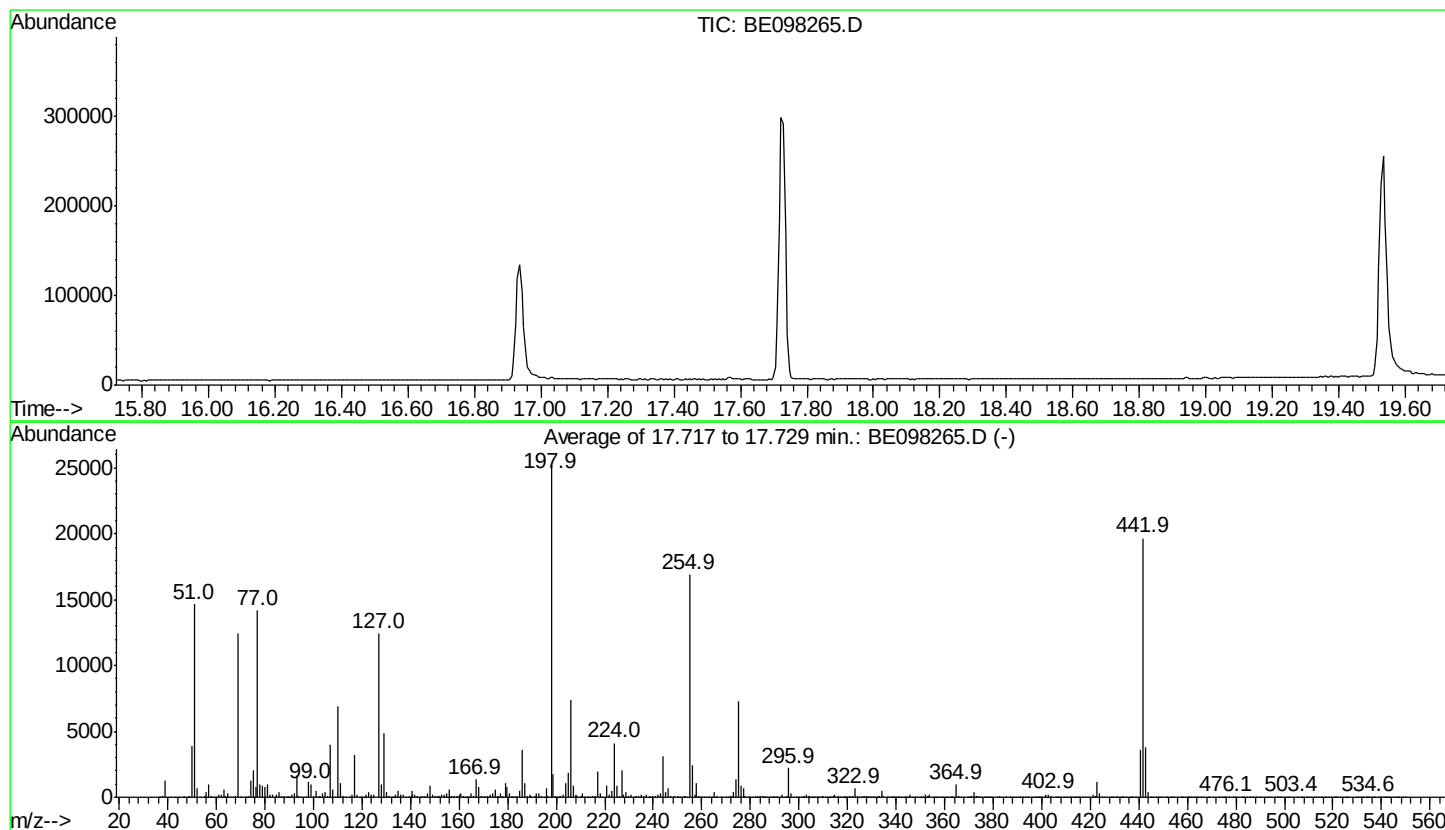

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.2	14645	PASS
68	69	0.00	2	1.1	142	PASS
69	198	0.00	100	49.5	12454	PASS
70	69	0.00	2	0.3	43	PASS
127	198	10	80	49.3	12422	PASS
197	198	0.00	2	0.6	147	PASS
198	198	100	100	100.0	25175	PASS
199	198	5	9	7.0	1773	PASS
275	198	10	60	29.1	7336	PASS
365	198	1	100	3.7	942	PASS
441	198	0.01	100	14.4	3625	PASS
442	198	50	100	78.2	19681	PASS
443	442	15	24	19.2	3783	PASS