


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE120419\
Data File : BE100770.D
Acq On : 4 Dec 2019 11:20
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE120419.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 04 17:18:11 2019

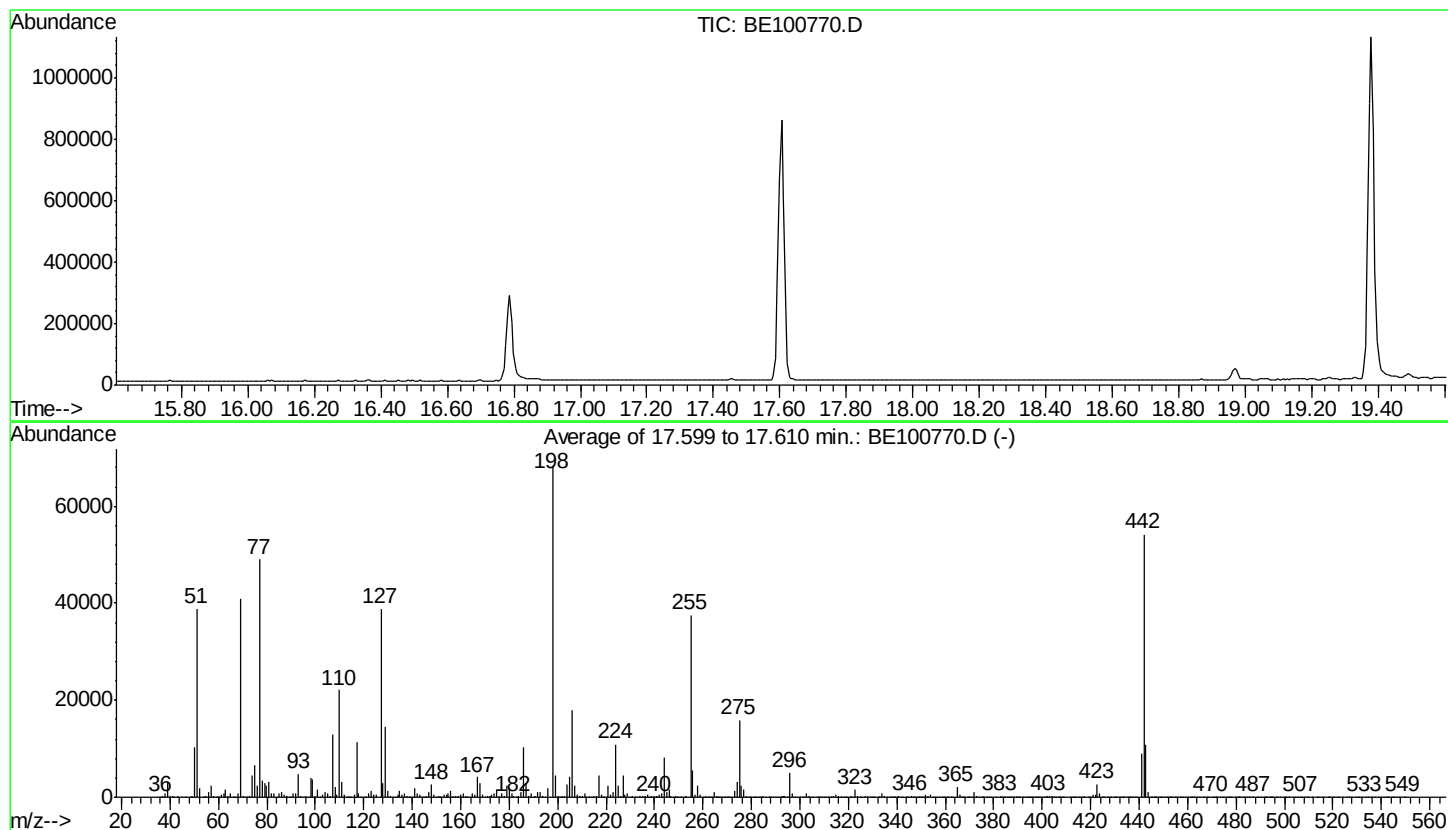

AutoFind: Scans 2555, 2556, 2557; Background Corrected with Scan 2549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.9	38924	PASS
68	69	0.00	2	1.9	764	PASS
69	198	0.00	100	59.8	40869	PASS
70	69	0.00	2	0.5	221	PASS
127	198	10	80	56.8	38835	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68378	PASS
199	198	5	9	6.7	4555	PASS
275	198	10	60	23.2	15882	PASS
365	198	1	100	3.1	2120	PASS
441	198	0.01	100	12.9	8853	PASS
442	198	50	100	79.2	54133	PASS
443	442	15	24	20.2	10922	PASS