

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE120519\
 Data File : BE100786.D
 Acq On : 5 Dec 2019 13:19
 Operator : JU
 Sample : PB125153BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Dec 05 14:37:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 04 17:18:11 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	5285	0.40	ng	0.00
7) Naphthalene-d8	10.54	136	21054	0.40	ng	0.00
13) Acenaphthene-d10	14.40	164	9536	0.40	ng	0.00
19) Phenanthrene-d10	17.12	188	21167	0.40	ng	-0.01
27) Chrysene-d12	21.31	240	18444	0.40	ng	0.00
34) Perylene-d12	23.76	264	20222	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.38	112	4541	0.36	ng	0.00
5) Phenol-d6	6.93	99	7309	0.39	ng	0.00
8) Nitrobenzene-d5	8.90	82	4228	0.42	ng	0.00
11) 2-Methylnaphthalene-d10	12.14	152	11518	0.38	ng	0.00
14) 2,4,6-Tribromophenol	15.88	330	238	0.22	ng	0.00
15) 2-Fluorobiphenyl	13.03	172	16968	0.45	ng	0.00
25) Fluoranthene-d10	19.16	212	93757	0.37	ng	0.00
29) Terphenyl-d14	19.76	244	20695	0.47	ng	0.00
Target Compounds						
3) n-Nitrosodimethylamine	3.70	42	239	0.030	ng	# 5
22) Pentachlorophenol	16.77	266	24	0.031	ng	93
32) Bis(2-ethylhexyl)phthalate	21.24	149	402	Below Cal	#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE120519\
Data File : BE100786.D
Acq On : 5 Dec 2019 13:19
Operator : JU
Sample : PB125153BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Dec 05 14:37:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 04 17:18:11 2019
Response via : Initial Calibration

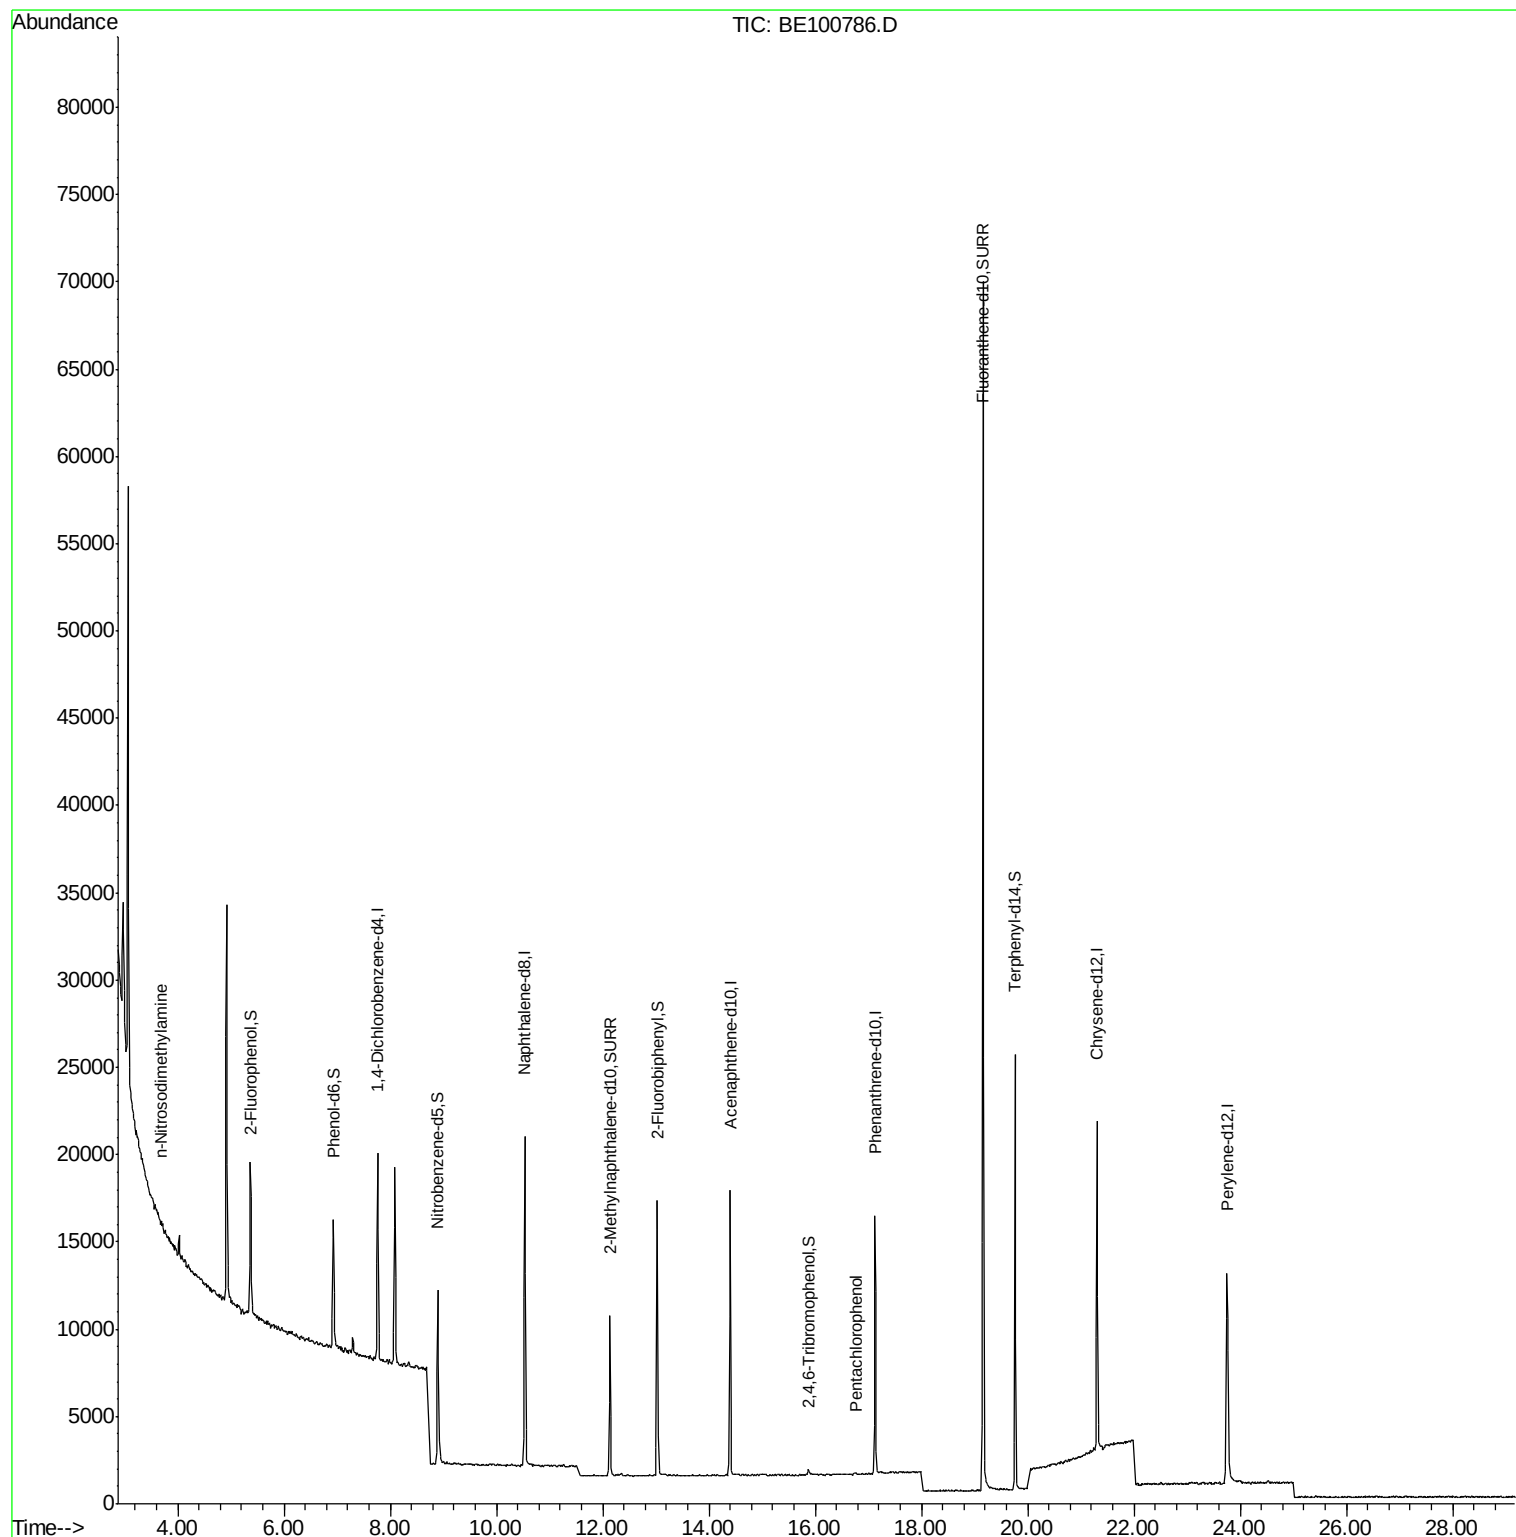

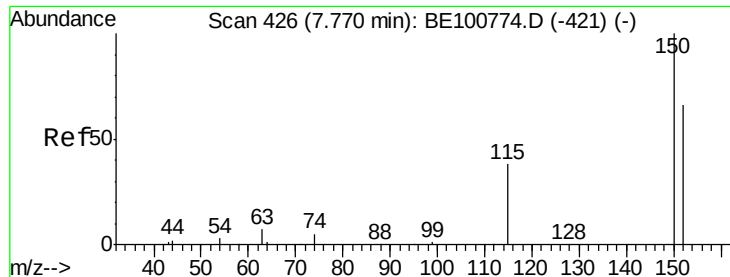


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.76 min Scan# 425
Delta R.T. -0.01 min
Lab File: BE100786.D
Acq: 5 Dec 2019 13:19

Instrument :
BNA_E
ClientSampleId :

Tot Ion:152 Resp: 5285
Ion Ratio Lower Upper
152 100
150 161.3 120.6 181.0
115 70.2 47.4 71.2

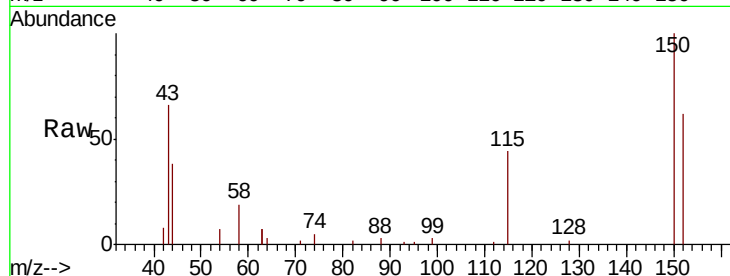


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

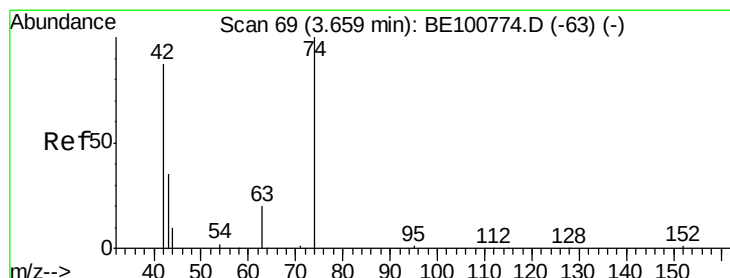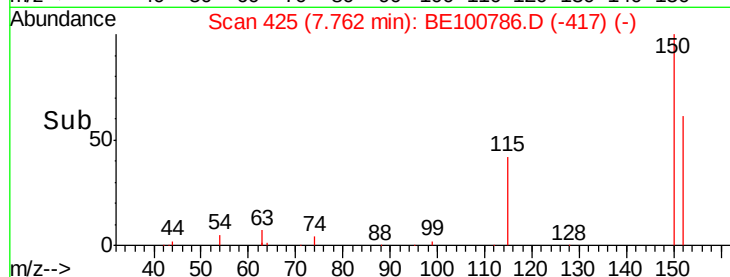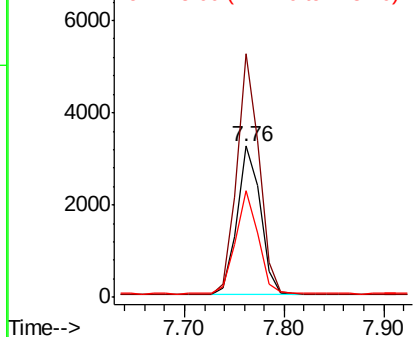



#3


n-Nitrosodimethylamine
Concen: 0.030 ng
RT: 3.70 min Scan# 72
Delta R.T. 0.04 min
Lab File: BE100786.D
Acq: 5 Dec 2019 13:19

Tgt Ion: 42 Resp: 239
Ion Ratio Lower Upper
42 100
74 0.0 86.3 129.5#
44 0.0 11.6 17.4#

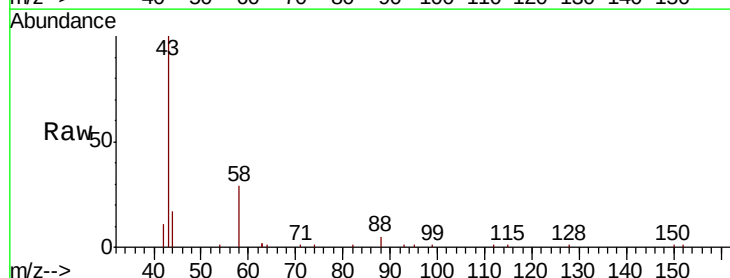

Abundance Ion 42.00 (41.70 to 42.70): BE1
Ion 74.00 (73.70 to 74.70): BE1
Ion 44.00 (43.70 to 44.70): BE1

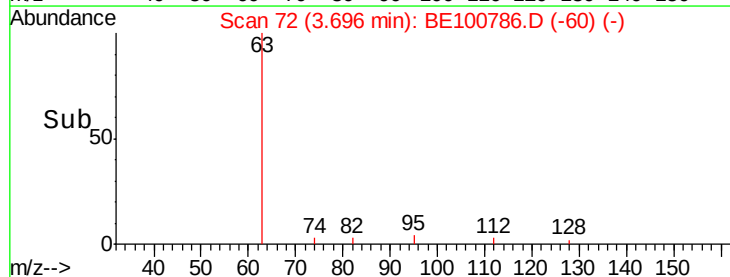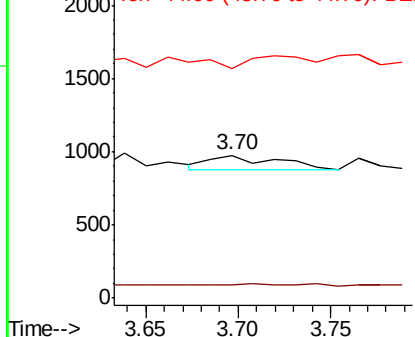



#4

2-Fluorophenol

Concen: 0.362 ng

RT: 5.38 min Scan# 218

Delta R.T. 0.00 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19

Instrument :

BNA_E

ClientSampleId :


Tot Ion:112 Resp: 4541

Ion Ratio Lower Upper

112 100

64 66.9 54.1 81.1




63 144.8 113.2 169.8



Abundance Ion 112.00 (111.70 to 112.70): BE1

Ion 64.00 (63.70 to 64.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

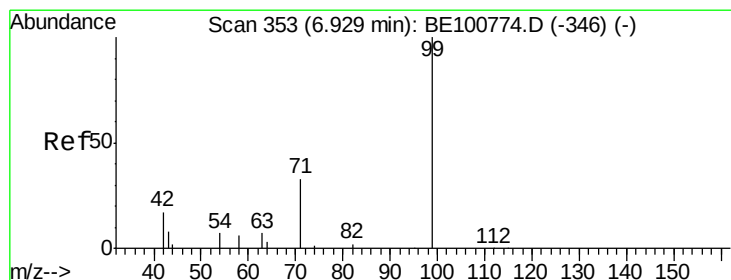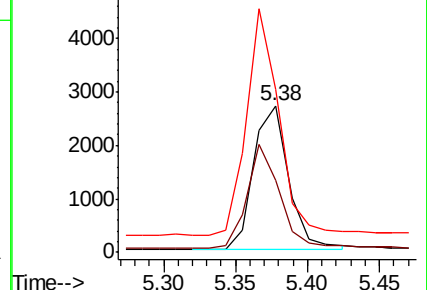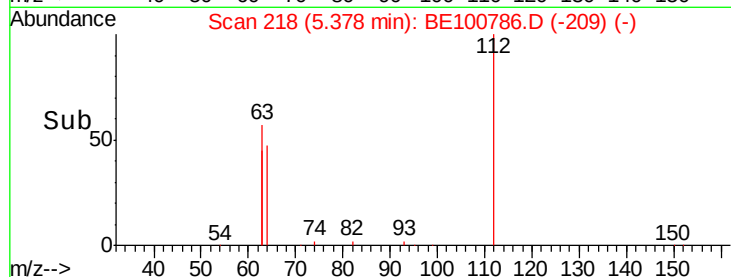

#5

Phenol-d6

Concen: 0.386 ng

RT: 6.93 min Scan# 353

Delta R.T. 0.00 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19


Tgt Ion: 99 Resp: 7309

Ion Ratio Lower Upper

99 100

42 24.1 19.1 28.7



71 36.4 27.7 41.5




Abundance Ion 99.00 (98.70 to 99.70): BE1

Ion 42.00 (41.70 to 42.70): BE1

Ion 71.00 (70.70 to 71.70): BE1

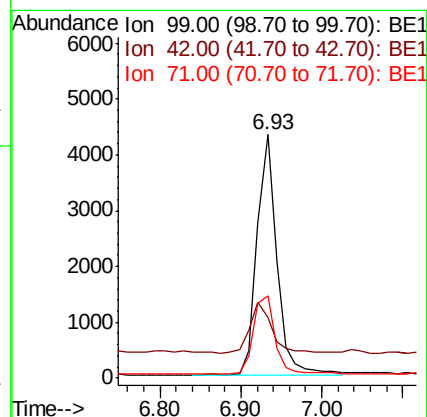

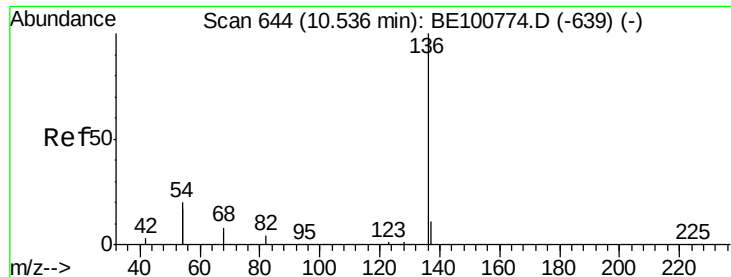

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.54 min Scan# 644

Delta R.T. 0.00 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19

Instrument :

BNA_E

ClientSampleId :

Tot Ion:136 Resp: 21054


Ion Ratio Lower Upper

136 100

137 11.2 9.4 14.0

54 33.9 31.1 46.7

68 7.9 6.6 10.0



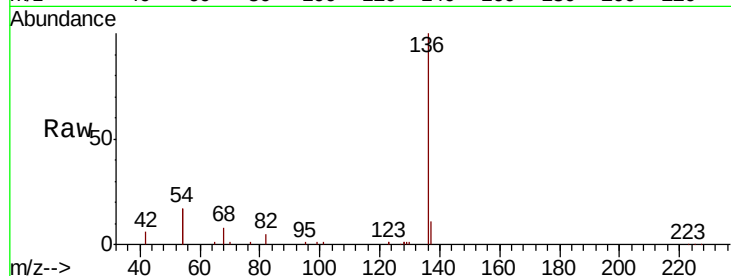


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE1

Ion 68.00 (67.70 to 68.70): BE1

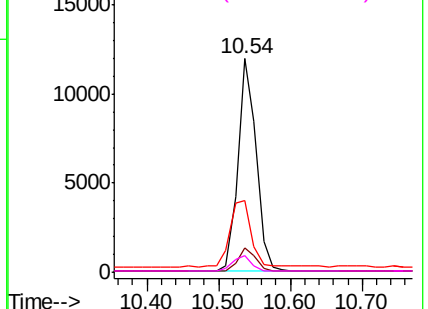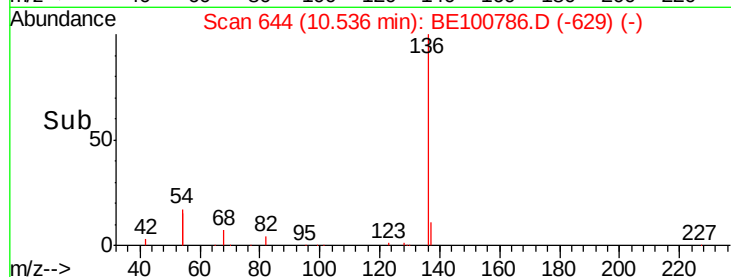

#8

Nitrobenzene-d5

Concen: 0.422 ng

RT: 8.90 min Scan# 518

Delta R.T. 0.00 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19


Tgt Ion: 82 Resp: 4228

Ion Ratio Lower Upper

82 100

128 123.2 97.0 145.4



54 203.0 171.8 257.6




Abundance Ion 82.00 (81.70 to 82.70): BE1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE1



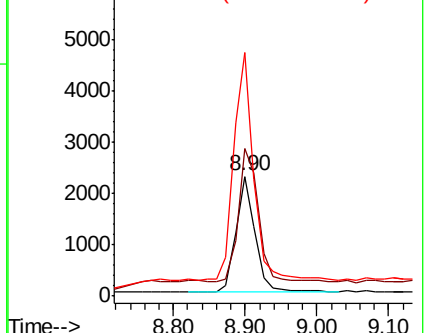
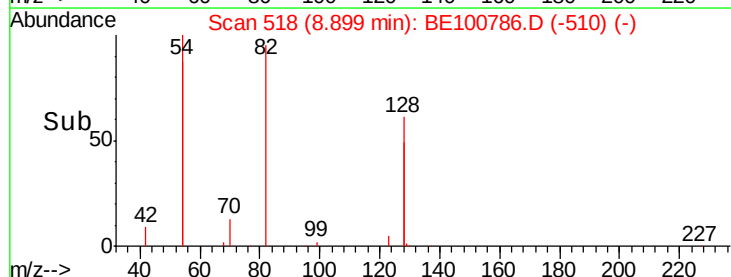


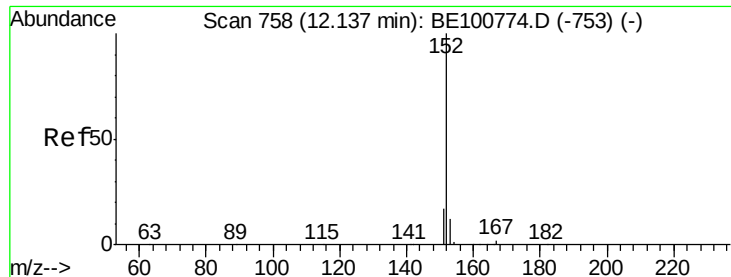

#11
 2-Methylnaphthalene-d10
 Concen: 0.378 ng
 RT: 12.14 min Scan# 758
 Delta R.T. 0.00 min
 Lab File: BE100786.D
 Acq: 5 Dec 2019 13:19




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:152 Resp: 11518
 Ion Ratio Lower Upper
 152 100
 151 19.3 15.8 23.8

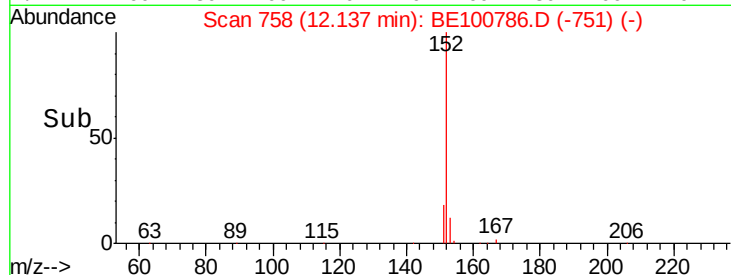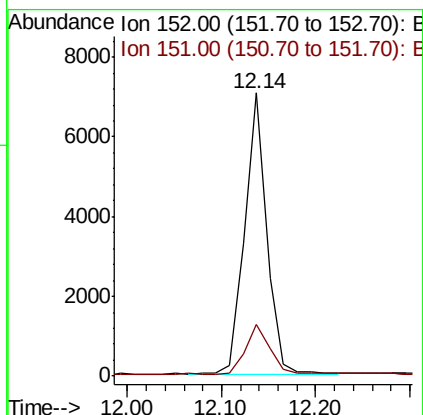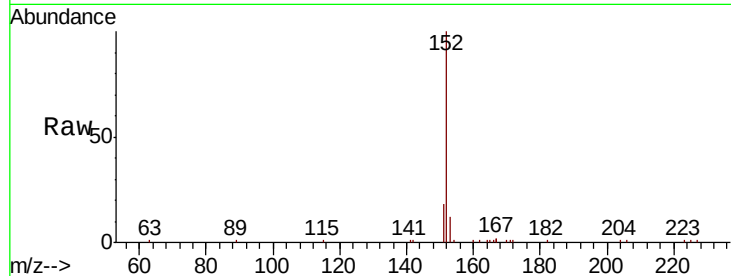

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.40 min Scan# 915
 Delta R.T. 0.00 min
 Lab File: BE100786.D
 Acq: 5 Dec 2019 13:19

Tgt Ion:164 Resp: 9536
 Ion Ratio Lower Upper
 164 100
 162 102.0 81.4 122.0
 160 49.0 39.4 59.0

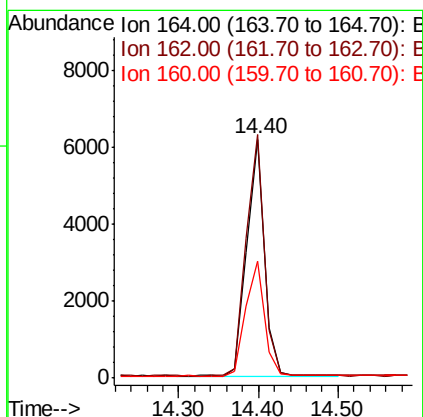







#14
 2,4,6-Tribromophenol
 Concen: 0.224 ng
 RT: 15.88 min Scan# 1019
 Delta R.T. -0.00 min
 Lab File: BE100786.D
 Acq: 5 Dec 2019 13:19

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:330 Resp: 238
 Ion Ratio Lower Upper
 330 100
 332 95.0 69.4 104.2
 141 90.3 51.1 76.7#




Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

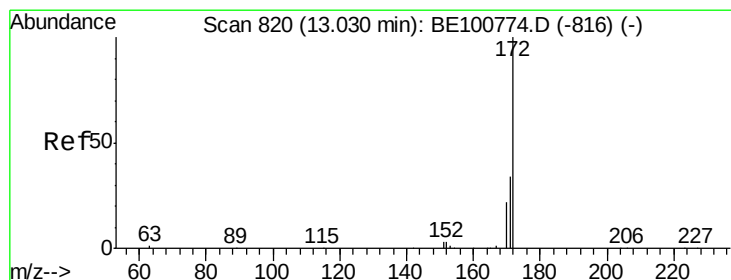
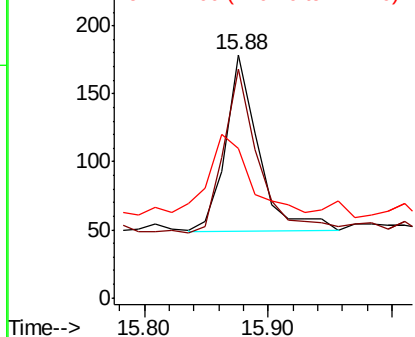



#15
 2-Fluorobiphenyl
 Concen: 0.449 ng
 RT: 13.03 min Scan# 820
 Delta R.T. 0.00 min
 Lab File: BE100786.D
 Acq: 5 Dec 2019 13:19

Tgt Ion:172 Resp: 16968
 Ion Ratio Lower Upper
 172 100
 171 32.8 27.2 40.8
 170 22.0 18.0 27.0

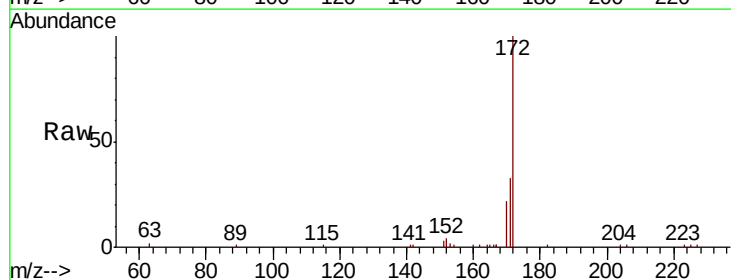

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

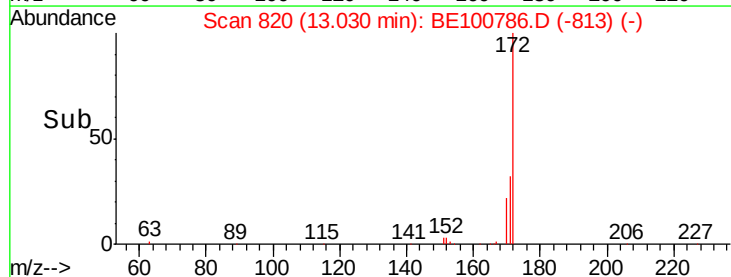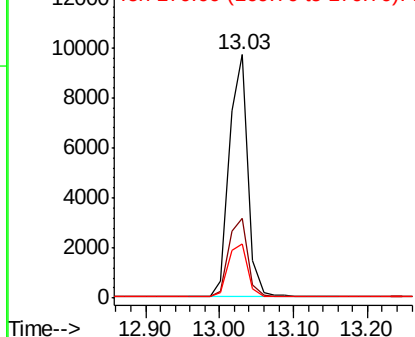



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.12 min Scan# 1112

Delta R.T. -0.01 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19

Instrument :

BNA_E

ClientSampleId :


Tot Ion:188 Resp: 21167

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 14.7 5.2 7.8#

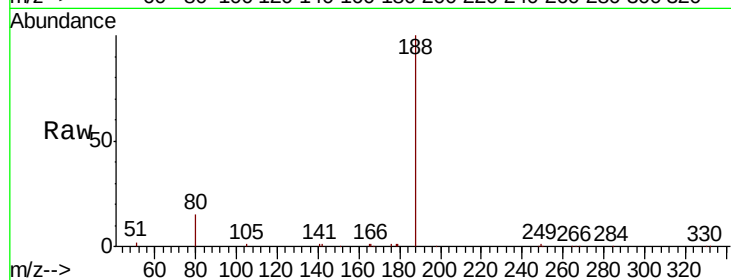

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE1

Ion 80.00 (79.70 to 80.70): BE1

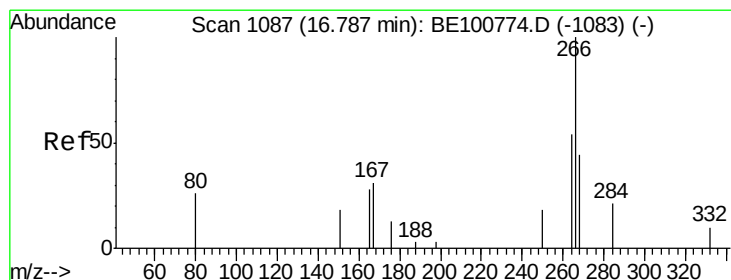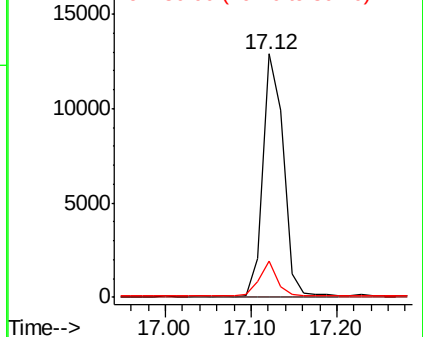

#22

Pentachlorophenol

Concen: 0.031 ng

RT: 16.77 min Scan# 1086

Delta R.T. -0.01 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19


Tgt Ion:266 Resp: 24

Ion Ratio Lower Upper

266 100

264 84.1 63.4 95.0



268 90.5 65.8 98.8

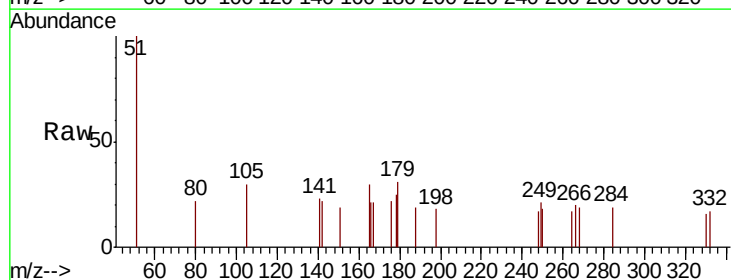


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

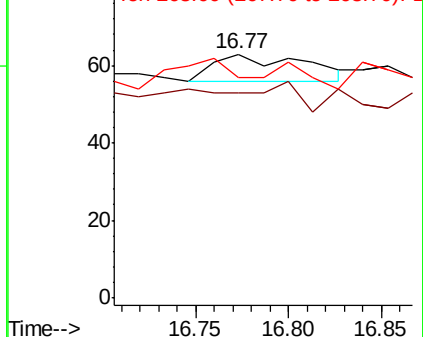



#25

Fluoranthene-d10

Concen: 0.375 ng

RT: 19.16 min Scan# 1374

Delta R.T. -0.00 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19

Instrument :

BNA_E

ClientSampleId :


Tot Ion:212 Resp: 93757

Ion Ratio Lower Upper

212 100

106 3.2 2.6 3.8




104 1.8 1.4 2.2

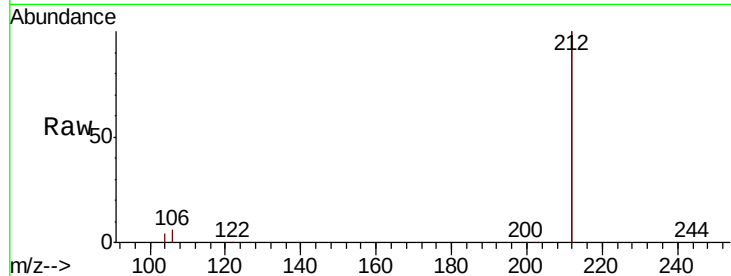

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

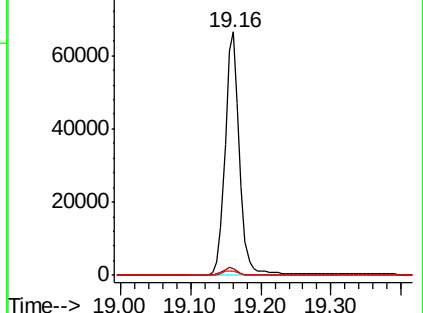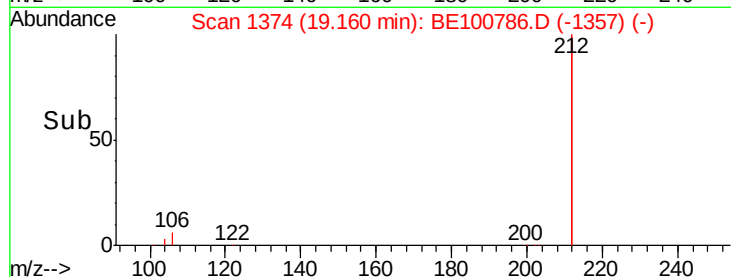

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.31 min Scan# 1625

Delta R.T. -0.00 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19


Tgt Ion:240 Resp: 18444

Ion Ratio Lower Upper

240 100

120 10.6 10.2 15.2



236 27.3 22.3 33.5




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

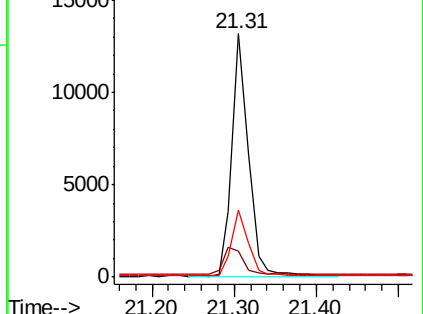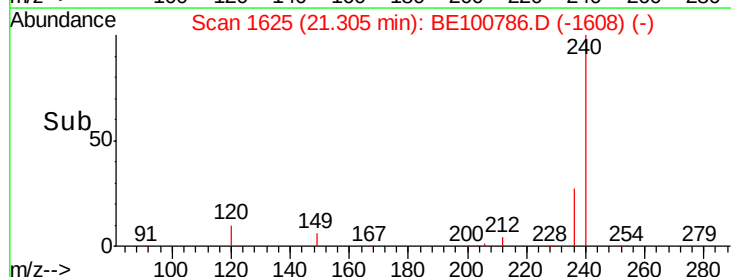

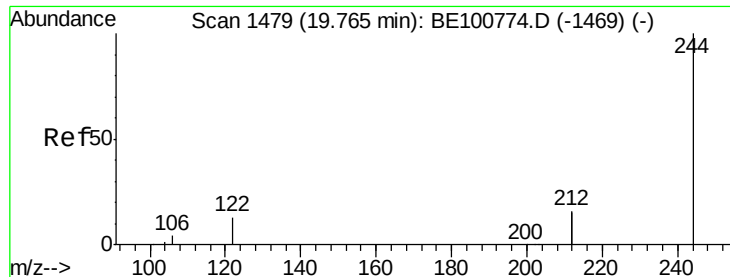

#29

Terphenyl-d14

Concen: 0.468 ng

RT: 19.76 min Scan# 1479

Delta R.T. -0.00 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19

Instrument :

BNA_E

ClientSampleId :


Tot Ion:244 Resp: 20695

Ion Ratio Lower Upper

244 100

212 32.4 26.2 39.4




122 11.7 10.2 15.4

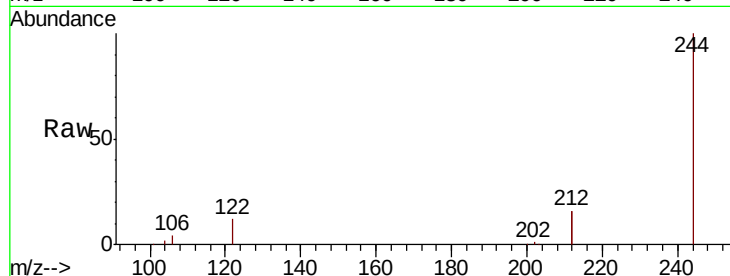

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

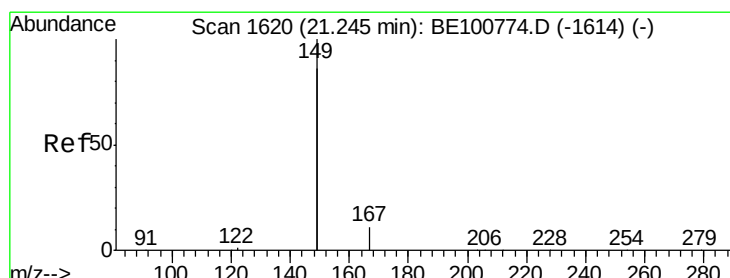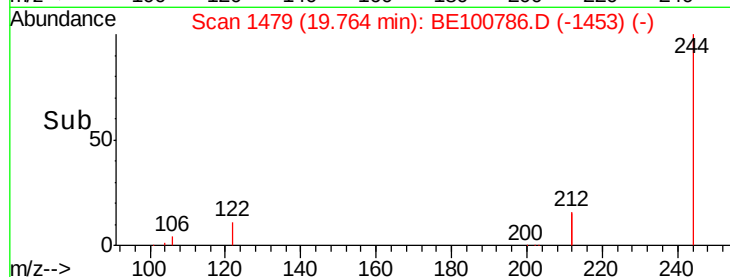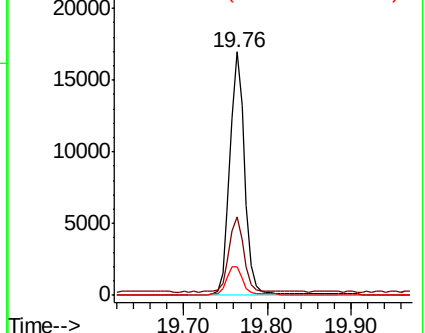

#32

Bis(2-ethylhexyl)phthalate

Concen: Below Cal

RT: 21.24 min Scan# 1620

Delta R.T. 0.00 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19


Tgt Ion:149 Resp: 402

Ion Ratio Lower Upper

149 100

167 9.5 5.0 7.6#



279 4.2 0.7 1.1#



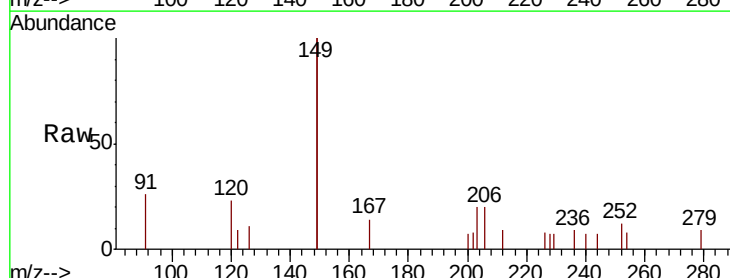


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

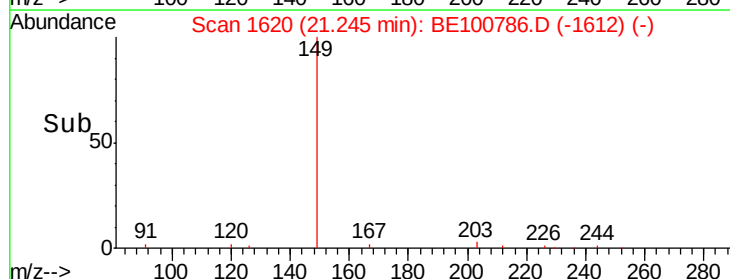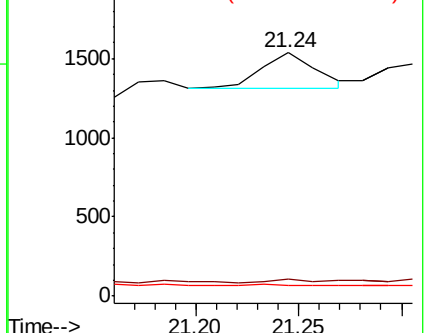



#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.76 min Scan# 2168

Delta R.T. -0.00 min

Lab File: BE100786.D

Acq: 5 Dec 2019 13:19

Instrument :

BNA_E

ClientSampleId :

Tot Ion:264 Resp: 20222

Ion Ratio Lower Upper

264 100

260 23.7 19.4 29.2

265 28.8 21.8 32.8

