


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE120519\
Data File : BE100780.D
Acq On : 5 Dec 2019 8:58
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE120419.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 04 17:18:11 2019

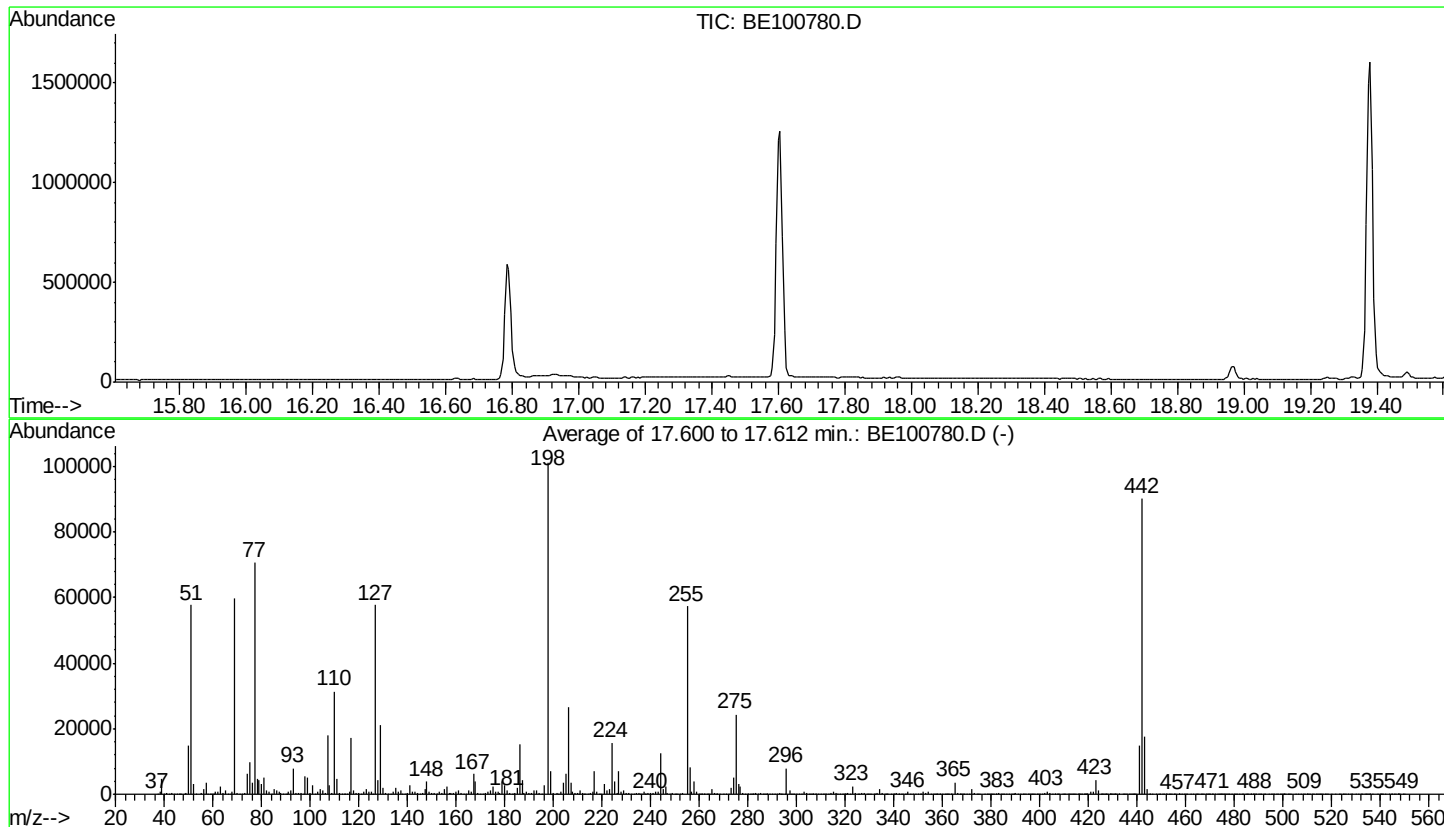

AutoFind: Scans 2555, 2556, 2557; Background Corrected with Scan 2546

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	57772	PASS
68	69	0.00	2	1.6	971	PASS
69	198	0.00	100	58.9	59585	PASS
70	69	0.00	2	0.6	342	PASS
127	198	10	80	57.0	57691	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101129	PASS
199	198	5	9	7.0	7082	PASS
275	198	10	60	24.0	24263	PASS
365	198	1	100	3.6	3680	PASS
441	198	0.01	100	14.6	14792	PASS
442	198	50	100	89.1	90089	PASS
443	442	15	24	19.3	17430	PASS