

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121018\
 Data File : BE098307.D
 Acq On : 10 Dec 2018 20:40
 Operator : SJ/JU
 Sample : J6259-18
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW302S-20181205

Quant Time: Dec 11 01:16:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	1243	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	4993	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	3281	0.40	ng	0.00
19) Phenanthrene-d10	17.28	188	8650	0.40	ng	0.00
27) Chrysene-d12	21.46	240	11786	0.40	ng	0.00
34) Perylene-d12	24.01	264	11305	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.45	112	461	0.16	ng	0.00
5) Phenol-d6	7.04	99	334	0.08	ng	0.00
8) Nitrobenzene-d5	9.03	82	1726	0.38	ng	0.01
11) 2-Methylnaphthalene-d10	12.27	152	3080	0.38	ng	0.00
14) 2,4,6-Tribromophenol	16.02	330	433	0.36	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	6230	0.45	ng	0.00
25) Fluoranthene-d10	19.31	212	48615	0.44	ng	0.00
29) Terphenyl-d14	19.91	244	10693	0.37	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.37	88	755	0.351	ng	Qvalue # 73
32) Bis(2-ethylhexyl)phthalate	21.37	149	13788	0.202	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121018\
Data File : BE098307.D
Acq On : 10 Dec 2018 20:40
Operator : SJ/JU
Sample : J6259-18
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW302S-20181205

Quant Time: Dec 11 01:16:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

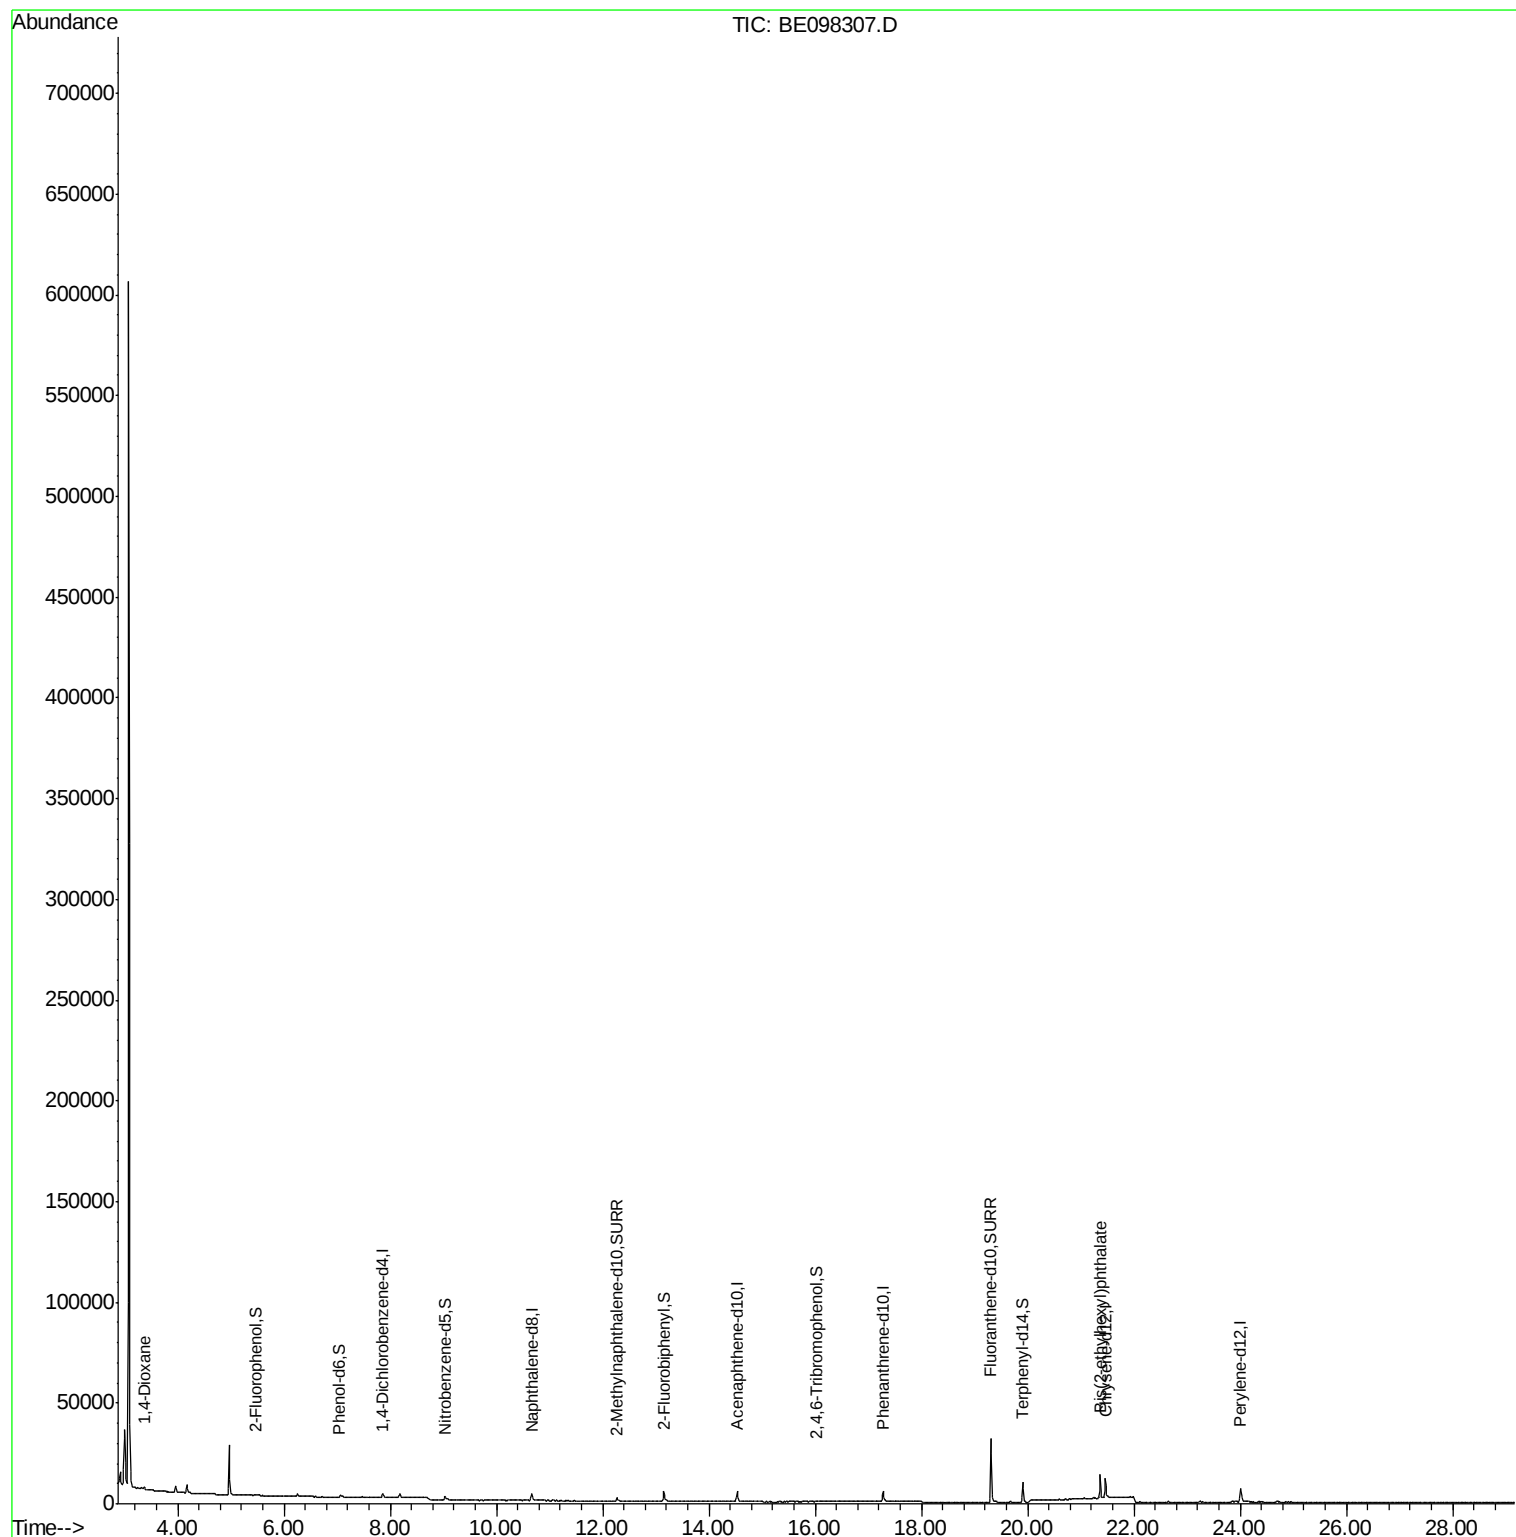



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.86 min Scan# 434

Delta R.T. -0.00 min

Lab File: BE098307.D

Acq: 10 Dec 2018 20:40

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW302S-20181205


Tot Ion:152 Resp: 1243

Ion Ratio Lower Upper

152 100

150 152.8 124.2 186.4



115 69.0 53.9 80.9

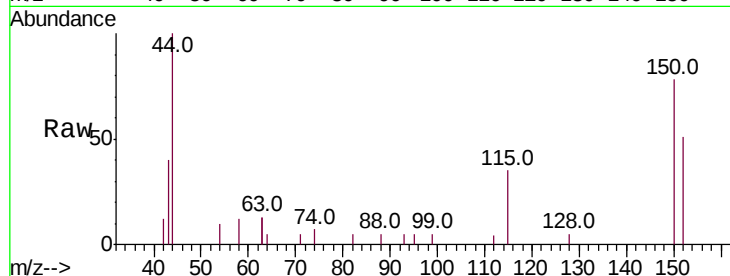

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

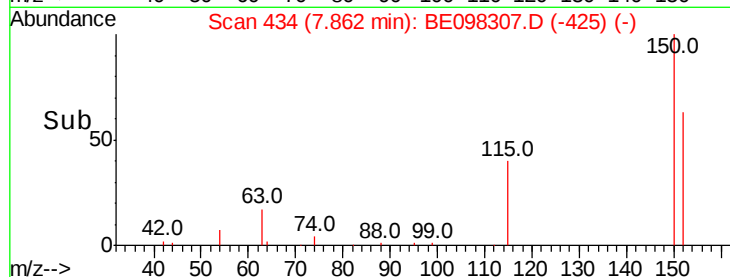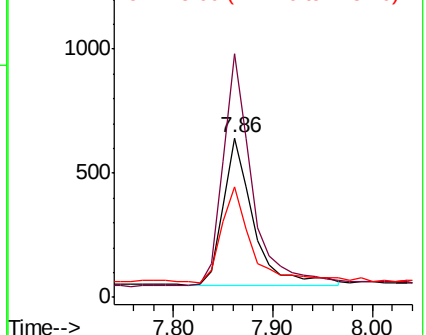

#2

1,4-Dioxane

Concen: 0.351 ng

RT: 3.37 min Scan# 44

Delta R.T. -0.00 min

Lab File: BE098307.D

Acq: 10 Dec 2018 20:40


Tgt Ion: 88 Resp: 755

Ion Ratio Lower Upper

88 100

58 96.4 75.0 112.6



43 98.1 38.3 57.5#

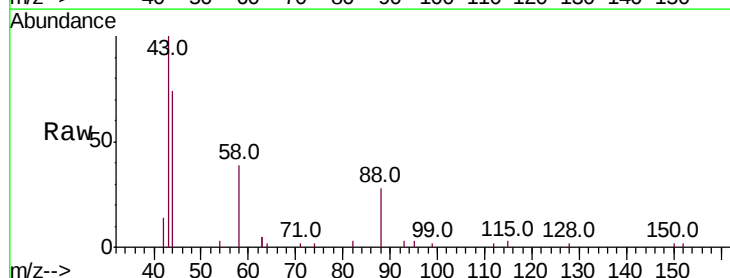

Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

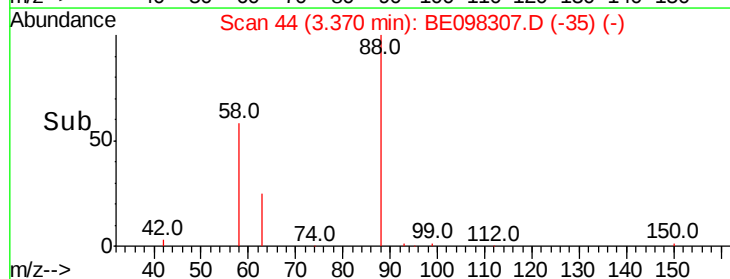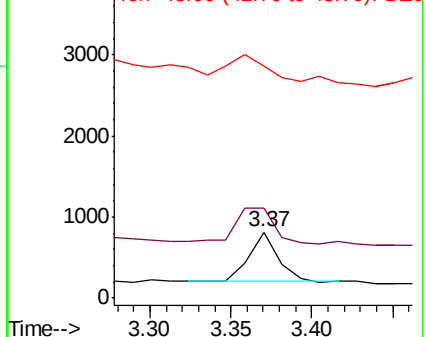



#4

2-Fluorophenol

Concen: 0.158 ng

RT: 5.45 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098307.D

Acq: 10 Dec 2018 20:40

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW302S-20181205


Tot Ion: 112 Resp: 461

Ion Ratio Lower Upper

112 100

64 77.0 59.8 89.8




63 178.3 133.7 200.5

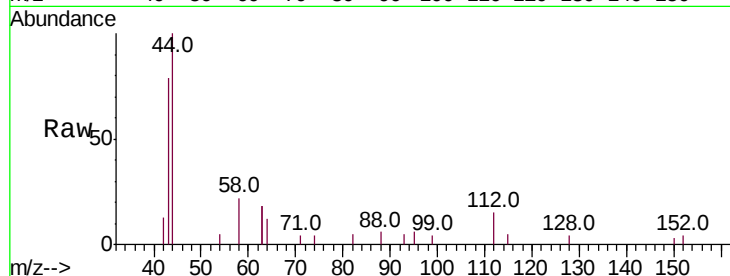

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

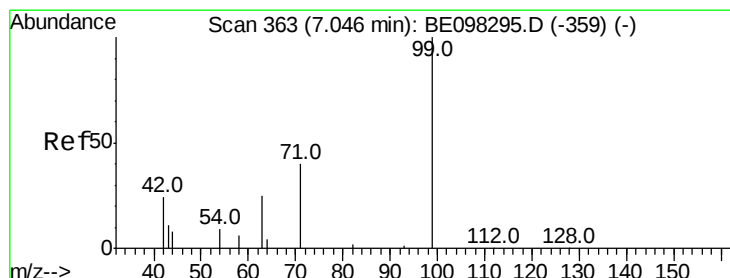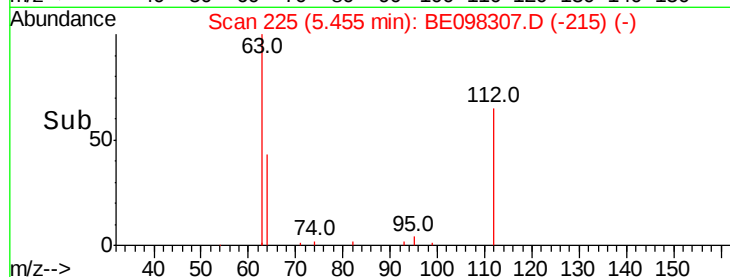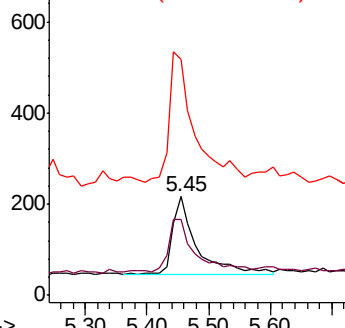

#5

Phenol-d6

Concen: 0.081 ng

RT: 7.04 min Scan# 363

Delta R.T. -0.00 min

Lab File: BE098307.D

Acq: 10 Dec 2018 20:40


Tgt Ion: 99 Resp: 334

Ion Ratio Lower Upper

99 100

42 62.0 26.3 39.5#



71 48.5 33.6 50.4

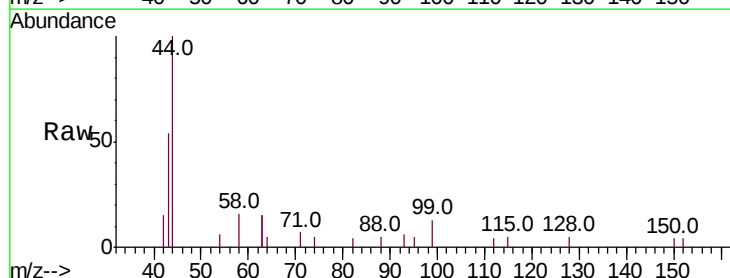


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

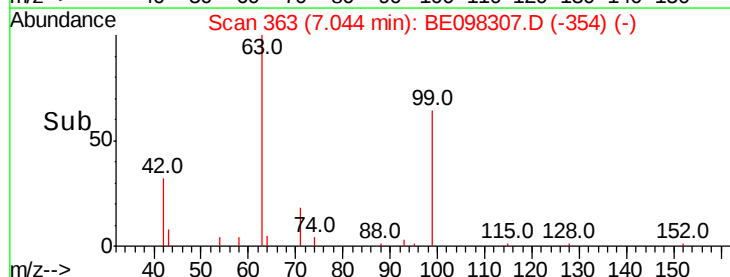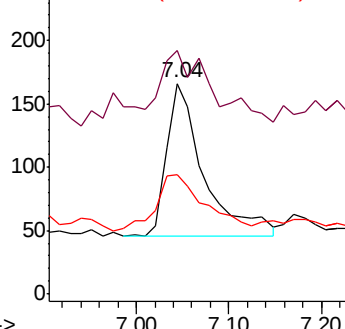

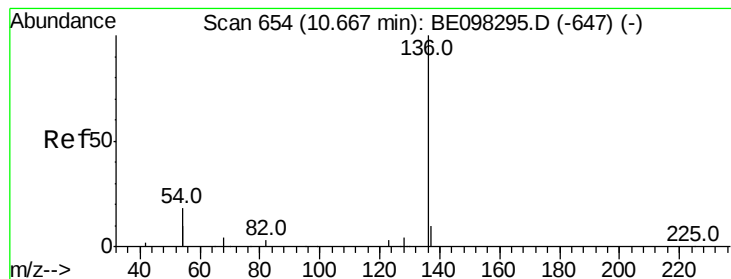

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. -0.00 min

Lab File: BE098307.D

Acq: 10 Dec 2018 20:40

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW302S-20181205

Tot Ion:136 Resp: 4993





Ion Ratio Lower Upper

136 100

137 11.7 9.2 13.8

54 46.6 28.4 42.6#

68 8.7 5.4 8.0#

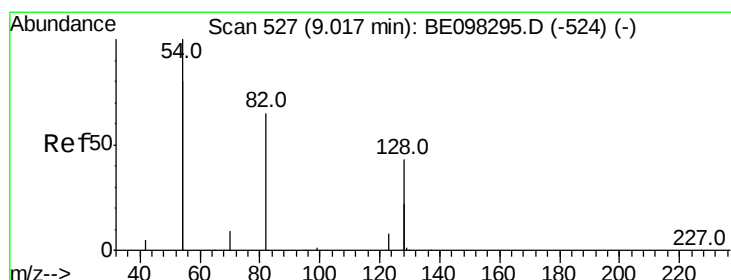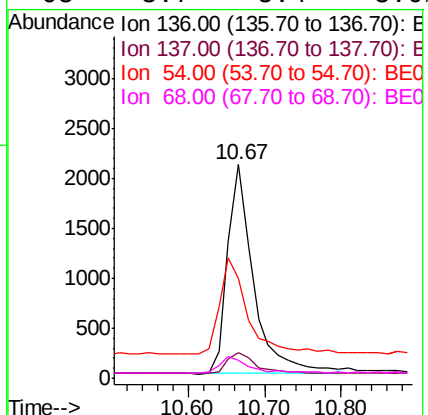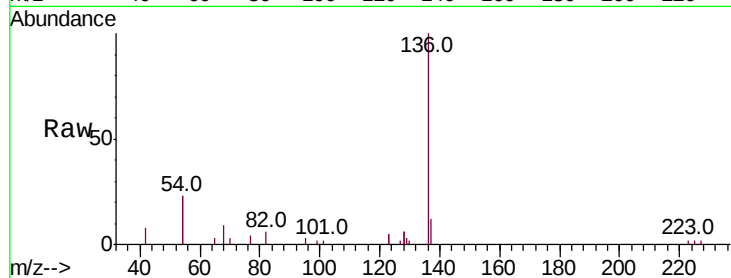

#8

Nitrobenzene-d5

Concen: 0.380 ng

RT: 9.03 min Scan# 528

Delta R.T. 0.01 min

Lab File: BE098307.D

Acq: 10 Dec 2018 20:40




Tgt Ion: 82 Resp: 1726


Ion Ratio Lower Upper

82 100

128 167.3 102.4 153.6#

54 283.0 221.8 332.8


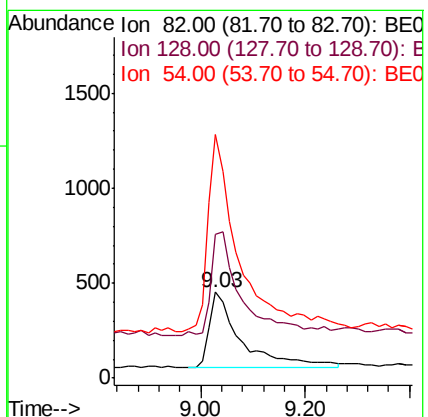

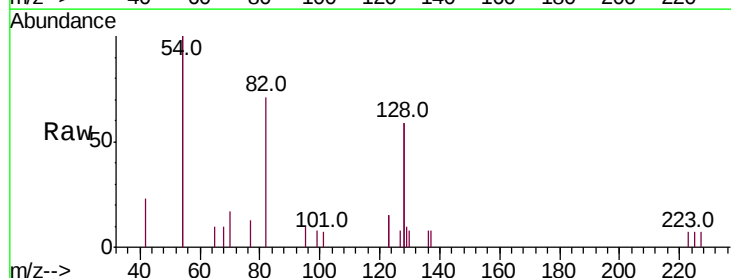


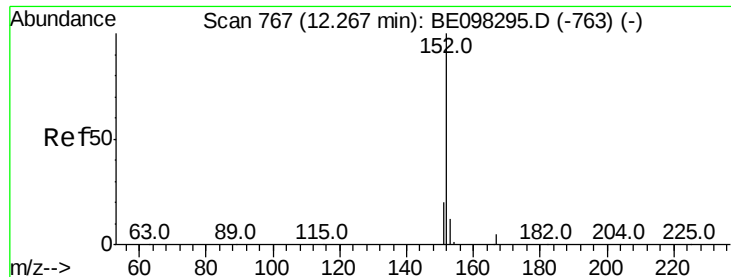

#11
2-Methylnaphthalene-d10
Concen: 0.379 ng
RT: 12.27 min Scan# 767
Delta R.T. -0.00 min
Lab File: BE098307.D
Acq: 10 Dec 2018 20:40




Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW302S-20181205

Tot Ion:152 Resp: 3080
Ion Ratio Lower Upper
152 100
151 19.2 16.2 24.4

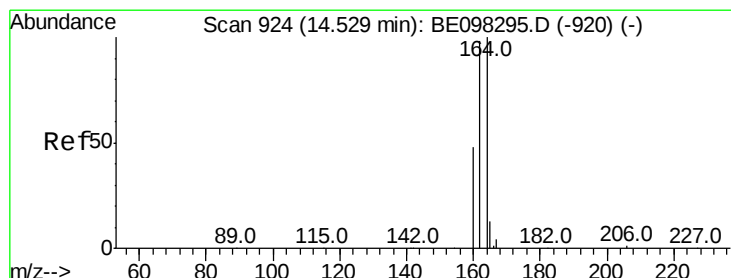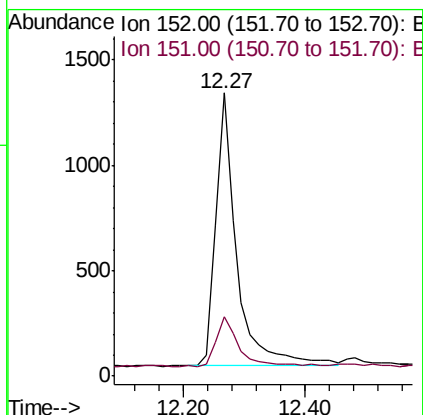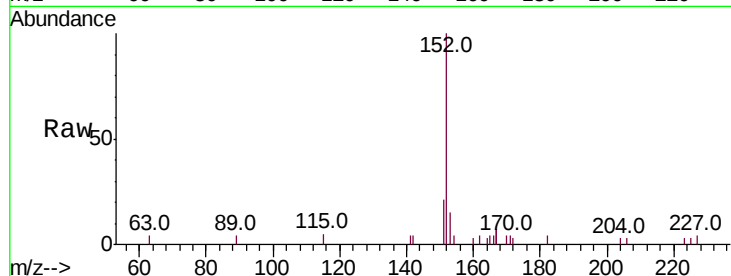

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.53 min Scan# 924
Delta R.T. -0.00 min
Lab File: BE098307.D
Acq: 10 Dec 2018 20:40

Tgt Ion:164 Resp: 3281
Ion Ratio Lower Upper
164 100
162 101.2 77.6 116.4
160 48.3 36.0 54.0

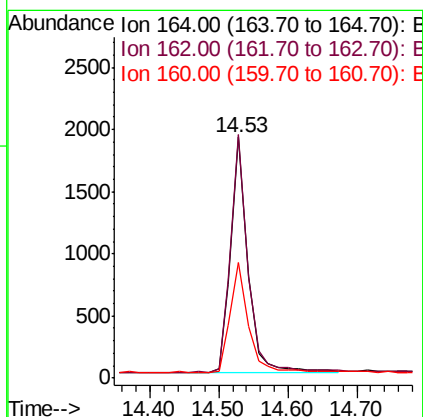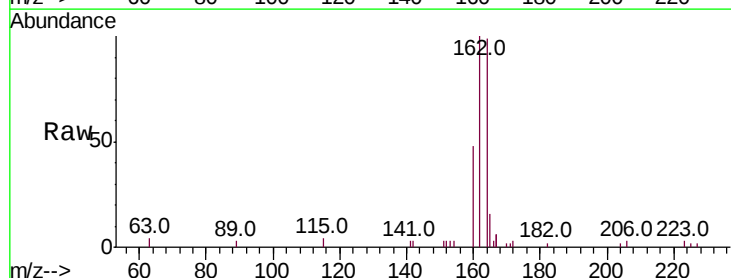



#14

2,4,6-Tribromophenol

Concen: 0.359 ng

RT: 16.02 min Scan# 1041

Delta R.T. -0.00 min

Lab File: BE098307.D

Acq: 10 Dec 2018 20:40

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW302S-20181205


Tot Ion:330 Resp: 433

Ion Ratio Lower Upper

330 100

332 104.8 76.2 114.4




141 47.3 39.0 58.4

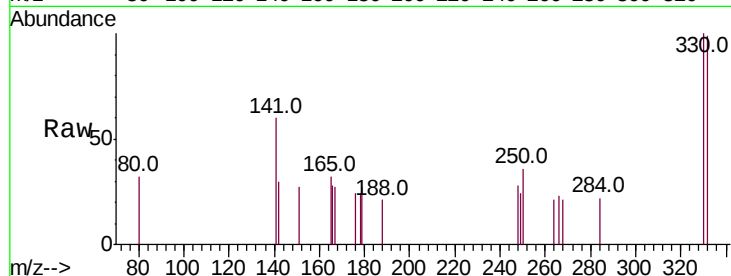

Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

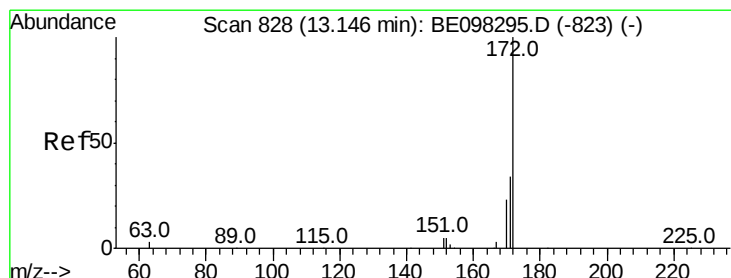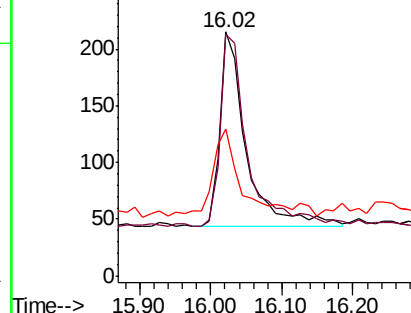

#15

2-Fluorobiphenyl

Concen: 0.450 ng

RT: 13.15 min Scan# 828

Delta R.T. -0.00 min

Lab File: BE098307.D

Acq: 10 Dec 2018 20:40


Tgt Ion:172 Resp: 6230

Ion Ratio Lower Upper

172 100

171 34.8 27.5 41.3



170 24.8 19.6 29.4

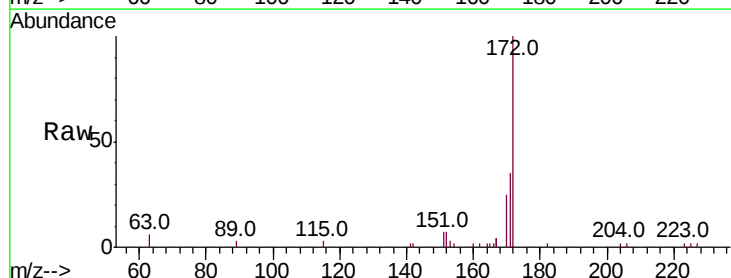


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

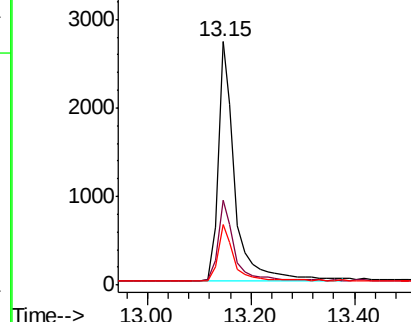

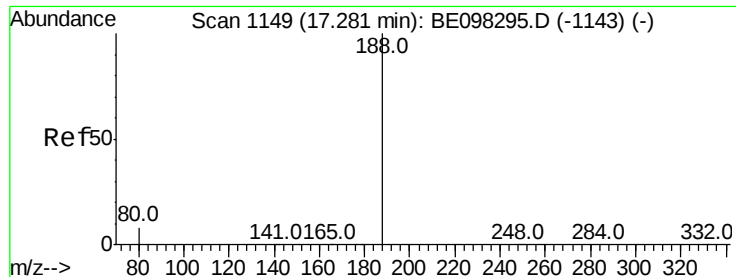

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.28 min Scan# 1149

Delta R.T. -0.00 min

Lab File: BE098307.D

Acq: 10 Dec 2018 20:40

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW302S-20181205


Tot Ion:188 Resp: 8650

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 9.5 7.2 10.8

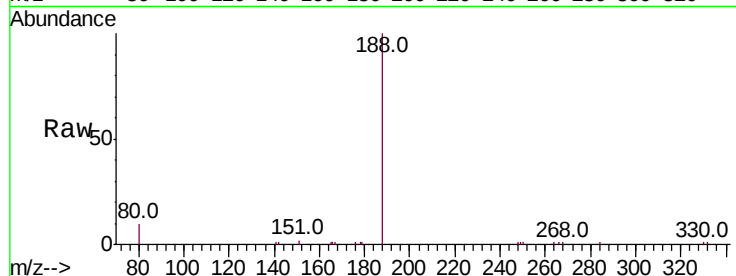

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

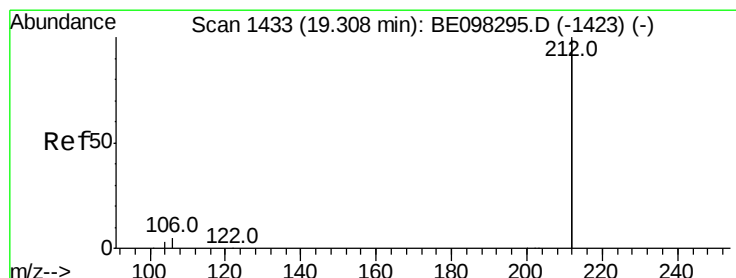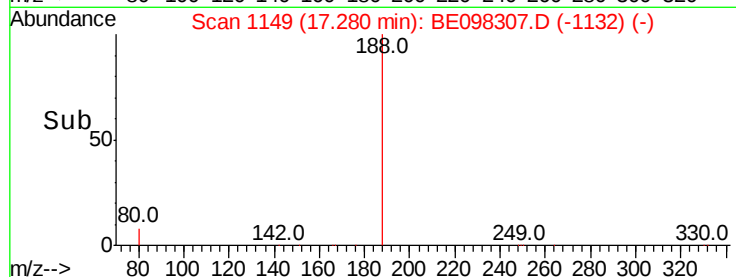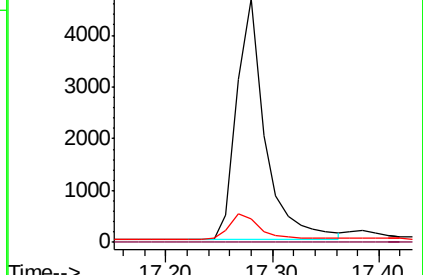

#25

Fluoranthene-d10

Concen: 0.438 ng

RT: 19.31 min Scan# 1433

Delta R.T. 0.00 min

Lab File: BE098307.D

Acq: 10 Dec 2018 20:40


Tgt Ion:212 Resp: 48615

Ion Ratio Lower Upper

212 100

106 2.8 2.2 3.2



104 1.6 1.3 1.9

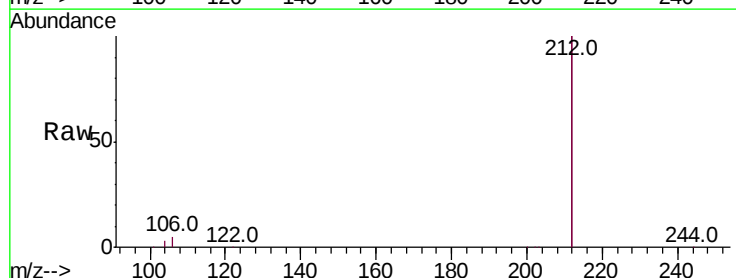

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E



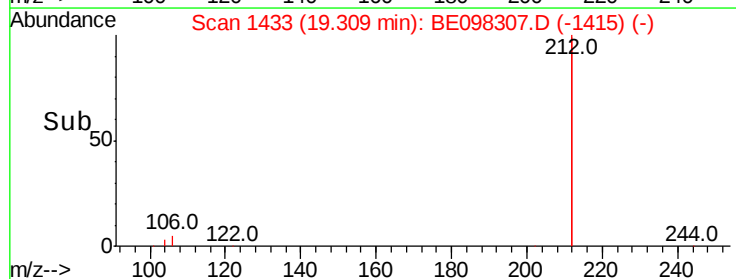
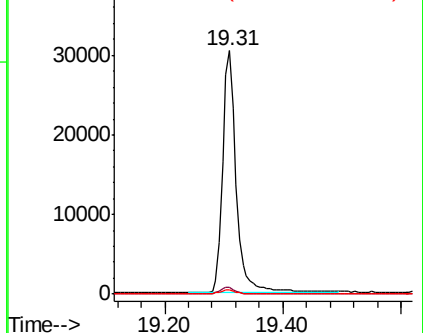




#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.46 min Scan# 1671
Delta R.T. -0.00 min
Lab File: BE098307.D
Acq: 10 Dec 2018 20:40




Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW302S-20181205


Tot Ion:240 Resp: 11786
Ion Ratio Lower Upper
240 100
120 9.6 9.5 14.3
236 27.3 22.7 34.1

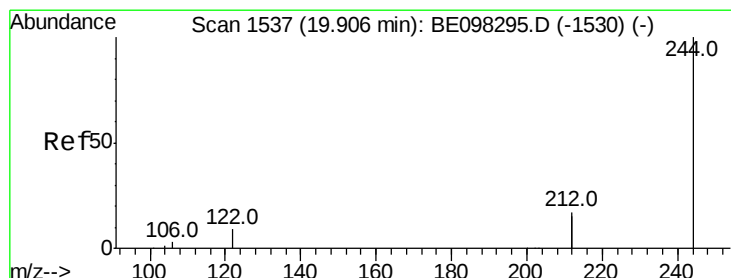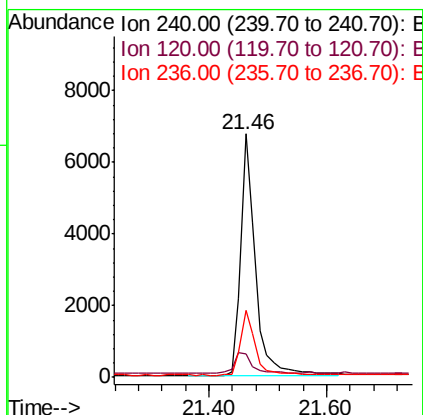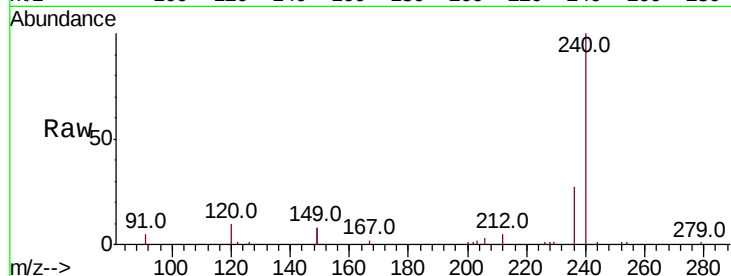

#29
Terphenyl-d14
Concen: 0.373 ng
RT: 19.91 min Scan# 1537
Delta R.T. 0.00 min
Lab File: BE098307.D
Acq: 10 Dec 2018 20:40

Tgt Ion:244 Resp: 10693
Ion Ratio Lower Upper
244 100
212 33.4 27.4 41.0
122 9.1 8.3 12.5



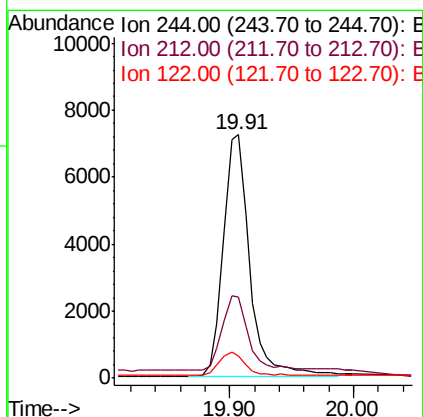
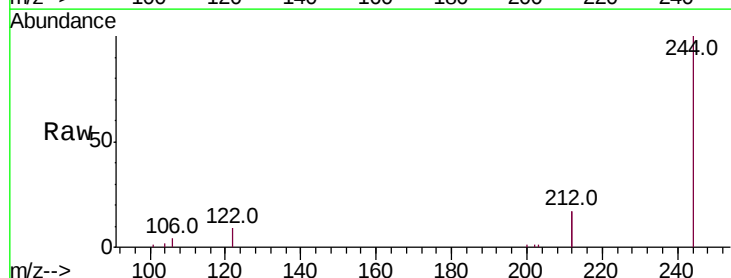


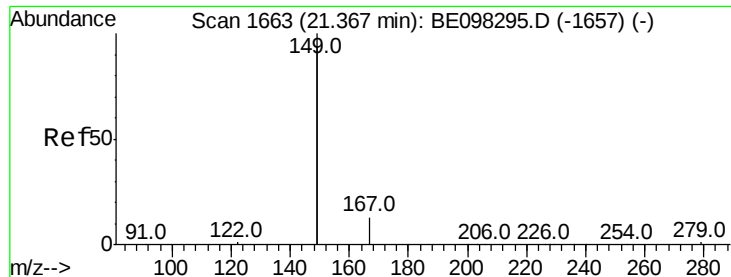

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.202 ng
 RT: 21.37 min Scan# 1663
 Delta R.T. -0.00 min
 Lab File: BE098307.D
 Acq: 10 Dec 2018 20:40

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW302S-20181205

Tot Ion	Ratio	Lower	Upper
149	100		
167	6.6	5.7	8.5
279	1.2	1.0	1.4

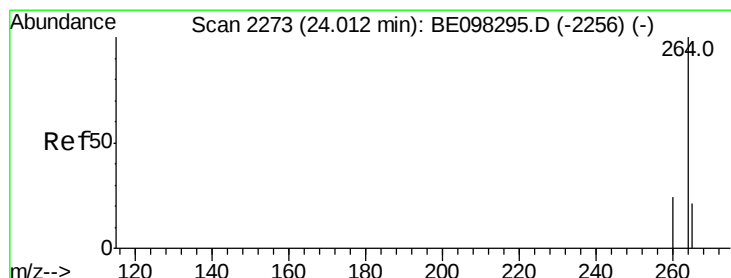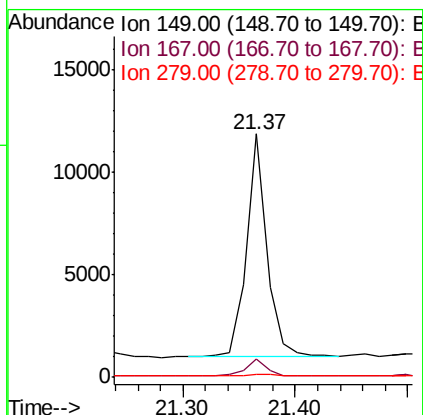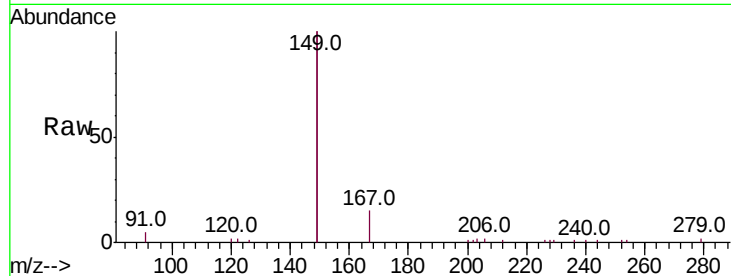

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.01 min Scan# 2272
 Delta R.T. -0.00 min
 Lab File: BE098307.D
 Acq: 10 Dec 2018 20:40

Tgt Ion	Ratio	Lower	Upper
264	100		
260	25.3	20.2	30.2
265	28.7	25.2	37.8

