

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121018\
 Data File : BE098312.D
 Acq On : 10 Dec 2018 23:45
 Operator : SJ/JU
 Sample : J6250-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW304S-20181204

Quant Time: Dec 11 01:23:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	1307	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	5721	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	3721	0.40	ng	0.00
19) Phenanthrene-d10	17.28	188	9395	0.40	ng	0.00
27) Chrysene-d12	21.46	240	11958	0.40	ng	0.00
34) Perylene-d12	24.00	264	11290	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.46	112	591	0.19	ng	0.01
5) Phenol-d6	7.06	99	399	0.09	ng	0.01
8) Nitrobenzene-d5	9.03	82	2480	0.48	ng	0.01
11) 2-Methylnaphthalene-d10	12.27	152	3893	0.42	ng	0.00
14) 2,4,6-Tribromophenol	16.02	330	583	0.43	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	11017	0.70	ng	0.00
25) Fluoranthene-d10	19.31	212	57272	0.48	ng	0.00
29) Terphenyl-d14	19.90	244	13456	0.46	ng	0.00
Target Compounds						
32) Bis(2-ethylhexyl)phthalate	21.37	149	5499	0.080	ng	Qvalue # 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121018\
Data File : BE098312.D
Acq On : 10 Dec 2018 23:45
Operator : SJ/JU
Sample : J6250-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW304S-20181204

Quant Time: Dec 11 01:23:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

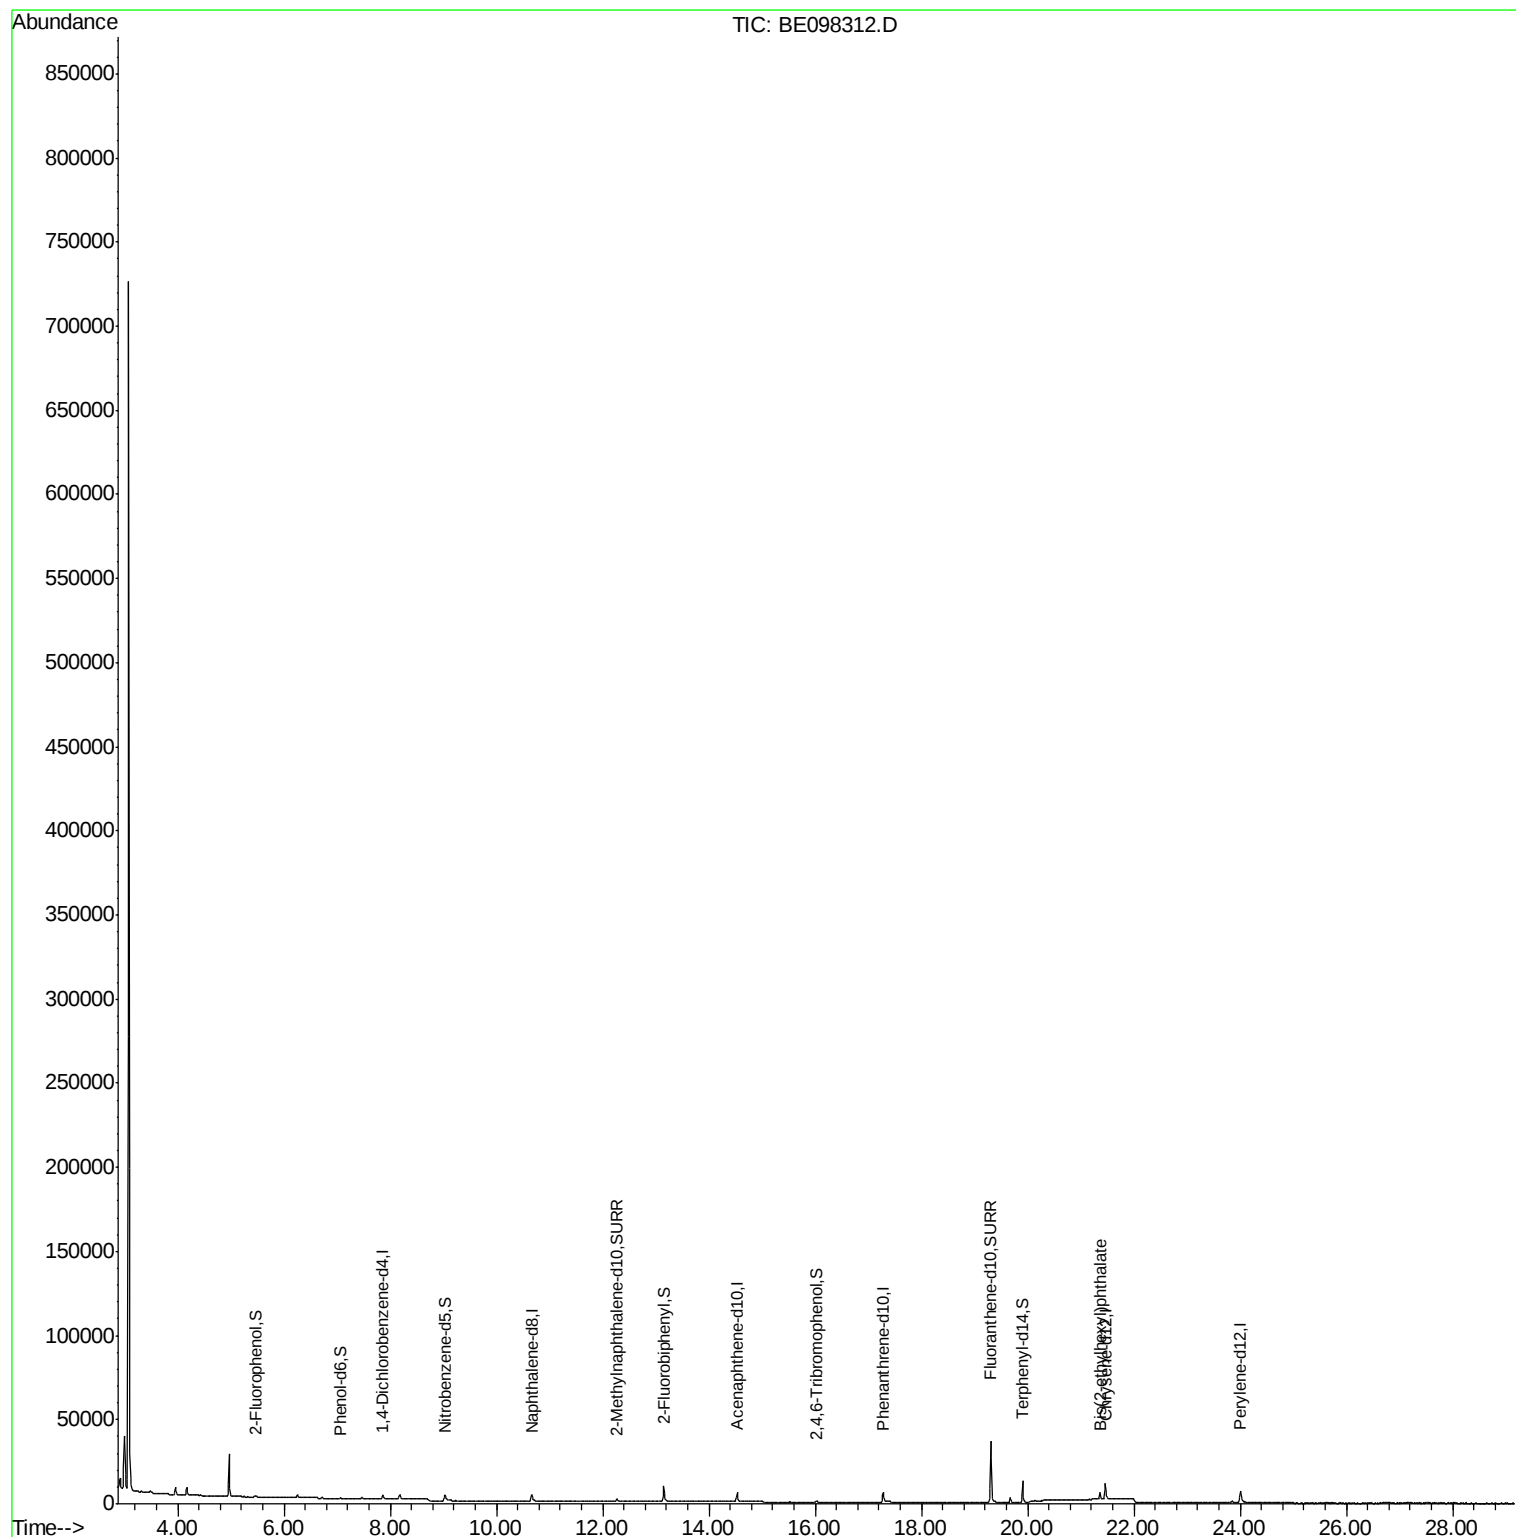




#1




1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.86 min Scan# 434
 Delta R.T. 0.00 min
 Lab File: BE098312.D
 Acq: 10 Dec 2018 23:45

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW304S-20181204

Tot Ion:152 Resp: 1307
 Ion Ratio Lower Upper
 152 100
 150 148.6 124.2 186.4
 115 65.4 53.9 80.9

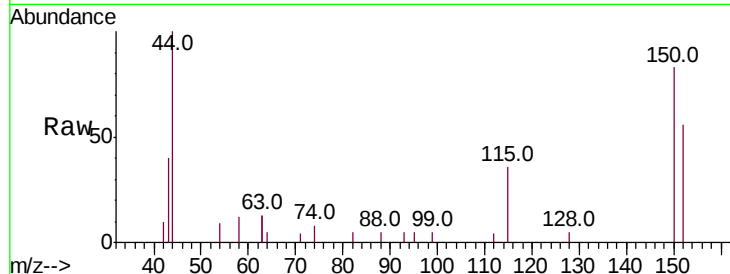


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

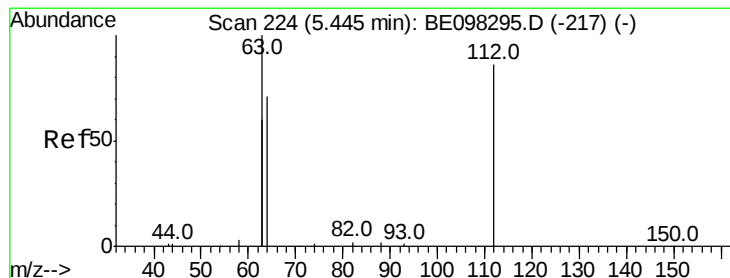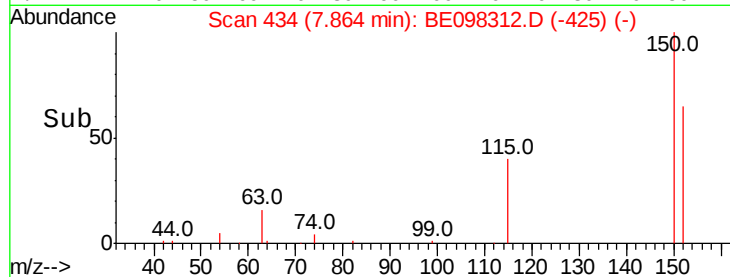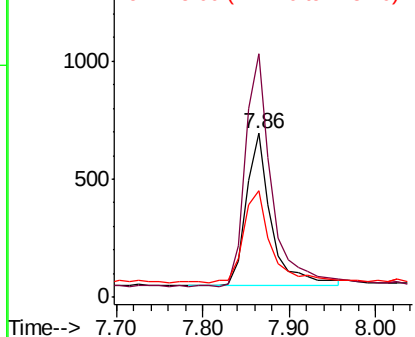



#4


2-Fluorophenol
 Concen: 0.193 ng
 RT: 5.46 min Scan# 225
 Delta R.T. 0.01 min
 Lab File: BE098312.D
 Acq: 10 Dec 2018 23:45

Tgt Ion:112 Resp: 591
 Ion Ratio Lower Upper
 112 100
 64 69.9 59.8 89.8
 63 161.6 133.7 200.5

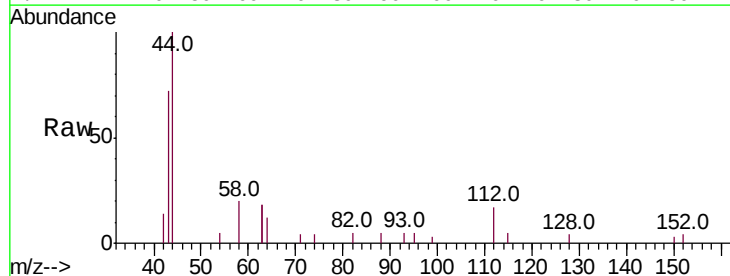

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BE0
 Ion 63.00 (62.70 to 63.70): BE0

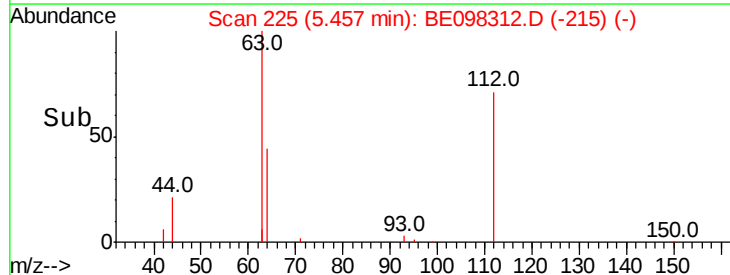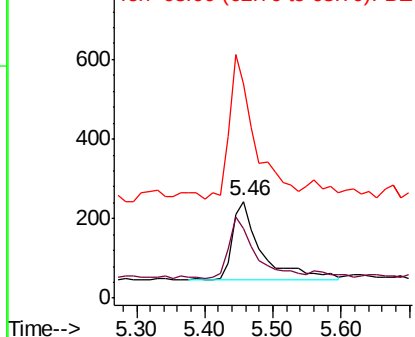

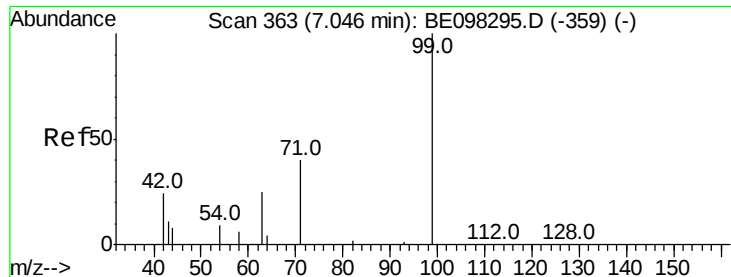

#5

Phenol-d6

Concen: 0.092 ng

RT: 7.06 min Scan# 364

Delta R.T. 0.01 min

Lab File: BE098312.D

Acq: 10 Dec 2018 23:45

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW304S-20181204


Tot Ion: 99 Resp: 399

Ion Ratio Lower Upper

99 100

42 0.0 26.3 39.5#




71 40.4 33.6 50.4

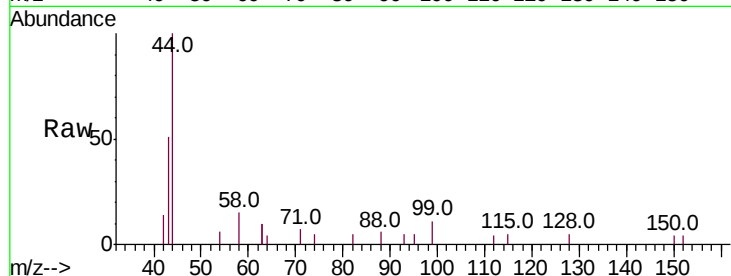

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

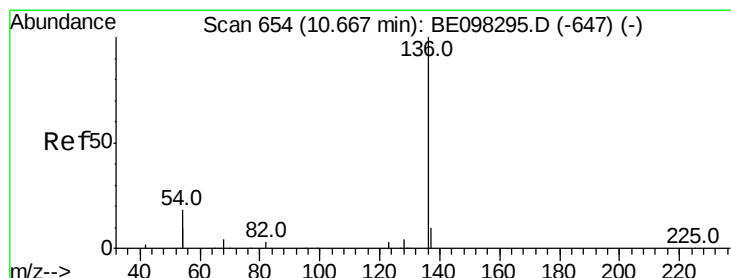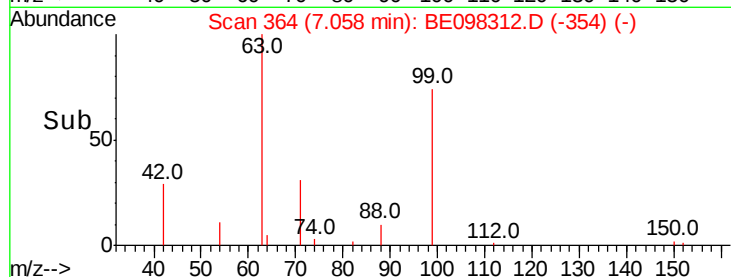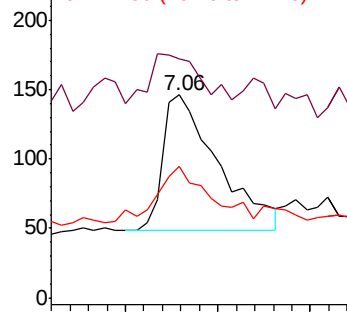

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. -0.00 min

Lab File: BE098312.D

Acq: 10 Dec 2018 23:45

Tgt Ion: 136 Resp: 5721


Ion Ratio Lower Upper

136 100

137 12.8 9.2 13.8

54 42.5 28.4 42.6

68 7.6 5.4 8.0


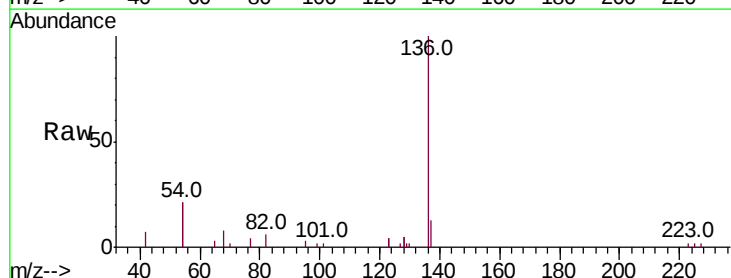


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

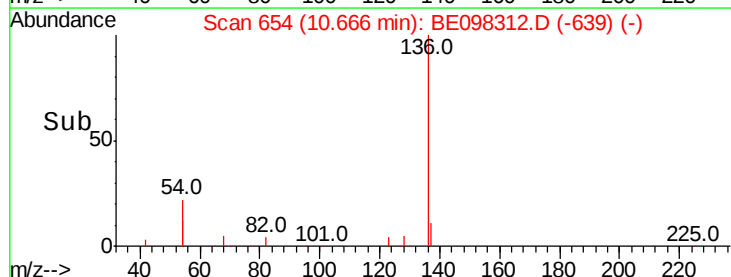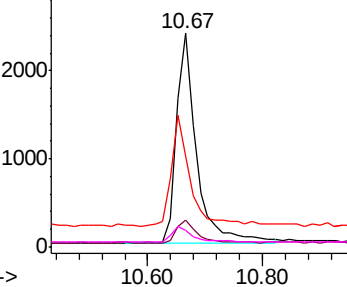



#8

Nitrobenzene-d5

Concen: 0.476 ng

RT: 9.03 min Scan# 528

Delta R.T. 0.01 min

Lab File: BE098312.D

Acq: 10 Dec 2018 23:45

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW304S-20181204


Tot Ion: 82 Resp: 2480

Ion Ratio Lower Upper

82 100

128 148.8 102.4 153.6



54 261.9 221.8 332.8

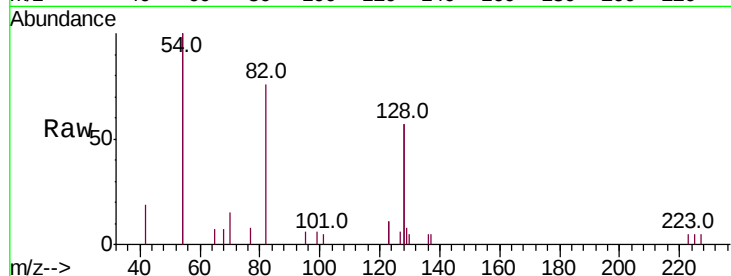

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

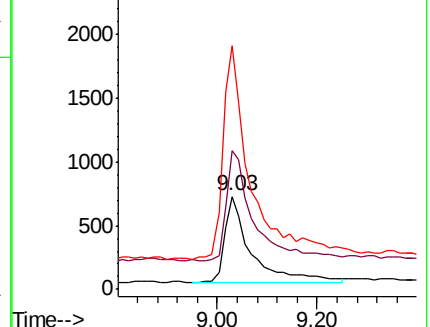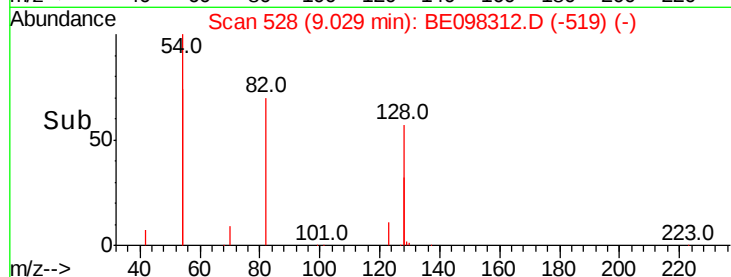

#11

2-Methylnaphthalene-d10

Concen: 0.418 ng

RT: 12.27 min Scan# 767

Delta R.T. 0.00 min

Lab File: BE098312.D


Acq: 10 Dec 2018 23:45

Tgt Ion: 152 Resp: 3893

Ion Ratio Lower Upper



152 100


151 17.6 16.2 24.4

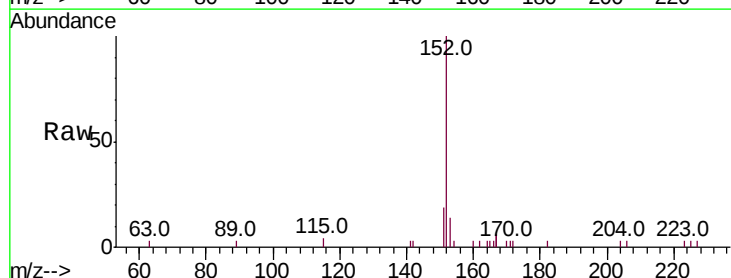

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

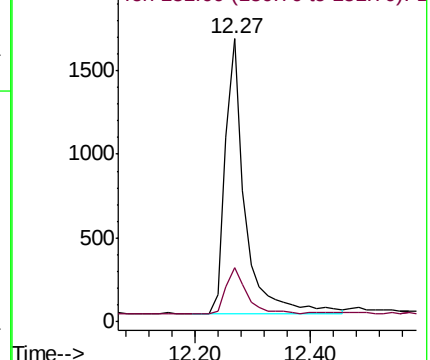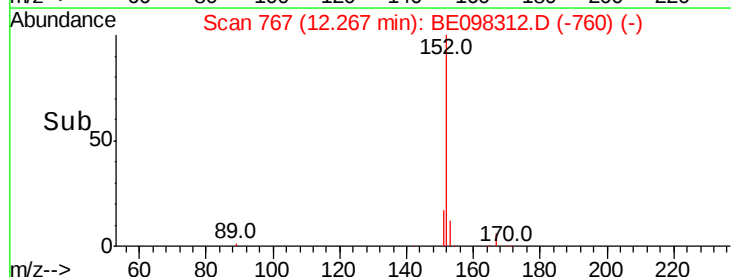

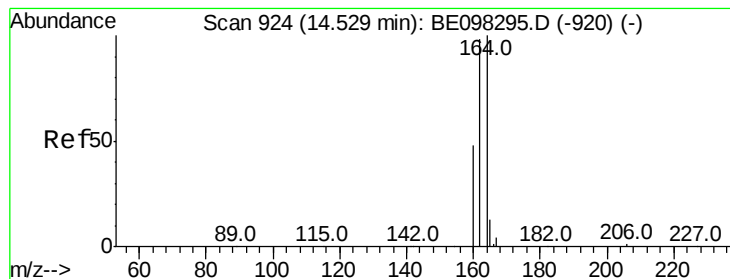

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.53 min Scan# 924

Delta R.T. 0.00 min

Lab File: BE098312.D

Acq: 10 Dec 2018 23:45

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW304S-20181204


Tot Ion:164 Resp: 3721

Ion Ratio Lower Upper

164 100

162 103.8 77.6 116.4




160 50.0 36.0 54.0

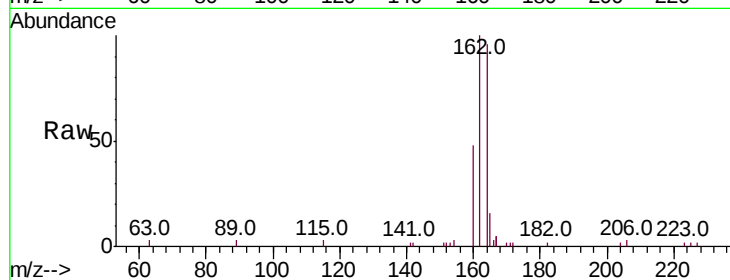

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

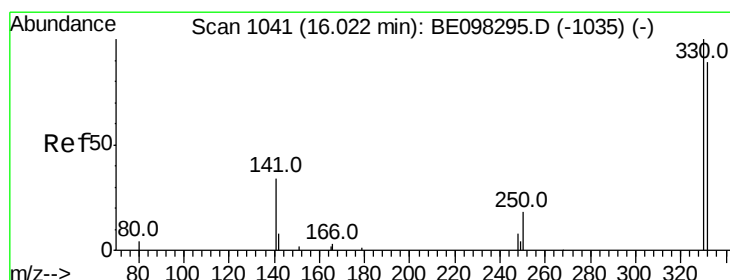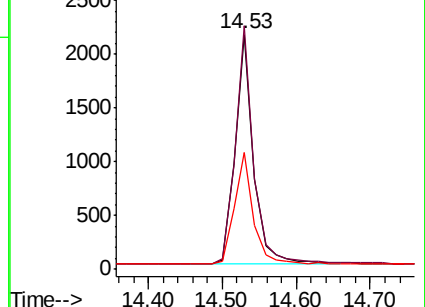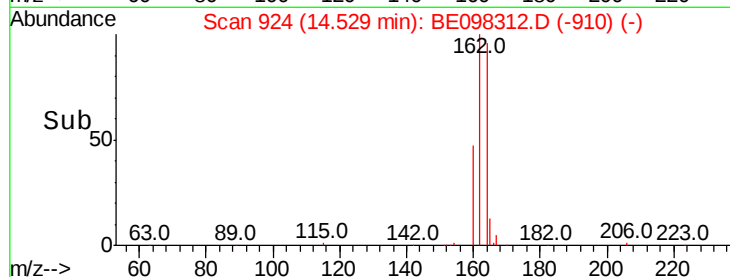

#14

2,4,6-Tribromophenol

Concen: 0.427 ng

RT: 16.02 min Scan# 1041

Delta R.T. -0.00 min

Lab File: BE098312.D

Acq: 10 Dec 2018 23:45


Tgt Ion:330 Resp: 583

Ion Ratio Lower Upper

330 100

332 106.3 76.2 114.4



141 40.7 39.0 58.4

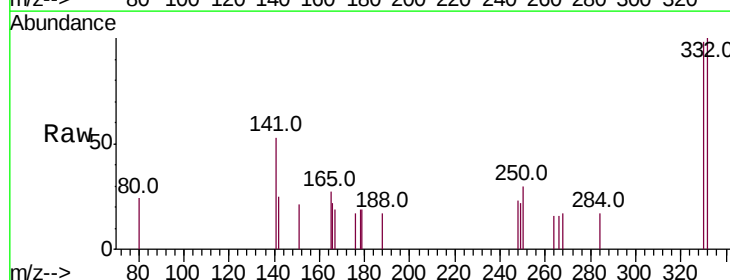


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

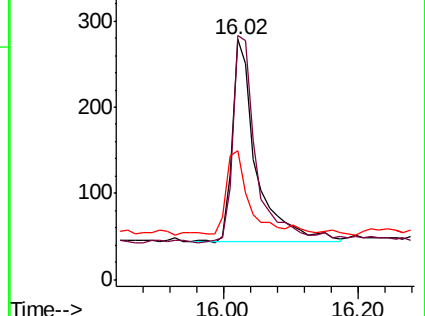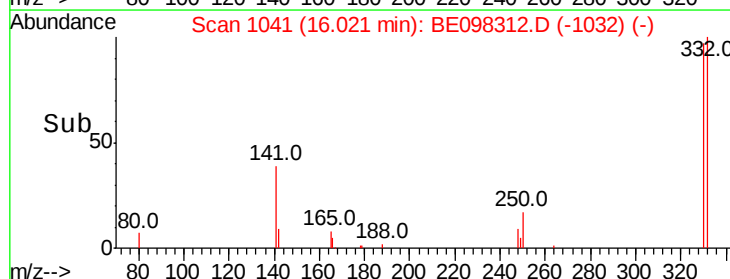


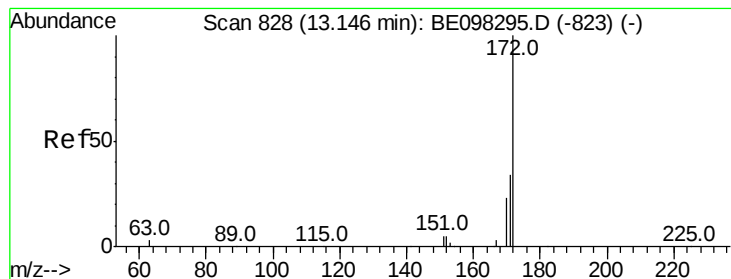




#15
2-Fluorobiphenyl
Concen: 0.702 ng
RT: 13.15 min Scan# 828
Delta R.T. 0.00 min
Lab File: BE098312.D
Acq: 10 Dec 2018 23:45

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW304S-20181204

Tot Ion:172 Resp: 11017
Ion Ratio Lower Upper
172 100
171 33.9 27.5 41.3
170 23.3 19.6 29.4

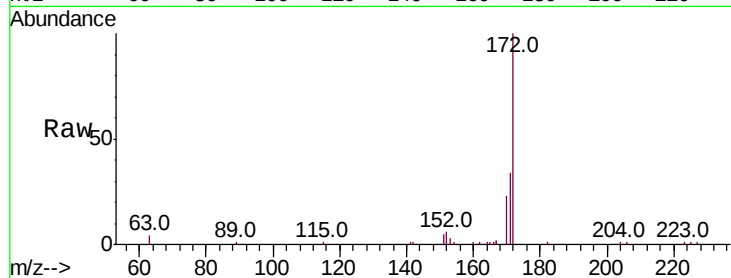


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

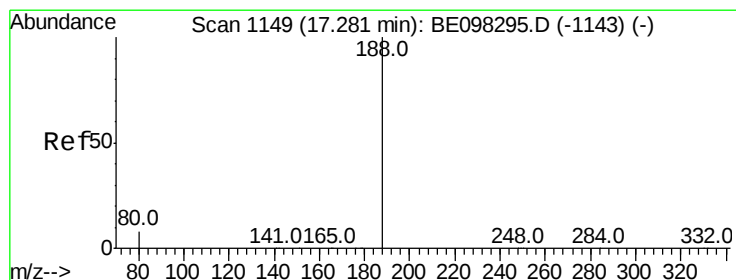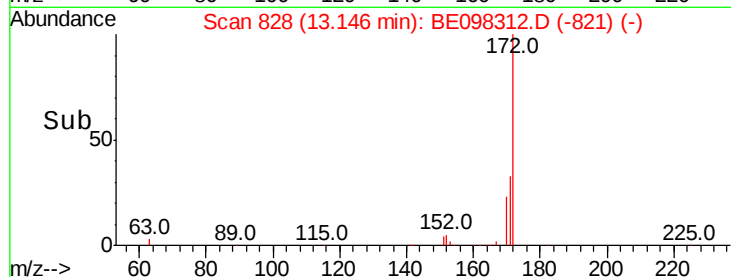
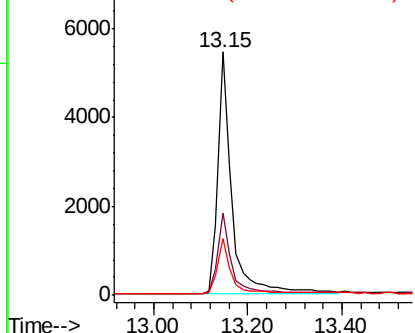



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.28 min Scan# 1149
Delta R.T. -0.00 min
Lab File: BE098312.D
Acq: 10 Dec 2018 23:45

Tgt Ion:188 Resp: 9395
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.7 7.2 10.8

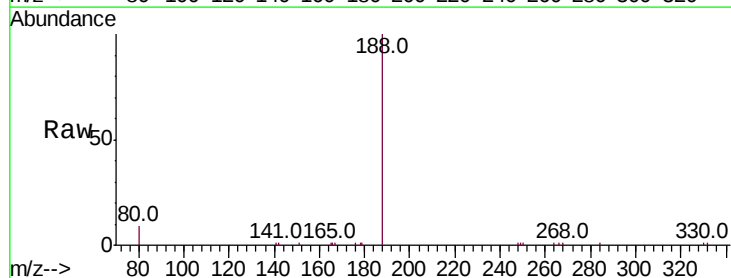

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0

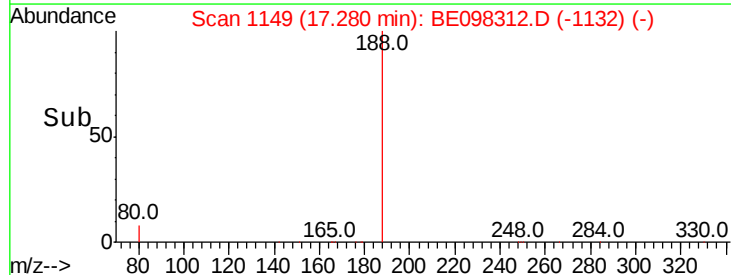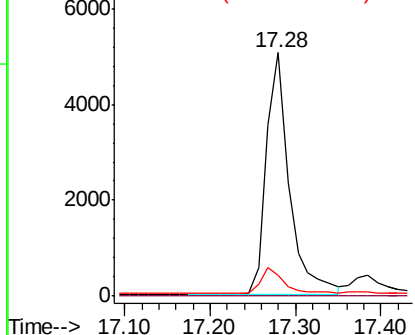


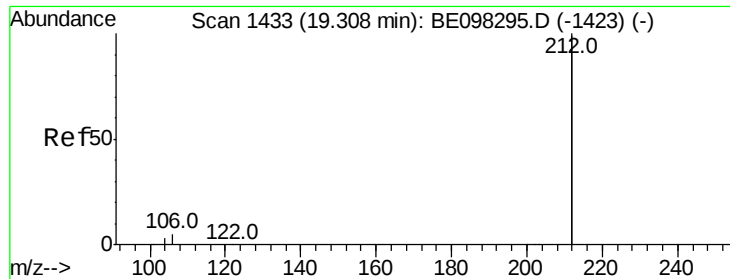




#25
 Fluoranthene-d10
 Concen: 0.475 ng
 RT: 19.31 min Scan# 1433
 Delta R.T. 0.00 min
 Lab File: BE098312.D
 Acq: 10 Dec 2018 23:45

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW304S-20181204

Tot Ion:212 Resp: 57272
 Ion Ratio Lower Upper
 212 100
 106 2.7 2.2 3.2
 104 1.6 1.3 1.9

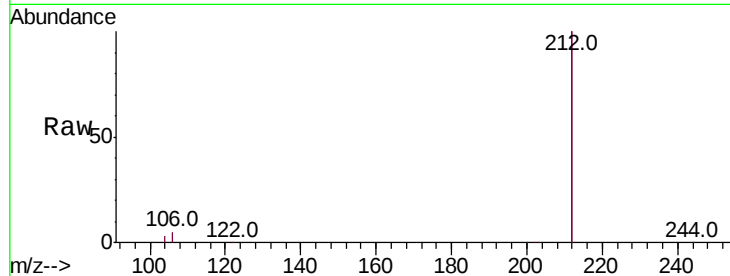


Abundance Ion 212.00 (211.70 to 212.70): E
 Ion 106.00 (105.70 to 106.70): E
 Ion 104.00 (103.70 to 104.70): E

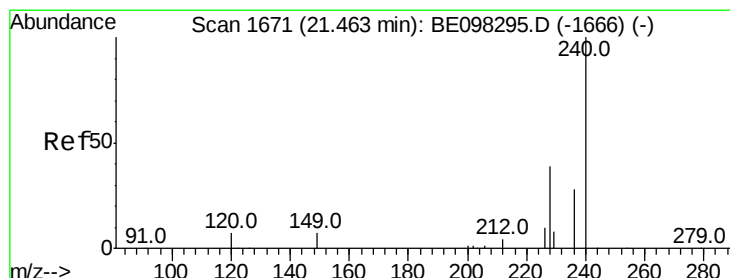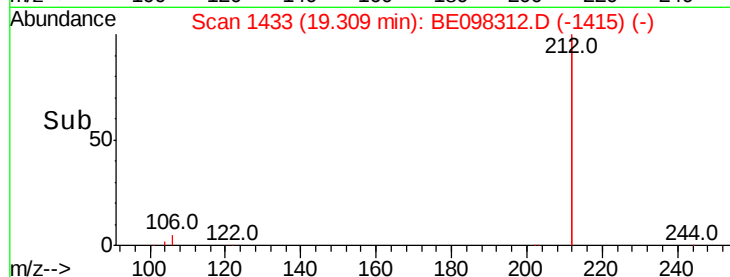
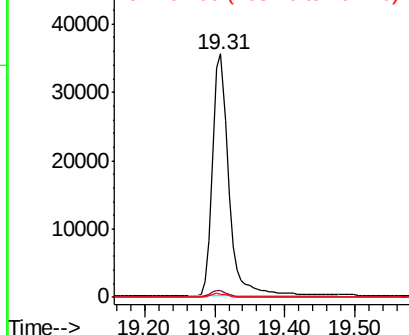



#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.46 min Scan# 1671
 Delta R.T. 0.00 min
 Lab File: BE098312.D
 Acq: 10 Dec 2018 23:45

Tgt Ion:240 Resp: 11958
 Ion Ratio Lower Upper
 240 100
 120 7.4 9.5 14.3#
 236 27.4 22.7 34.1

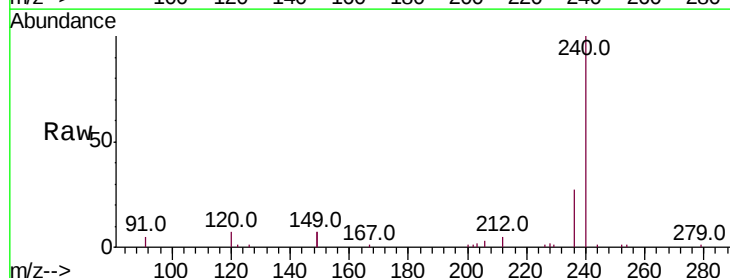

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

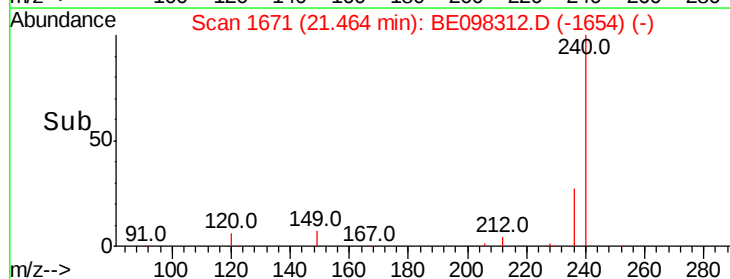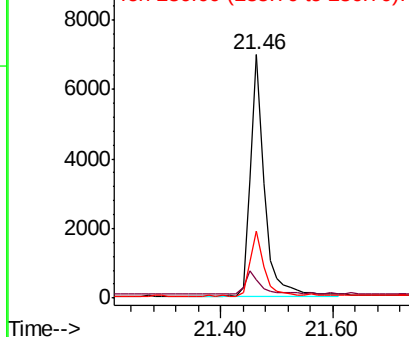

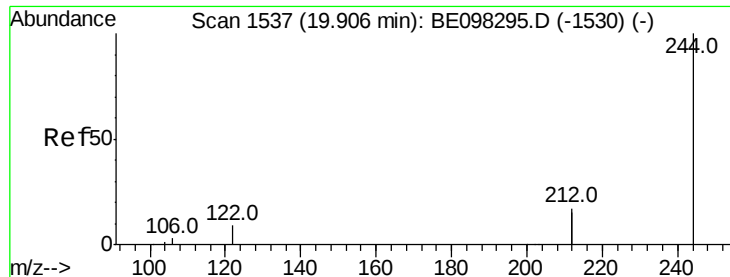

#29

Terphenyl-d14

Concen: 0.463 ng

RT: 19.90 min Scan# 1536

Delta R.T. -0.01 min

Lab File: BE098312.D

Acq: 10 Dec 2018 23:45

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW304S-20181204


Tot Ion:244 Resp: 13456

Ion Ratio Lower Upper

244 100

212 33.7 27.4 41.0




122 10.6 8.3 12.5

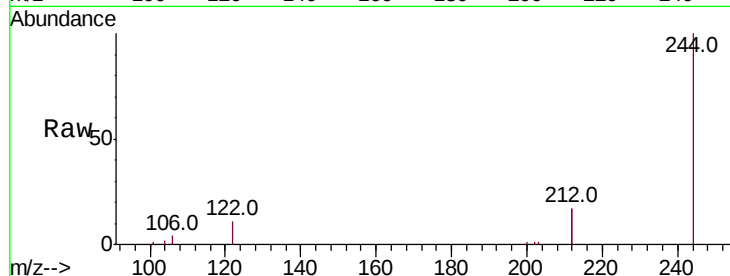

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

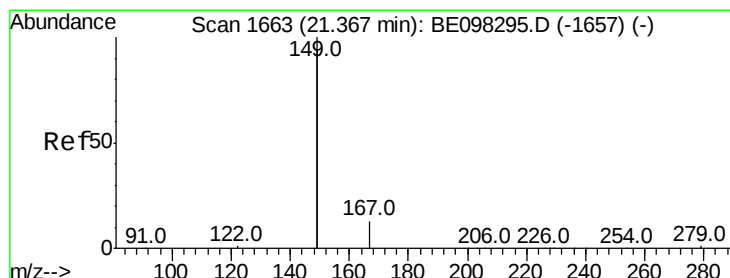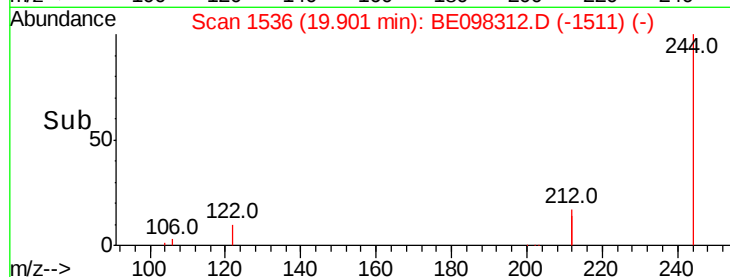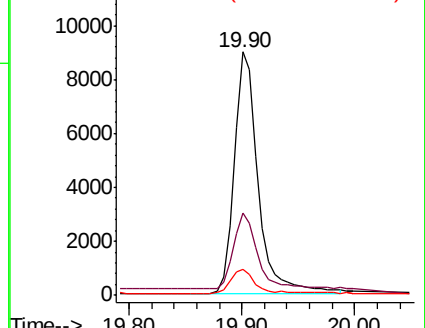

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.080 ng

RT: 21.37 min Scan# 1663

Delta R.T. 0.00 min

Lab File: BE098312.D

Acq: 10 Dec 2018 23:45


Tgt Ion:149 Resp: 5499

Ion Ratio Lower Upper

149 100

167 6.5 5.7 8.5



279 1.6 1.0 1.4#


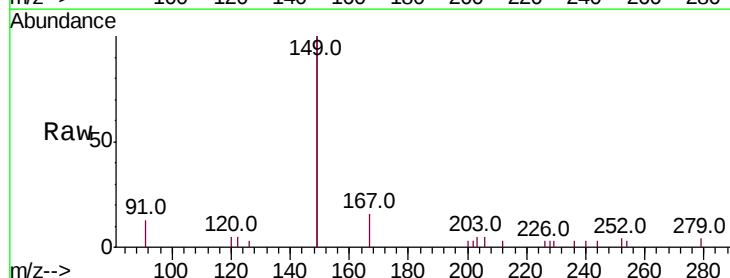


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

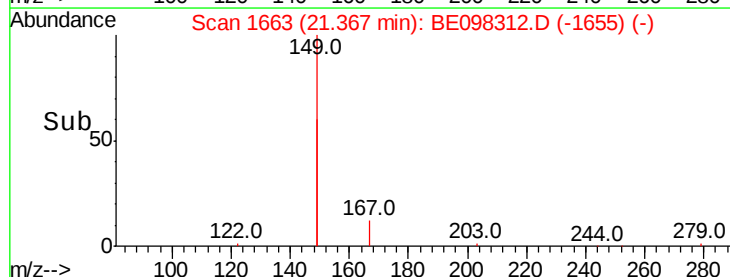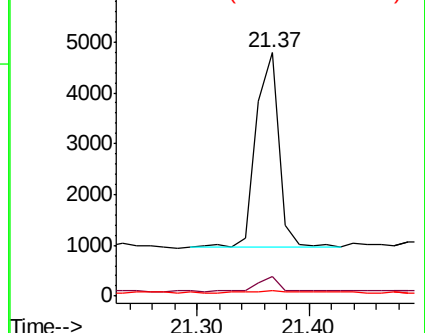

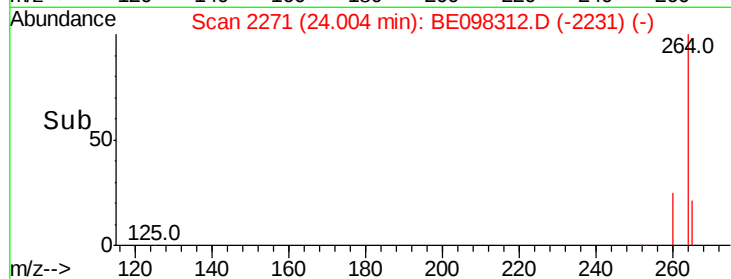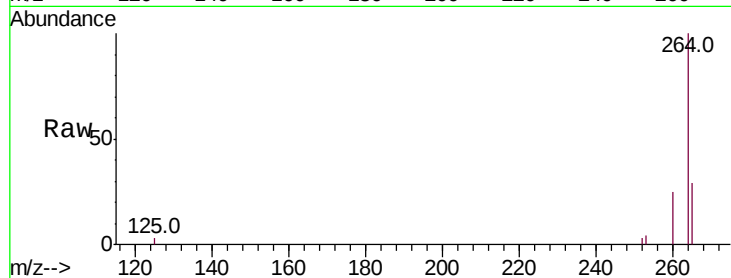

#34
 Pervlene-d12
 Concen: 0.400 ng
 RT: 24.00 min Scan# 2271
 Delta R.T. -0.01 min
 Lab File: BE098312.D
 Acq: 10 Dec 2018 23:45

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW304S-20181204

Tot Ion:264 Resp: 11290
 Ion Ratio Lower Upper
 264 100
 260 25.1 20.2 30.2
 265 29.2 25.2 37.8

