

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121018\
 Data File : BE098326.D
 Acq On : 11 Dec 2018 10:06
 Operator : SJ/JU
 Sample : J6259-22DL 2X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP02-20181205DL

Quant Time: Dec 11 11:01:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	1262	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	5552	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	3722	0.40	ng	0.00
19) Phenanthrene-d10	17.28	188	9874	0.40	ng	0.00
27) Chrysene-d12	21.46	240	12347	0.40	ng	0.00
34) Perylene-d12	24.01	264	11543	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.45	112	276	0.09	ng	0.00
5) Phenol-d6	7.05	99	184	0.04	ng	0.00
8) Nitrobenzene-d5	9.04	82	1000	0.20	ng	0.03
11) 2-Methylnaphthalene-d10	12.27	152	1813	0.20	ng	0.00
14) 2,4,6-Tribromophenol	16.03	330	260	0.19	ng	0.01
15) 2-Fluorobiphenyl	13.15	172	4135	0.26	ng	0.00
25) Fluoranthene-d10	19.31	212	28180	0.22	ng	0.00
29) Terphenyl-d14	19.91	244	6495	0.22	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.37	88	3604	1.651	ng	98
32) Bis(2-ethylhexyl)phthalate	21.37	149	5022	0.070	ng	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121018\
Data File : BE098326.D
Acq On : 11 Dec 2018 10:06
Operator : SJ/JU
Sample : J6259-22DL 2X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-DUP02-20181205DL

Quant Time: Dec 11 11:01:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

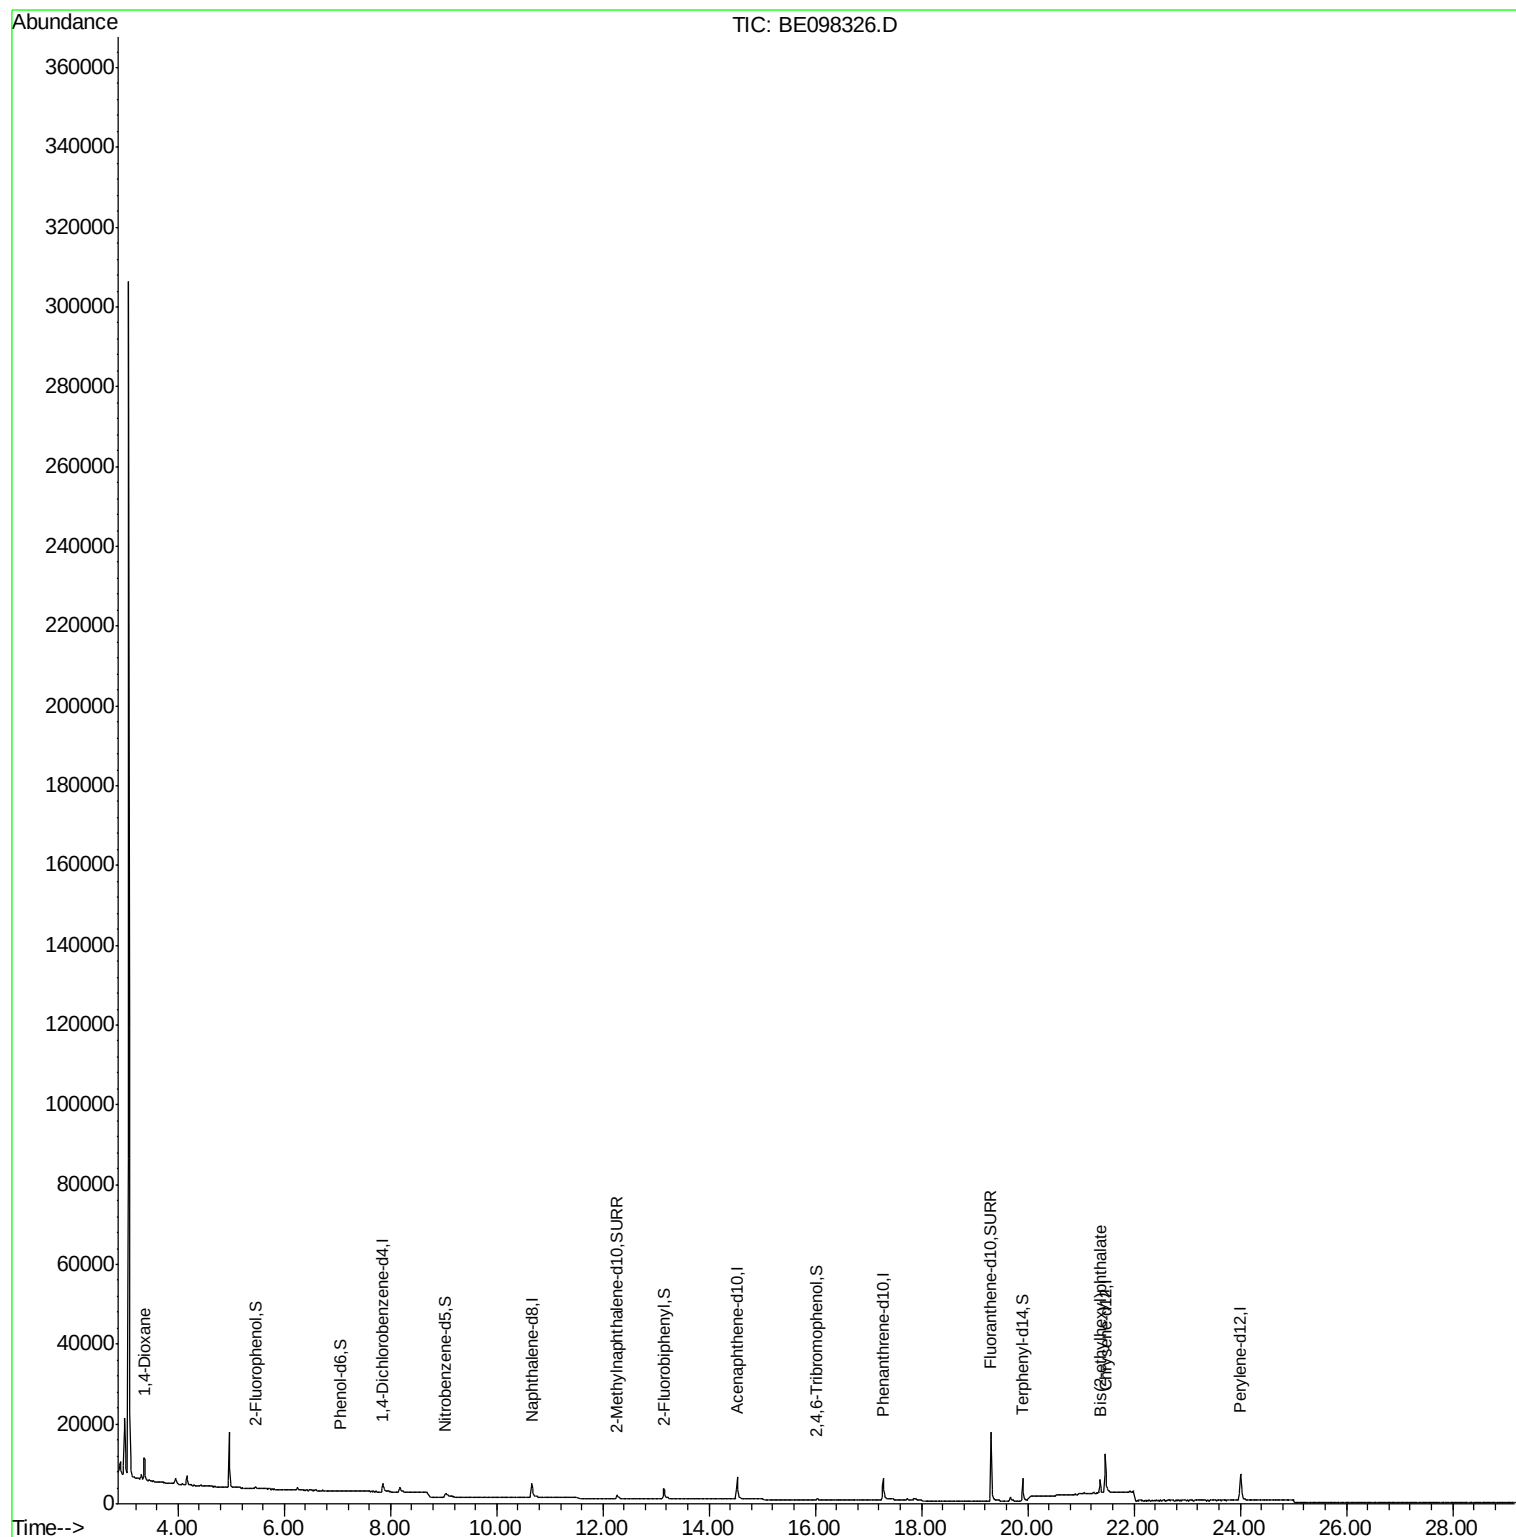

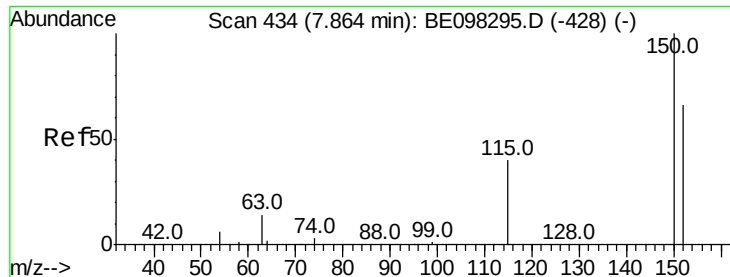

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.86 min Scan# 434

Delta R.T. -0.00 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06

Instrument :

BNA_E

ClientSampleId :

BP-DUP02-20181205DL


Tot Ion:152 Resp: 1262

Ion Ratio Lower Upper




152 100

150 152.3 124.2 186.4

115 70.8 53.9 80.9

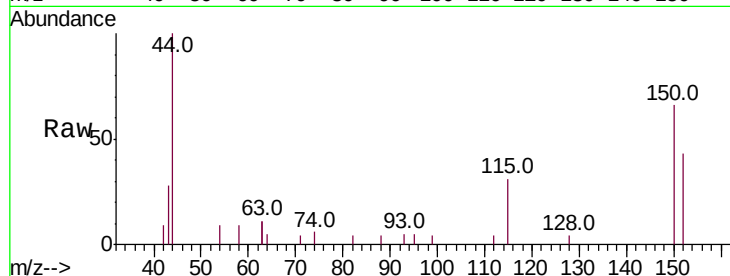

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

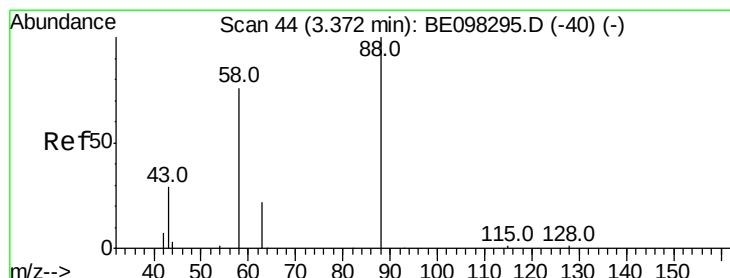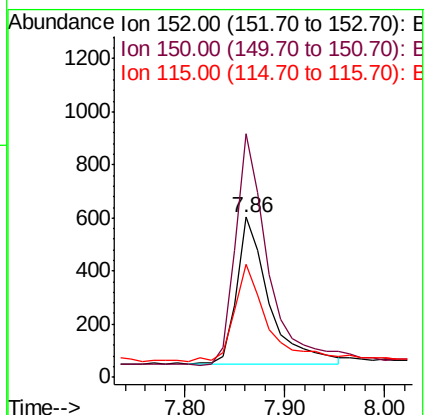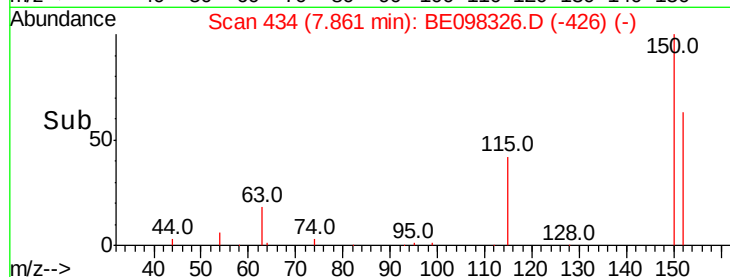

#2

1,4-Dioxane

Concen: 1.651 ng

RT: 3.37 min Scan# 44

Delta R.T. -0.00 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06


Tgt Ion: 88 Resp: 3604

Ion Ratio Lower Upper



88 100


58 95.3 75.0 112.6

43 49.1 38.3 57.5

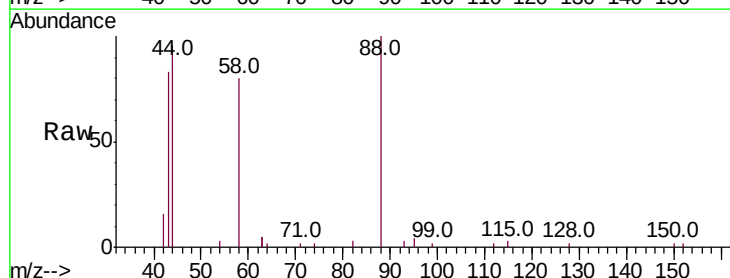

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

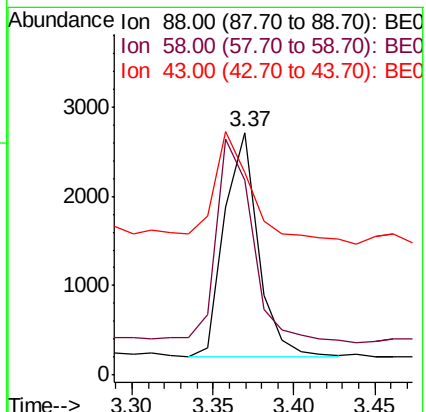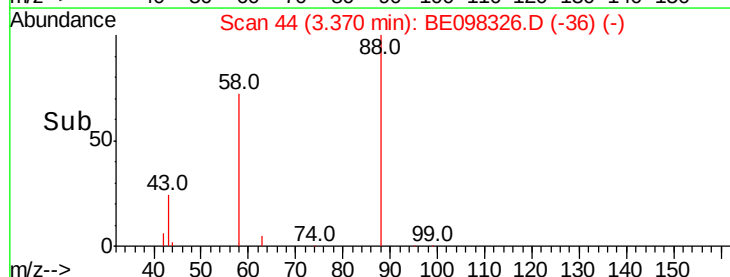

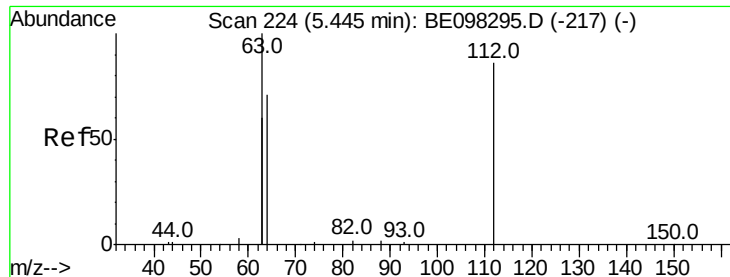

#4

2-Fluorophenol

Concen: 0.093 ng

RT: 5.45 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06

Instrument :

BNA_E

ClientSampleId :

BP-DUP02-20181205DL


Tot Ion:112 Resp: 276

Ion Ratio Lower Upper

112 100

64 71.4 59.8 89.8




63 147.8 133.7 200.5

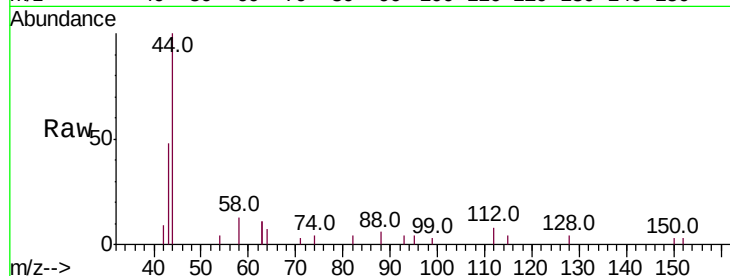

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

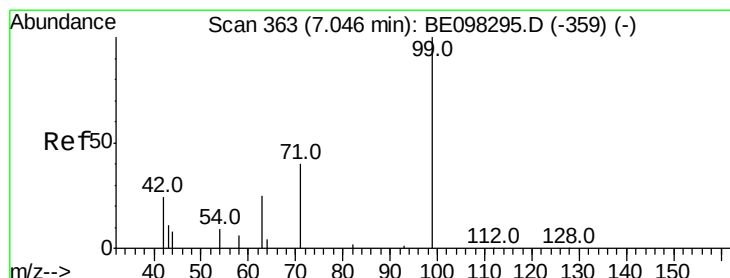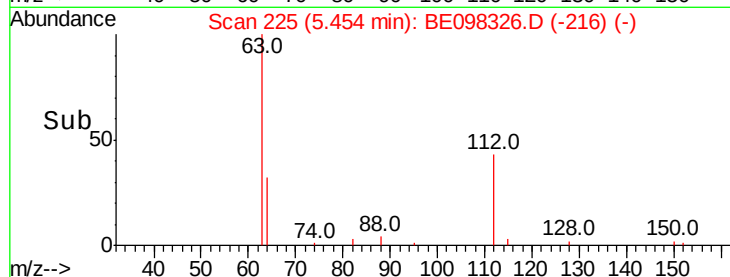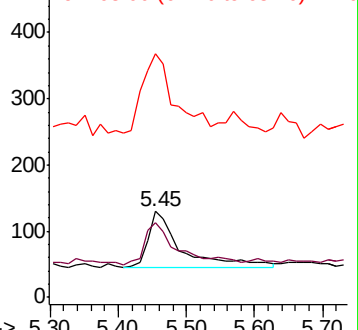

#5

Phenol-d6

Concen: 0.044 ng

RT: 7.05 min Scan# 364

Delta R.T. 0.01 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06


Tgt Ion: 99 Resp: 184

Ion Ratio Lower Upper

99 100

42 0.0 26.3 39.5#



71 36.4 33.6 50.4

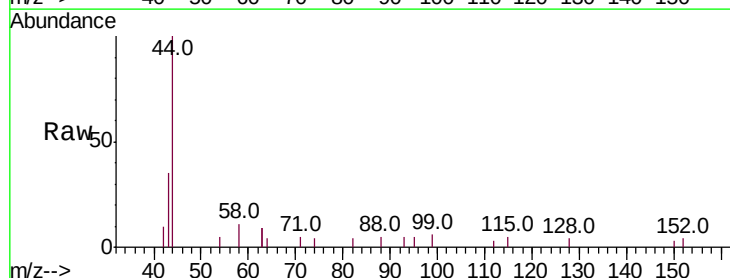


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

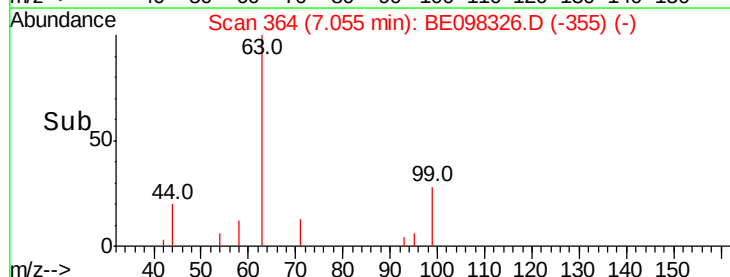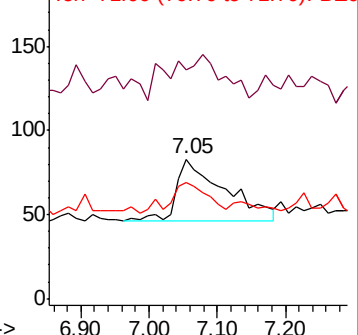



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. -0.00 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06

Instrument :

BNA_E

ClientSampleId :

BP-DUP02-20181205DL

Tot Ion:136 Resp: 5552



Ion Ratio Lower Upper

136 100

137 13.4 9.2 13.8

54 45.1 28.4 42.6#

68 8.0 5.4 8.0


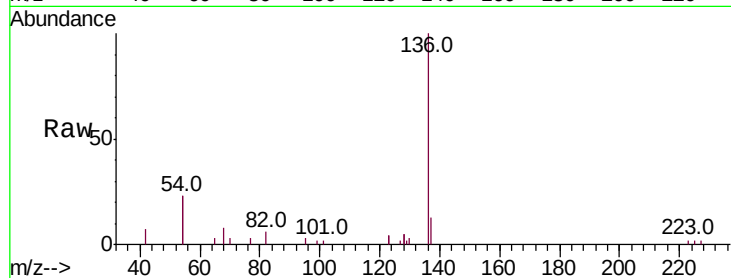


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

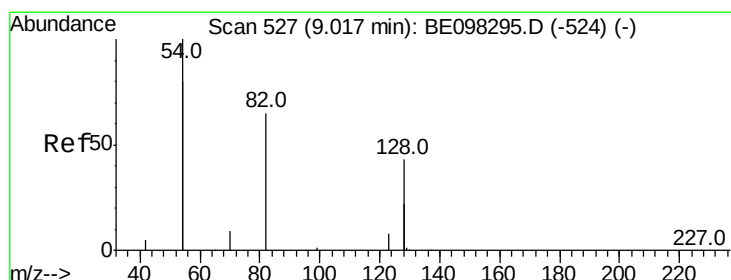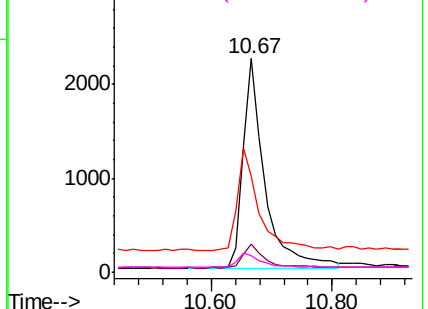

#8

Nitrobenzene-d5

Concen: 0.198 ng

RT: 9.04 min Scan# 529

Delta R.T. 0.03 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06



Tgt Ion: 82 Resp: 1000

Ion Ratio Lower Upper

82 100

128 185.7 102.4 153.6#


54 286.5 221.8 332.8

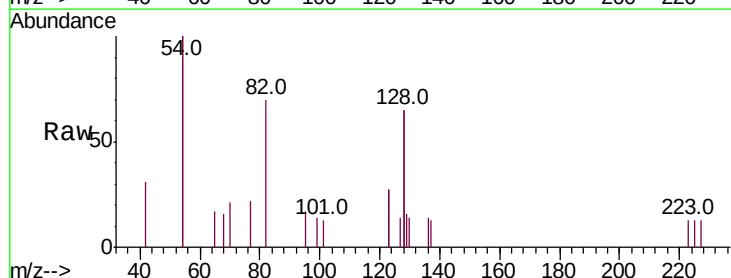


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0




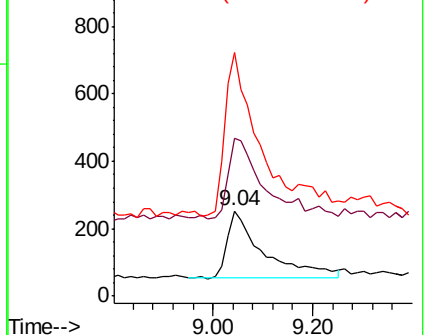




#11
 2-Methylnaphthalene-d10
 Concen: 0.201 ng
 RT: 12.27 min Scan# 767
 Delta R.T. 0.00 min
 Lab File: BE098326.D
 Acq: 11 Dec 2018 10:06




Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP02-20181205DL


Tot Ion:152 Resp: 1813
 Ion Ratio Lower Upper
 152 100
 151 19.1 16.2 24.4

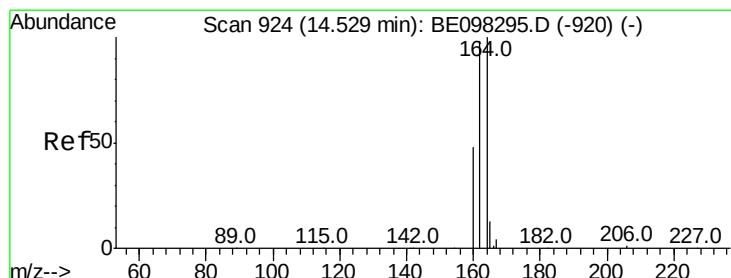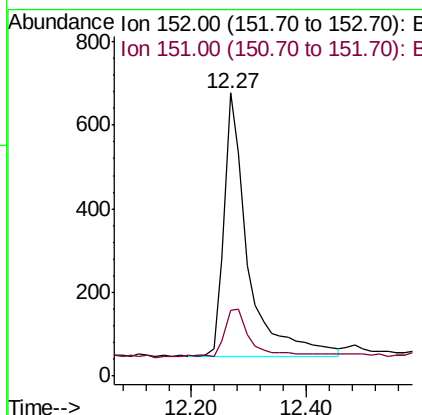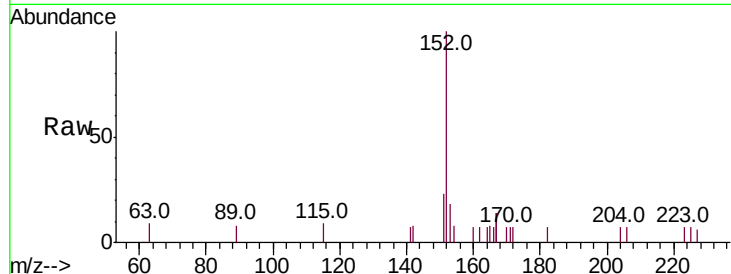

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.53 min Scan# 924
 Delta R.T. 0.00 min
 Lab File: BE098326.D
 Acq: 11 Dec 2018 10:06

Tgt Ion:164 Resp: 3722
 Ion Ratio Lower Upper
 164 100
 162 97.5 77.6 116.4
 160 47.4 36.0 54.0

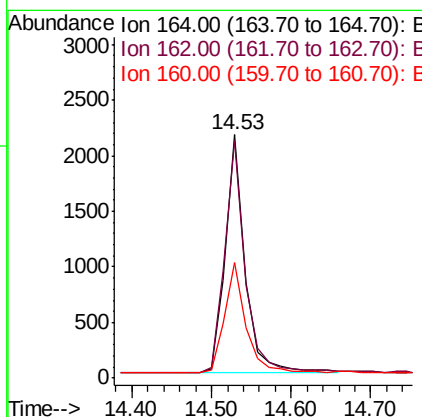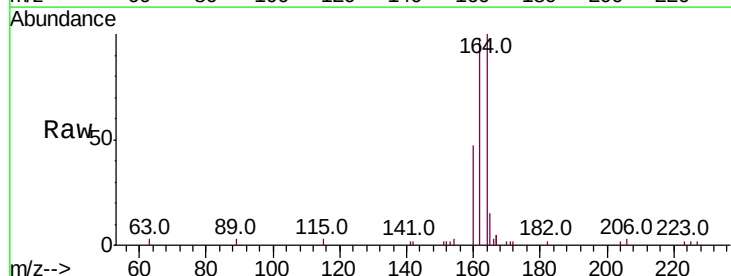



#14

2,4,6-Tribromophenol

Concen: 0.190 ng

RT: 16.03 min Scan# 1042

Delta R.T. 0.01 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06

Instrument :

BNA_E

ClientSampleId :

BP-DUP02-20181205DL


Tot Ion:330 Resp: 260

Ion Ratio Lower Upper

330 100

332 98.5 76.2 114.4




141 41.5 39.0 58.4

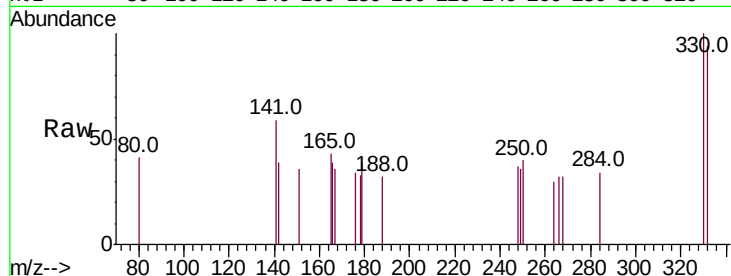

Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

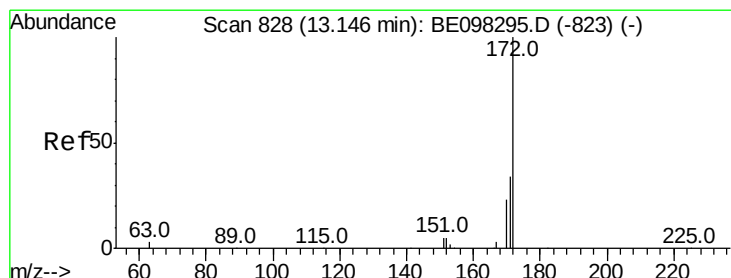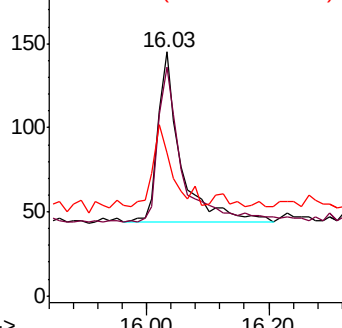

#15

2-Fluorobiphenyl

Concen: 0.263 ng

RT: 13.15 min Scan# 828

Delta R.T. 0.00 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06


Tgt Ion:172 Resp: 4135

Ion Ratio Lower Upper

172 100

171 36.2 27.5 41.3



170 27.0 19.6 29.4

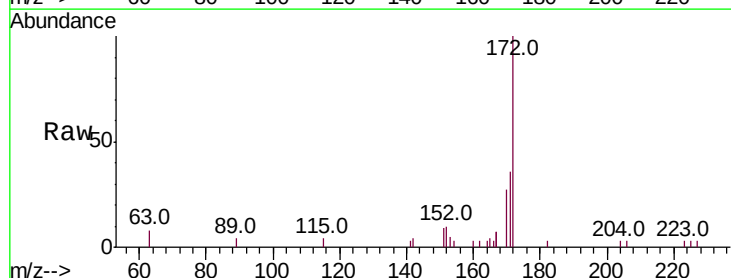


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

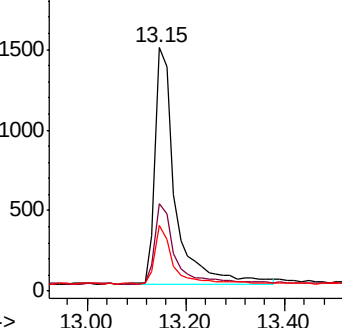

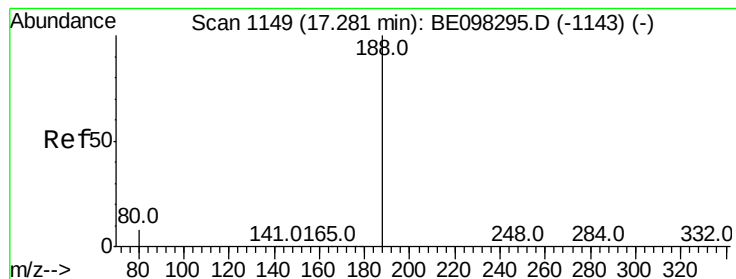

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.28 min Scan# 1149

Delta R.T. -0.00 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06

Instrument :

BNA_E

ClientSampleId :

BP-DUP02-20181205DL


Tot Ion:188 Resp: 9874

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 10.1 7.2 10.8

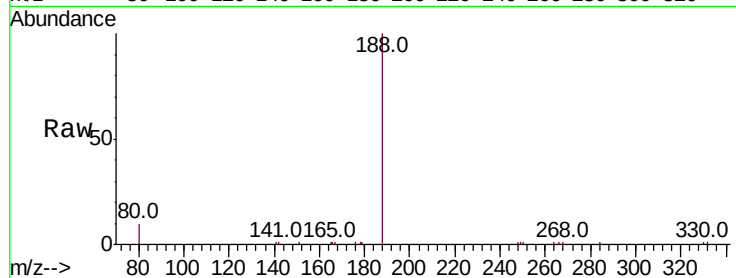

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

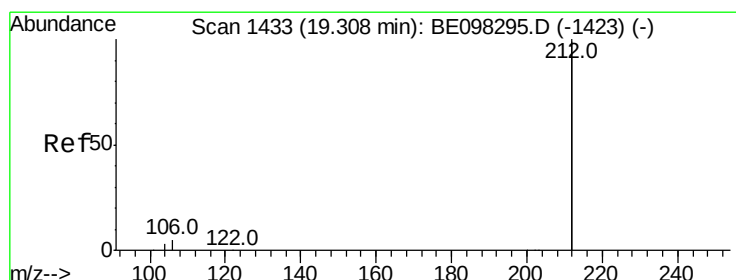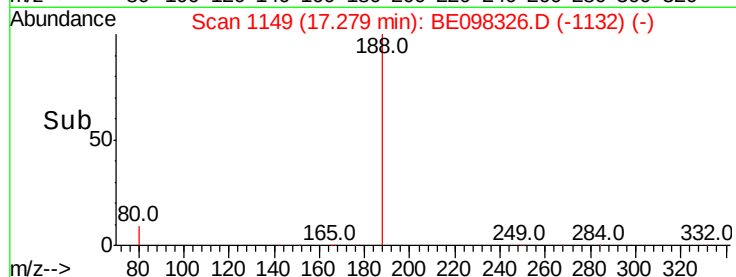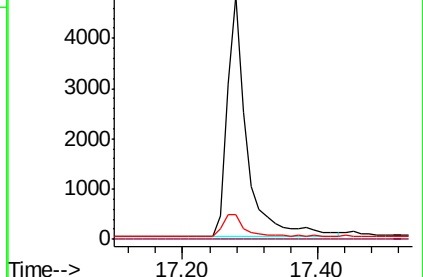

#25

Fluoranthene-d10

Concen: 0.222 ng

RT: 19.31 min Scan# 1433

Delta R.T. 0.00 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06


Tgt Ion:212 Resp: 28180

Ion Ratio Lower Upper

212 100

106 2.6 2.2 3.2



104 1.5 1.3 1.9

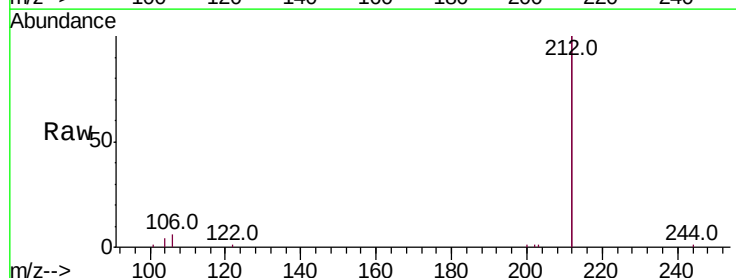


Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

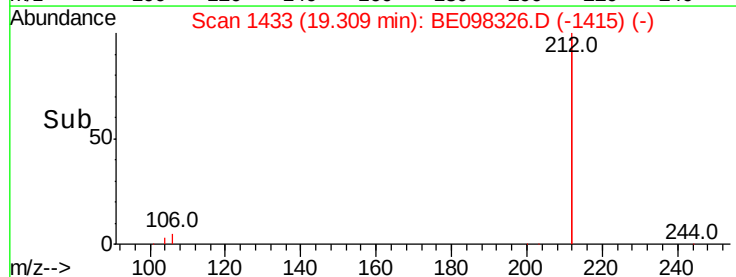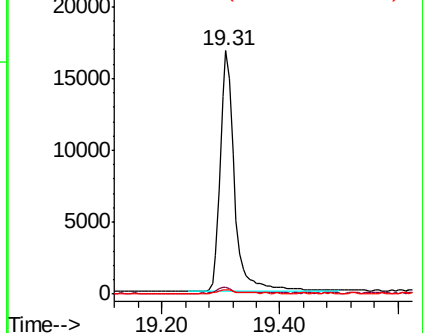



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.46 min Scan# 1671

Delta R.T. -0.00 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06

Instrument :

BNA_E

ClientSampleId :

BP-DUP02-20181205DL


Tot Ion:240 Resp: 12347

Ion Ratio Lower Upper

240 100

120 8.2 9.5 14.3#




236 27.7 22.7 34.1

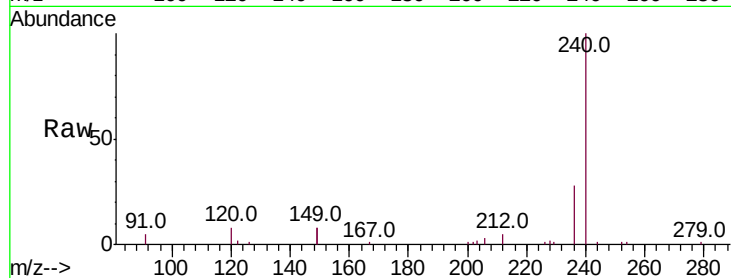

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

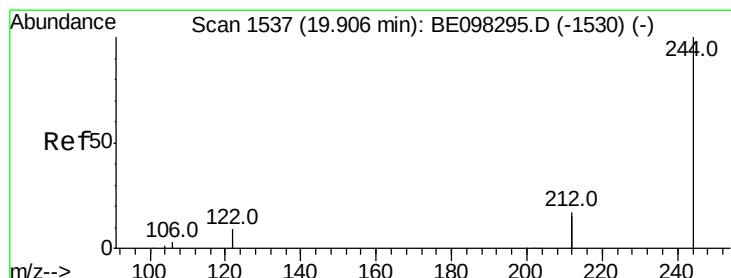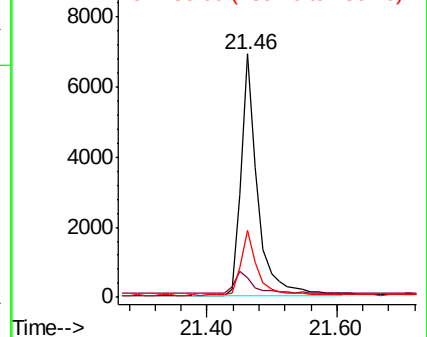

#29

Terphenyl-d14

Concen: 0.216 ng

RT: 19.91 min Scan# 1537

Delta R.T. 0.00 min

Lab File: BE098326.D

Acq: 11 Dec 2018 10:06


Tgt Ion:244 Resp: 6495

Ion Ratio Lower Upper

244 100

212 36.3 27.4 41.0



122 10.8 8.3 12.5

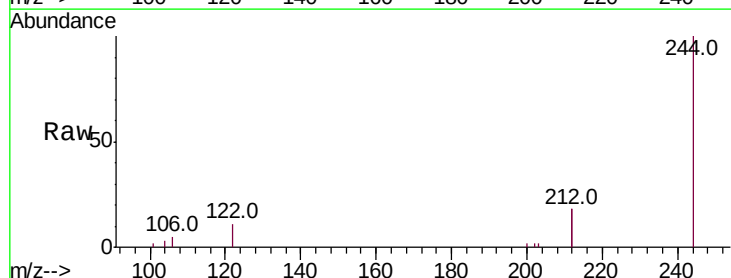


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E




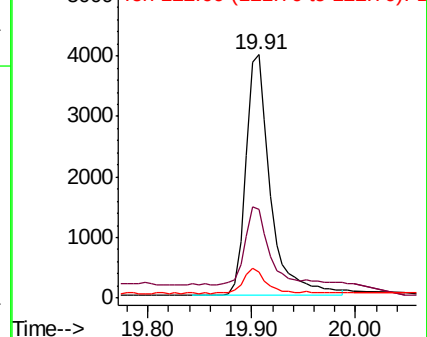




#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.070 ng
 RT: 21.37 min Scan# 1663
 Delta R.T. -0.00 min
 Lab File: BE098326.D
 Acq: 11 Dec 2018 10:06

Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP02-20181205DL

Tot Ion:149 Resp: 5022
 Ion Ratio Lower Upper
 149 100
 167 5.7 5.7 8.5#
 279 1.3 1.0 1.4

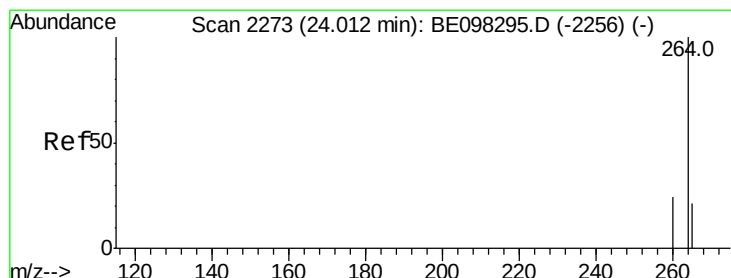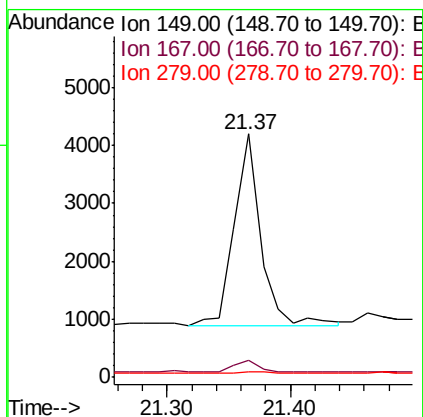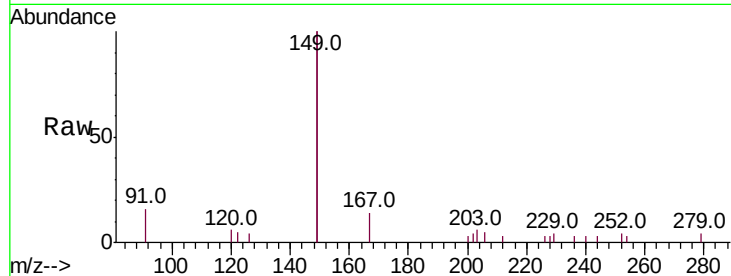

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.01 min Scan# 2272
 Delta R.T. -0.00 min
 Lab File: BE098326.D
 Acq: 11 Dec 2018 10:06

Tgt Ion:264 Resp: 11543
 Ion Ratio Lower Upper
 264 100
 260 24.7 20.2 30.2
 265 28.0 25.2 37.8

