


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE121018\
 Data File : BE098300.D
 Acq On : 10 Dec 2018 16:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

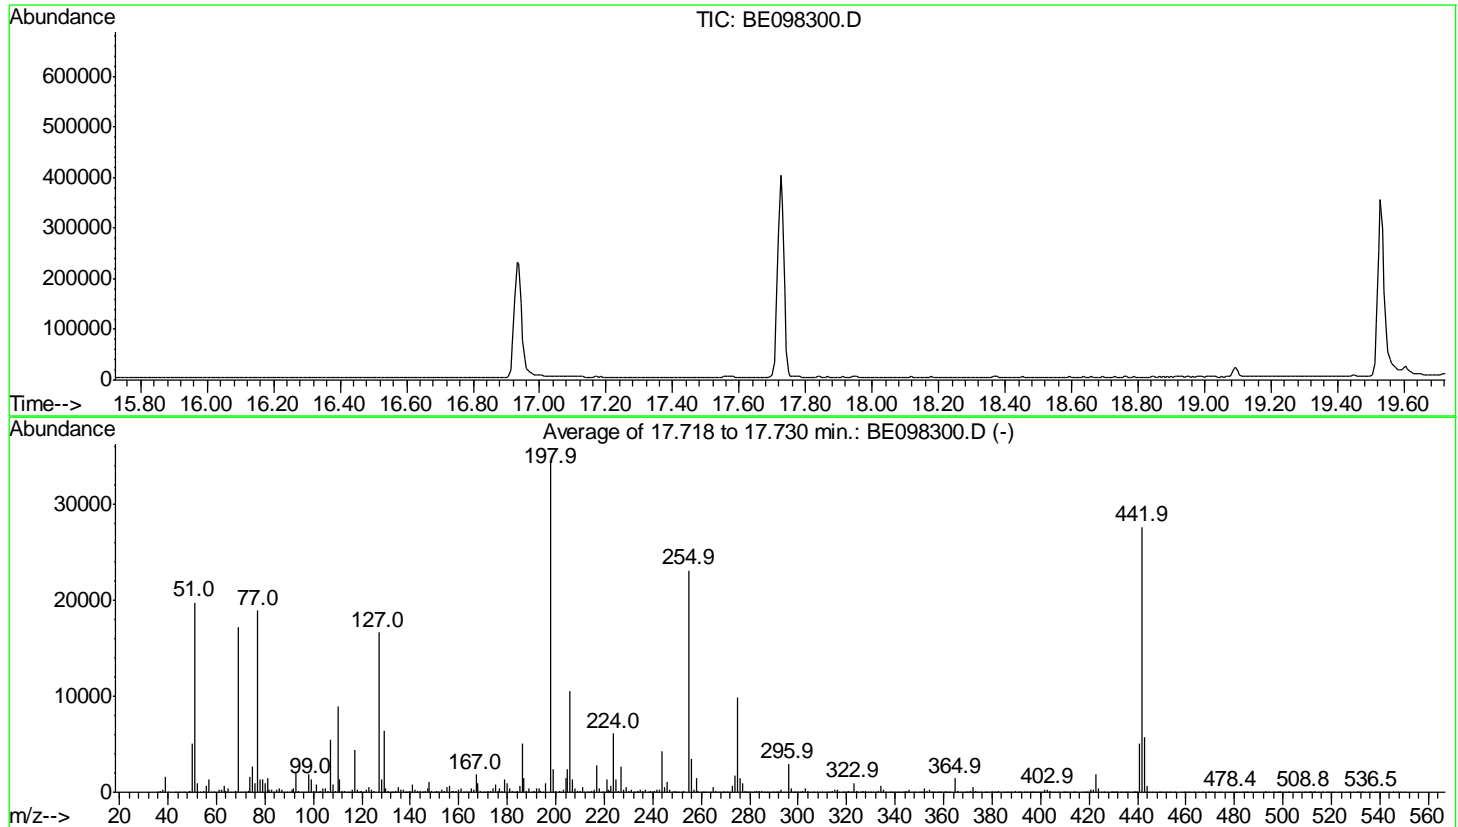

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.2	19779	PASS
68	69	0.00	2	1.2	204	PASS
69	198	0.00	100	50.0	17267	PASS
70	69	0.00	2	0.2	37	PASS
127	198	10	80	48.2	16673	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34556	PASS
199	198	5	9	6.9	2378	PASS
275	198	10	60	28.7	9921	PASS
365	198	1	100	4.2	1447	PASS
441	198	0.01	100	14.7	5067	PASS
442	198	50	100	79.9	27626	PASS
443	442	15	24	20.7	5710	PASS