

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121218\
 Data File : BE098373.D
 Acq On : 12 Dec 2018 22:30
 Operator : SJ/JU
 Sample : J6324-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE-109D3-20181206

Quant Time: Dec 13 06:59:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	1115	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	4843	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	3268	0.40	ng	0.00
19) Phenanthrene-d10	17.27	188	8732	0.40	ng	-0.01
27) Chrysene-d12	21.46	240	10264	0.40	ng	0.00
34) Perylene-d12	24.00	264	9860	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.46	112	558	0.21	ng	0.01
5) Phenol-d6	7.05	99	433	0.12	ng	0.00
8) Nitrobenzene-d5	9.04	82	1533	0.35	ng	0.03
11) 2-Methylnaphthalene-d10	12.27	152	3203	0.41	ng	0.00
14) 2,4,6-Tribromophenol	16.02	330	572	0.48	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	5096	0.37	ng	0.00
25) Fluoranthene-d10	19.30	212	48943	0.44	ng	0.00
29) Terphenyl-d14	19.90	244	8624	0.35	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.36	88	6487	3.364	ng	98
32) Bis(2-ethylhexyl)phthalate	21.35	149	6267	0.106	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121218\
Data File : BE098373.D
Acq On : 12 Dec 2018 22:30
Operator : SJ/JU
Sample : J6324-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE-109D3-20181206

Quant Time: Dec 13 06:59:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

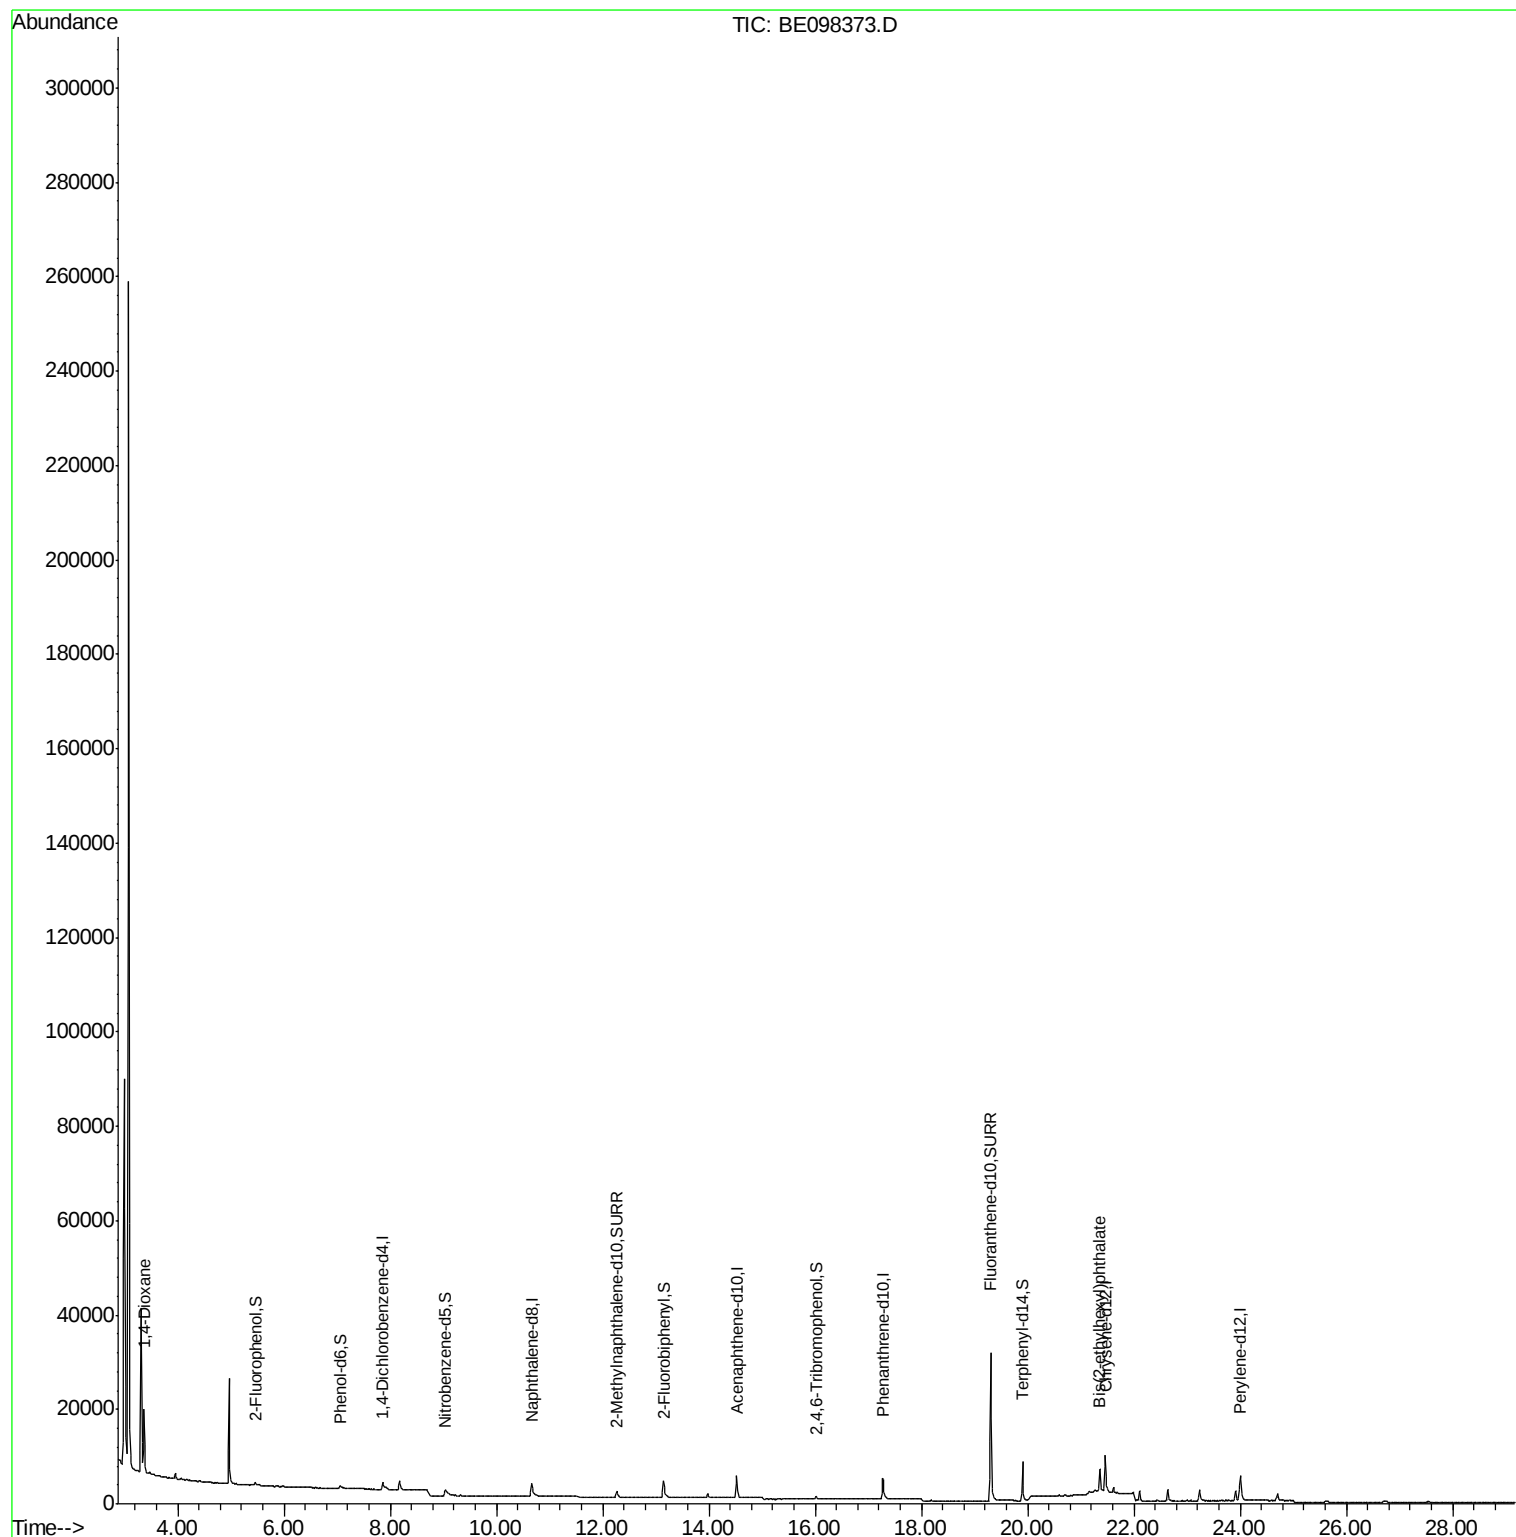

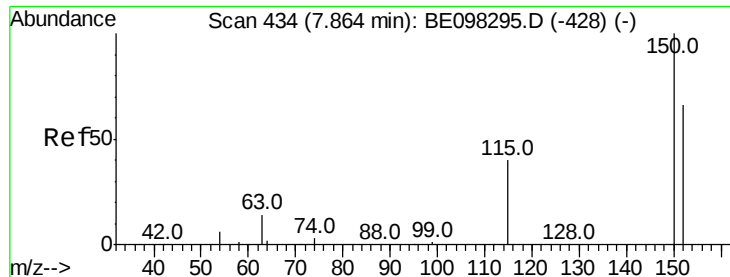


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.86 min Scan# 434
Delta R.T. 0.00 min
Lab File: BE098373.D
Acq: 12 Dec 2018 22:30

Instrument :
BNA_E
ClientSampleId :
RE-109D3-20181206

Tot Ion:152 Resp: 1115
Ion Ratio Lower Upper
152 100
150 149.6 124.2 186.4
115 63.6 53.9 80.9

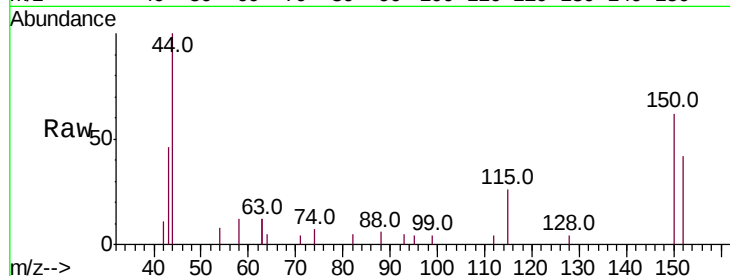


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

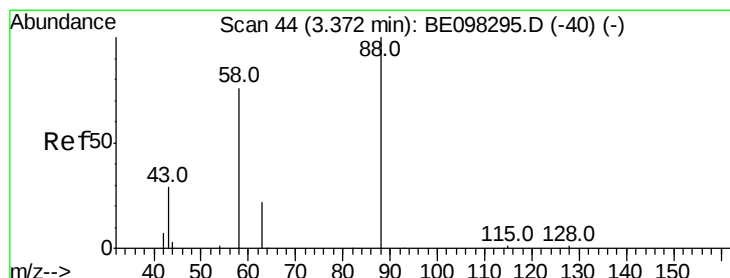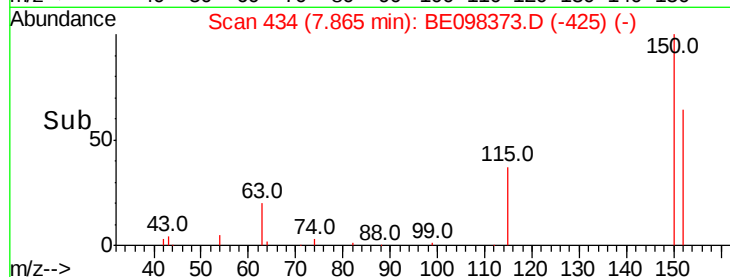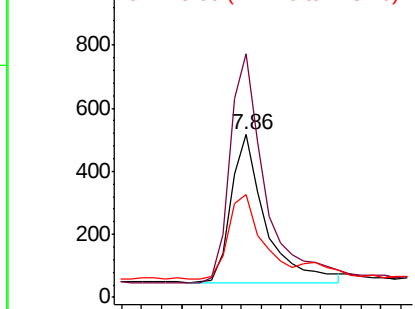



#2


1,4-Dioxane
Concen: 3.364 ng
RT: 3.36 min Scan# 43
Delta R.T. -0.01 min
Lab File: BE098373.D
Acq: 12 Dec 2018 22:30

Tgt Ion: 88 Resp: 6487
Ion Ratio Lower Upper
88 100
58 94.1 75.0 112.6
43 51.1 38.3 57.5

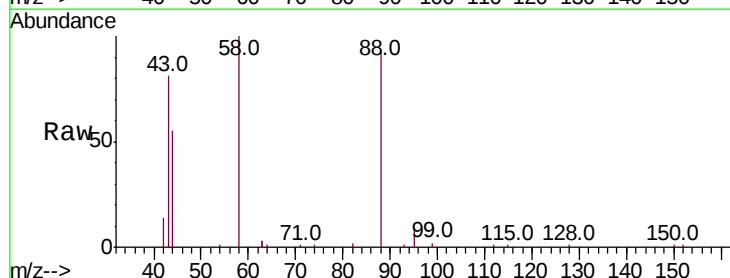

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

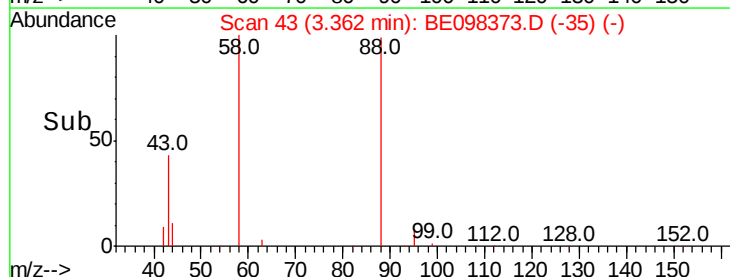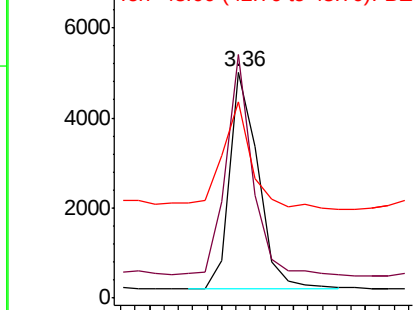

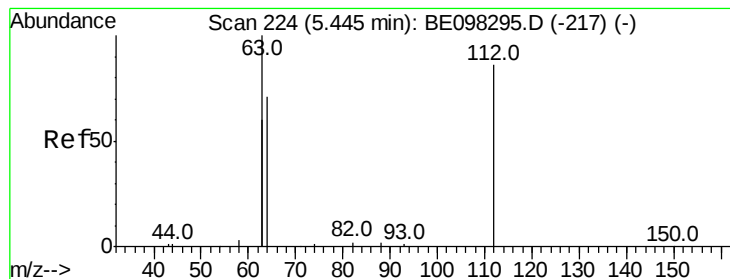

#4

2-Fluorophenol

Concen: 0.214 ng

RT: 5.46 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098373.D

Acq: 12 Dec 2018 22:30

Instrument :

BNA_E

ClientSampleId :

RE-109D3-20181206


Tot Ion:112 Resp: 558

Ion Ratio Lower Upper

112 100

64 69.4 59.8 89.8




63 194.6 133.7 200.5

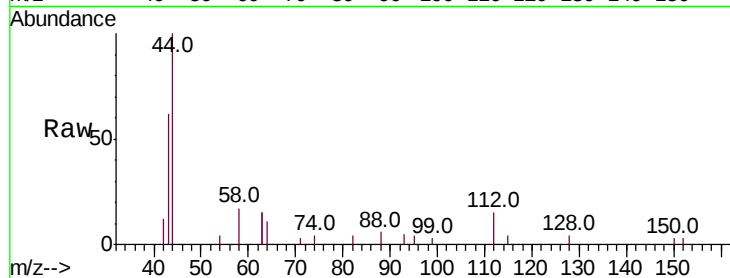

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

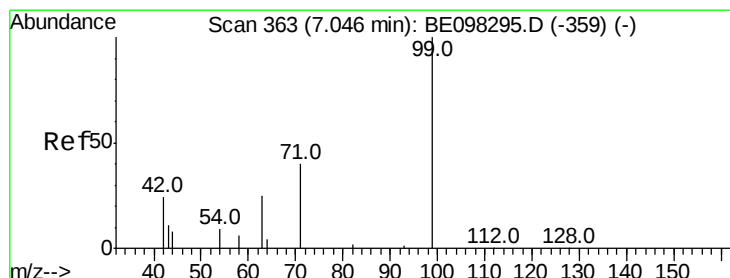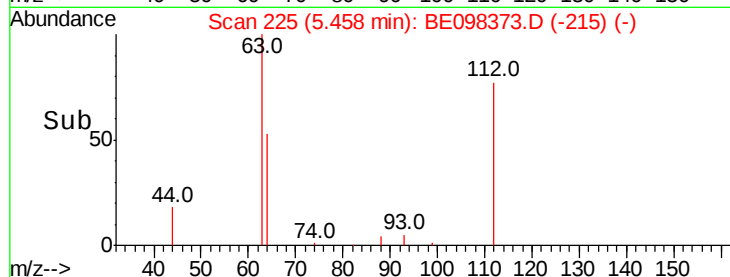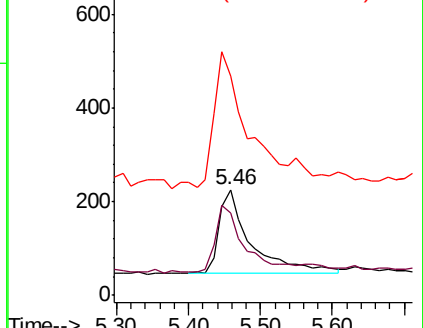

#5

Phenol-d6

Concen: 0.117 ng

RT: 7.05 min Scan# 363

Delta R.T. 0.00 min

Lab File: BE098373.D

Acq: 12 Dec 2018 22:30


Tgt Ion: 99 Resp: 433

Ion Ratio Lower Upper

99 100

42 50.8 26.3 39.5#



71 39.3 33.6 50.4

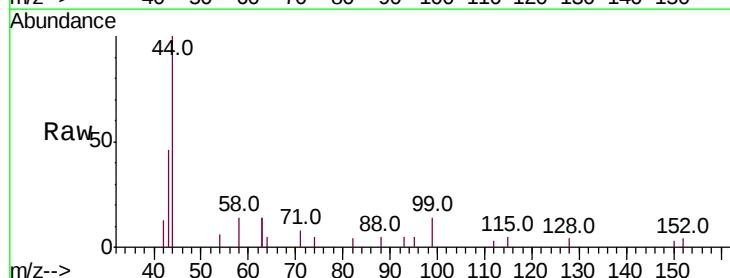


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

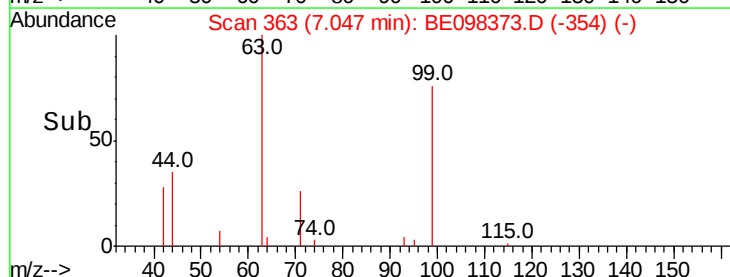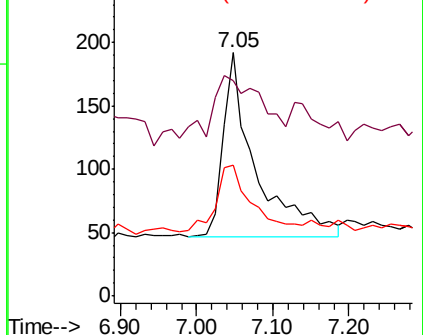

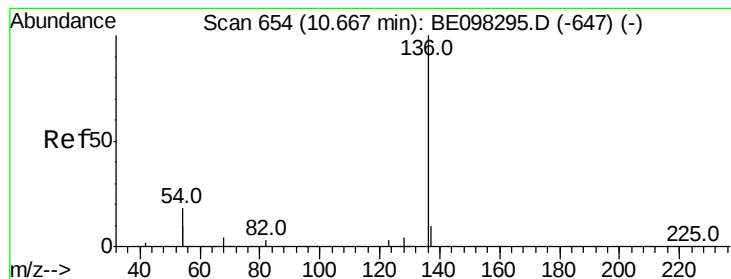

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. -0.00 min

Lab File: BE098373.D

Acq: 12 Dec 2018 22:30

Instrument :

BNA_E

ClientSampleId :

RE-109D3-20181206

Tot Ion:136 Resp: 4843





Ion Ratio Lower Upper

136 100

137 14.3 9.2 13.8#

54 47.4 28.4 42.6#

68 8.7 5.4 8.0#

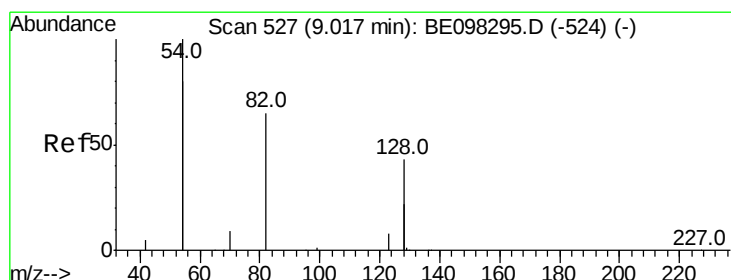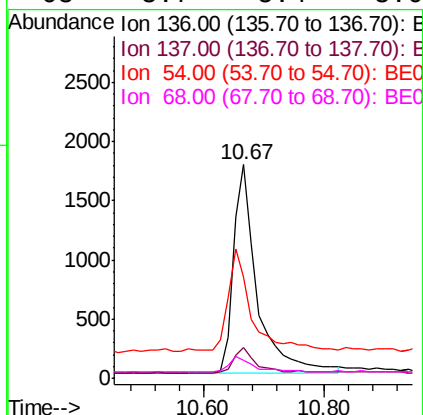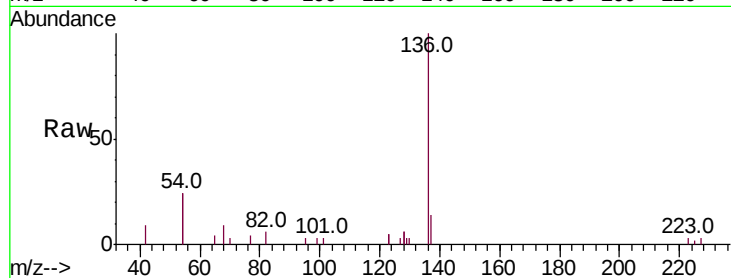

#8

Nitrobenzene-d5

Concen: 0.348 ng

RT: 9.04 min Scan# 529

Delta R.T. 0.03 min

Lab File: BE098373.D

Acq: 12 Dec 2018 22:30




Tgt Ion: 82 Resp: 1533


Ion Ratio Lower Upper

82 100

128 182.8 102.4 153.6#

54 281.1 221.8 332.8


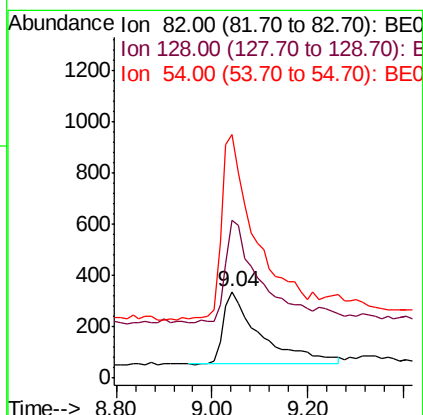

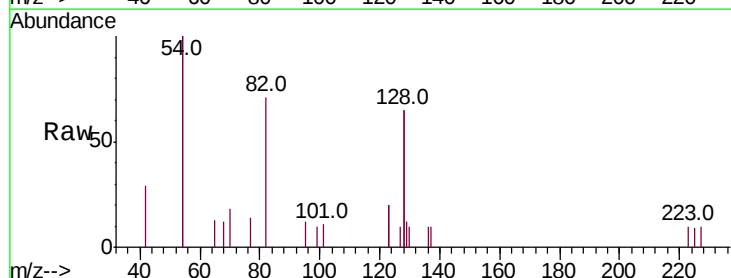




#11
2-Methylnaphthalene-d10
Concen: 0.407 ng
RT: 12.27 min Scan# 767
Delta R.T. -0.00 min
Lab File: BE098373.D
Acq: 12 Dec 2018 22:30




Instrument :
BNA_E
ClientSampleId :
RE-109D3-20181206


Tot Ion:152 Resp: 3203
Ion Ratio Lower Upper
152 100
151 21.1 16.2 24.4

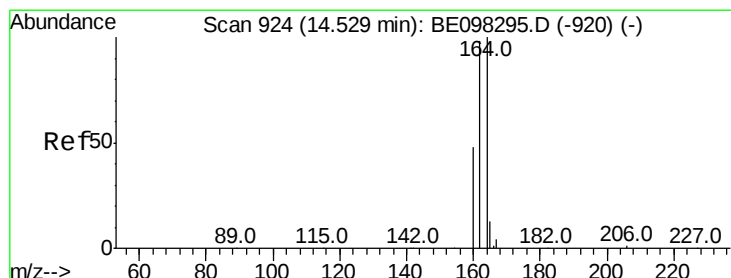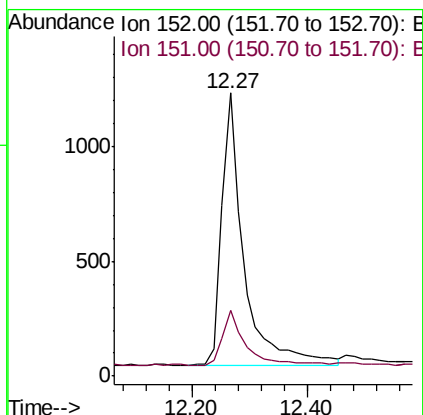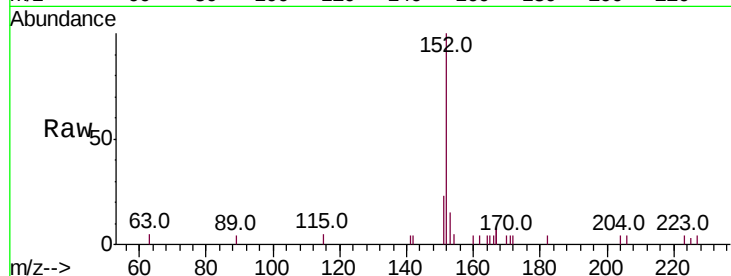

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.53 min Scan# 924
Delta R.T. -0.00 min
Lab File: BE098373.D
Acq: 12 Dec 2018 22:30

Tgt Ion:164 Resp: 3268
Ion Ratio Lower Upper
164 100
162 96.6 77.6 116.4
160 46.8 36.0 54.0

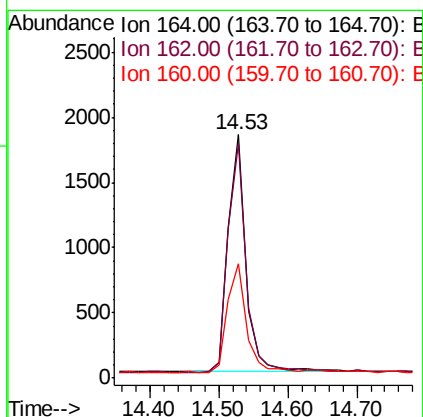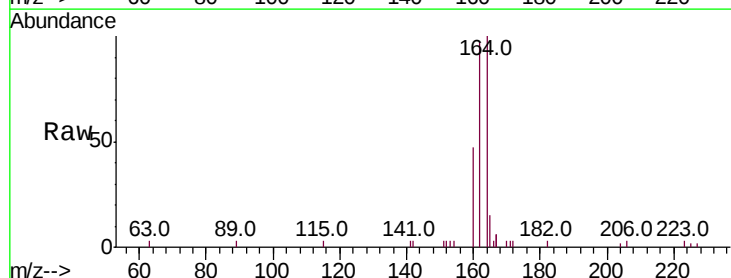







#14
 2,4,6-Tribromophenol
 Concen: 0.477 ng
 RT: 16.02 min Scan# 1041
 Delta R.T. -0.00 min
 Lab File: BE098373.D
 Acq: 12 Dec 2018 22:30

Instrument :
 BNA_E
 ClientSampleId :
 RE-109D3-20181206

Tot Ion:330 Resp: 572
 Ion Ratio Lower Upper
 330 100
 332 93.0 76.2 114.4
 141 39.5 39.0 58.4

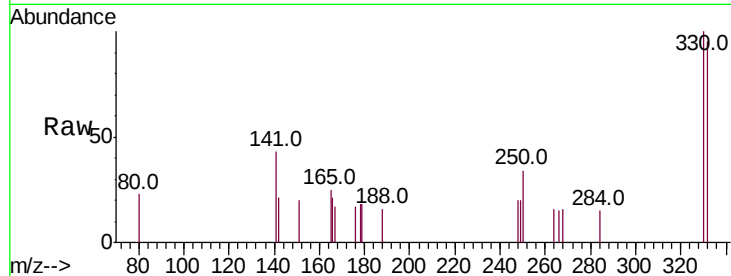


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

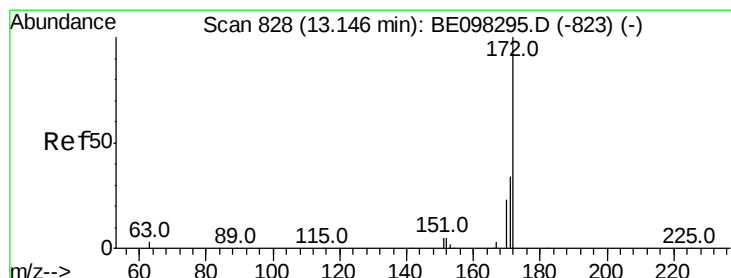
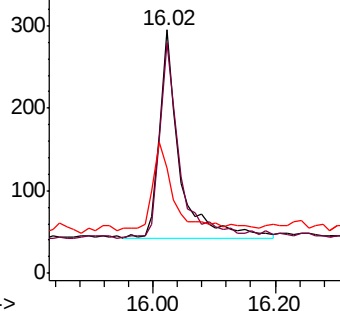



#15
 2-Fluorobiphenyl
 Concen: 0.370 ng
 RT: 13.15 min Scan# 828
 Delta R.T. -0.00 min
 Lab File: BE098373.D
 Acq: 12 Dec 2018 22:30

Tgt Ion:172 Resp: 5096
 Ion Ratio Lower Upper
 172 100
 171 35.1 27.5 41.3
 170 23.4 19.6 29.4

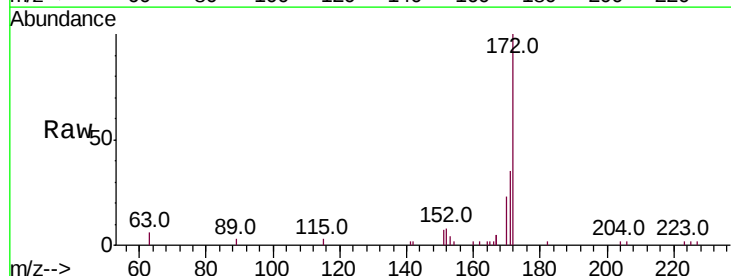

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

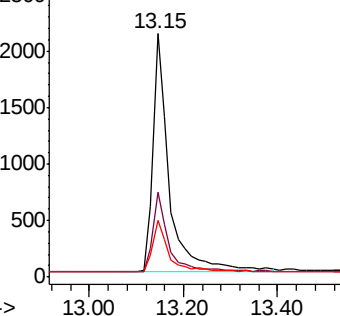

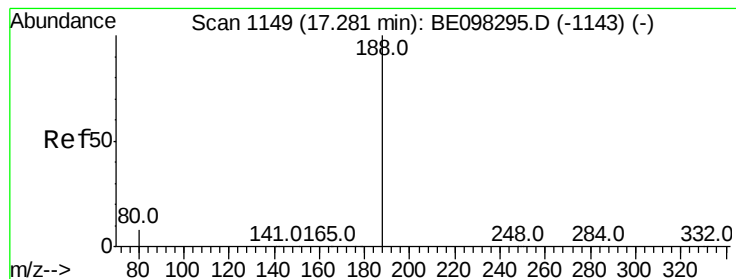

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.27 min Scan# 1148

Delta R.T. -0.01 min

Lab File: BE098373.D

Acq: 12 Dec 2018 22:30

Instrument :

BNA_E

ClientSampleId :

RE-109D3-20181206


Tot Ion:188 Resp: 8732

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 13.5 7.2 10.8#

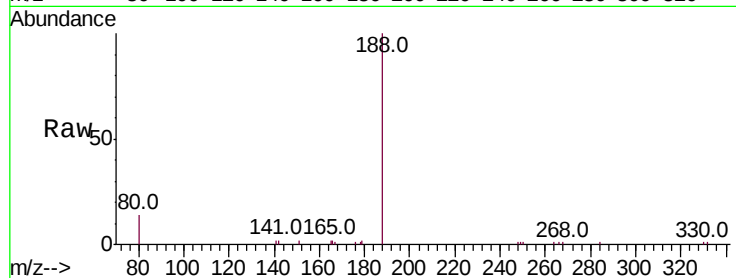

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

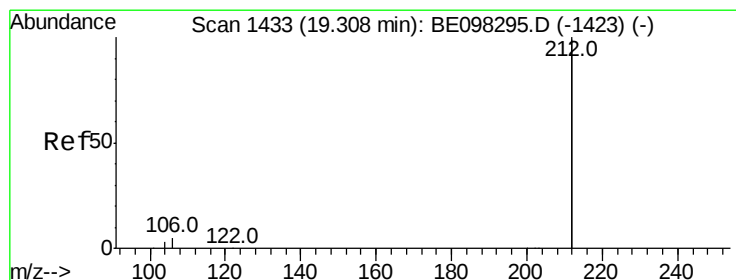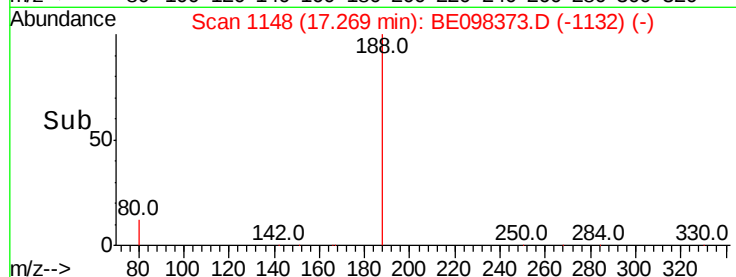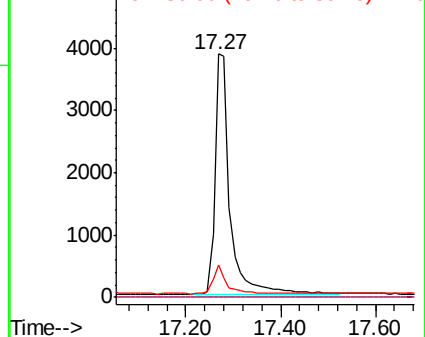

#25

Fluoranthene-d10

Concen: 0.437 ng

RT: 19.30 min Scan# 1432

Delta R.T. -0.00 min

Lab File: BE098373.D

Acq: 12 Dec 2018 22:30


Tgt Ion:212 Resp: 48943

Ion Ratio Lower Upper

212 100

106 2.6 2.2 3.2



104 1.5 1.3 1.9

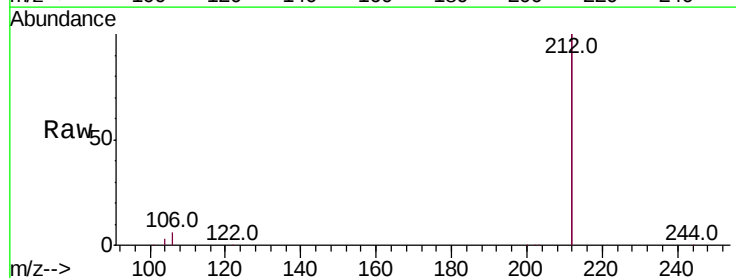


Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

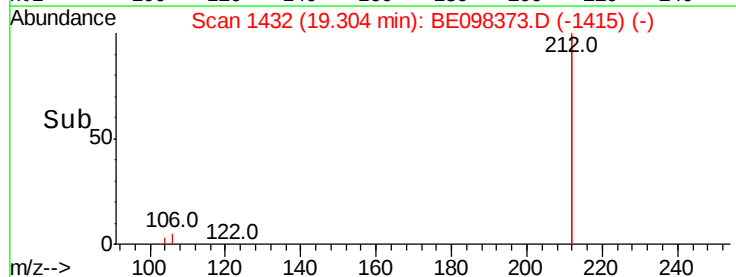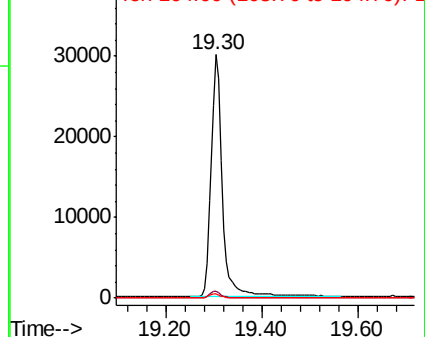



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.46 min Scan# 1671

Delta R.T. -0.00 min

Lab File: BE098373.D

Acq: 12 Dec 2018 22:30

Instrument :

BNA_E

ClientSampleId :

RE-109D3-20181206


Tot Ion:240 Resp: 10264

Ion Ratio Lower Upper

240 100

120 7.4 9.5 14.3#




236 27.0 22.7 34.1

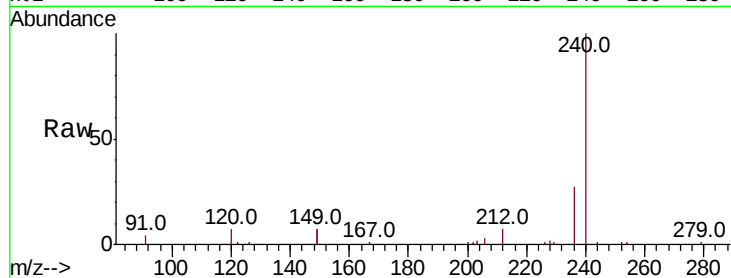

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

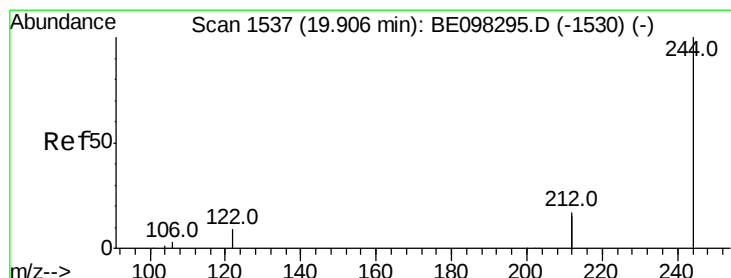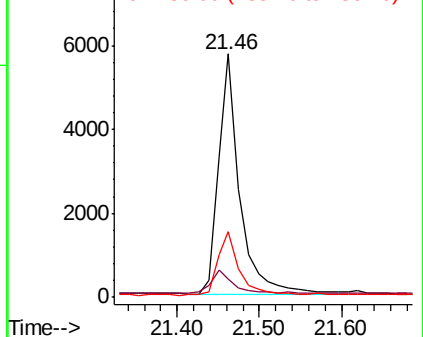

#29

Terphenyl-d14

Concen: 0.346 ng

RT: 19.90 min Scan# 1536

Delta R.T. -0.00 min

Lab File: BE098373.D

Acq: 12 Dec 2018 22:30


Tgt Ion:244 Resp: 8624

Ion Ratio Lower Upper

244 100

212 35.0 27.4 41.0



122 10.2 8.3 12.5

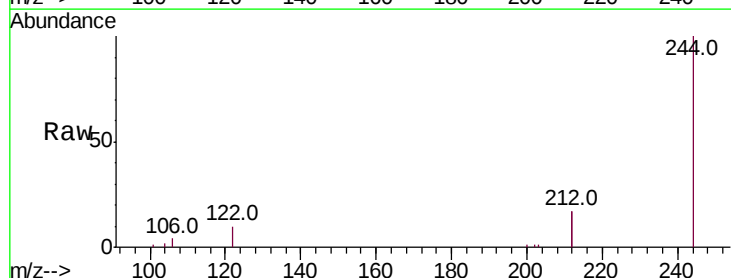


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E




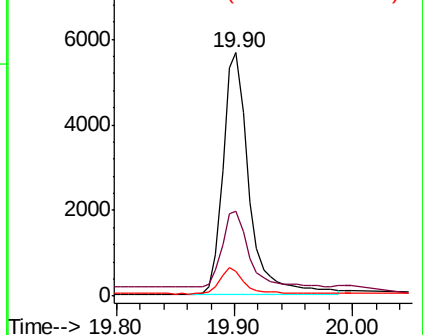




#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.106 ng
 RT: 21.35 min Scan# 1662
 Delta R.T. -0.01 min
 Lab File: BE098373.D
 Acq: 12 Dec 2018 22:30

Instrument :
 BNA_E
 ClientSampleId :
 RE-109D3-20181206

Tot Ion:149 Resp: 6267
 Ion Ratio Lower Upper
 149 100
 167 7.5 5.7 8.5
 279 1.6 1.0 1.4#

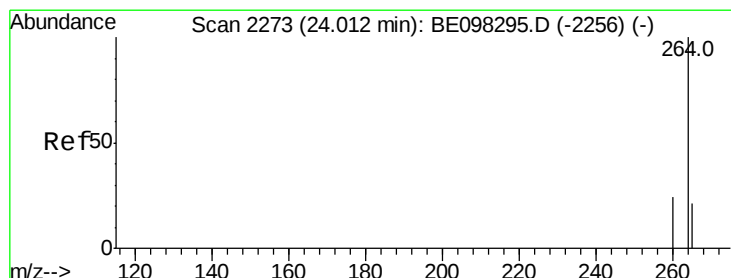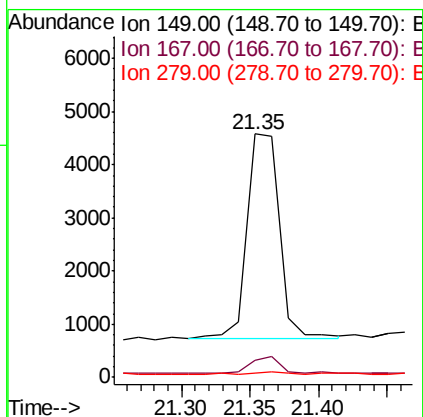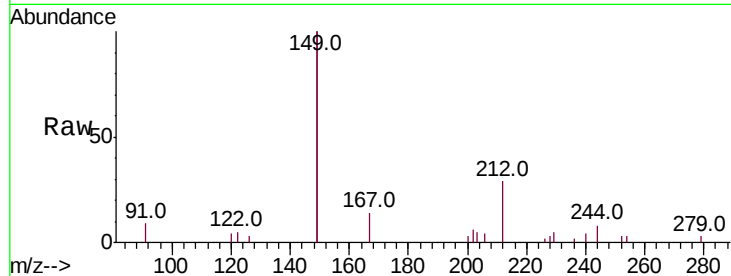

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.00 min Scan# 2270
 Delta R.T. -0.01 min
 Lab File: BE098373.D
 Acq: 12 Dec 2018 22:30

Tgt Ion:264 Resp: 9860
 Ion Ratio Lower Upper
 264 100
 260 25.5 20.2 30.2
 265 27.0 25.2 37.8

