


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE121218\
 Data File : BE098361.D
 Acq On : 12 Dec 2018 15:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

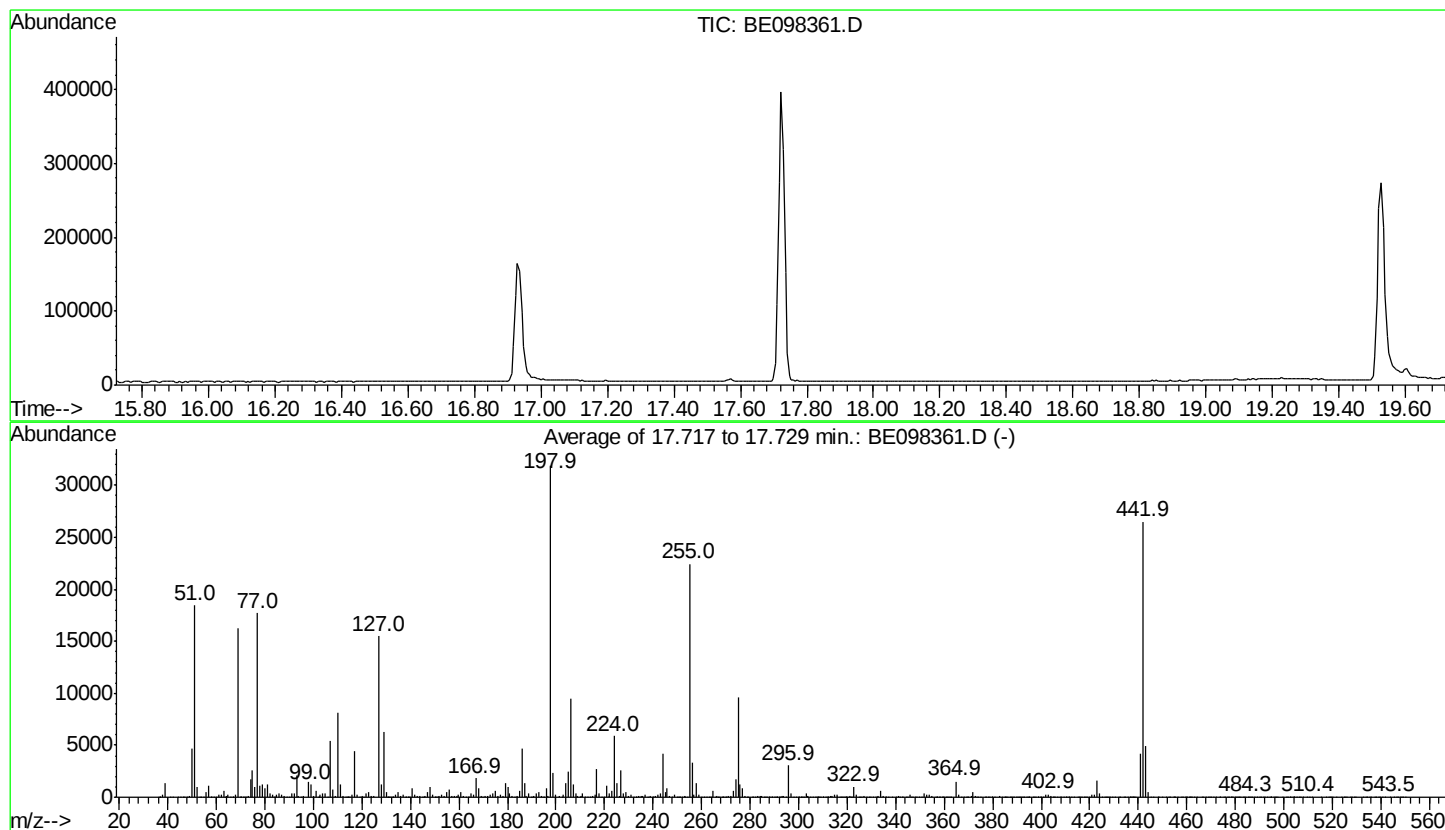

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.8	18437	PASS
68	69	0.00	2	1.4	221	PASS
69	198	0.00	100	51.2	16315	PASS
70	69	0.00	2	0.2	32	PASS
127	198	10	80	48.5	15466	PASS
197	198	0.00	2	0.2	73	PASS
198	198	100	100	100.0	31889	PASS
199	198	5	9	7.3	2313	PASS
275	198	10	60	30.3	9651	PASS
365	198	1	100	4.7	1501	PASS
441	198	0.01	100	13.1	4188	PASS
442	198	50	100	83.1	26504	PASS
443	442	15	24	18.7	4953	PASS