

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE121318\
 Data File : BE098408.D
 Acq On : 13 Dec 2018 22:03
 Operator : SJ/JU
 Sample : J6323-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE-126D3-20181207

Quant Time: Dec 13 23:09:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	944	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	4120	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	2859	0.40	ng	0.00
19) Phenanthrene-d10	17.27	188	7361	0.40	ng	-0.01
27) Chrysene-d12	21.46	240	8558	0.40	ng	0.00
34) Perylene-d12	24.01	264	7934	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.46	112	131	0.06	ng	0.01
5) Phenol-d6	7.07	99	231	0.07	ng	0.02
8) Nitrobenzene-d5	9.04	82	1549	0.41	ng	0.03
11) 2-Methylnaphthalene-d10	12.27	152	3070	0.46	ng	0.00
14) 2,4,6-Tribromophenol	16.02	330	613	0.58	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	5401	0.45	ng	0.00
25) Fluoranthene-d10	19.30	212	41908	0.44	ng	0.00
29) Terphenyl-d14	19.90	244	8175	0.39	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.36	88	1625	0.995	ng	Qvalue # 81
3) n-Nitrosodimethylamine	3.68	42	30	0.020	ng	# 100
22) Pentachlorophenol	16.95	266	22	0.050	ng	# 71
32) Bis(2-ethylhexyl)phthalate	21.35	149	3601	0.073	ng	# 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE121318\
Data File : BE098408.D
Acq On : 13 Dec 2018 22:03
Operator : SJ/JU
Sample : J6323-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE-126D3-20181207

Quant Time: Dec 13 23:09:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

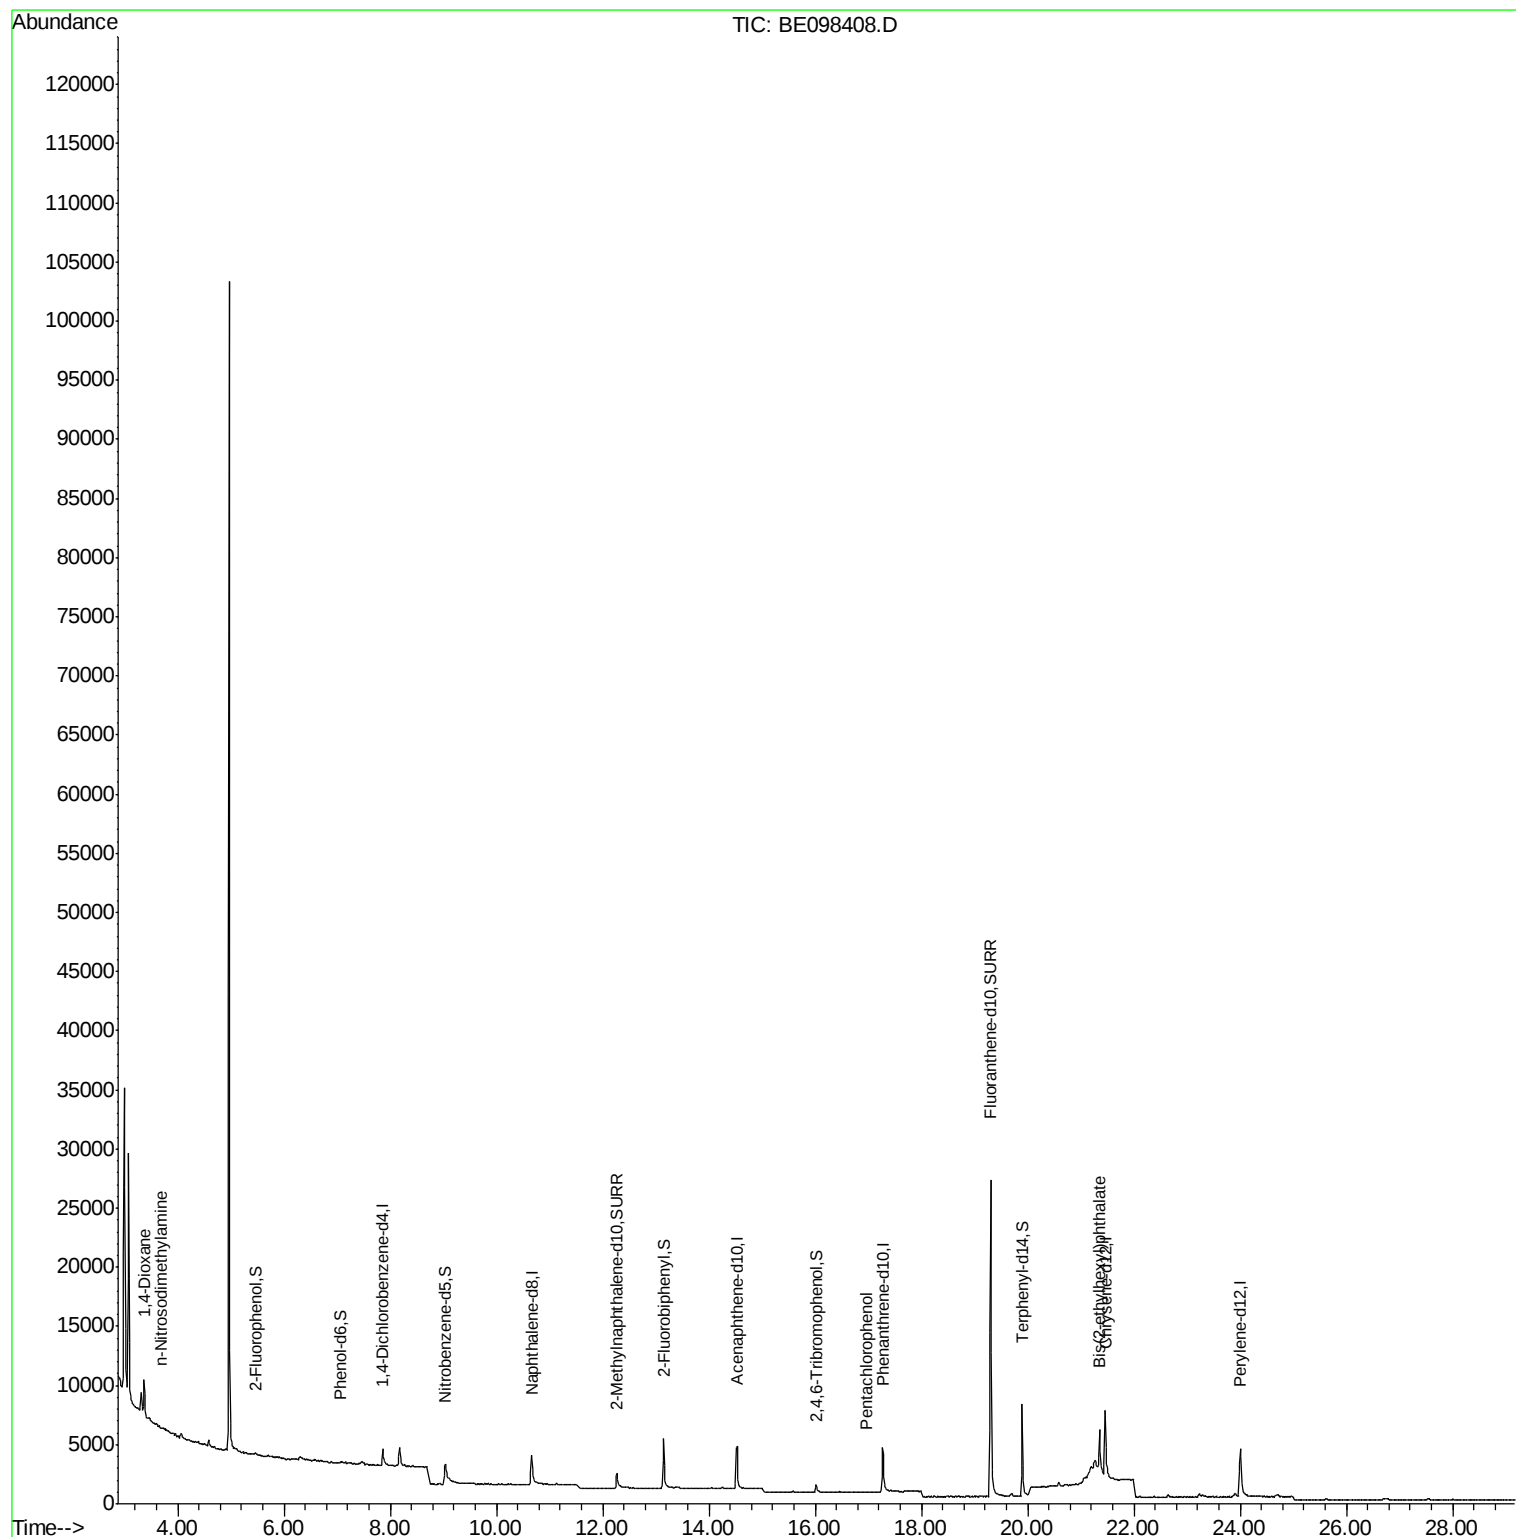




#1


1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.86 min Scan# 434
Delta R.T. 0.00 min
Lab File: BE098408.D
Acq: 13 Dec 2018 22:03

Instrument :
BNA_E
ClientSampleId :
RE-126D3-20181207



Tgt Ion:152 Resp: 944
Ion Ratio Lower Upper
152 100
150 160.3 124.2 186.4
115 69.7 53.9 80.9

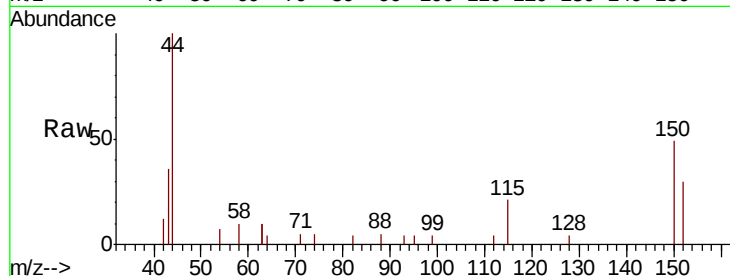

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

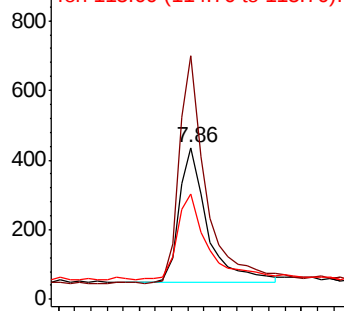


Time--> 7.70 7.80 7.90 8.00

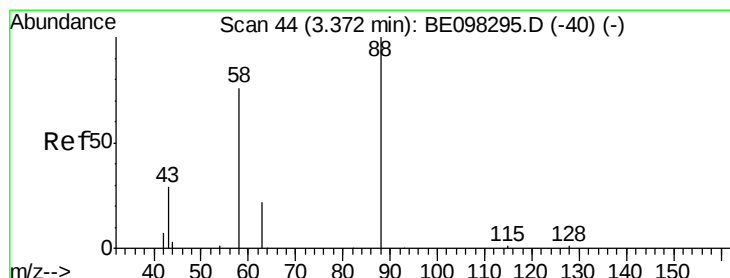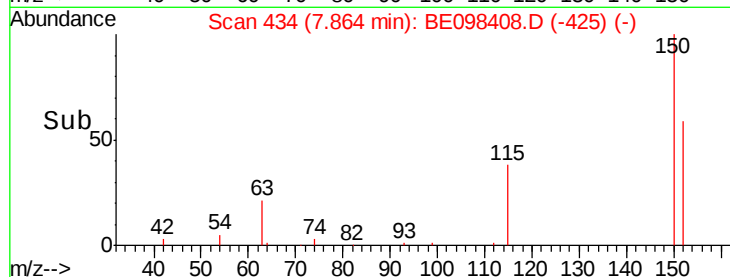


#2

1,4-Dioxane
Concen: 0.995 ng
RT: 3.36 min Scan# 43
Delta R.T. -0.01 min
Lab File: BE098408.D
Acq: 13 Dec 2018 22:03


Tgt Ion: 88 Resp: 1625
Ion Ratio Lower Upper
88 100
58 101.1 75.0 112.6
43 75.9 38.3 57.5#

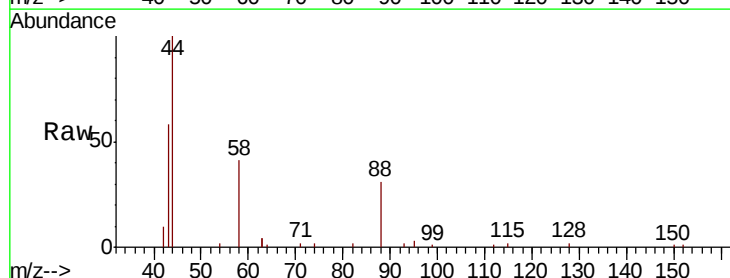

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

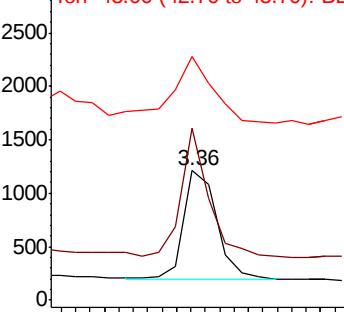

Time--> 3.30 3.35 3.40 3.45

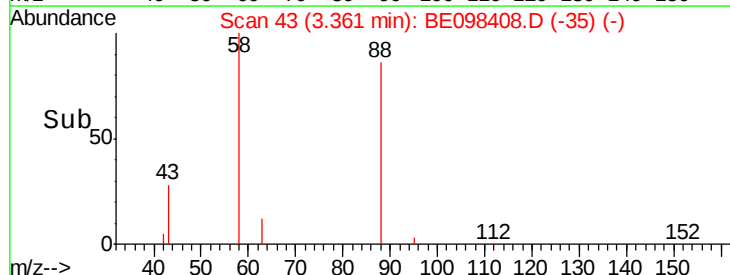



#3

n-Nitrosodimethylamine

Concen: 0.020 ng

RT: 3.68 min Scan# 71

Delta R.T. -0.01 min

Lab File: BE098408.D

Acq: 13 Dec 2018 22:03

Instrument :

BNA_E

ClientSampleId :

RE-126D3-20181207


Tgt Ion: 42 Resp: 30

Ion Ratio Lower Upper

42 100

74 16.7 0.0 0.0#



44 0.0 0.0 0.0

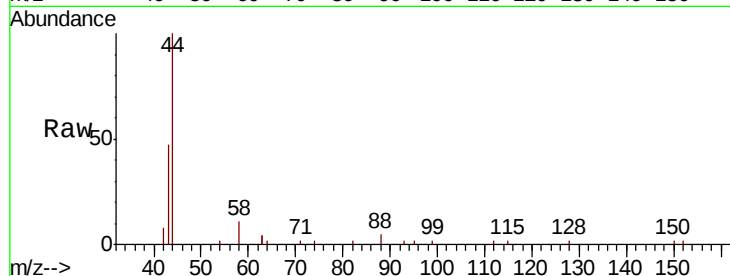

Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

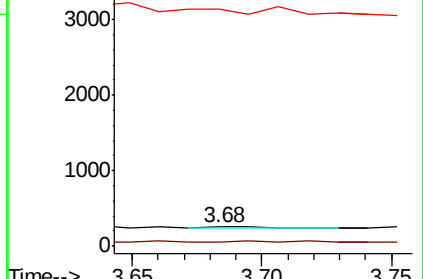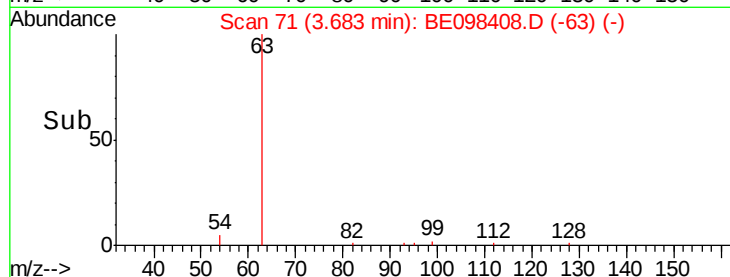

#4

2-Fluorophenol

Concen: 0.059 ng

RT: 5.46 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098408.D

Acq: 13 Dec 2018 22:03


Tgt Ion: 112 Resp: 131

Ion Ratio Lower Upper

112 100

64 75.6 59.8 89.8



63 177.9 133.7 200.5

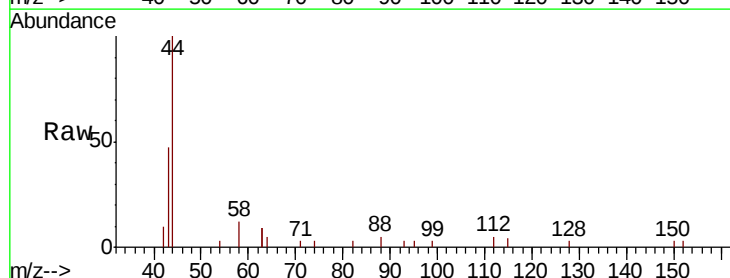


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

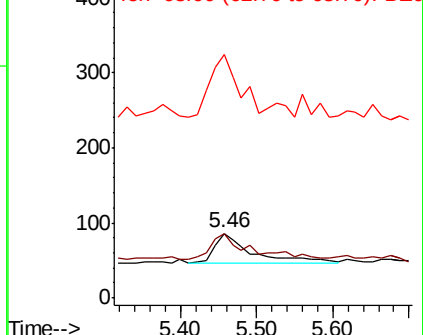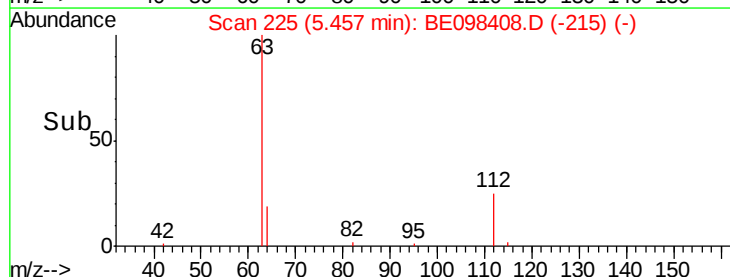

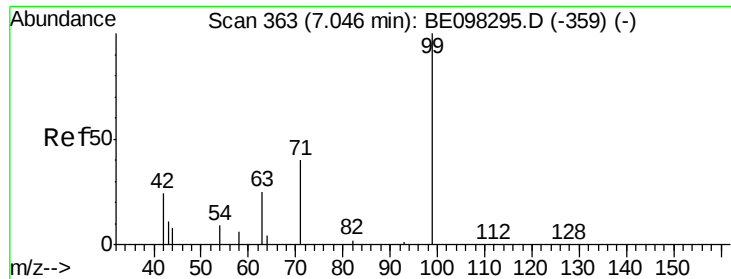

#5

Phenol-d6

Concen: 0.074 ng

RT: 7.07 min Scan# 365

Delta R.T. 0.02 min

Lab File: BE098408.D

Acq: 13 Dec 2018 22:03

Instrument :

BNA_E

ClientSampleId :

RE-126D3-20181207


Tgt Ion: 99 Resp: 231

Ion Ratio Lower Upper

99 100

42 0.0 26.3 39.5#




71 0.0 33.6 50.4#

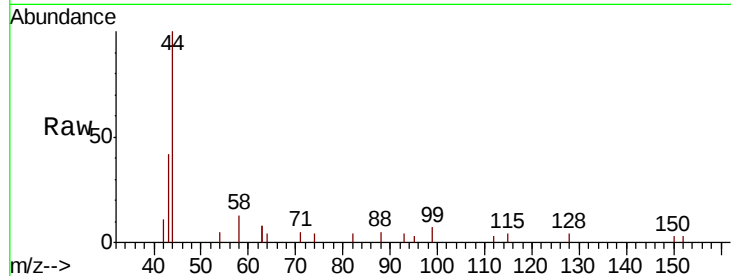

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

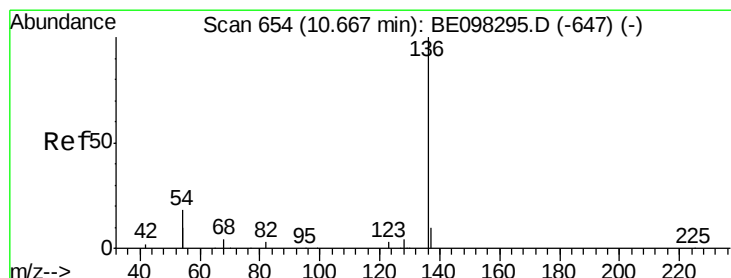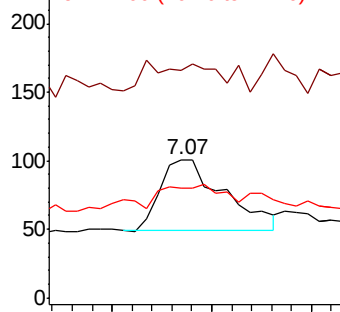

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. 0.00 min

Lab File: BE098408.D

Acq: 13 Dec 2018 22:03

Tgt Ion: 136 Resp: 4120


Ion Ratio Lower Upper

136 100

137 13.8 9.2 13.8#

54 48.3 28.4 42.6#

68 12.8 5.4 8.0#


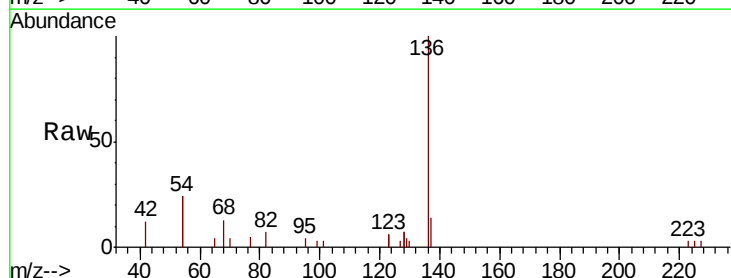


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

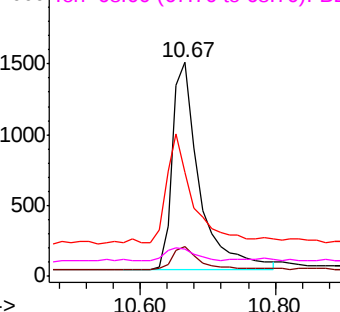







#8
 Nitrobenzene-d5
 Concen: 0.413 ng
 RT: 9.04 min Scan# 529
 Delta R.T. 0.03 min
 Lab File: BE098408.D
 Acq: 13 Dec 2018 22:03

Instrument :
 BNA_E
 ClientSampleId :
 RE-126D3-20181207

Tgt Ion: 82 Resp: 1549
 Ion Ratio Lower Upper
 82 100
 128 169.4 102.4 153.6#
 54 279.0 221.8 332.8

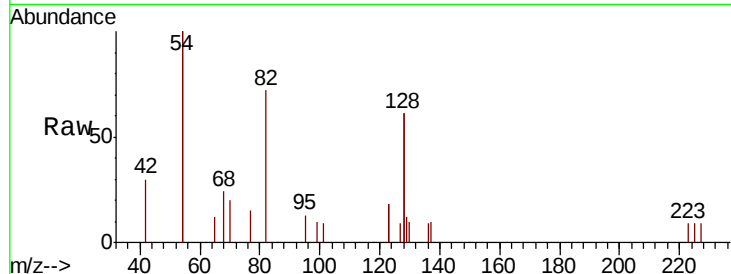


Abundance Ion 82.00 (81.70 to 82.70): BE0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BE0

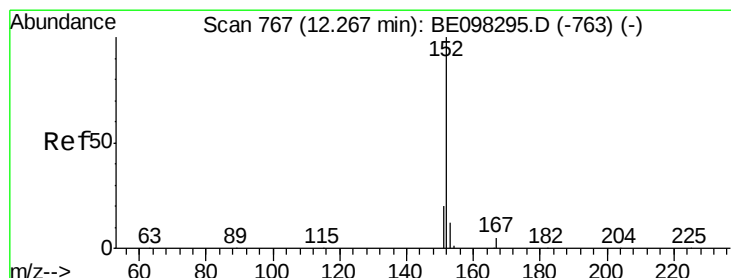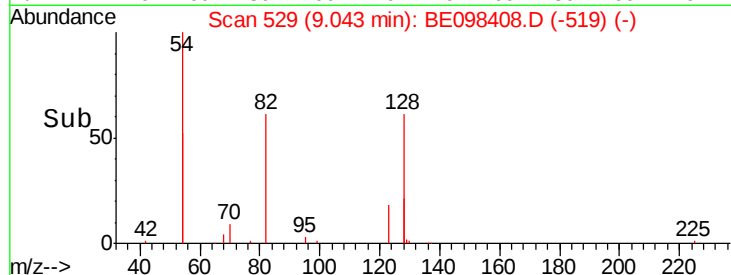
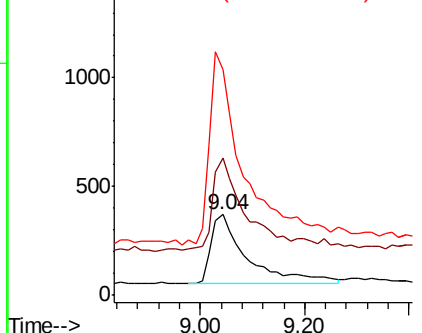



#11
 2-Methylnaphthalene-d10
 Concen: 0.458 ng
 RT: 12.27 min Scan# 767
 Delta R.T. 0.00 min
 Lab File: BE098408.D
 Acq: 13 Dec 2018 22:03

Tgt Ion: 152 Resp: 3070
 Ion Ratio Lower Upper
 152 100
 151 20.3 16.2 24.4

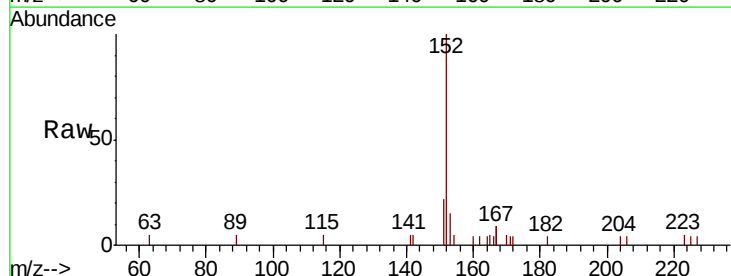

Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 151.00 (150.70 to 151.70): E

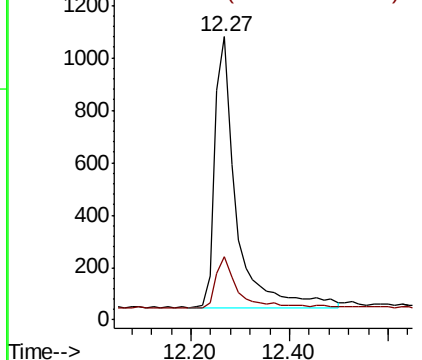


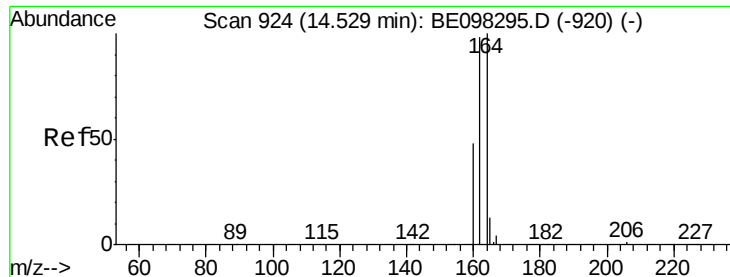




#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.53 min Scan# 924
 Delta R.T. 0.00 min
 Lab File: BE098408.D
 Acq: 13 Dec 2018 22:03

Instrument :
 BNA_E
 ClientSampleId :
 RE-126D3-20181207

Tgt Ion:164 Resp: 2859
 Ion Ratio Lower Upper
 164 100
 162 96.2 77.6 116.4
 160 48.7 36.0 54.0

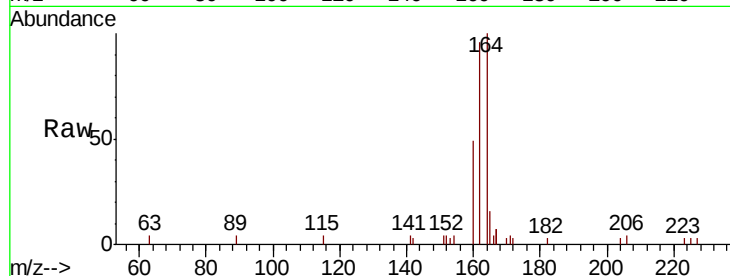


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

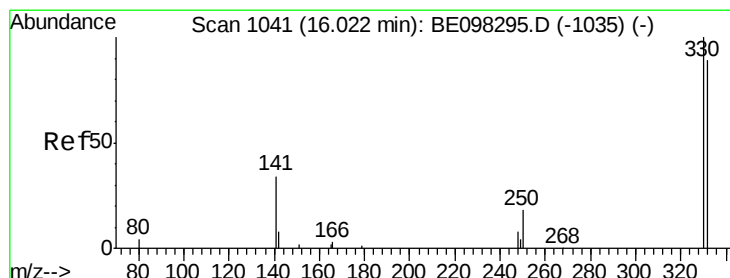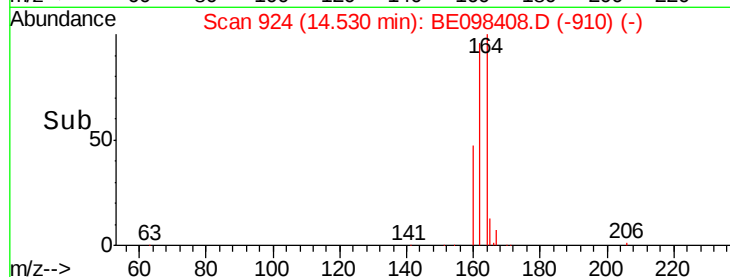
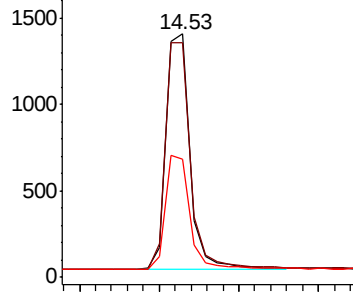



#14
 2,4,6-Tribromophenol
 Concen: 0.584 ng
 RT: 16.02 min Scan# 1041
 Delta R.T. -0.00 min
 Lab File: BE098408.D
 Acq: 13 Dec 2018 22:03

Tgt Ion:330 Resp: 613
 Ion Ratio Lower Upper
 330 100
 332 92.3 76.2 114.4
 141 43.1 39.0 58.4

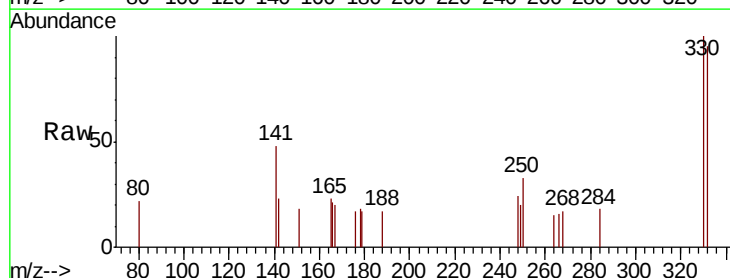

Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



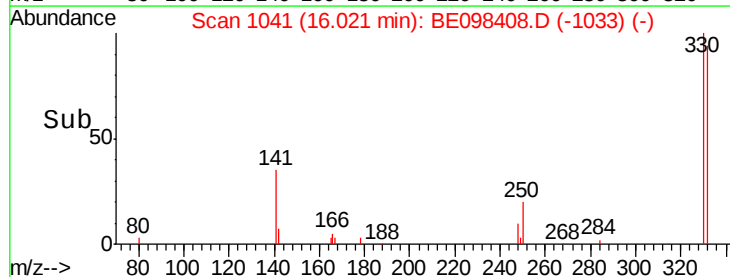
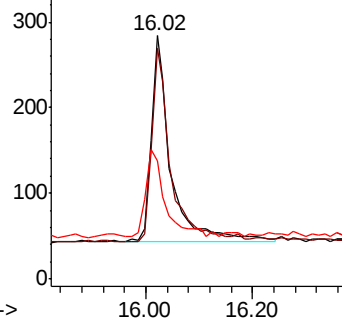


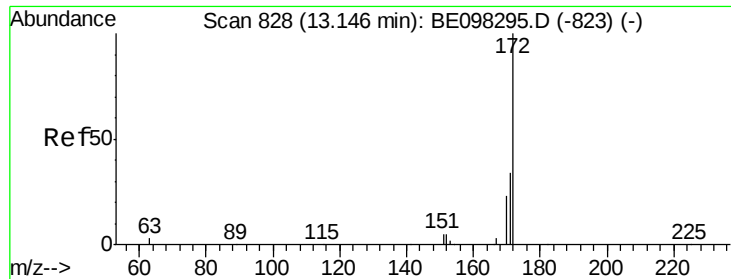

#15
2-Fluorobiphenyl
Concen: 0.448 ng
RT: 13.15 min Scan# 828
Delta R.T. 0.00 min
Lab File: BE098408.D
Acq: 13 Dec 2018 22:03




Instrument :
BNA_E
ClientSampleId :
RE-126D3-20181207


Tgt Ion:172 Resp: 5401
Ion Ratio Lower Upper
172 100
171 33.2 27.5 41.3
170 23.1 19.6 29.4

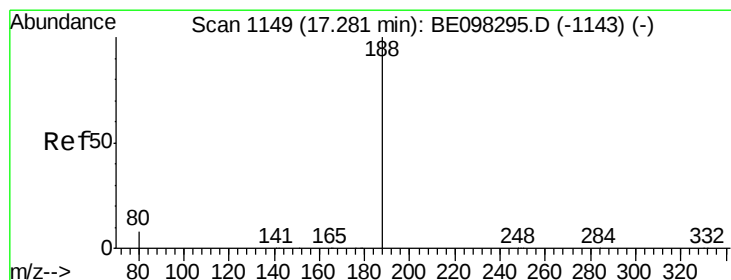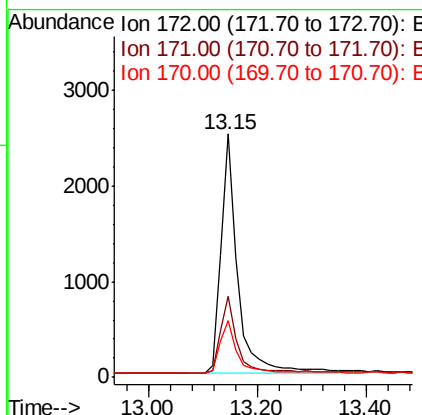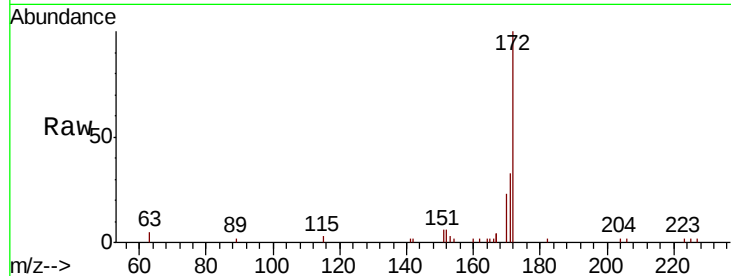

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.27 min Scan# 1148
Delta R.T. -0.01 min
Lab File: BE098408.D
Acq: 13 Dec 2018 22:03

Tgt Ion:188 Resp: 7361
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.9 7.2 10.8#


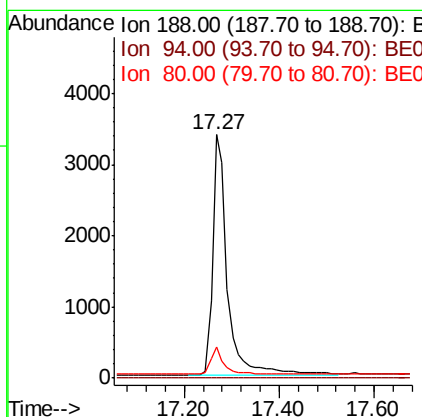

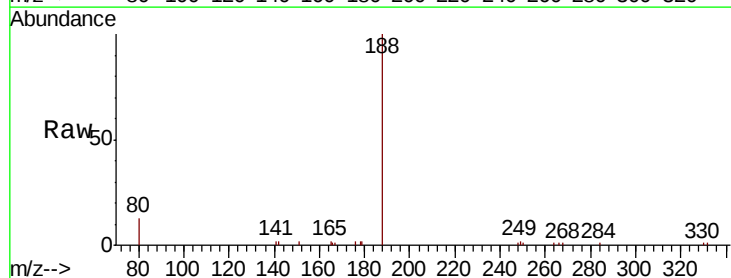




#22
 Pentachlorophenol
 Concen: 0.050 ng
 RT: 16.95 min Scan# 1121
 Delta R.T. 0.01 min
 Lab File: BE098408.D
 Acq: 13 Dec 2018 22:03




Instrument :
 BNA_E
 ClientSampleId :
 RE-126D3-20181207

Tgt Ion: 266 Resp: 22
 Ion Ratio Lower Upper
 266 100
 264 92.5 59.0 88.4#
 268 98.1 55.1 82.7#

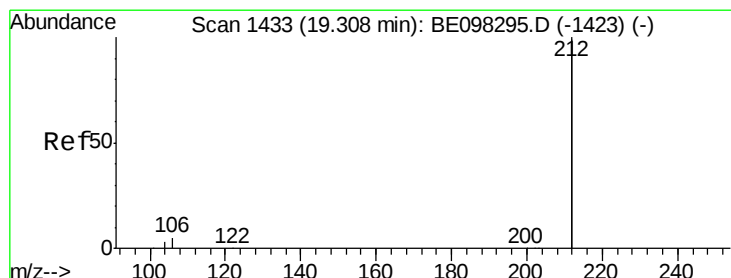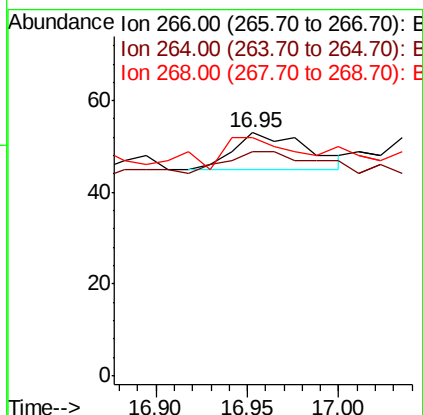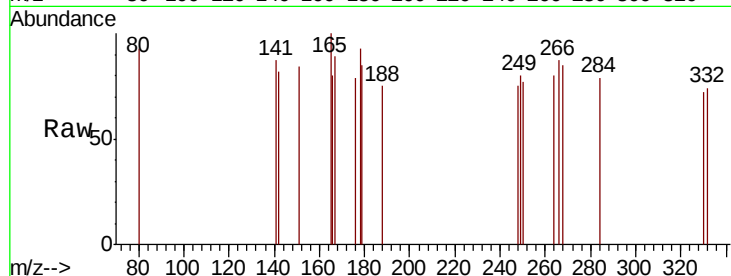

#25
 Fluoranthene-d10
 Concen: 0.444 ng
 RT: 19.30 min Scan# 1432
 Delta R.T. -0.01 min
 Lab File: BE098408.D
 Acq: 13 Dec 2018 22:03

Tgt Ion: 212 Resp: 41908
 Ion Ratio Lower Upper
 212 100
 106 2.7 2.2 3.2
 104 1.4 1.3 1.9

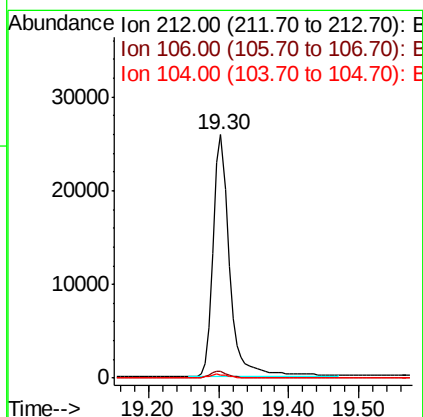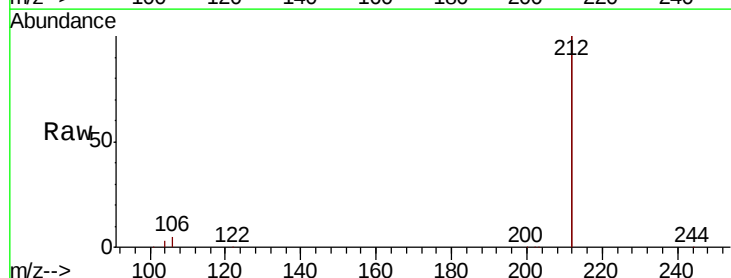



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.46 min Scan# 1671

Delta R.T. -0.00 min

Lab File: BE098408.D

Acq: 13 Dec 2018 22:03

Instrument :

BNA_E

ClientSampleId :

RE-126D3-20181207


Tgt Ion:240 Resp: 8558

Ion Ratio Lower Upper

240 100

120 8.3 9.5 14.3#




236 28.4 22.7 34.1

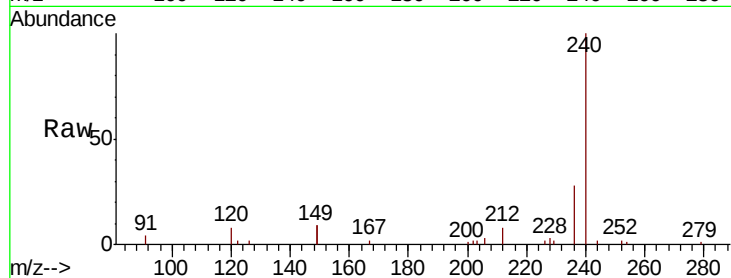

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

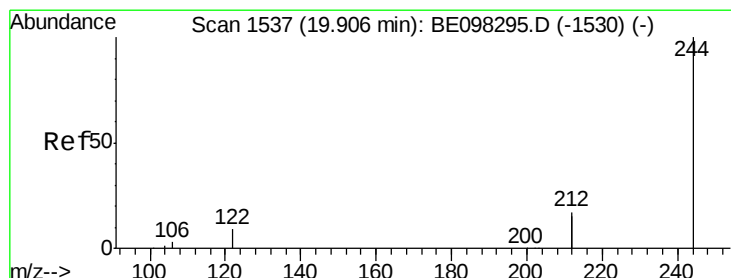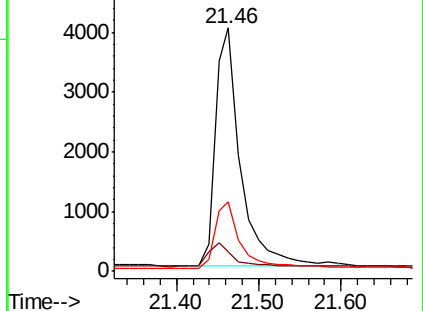

#29

Terphenyl-d14

Concen: 0.393 ng

RT: 19.90 min Scan# 1536

Delta R.T. -0.00 min

Lab File: BE098408.D

Acq: 13 Dec 2018 22:03


Tgt Ion:244 Resp: 8175

Ion Ratio Lower Upper

244 100

212 35.5 27.4 41.0



122 9.3 8.3 12.5

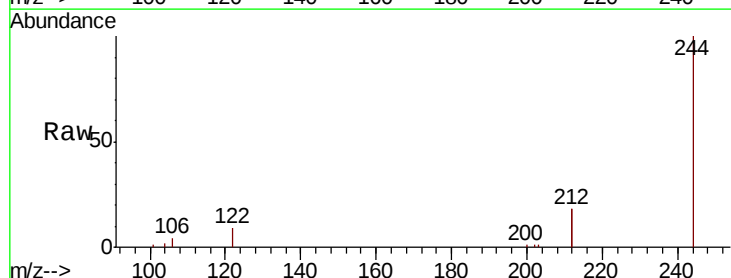


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E




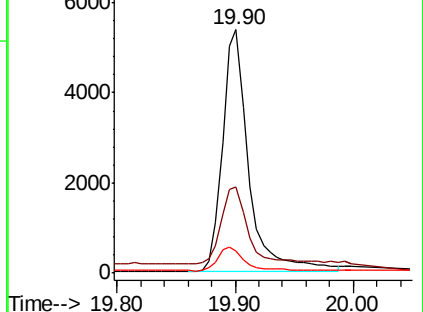


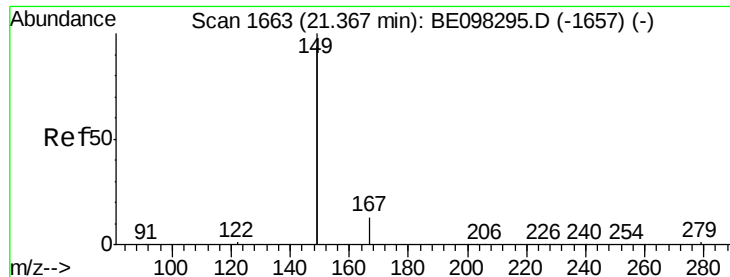

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.073 ng
 RT: 21.35 min Scan# 1662
 Delta R.T. -0.01 min
 Lab File: BE098408.D
 Acq: 13 Dec 2018 22:03

Instrument :
 BNA_E
 ClientSampleId :
 RE-126D3-20181207

Tgt Ion:149 Resp: 3601
 Ion Ratio Lower Upper
 149 100
 167 9.4 5.7 8.5#
 279 1.8 1.0 1.4#

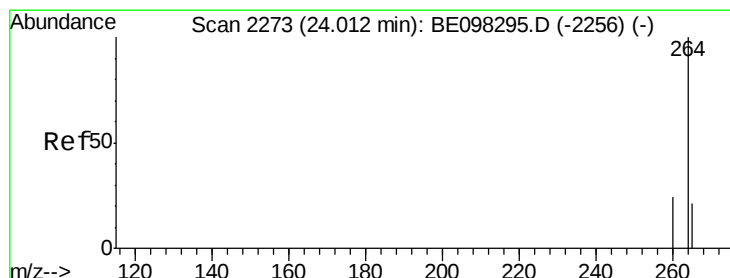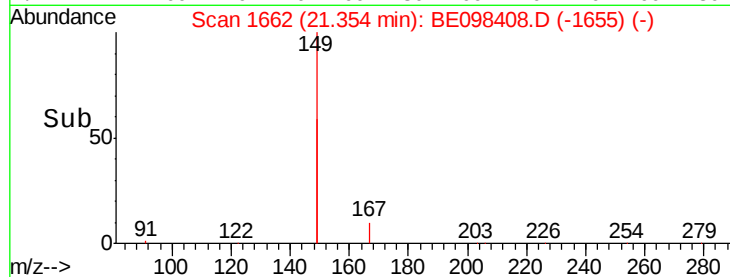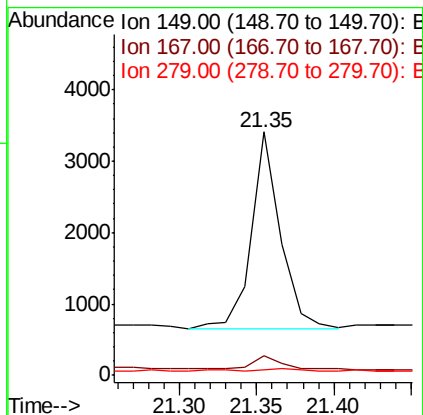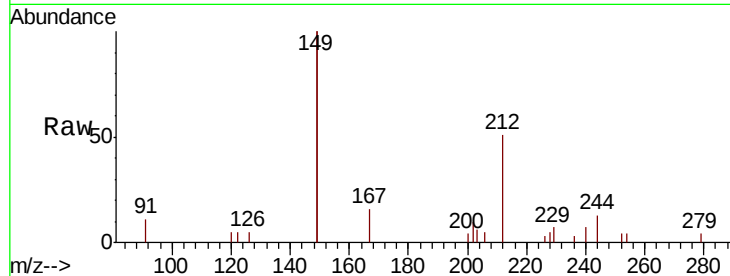

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.01 min Scan# 2271
 Delta R.T. -0.01 min
 Lab File: BE098408.D
 Acq: 13 Dec 2018 22:03

Tgt Ion:264 Resp: 7934
 Ion Ratio Lower Upper
 264 100
 260 25.7 20.2 30.2
 265 27.1 25.2 37.8

