

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE121318\
 Data File : BE098427.D
 Acq On : 14 Dec 2018 9:44
 Operator : SJ/JU
 Sample : J6343-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW311S-20181209

Quant Time: Dec 14 15:15:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	888	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	3810	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	2452	0.40	ng	0.00
19) Phenanthrene-d10	17.27	188	6575	0.40	ng	-0.01
27) Chrysene-d12	21.46	240	7844	0.40	ng	0.00
34) Perylene-d12	24.00	264	7343	0.40	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.45	112	382	0.18	ng	0.00
5) Phenol-d6	7.04	99	370	0.13	ng	0.00
8) Nitrobenzene-d5	9.04	82	1209	0.35	ng	0.03
11) 2-Methylnaphthalene-d10	12.27	152	2234	0.36	ng	0.00
14) 2,4,6-Tribromophenol	16.02	330	443	0.49	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	4627	0.45	ng	0.00
25) Fluoranthene-d10	19.30	212	32490	0.39	ng	0.00
29) Terphenyl-d14	19.90	244	7235	0.38	ng	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.38	88	68	0.044	ng	# 12
3) n-Nitrosodimethylamine	3.67	42	82	0.059	ng	# 100
32) Bis(2-ethylhexyl)phthalate	21.35	149	2240	0.049	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE121318\
Data File : BE098427.D
Acq On : 14 Dec 2018 9:44
Operator : SJ/JU
Sample : J6343-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW311S-20181209

Quant Time: Dec 14 15:15:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

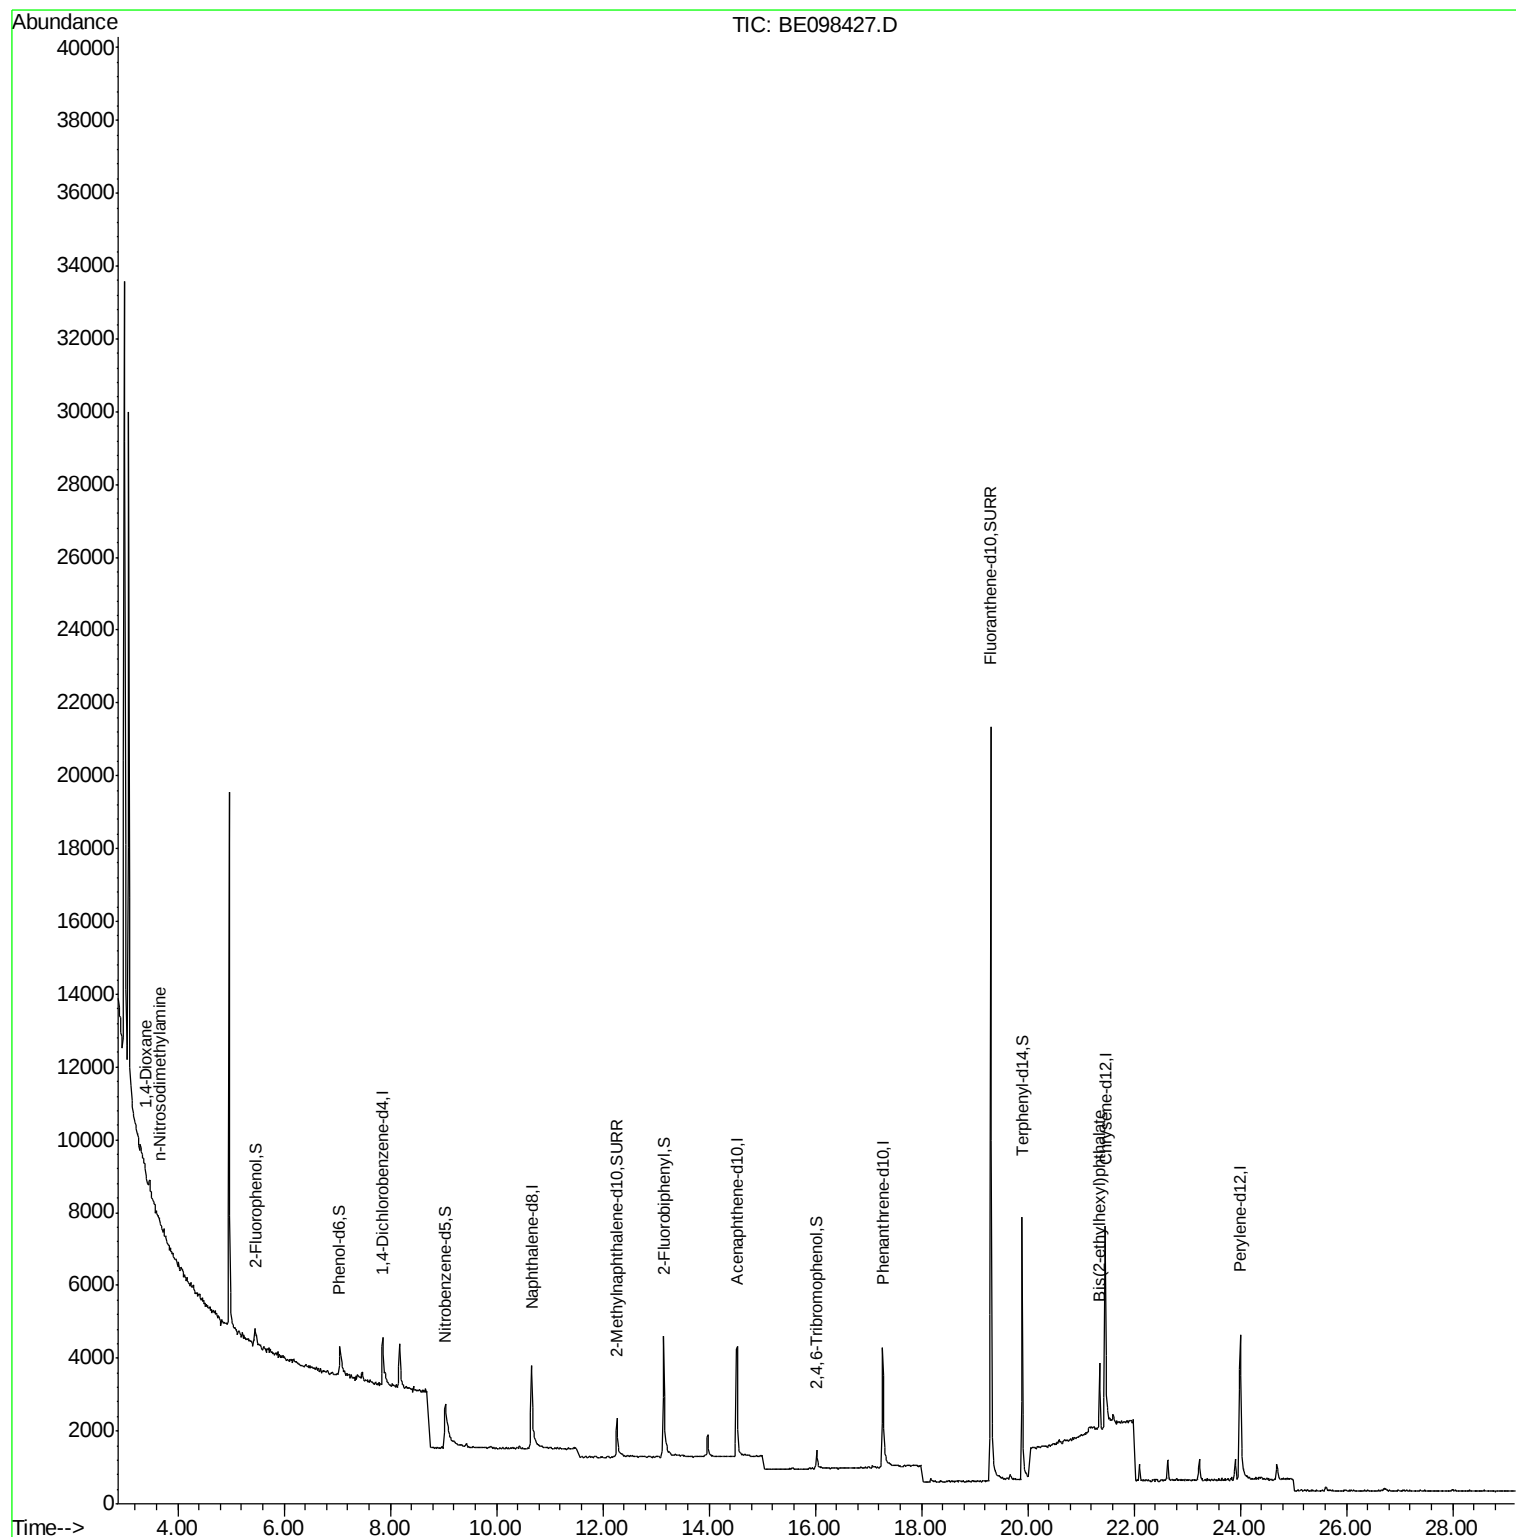




#1



1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.86 min Scan# 434
Delta R.T. -0.00 min
Lab File: BE098427.D
Acq: 14 Dec 2018 9:44

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW311S-20181209

Tgt Ion: 152 Resp: 888
Ion Ratio Lower Upper
152 100
150 144.5 124.2 186.4
115 67.8 53.9 80.9

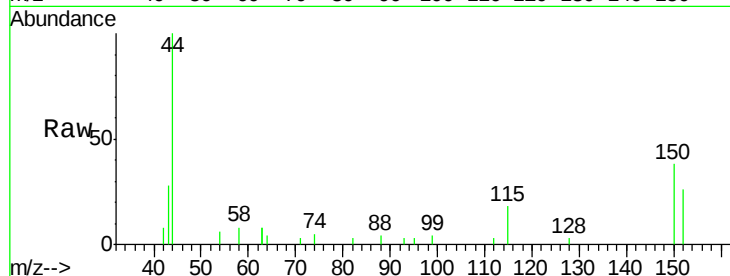


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

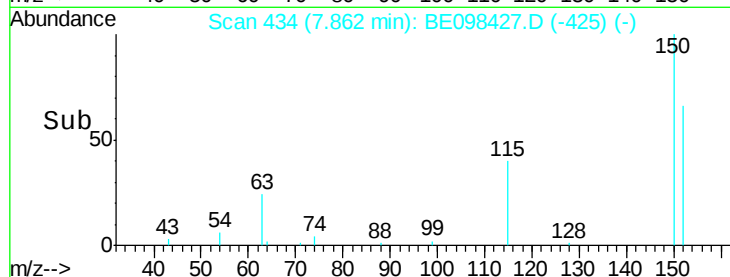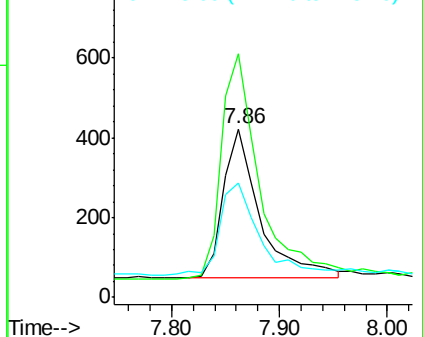



#2

1,4-Dioxane
Concen: 0.044 ng
RT: 3.38 min Scan# 45
Delta R.T. 0.01 min
Lab File: BE098427.D
Acq: 14 Dec 2018 9:44

Tgt Ion: 88 Resp: 68
Ion Ratio Lower Upper
88 100
58 0.0 75.0 112.6#
43 0.0 38.3 57.5#

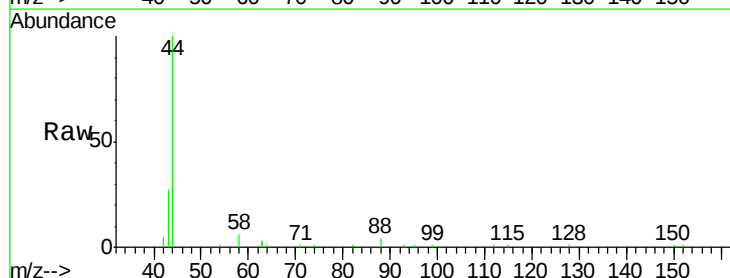

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

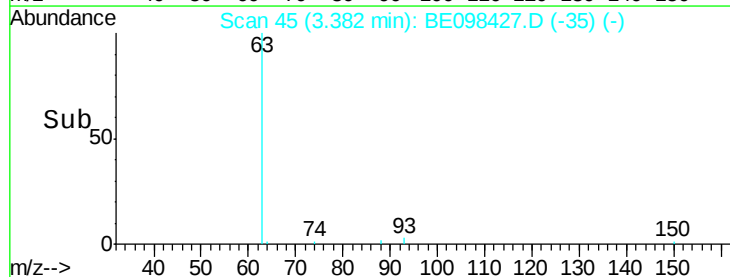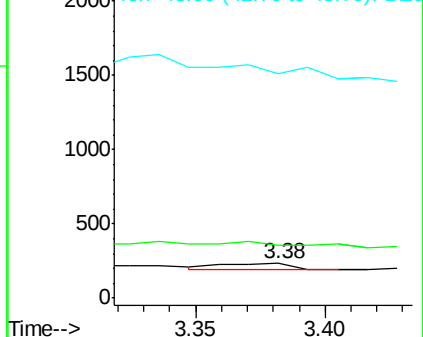



#3

n-Nitrosodimethylamine

Concen: 0.059 ng

RT: 3.67 min Scan# 70

Delta R.T. -0.02 min

Lab File: BE098427.D

Acq: 14 Dec 2018 9:44

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW311S-20181209


Tgt Ion: 42 Resp: 82

Ion Ratio Lower Upper

42 100

74 0.0 0.0 0.0



44 0.0 0.0 0.0

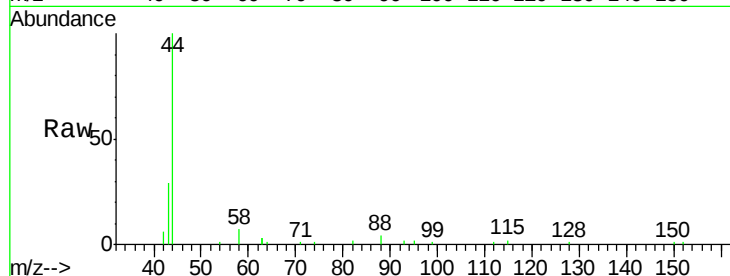

Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

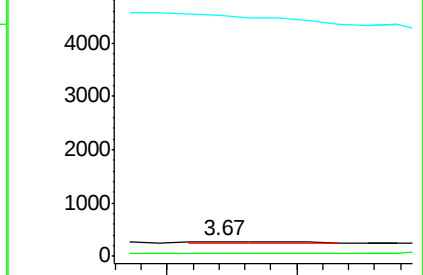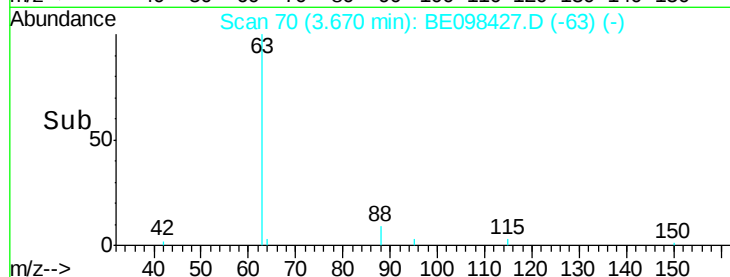

#4

2-Fluorophenol

Concen: 0.184 ng

RT: 5.45 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098427.D

Acq: 14 Dec 2018 9:44


Tgt Ion: 112 Resp: 382

Ion Ratio Lower Upper

112 100

64 76.7 59.8 89.8



63 168.3 133.7 200.5

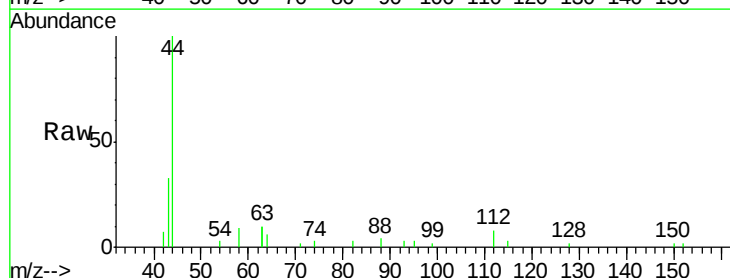


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

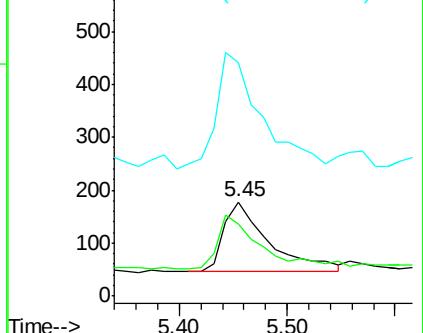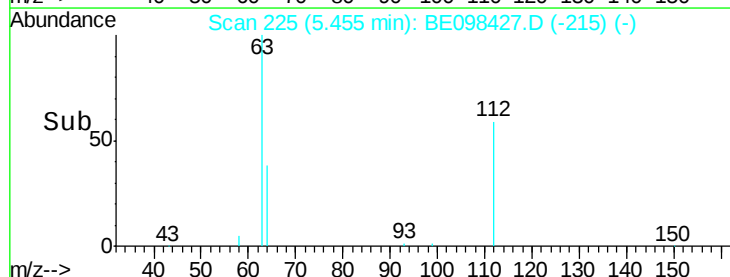

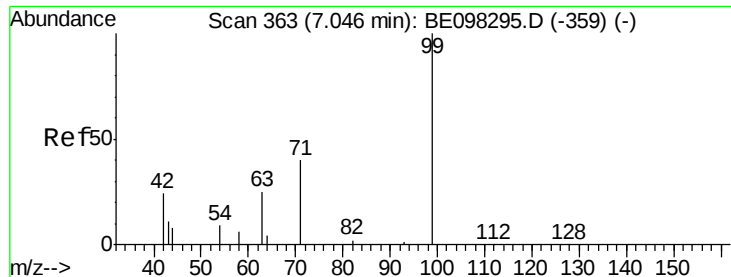

#5

Phenol-d6

Concen: 0.126 ng

RT: 7.04 min Scan# 363

Delta R.T. -0.00 min

Lab File: BE098427.D

Acq: 14 Dec 2018 9:44

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW311S-20181209


Tgt Ion: 99 Resp: 370

Ion Ratio Lower Upper

99 100

42 66.2 26.3 39.5#


71 45.4 33.6 50.4

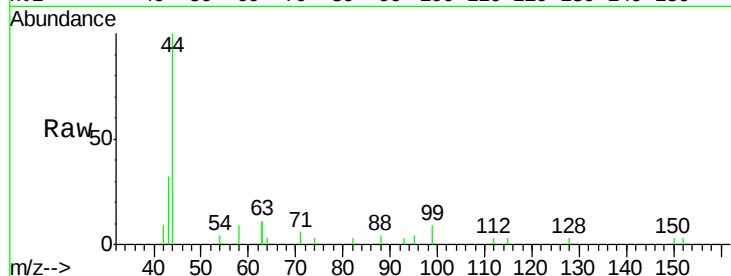



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

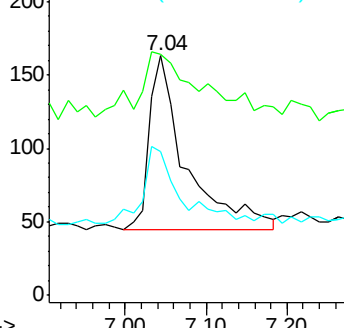

Time-->

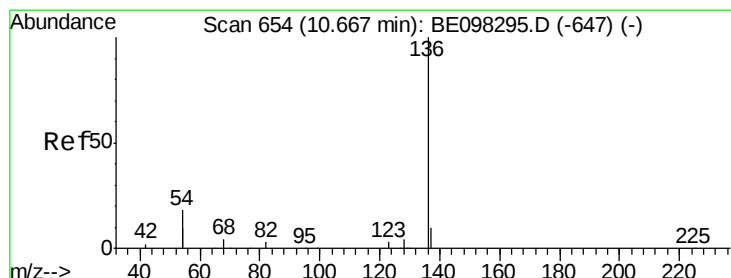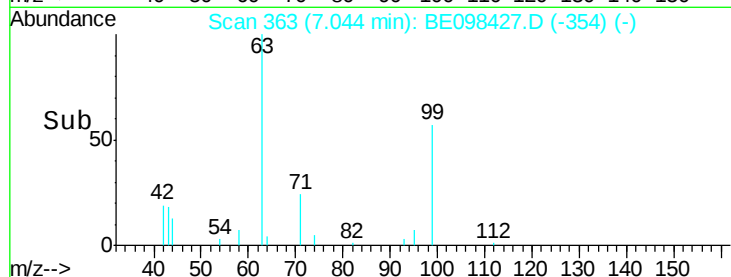

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. -0.00 min

Lab File: BE098427.D

Acq: 14 Dec 2018 9:44

Tgt Ion: 136 Resp: 3810


Ion Ratio Lower Upper

136 100

137 13.1 9.2 13.8

54 44.7 28.4 42.6#

68 8.5 5.4 8.0#

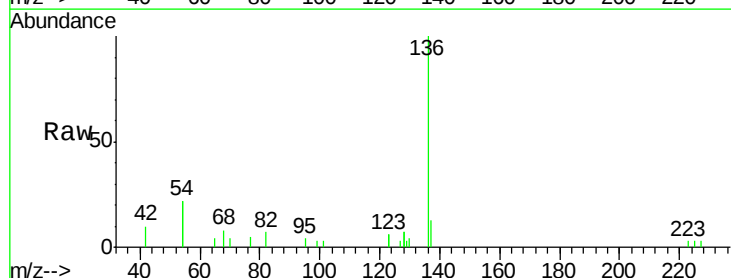


Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

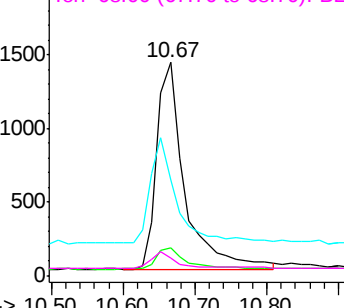

Time-->

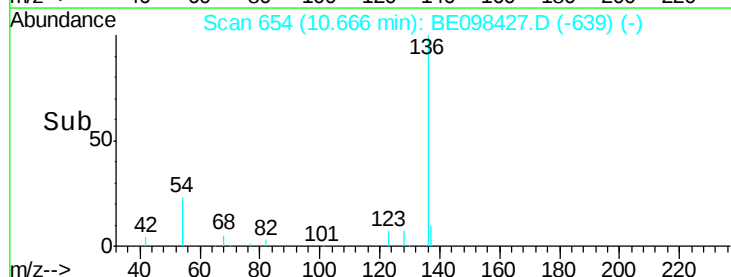



#8

Nitrobenzene-d5

Concen: 0.349 ng

RT: 9.04 min Scan# 529

Delta R.T. 0.03 min

Lab File: BE098427.D

Acq: 14 Dec 2018 9:44

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW311S-20181209


Tgt Ion: 82 Resp: 1209

Ion Ratio Lower Upper




82 100

128 181.6 102.4 153.6#

54 285.5 221.8 332.8

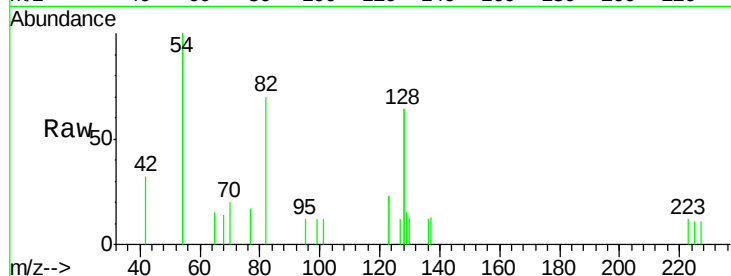

Abundance Ion 82.00 (81.70 to 82.70): BE098427.D (-519) (-)

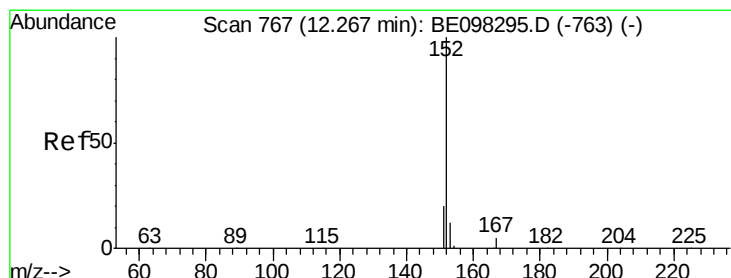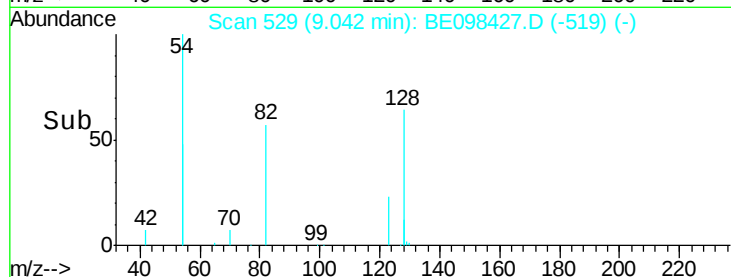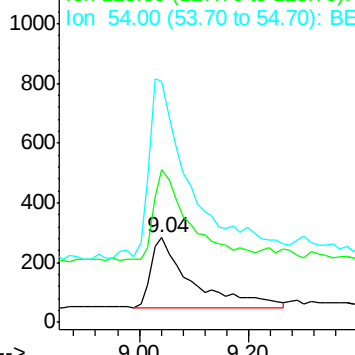

#11

2-Methylnaphthalene-d10

Concen: 0.361 ng

RT: 12.27 min Scan# 767

Delta R.T. -0.00 min

Lab File: BE098427.D


Acq: 14 Dec 2018 9:44

Tgt Ion: 152 Resp: 2234



Ion Ratio Lower Upper


152 100

151 18.9 16.2 24.4

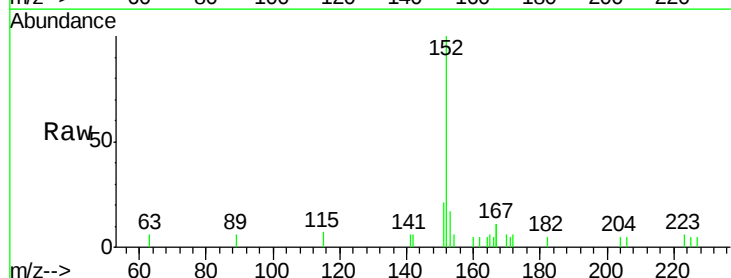

Abundance Ion 152.00 (151.70 to 152.70): BE098427.D (-760) (-)

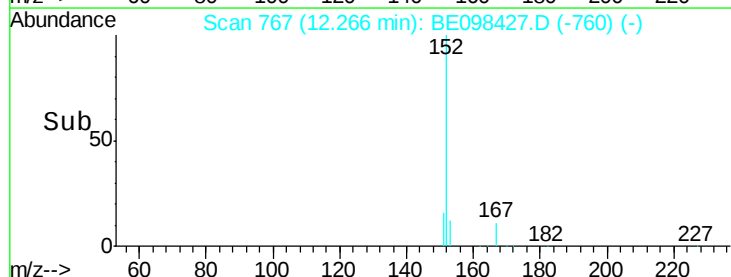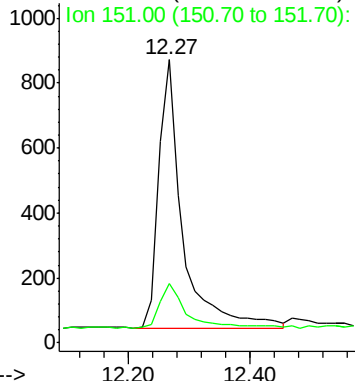


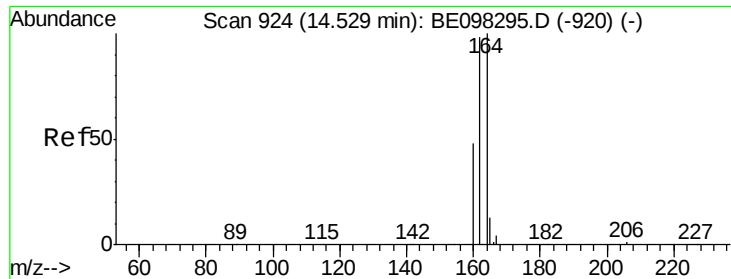




#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.53 min Scan# 924
 Delta R.T. -0.00 min
 Lab File: BE098427.D
 Acq: 14 Dec 2018 9:44

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW311S-20181209

Tgt Ion:164 Resp: 2452
 Ion Ratio Lower Upper
 164 100
 162 97.5 77.6 116.4
 160 51.3 36.0 54.0

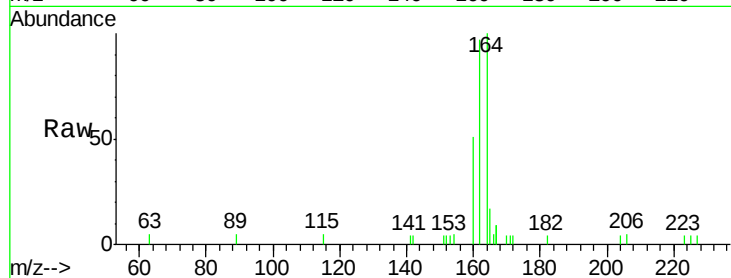


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

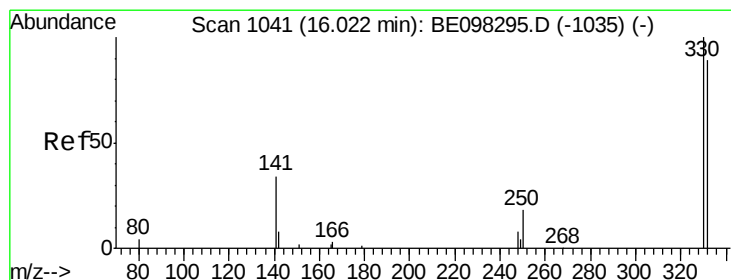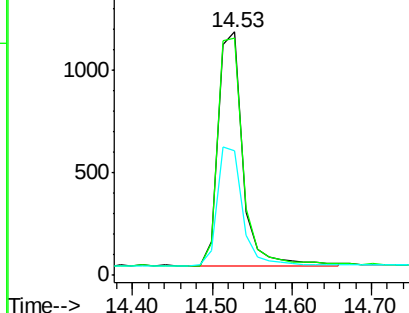
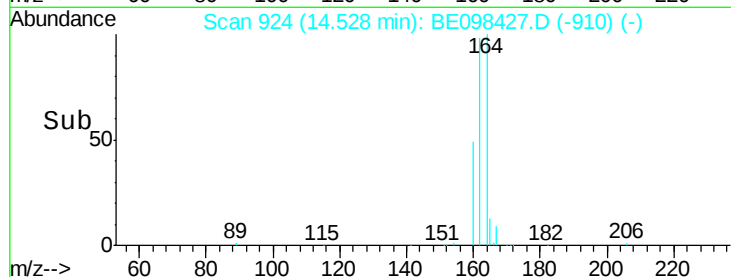



#14
 2,4,6-Tribromophenol
 Concen: 0.492 ng
 RT: 16.02 min Scan# 1041
 Delta R.T. -0.00 min
 Lab File: BE098427.D
 Acq: 14 Dec 2018 9:44

Tgt Ion:330 Resp: 443
 Ion Ratio Lower Upper
 330 100
 332 92.1 76.2 114.4
 141 42.4 39.0 58.4

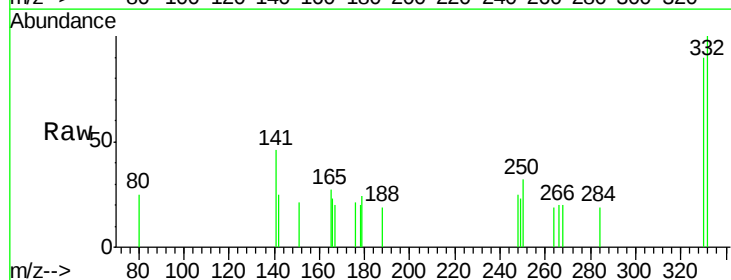

Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



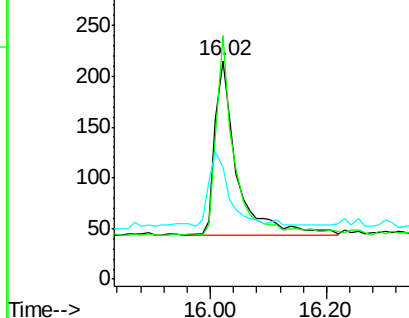
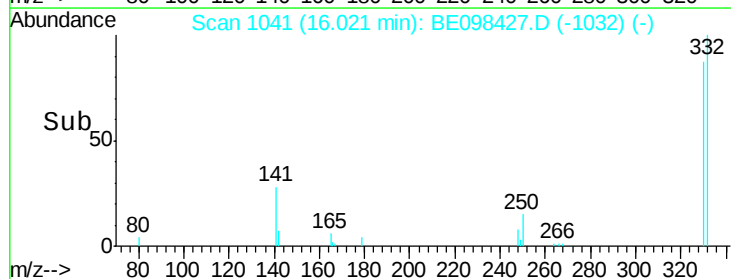


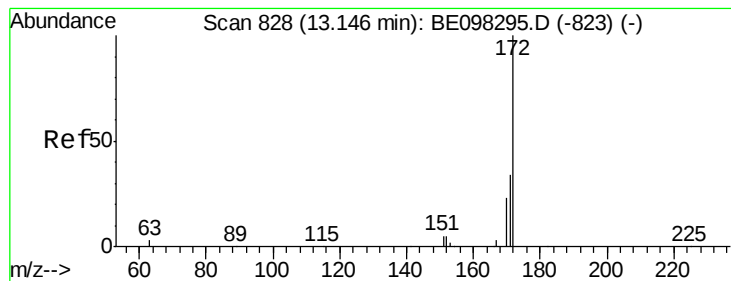

#15
2-Fluorobiphenyl
Concen: 0.447 ng
RT: 13.15 min Scan# 828
Delta R.T. -0.00 min
Lab File: BE098427.D
Acq: 14 Dec 2018 9:44




Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW311S-20181209


Tgt Ion:172 Resp: 4627
Ion Ratio Lower Upper
172 100
171 33.4 27.5 41.3
170 25.5 19.6 29.4

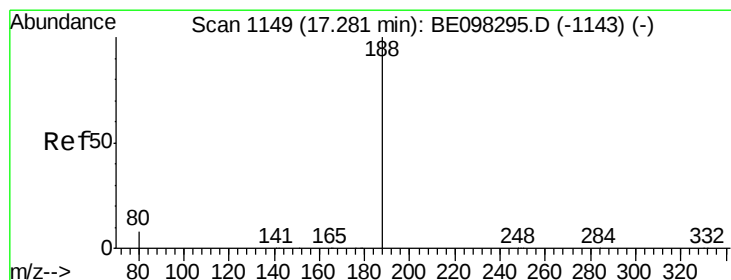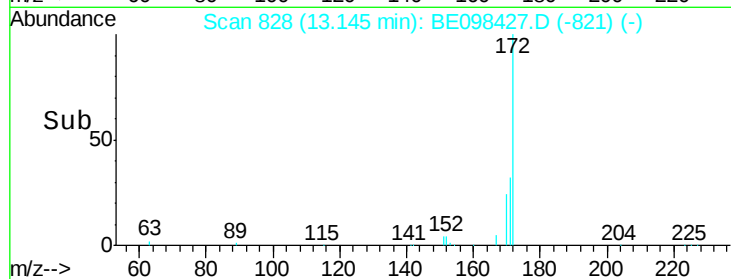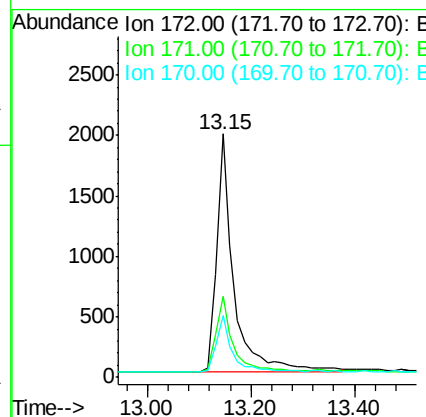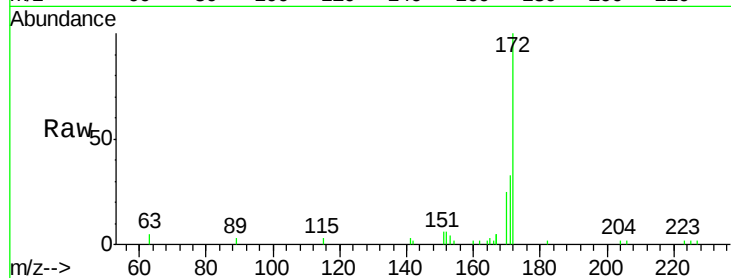

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.27 min Scan# 1148
Delta R.T. -0.01 min
Lab File: BE098427.D
Acq: 14 Dec 2018 9:44

Tgt Ion:188 Resp: 6575
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.2 7.2 10.8#


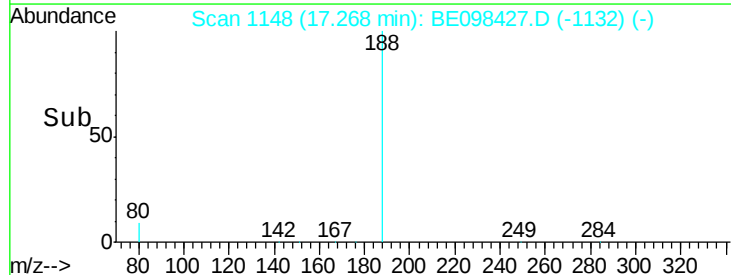
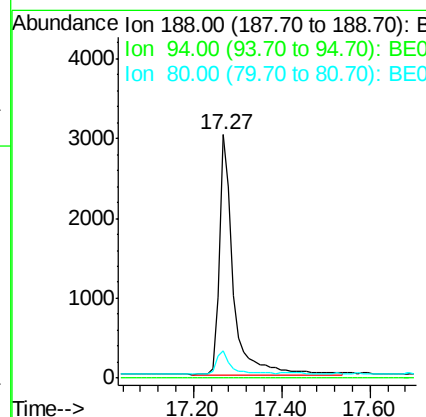
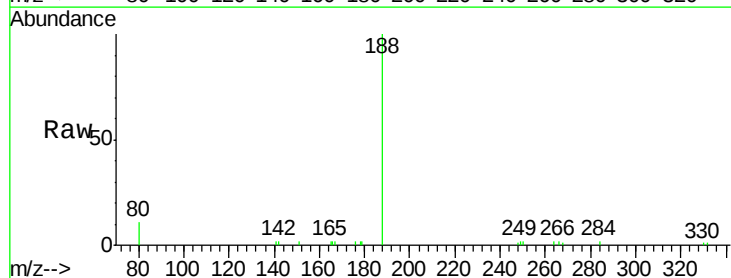


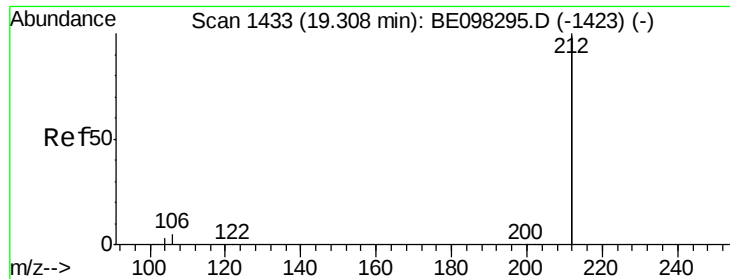

#25
 Fluoranthene-d10
 Concen: 0.385 ng
 RT: 19.30 min Scan# 1432
 Delta R.T. -0.00 min
 Lab File: BE098427.D
 Acq: 14 Dec 2018 9:44




Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW311S-20181209


Tgt Ion:212 Resp: 32490
 Ion Ratio Lower Upper
 212 100
 106 2.5 2.2 3.2
 104 1.5 1.3 1.9

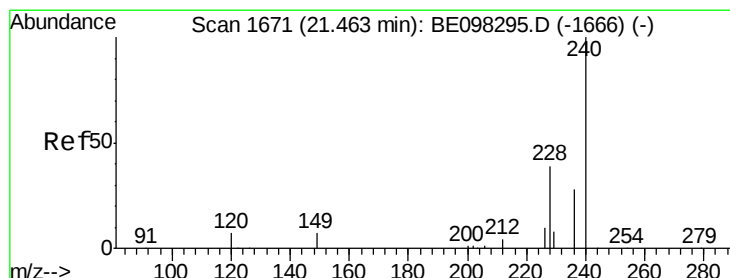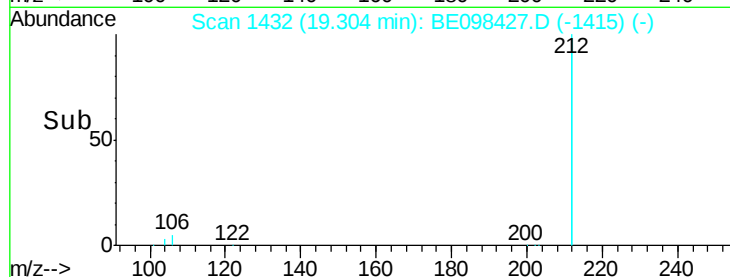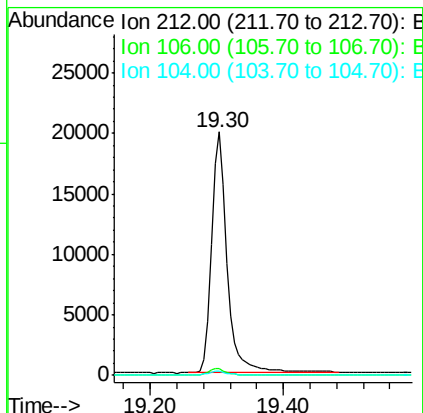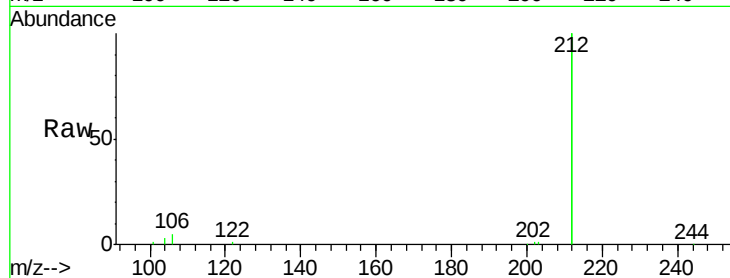

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.46 min Scan# 1671
 Delta R.T. -0.00 min
 Lab File: BE098427.D
 Acq: 14 Dec 2018 9:44

Tgt Ion:240 Resp: 7844
 Ion Ratio Lower Upper
 240 100
 120 7.1 9.5 14.3#
 236 27.4 22.7 34.1

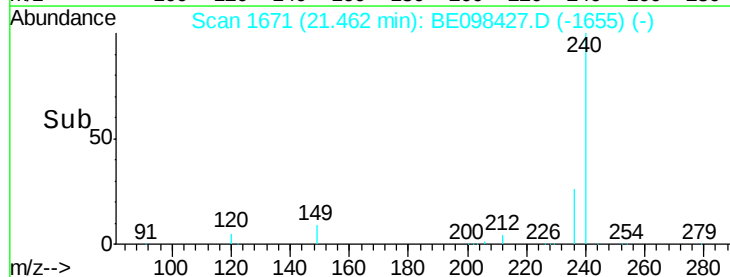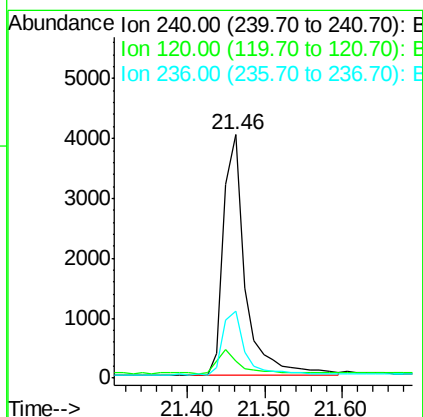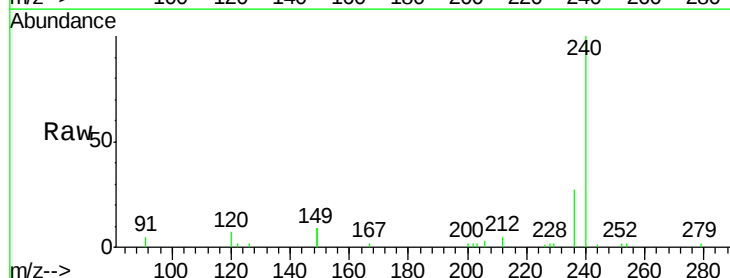

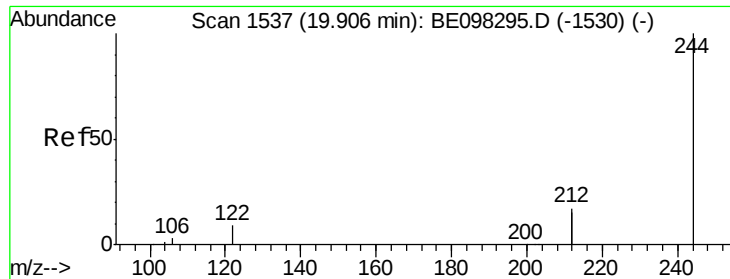

#29

Terphenyl-d14

Concen: 0.380 ng

RT: 19.90 min Scan# 1535

Delta R.T. -0.01 min

Lab File: BE098427.D

Acq: 14 Dec 2018 9:44

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW311S-20181209


Tgt Ion:244 Resp: 7235

Ion Ratio Lower Upper

244 100

212 36.6 27.4 41.0




122 10.7 8.3 12.5

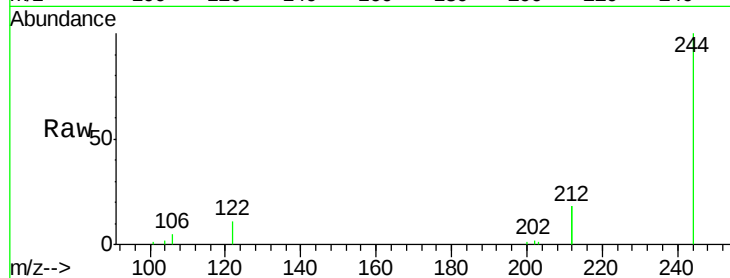

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

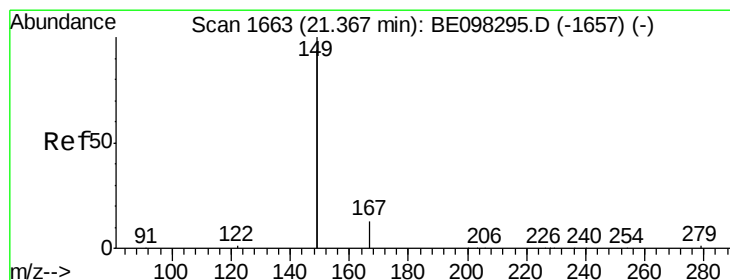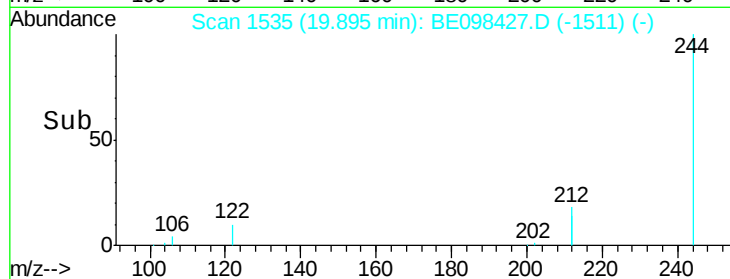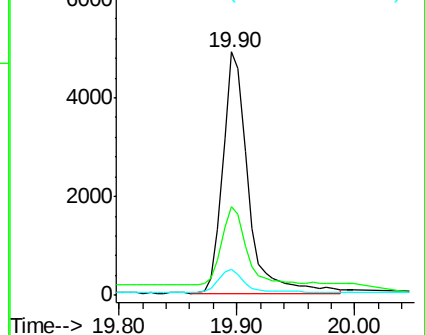

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.049 ng

RT: 21.35 min Scan# 1662

Delta R.T. -0.01 min

Lab File: BE098427.D

Acq: 14 Dec 2018 9:44


Tgt Ion:149 Resp: 2240

Ion Ratio Lower Upper

149 100

167 7.5 5.7 8.5



279 1.8 1.0 1.4#


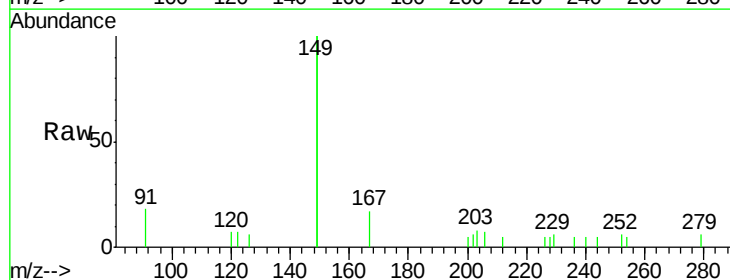


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

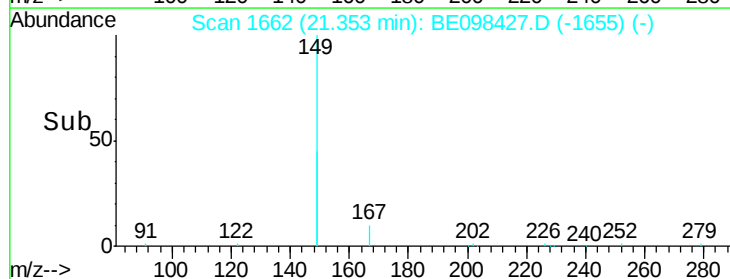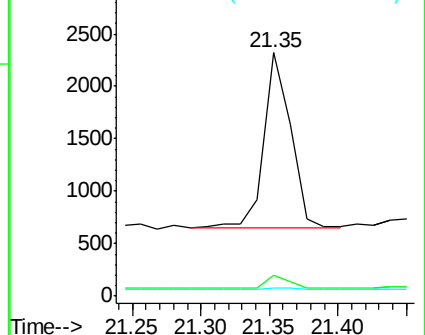

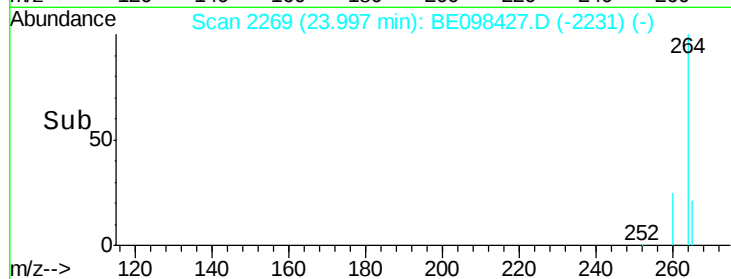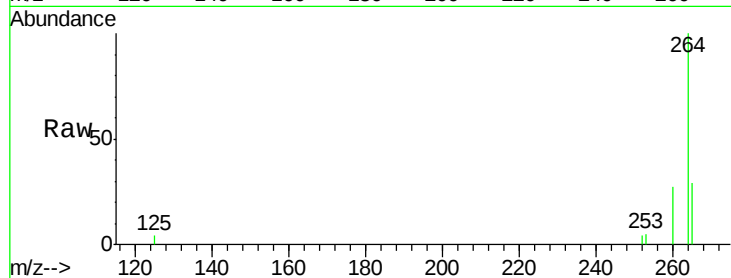

#34

Perylene-d12

Concen: 0.400 ng

RT: 24.00 min Scan# 2269

Delta R.T. -0.01 min

Lab File: BE098427.D

Acq: 14 Dec 2018 9:44

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW311S-20181209

Tgt Ion: 264 Resp: 7343

Ion Ratio Lower Upper

264 100

260 26.6 20.2 30.2

265 28.6 25.2 37.8

