


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE121318\
 Data File : BE098415.D
 Acq On : 14 Dec 2018 2:23
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

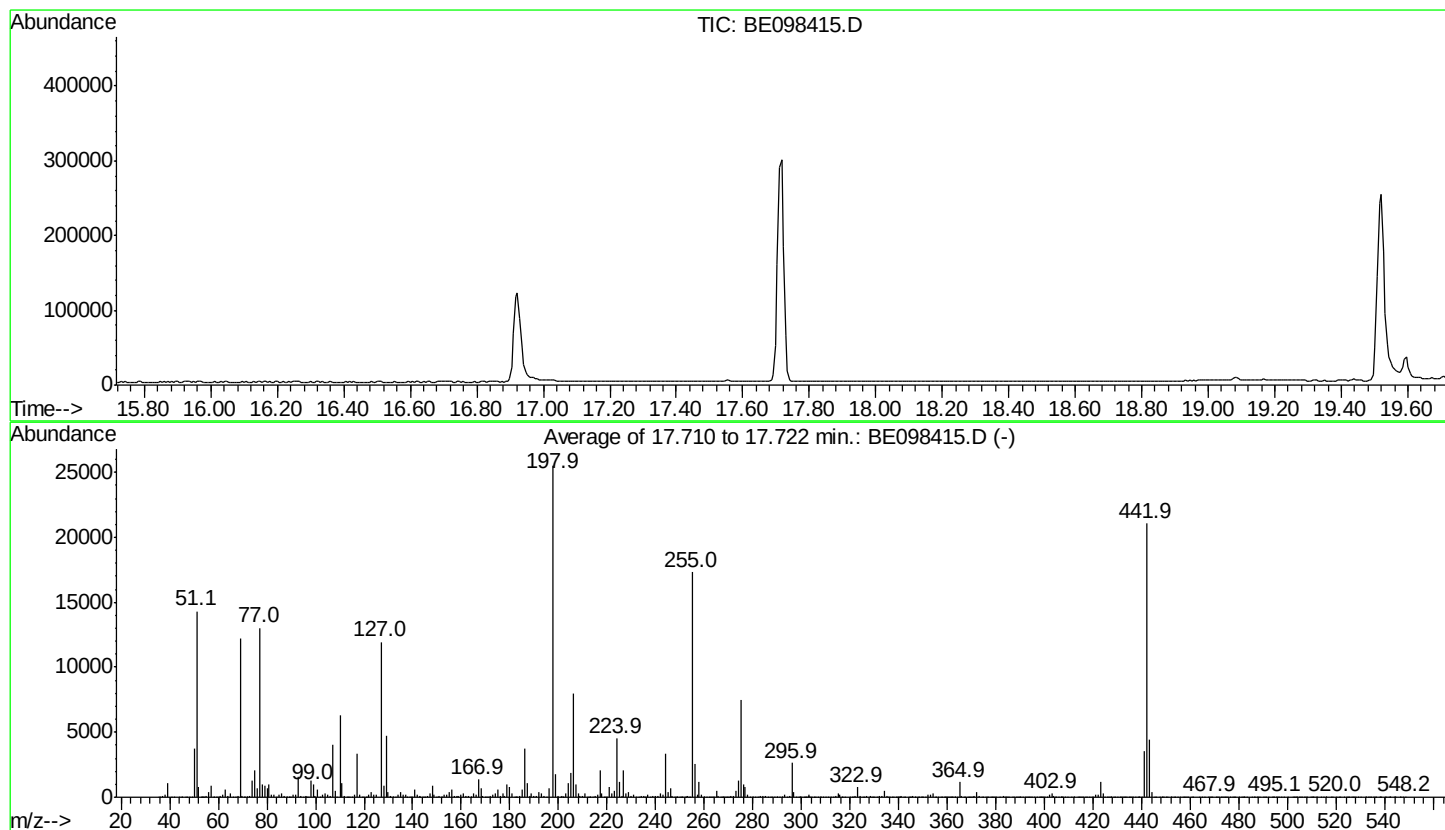

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.1	14323	PASS
68	69	0.00	2	0.7	91	PASS
69	198	0.00	100	47.8	12192	PASS
70	69	0.00	2	0.7	82	PASS
127	198	10	80	46.9	11957	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25513	PASS
199	198	5	9	7.0	1779	PASS
275	198	10	60	29.2	7456	PASS
365	198	1	100	4.6	1176	PASS
441	198	0.01	100	14.0	3576	PASS
442	198	50	100	82.6	21064	PASS
443	442	15	24	21.2	4462	PASS