


Data Path : Z:\HPCHEM1\BNA E\Data\BE121417\
 Data File : BE094975.D
 Acq On : 14 Dec 2017 14:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 14 18:42:53 2017

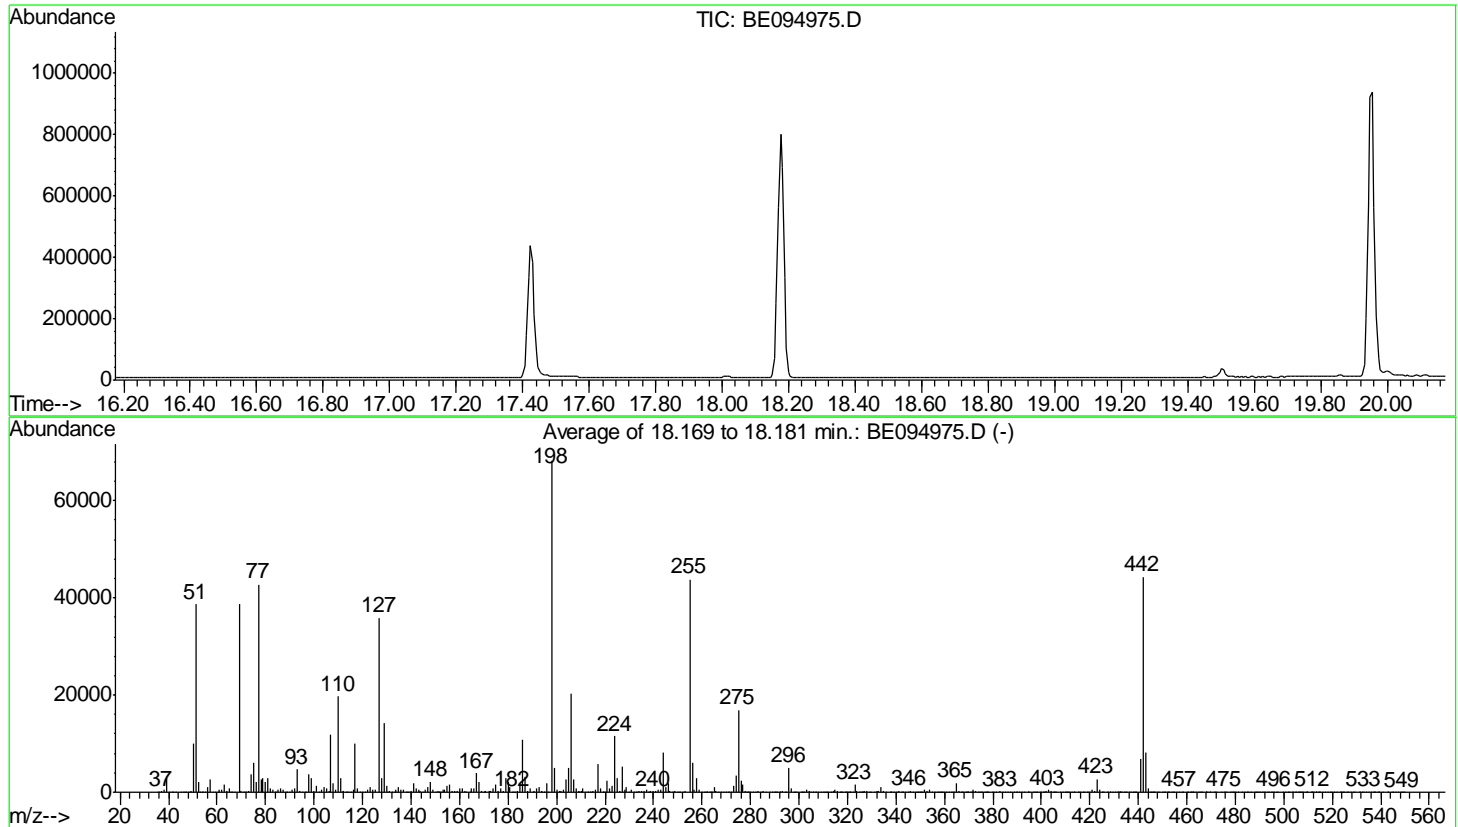

AutoFind: Scans 2652, 2653, 2654; Background Corrected with Scan 2643

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.6	38637	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.7	38691	PASS
70	69	0.00	2	0.5	200	PASS
127	198	10	80	52.7	35956	PASS
197	198	0.00	2	0.2	117	PASS
198	198	100	100	100.0	68247	PASS
199	198	5	9	7.3	5007	PASS
275	198	10	60	24.8	16940	PASS
365	198	1	100	2.9	1974	PASS
441	442	0.01	24	15.8	6988	PASS
442	198	50	100	65.0	44330	PASS
443	442	15	24	18.4	8178	PASS