


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121618\
Data File : BE098503.D
Acq On : 16 Dec 2018 11:47
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 10 14:59:55 2018

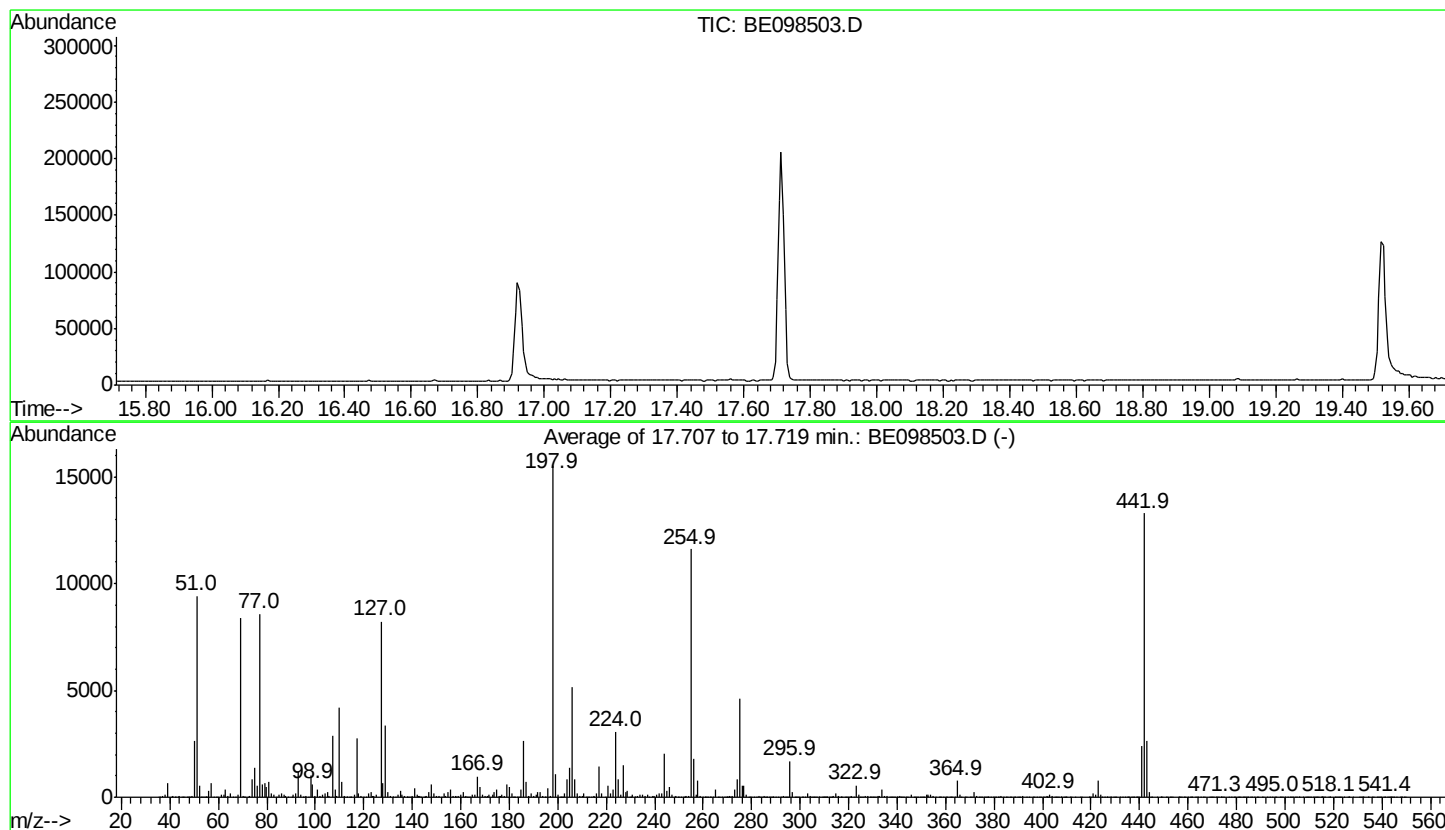

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.8	9432	PASS
68	69	0.00	2	1.4	118	PASS
69	198	0.00	100	54.0	8389	PASS
70	69	0.00	2	0.7	58	PASS
127	198	10	80	53.0	8227	PASS
197	198	0.00	2	0.2	37	PASS
198	198	100	100	100.0	15523	PASS
199	198	5	9	6.9	1074	PASS
275	198	10	60	29.8	4631	PASS
365	198	1	100	4.8	751	PASS
441	198	0.01	100	15.5	2399	PASS
442	198	50	100	85.6	13282	PASS
443	442	15	24	19.8	2629	PASS