

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121619\
 Data File : BE100932.D
 Acq On : 16 Dec 2019 23:46
 Operator : JU
 Sample : K6252-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE135D1-20191210

Quant Time: Dec 17 06:20:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 13 10:42:38 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	4559	0.40	ng	0.00
7) Naphthalene-d8	10.54	136	20489	0.40	ng	0.00
13) Acenaphthene-d10	14.38	164	11958	0.40	ng	0.00
19) Phenanthrene-d10	17.12	188	30174	0.40	ng	0.00
27) Chrysene-d12	21.29	240	27592	0.40	ng	-0.01
34) Perylene-d12	23.74	264	31165	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.36	112	1781	0.16	ng	-0.01
5) Phenol-d6	6.93	99	1581	0.10	ng	0.00
8) Nitrobenzene-d5	8.90	82	5231	0.54	ng	0.00
11) 2-Methylnaphthalene-d10	12.12	152	12285	0.41	ng	-0.01
14) 2,4,6-Tribromophenol	15.86	330	599	0.45	ng	-0.01
15) 2-Fluorobiphenyl	13.02	172	16335	0.34	ng	0.00
25) Fluoranthene-d10	19.15	212	138541	0.39	ng	0.00
29) Terphenyl-d14	19.75	244	26242	0.40	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.34	88	2439	0.293	ng	# 33
22) Pentachlorophenol	16.83	266	26	0.023	ng	# 74
32) Bis(2-ethylhexyl)phthalate	21.23	149	105780	1.500	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121619\
Data File : BE100932.D
Acq On : 16 Dec 2019 23:46
Operator : JU
Sample : K6252-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE135D1-20191210

Quant Time: Dec 17 06:20:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 13 10:42:38 2019
Response via : Initial Calibration

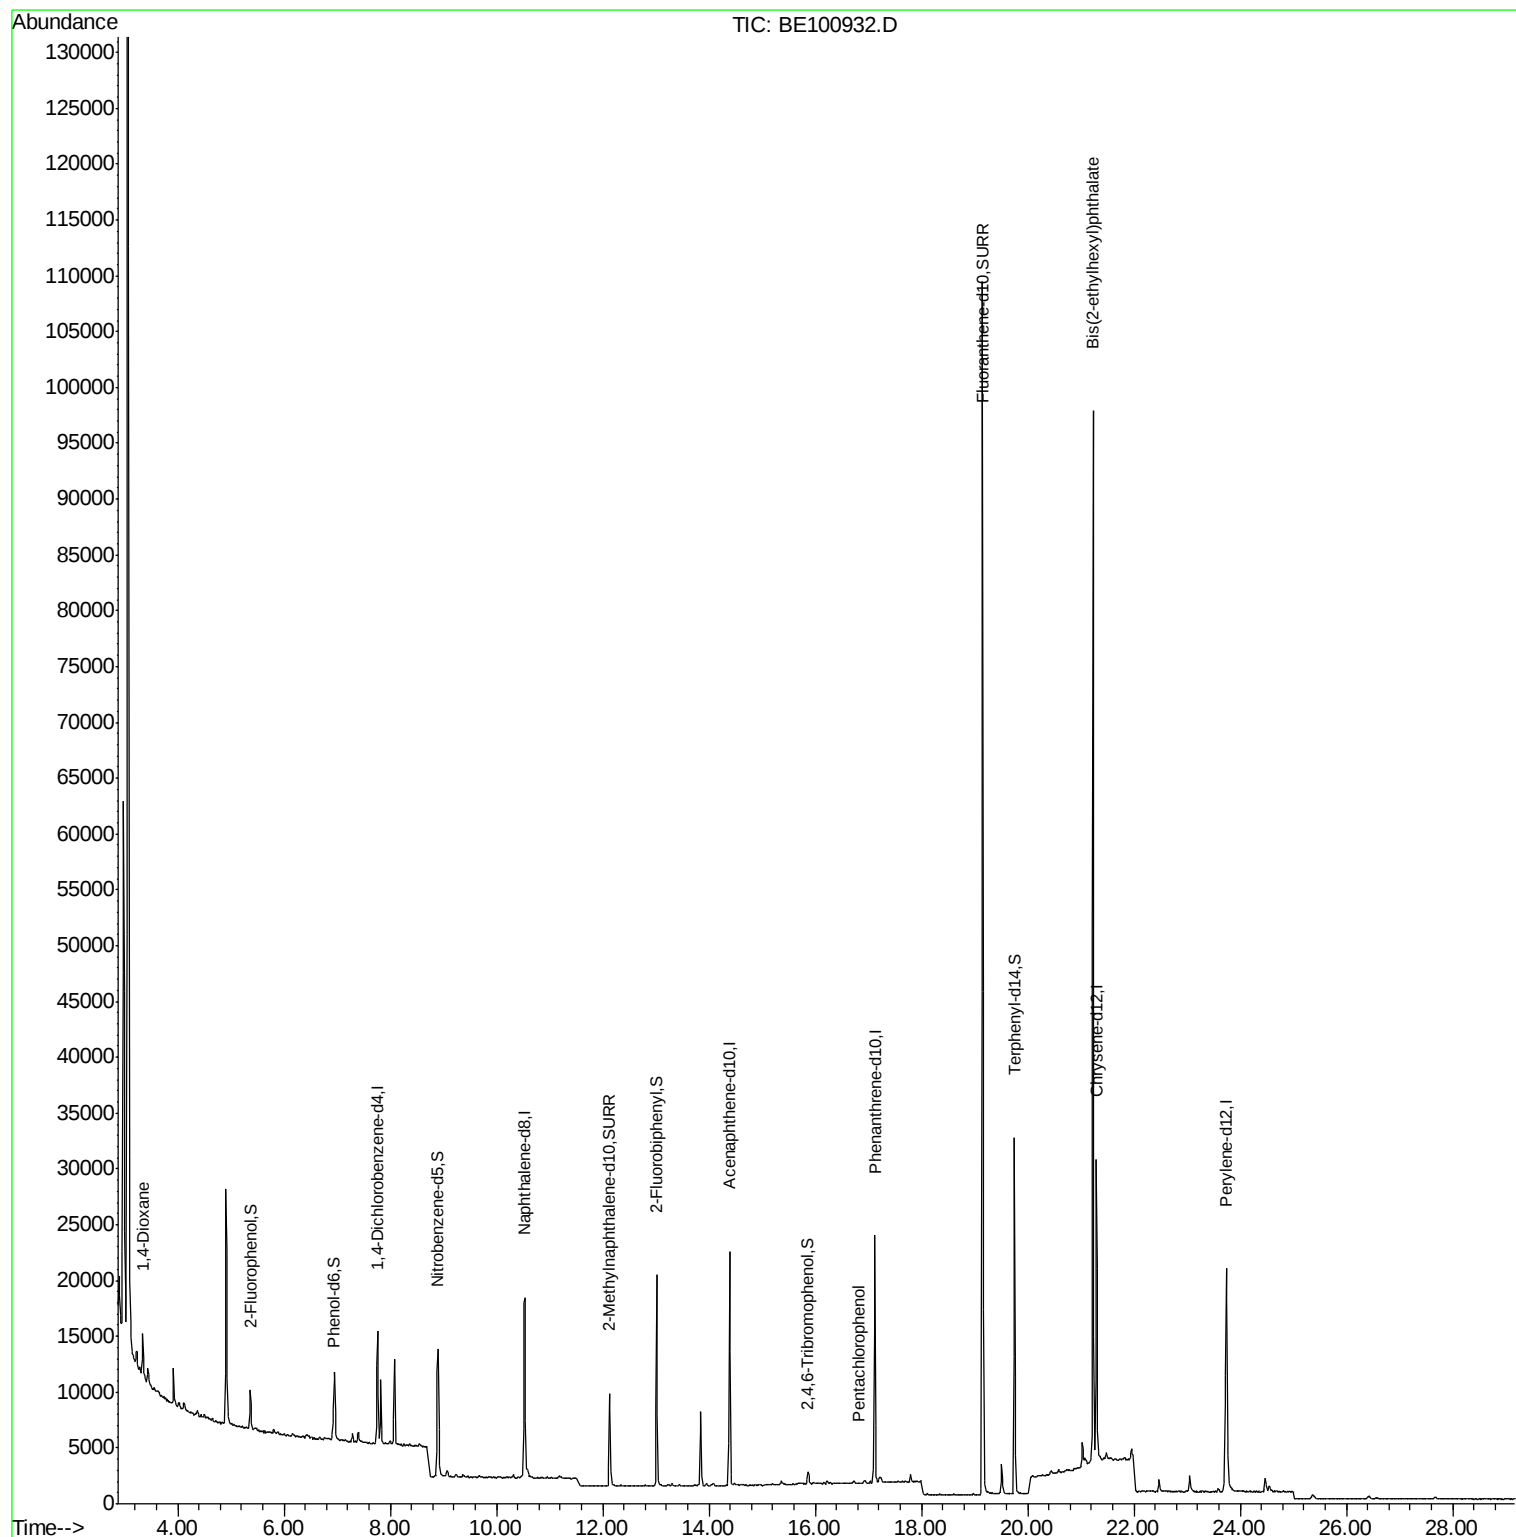




#1



1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.76 min Scan# 425
Delta R.T. 0.00 min
Lab File: BE100932.D
Acq: 16 Dec 2019 23:46

Instrument :
BNA_E
ClientSampleId :
RE135D1-20191210

Tot Ion:152 Resp: 4559
Ion Ratio Lower Upper
152 100
150 155.1 125.5 188.3
115 65.3 55.7 83.5

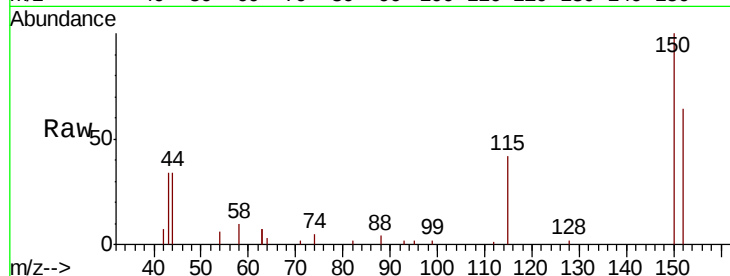


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

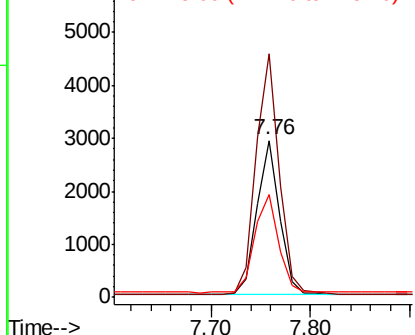



#2

1,4-Dioxane
Concen: 0.293 ng
RT: 3.34 min Scan# 41
Delta R.T. 0.00 min
Lab File: BE100932.D
Acq: 16 Dec 2019 23:46

Tgt Ion: 88 Resp: 2439
Ion Ratio Lower Upper
88 100
58 92.5 52.3 78.5#
43 103.7 23.5 35.3#



Abundance Ion 88.00 (87.70 to 88.70): BE1
Ion 58.00 (57.70 to 58.70): BE1
Ion 43.00 (42.70 to 43.70): BE1

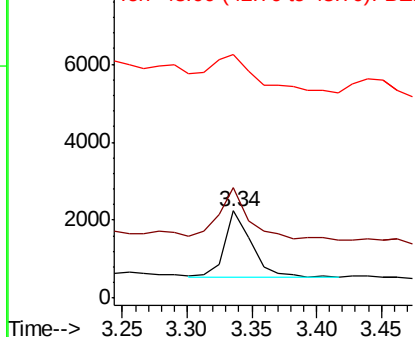



#4

2-Fluorophenol

Concen: 0.165 ng

RT: 5.36 min Scan# 217

Delta R.T. -0.01 min

Lab File: BE100932.D

Acq: 16 Dec 2019 23:46

Instrument :

BNA_E

ClientSampleId :

RE135D1-20191210


Tot Ion:112 Resp: 1781

Ion Ratio Lower Upper

112 100

64 66.5 54.5 81.7



63 139.9 116.1 174.1



Abundance Ion 112.00 (111.70 to 112.70): BE1

Ion 64.00 (63.70 to 64.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

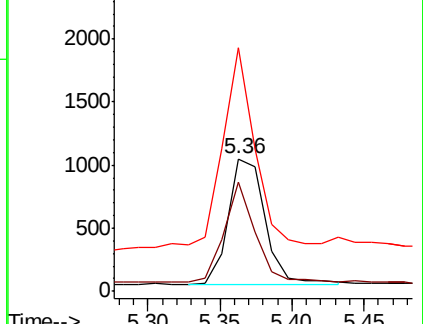

#5

Phenol-d6

Concen: 0.097 ng

RT: 6.93 min Scan# 353

Delta R.T. 0.00 min

Lab File: BE100932.D

Acq: 16 Dec 2019 23:46


Tgt Ion: 99 Resp: 1581

Ion Ratio Lower Upper

99 100

42 45.2 18.2 27.2#



71 40.9 29.1 43.7




Abundance Ion 99.00 (98.70 to 99.70): BE1

Ion 42.00 (41.70 to 42.70): BE1

Ion 71.00 (70.70 to 71.70): BE1

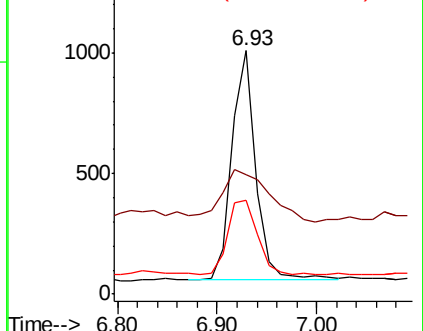

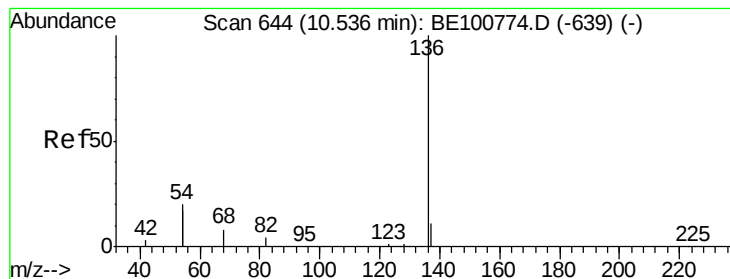

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.54 min Scan# 644

Delta R.T. -0.00 min

Lab File: BE100932.D

Acq: 16 Dec 2019 23:46

Instrument :

BNA_E

ClientSampleId :

RE135D1-20191210

Tot Ion:136 Resp: 20489


Ion Ratio Lower Upper

136 100

137 11.2 9.1 13.7

54 24.4 18.9 28.3

68 5.4 4.6 6.8






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE1

Ion 68.00 (67.70 to 68.70): BE1

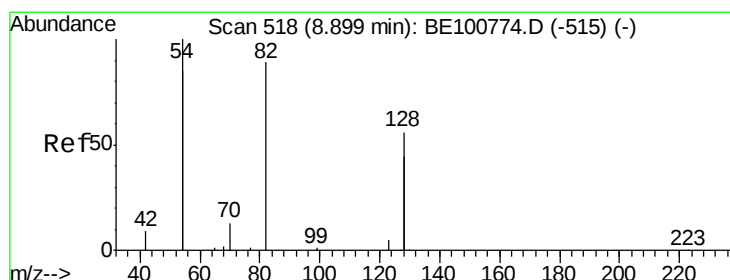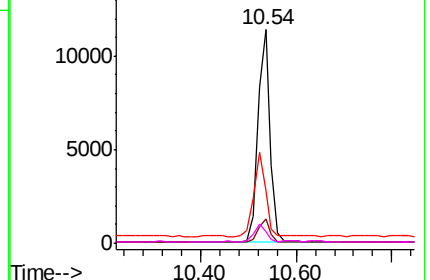

#8

Nitrobenzene-d5

Concen: 0.536 ng

RT: 8.90 min Scan# 518

Delta R.T. -0.00 min

Lab File: BE100932.D

Acq: 16 Dec 2019 23:46


Tgt Ion: 82 Resp: 5231

Ion Ratio Lower Upper

82 100

128 141.9 113.5 170.3



54 190.1 138.9 208.3




Abundance Ion 82.00 (81.70 to 82.70): BE1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE1



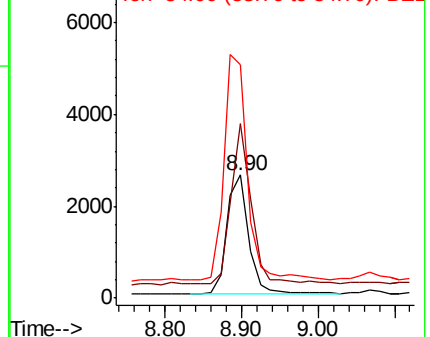
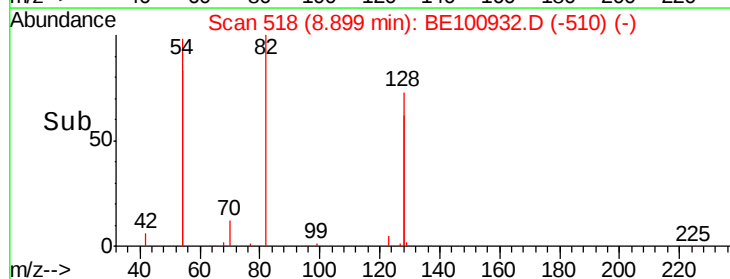


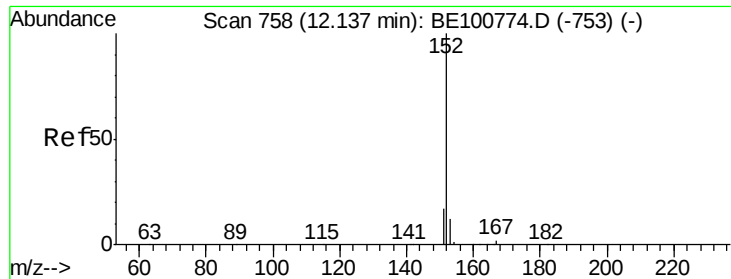

#11
 2-Methylnaphthalene-d10
 Concen: 0.414 ng
 RT: 12.12 min Scan# 757
 Delta R.T. -0.01 min
 Lab File: BE100932.D
 Acq: 16 Dec 2019 23:46




Instrument :
 BNA_E
 ClientSampleId :
 RE135D1-20191210


Tot Ion:152 Resp: 12285
 Ion Ratio Lower Upper
 152 100
 151 19.7 15.1 22.7

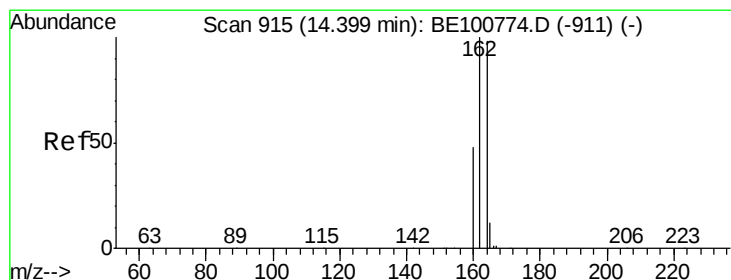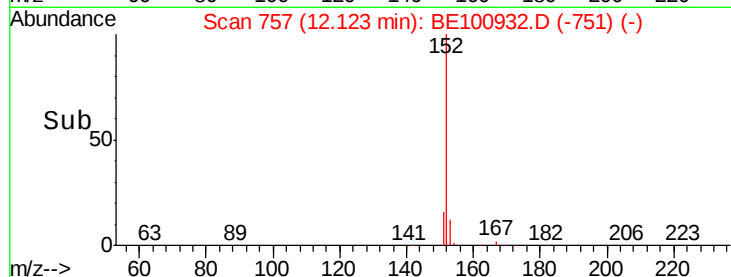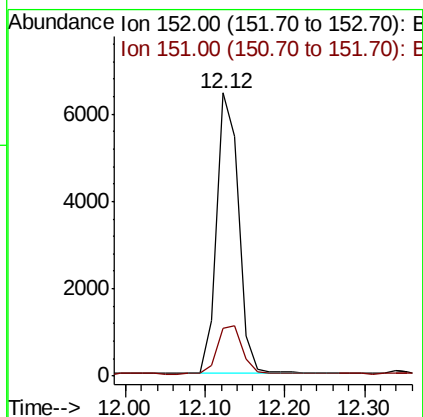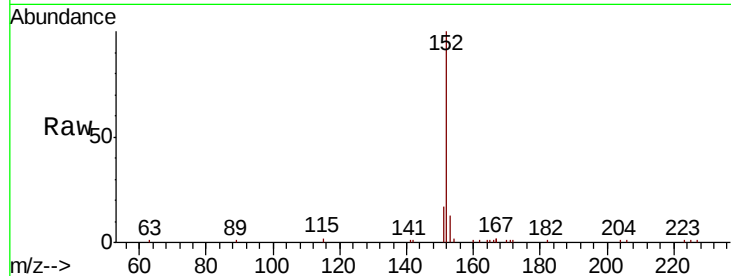

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.38 min Scan# 914
 Delta R.T. -0.00 min
 Lab File: BE100932.D
 Acq: 16 Dec 2019 23:46

Tgt Ion:164 Resp: 11958
 Ion Ratio Lower Upper
 164 100
 162 105.8 86.0 129.0
 160 50.4 42.3 63.5

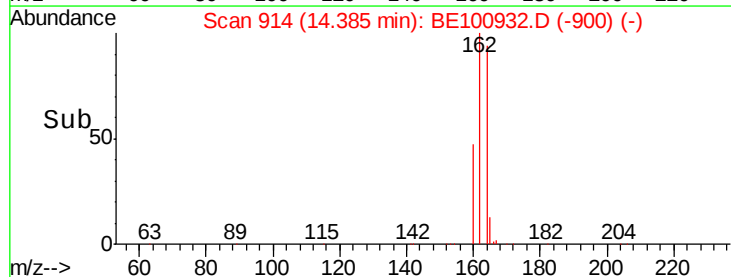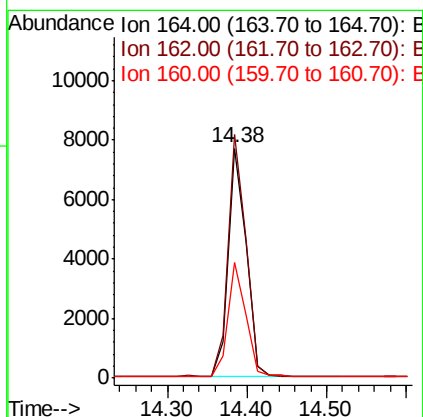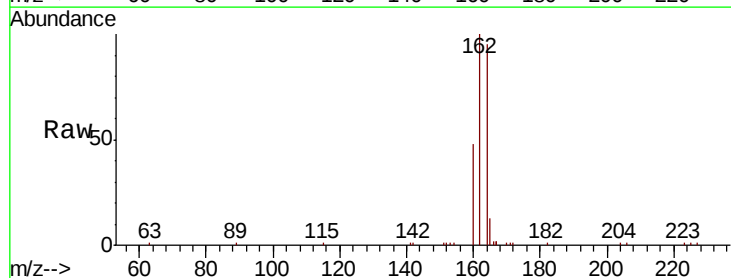


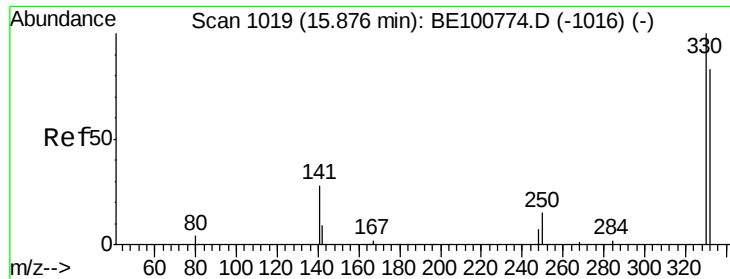




#14
2,4,6-Tribromophenol
Concen: 0.450 ng
RT: 15.86 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BE100932.D
Acq: 16 Dec 2019 23:46

Instrument :
BNA_E
ClientSampleId :
RE135D1-20191210

Tot Ion:330 Resp: 599
Ion Ratio Lower Upper
330 100
332 108.7 74.1 111.1
141 57.3 46.7 70.1




Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

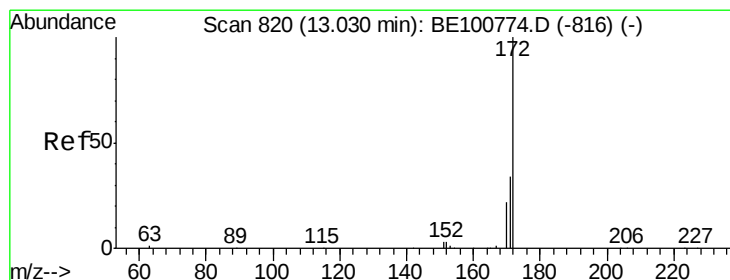
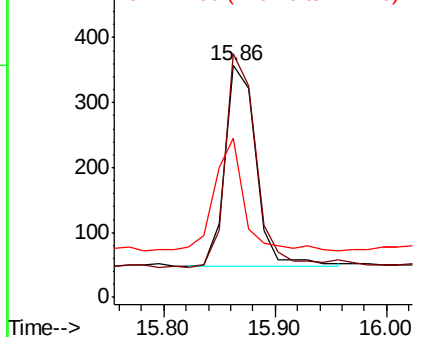



#15
2-Fluorobiphenyl
Concen: 0.344 ng
RT: 13.02 min Scan# 819
Delta R.T. -0.00 min
Lab File: BE100932.D
Acq: 16 Dec 2019 23:46

Tgt Ion:172 Resp: 16335
Ion Ratio Lower Upper
172 100
171 34.6 28.2 42.4
170 23.6 19.4 29.0



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

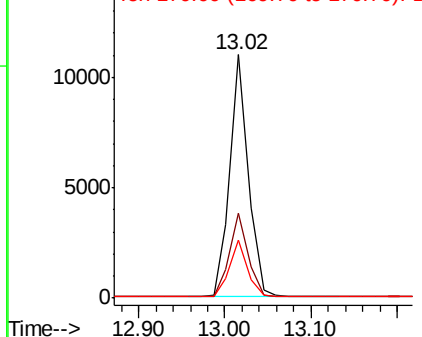

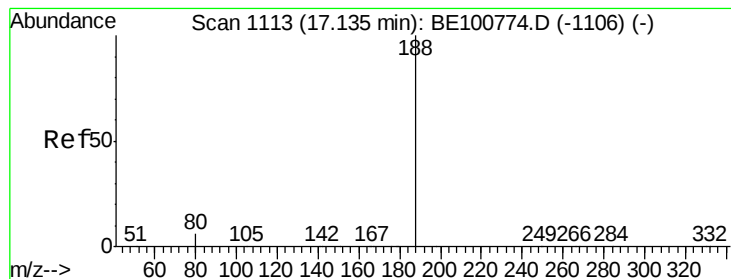

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.12 min Scan# 1112

Delta R.T. 0.00 min

Lab File: BE100932.D

Acq: 16 Dec 2019 23:46

Instrument :

BNA_E

ClientSampleId :

RE135D1-20191210


Tot Ion:188 Resp: 30174

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 8.8 7.9 11.9

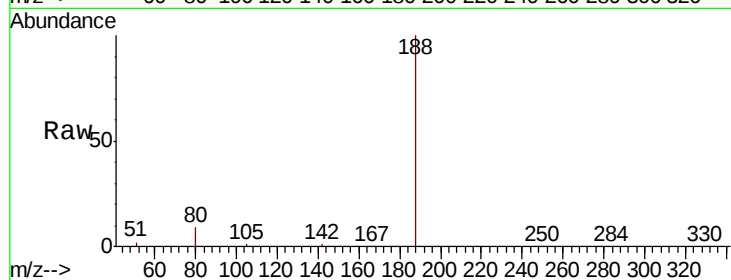

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE1

Ion 80.00 (79.70 to 80.70): BE1

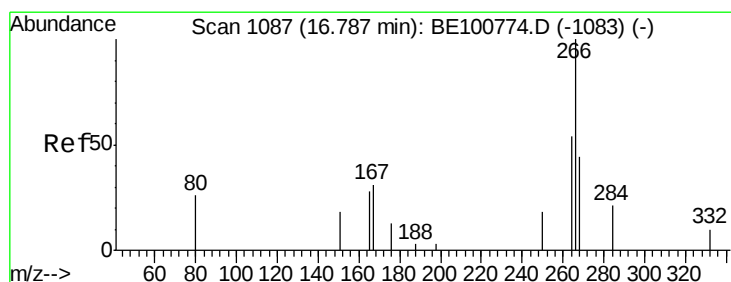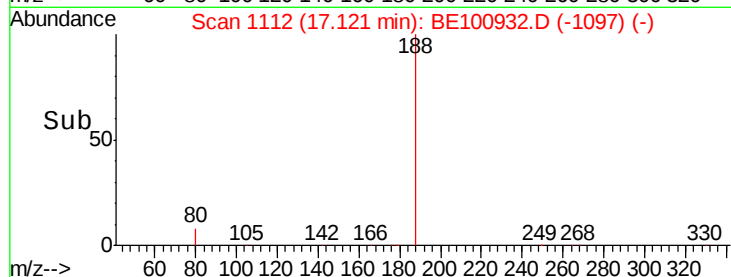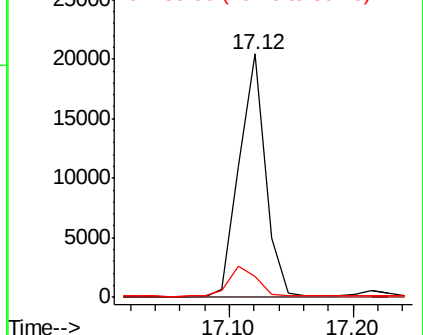

#22

Pentachlorophenol

Concen: 0.023 ng

RT: 16.83 min Scan# 1090

Delta R.T. 0.04 min

Lab File: BE100932.D

Acq: 16 Dec 2019 23:46


Tgt Ion:266 Resp: 26

Ion Ratio Lower Upper

266 100

264 85.2 55.1 82.7#



268 88.5 50.7 76.1#

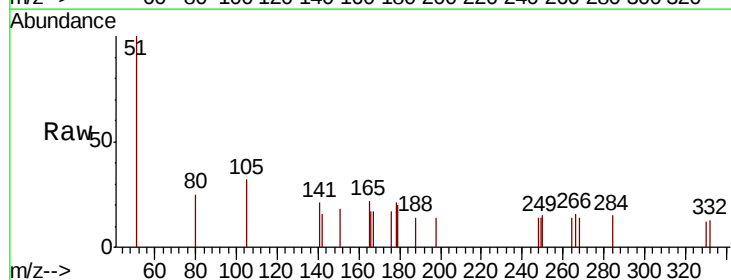


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E



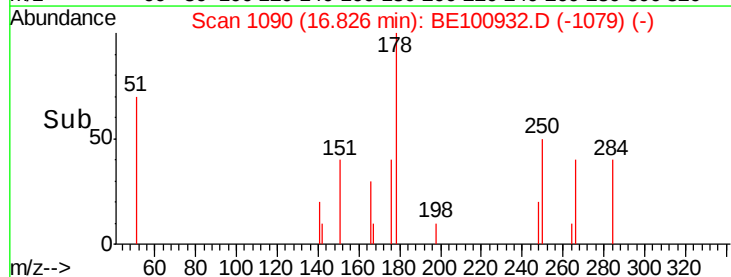
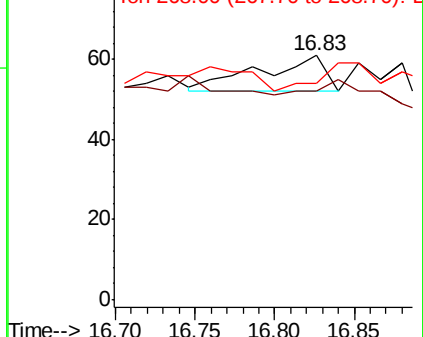




#25
 Fluoranthene-d10
 Concen: 0.388 ng
 RT: 19.15 min Scan# 1372
 Delta R.T. 0.00 min
 Lab File: BE100932.D
 Acq: 16 Dec 2019 23:46




Instrument :
 BNA_E
 ClientSampleId :
 RE135D1-20191210


Tot Ion:212 Resp: 138541
 Ion Ratio Lower Upper
 212 100
 106 3.5 2.6 4.0
 104 1.9 1.4 2.2

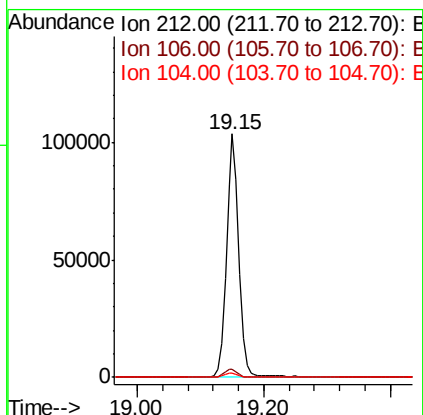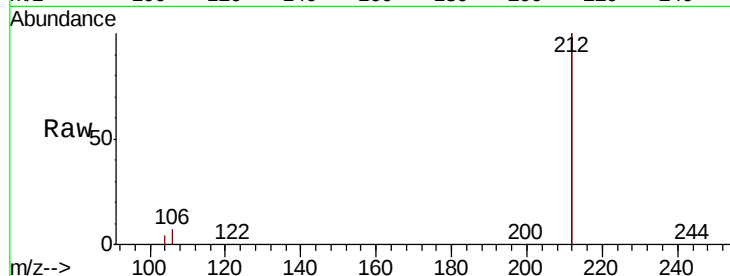

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.29 min Scan# 1624
 Delta R.T. -0.01 min
 Lab File: BE100932.D
 Acq: 16 Dec 2019 23:46

Tgt Ion:240 Resp: 27592
 Ion Ratio Lower Upper
 240 100
 120 13.1 4.0 6.0#
 236 27.9 21.6 32.4

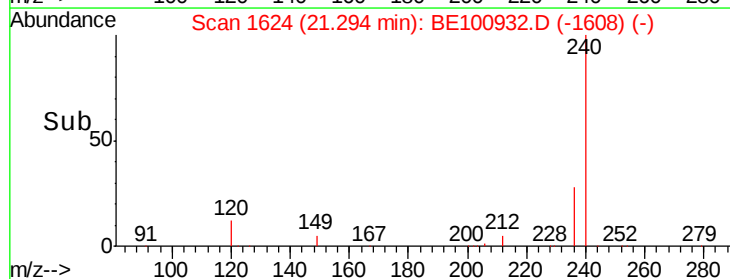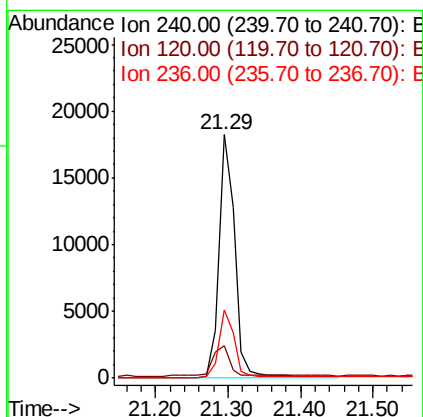

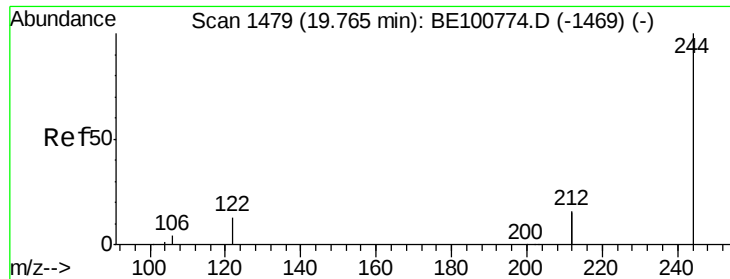

#29

Terphenyl-d14

Concen: 0.397 ng

RT: 19.75 min Scan# 1477

Delta R.T. -0.00 min

Lab File: BE100932.D

Acq: 16 Dec 2019 23:46

Instrument :

BNA_E

ClientSampleId :

RE135D1-20191210


Tot Ion:244 Resp: 26242

Ion Ratio Lower Upper




244 100

212 32.0 25.2 37.8

122 12.2 8.9 13.3



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

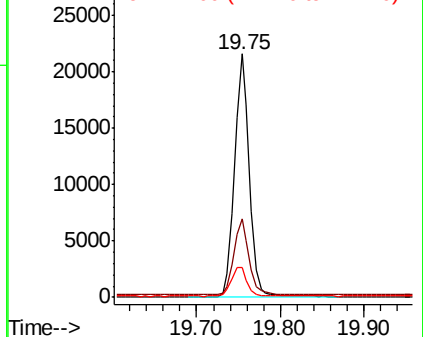

#32

Bis(2-ethylhexyl)phthalate

Concen: 1.500 ng

RT: 21.23 min Scan# 1619

Delta R.T. 0.00 min

Lab File: BE100932.D

Acq: 16 Dec 2019 23:46


Tgt Ion:149 Resp: 105780

Ion Ratio Lower Upper



149 100




167 6.7 5.0 7.4

279 0.8 0.6 1.0



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

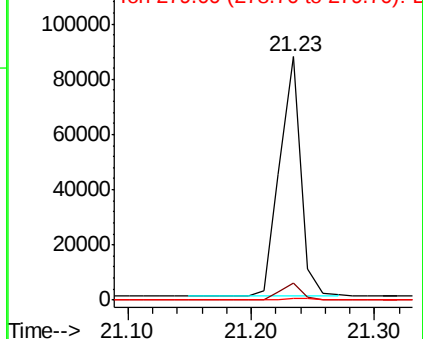

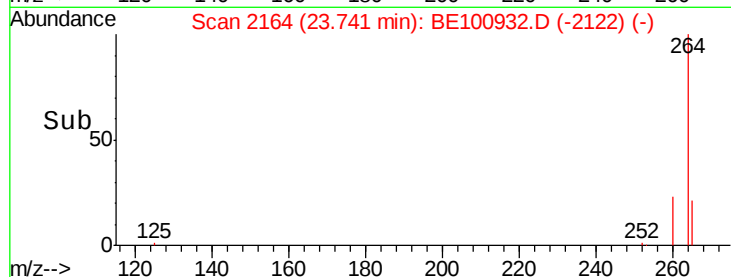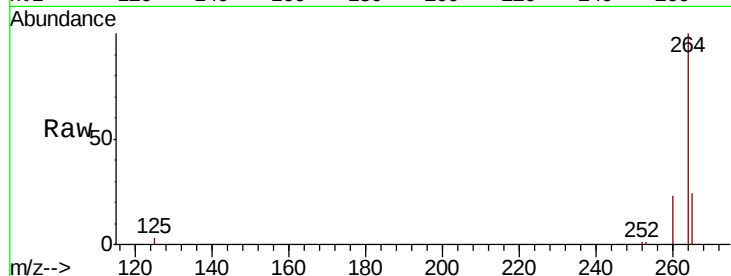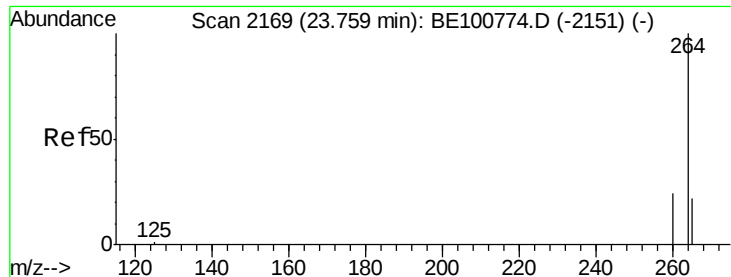

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.74 min Scan# 2164

Delta R.T. -0.00 min

Lab File: BE100932.D

Acq: 16 Dec 2019 23:46

Instrument :

BNA_E

ClientSampleId :

RE135D1-20191210

Tot Ion: 264 Resp: 31165

Ion Ratio Lower Upper

264 100

260 23.2 19.4 29.0

265 23.9 20.1 30.1

