
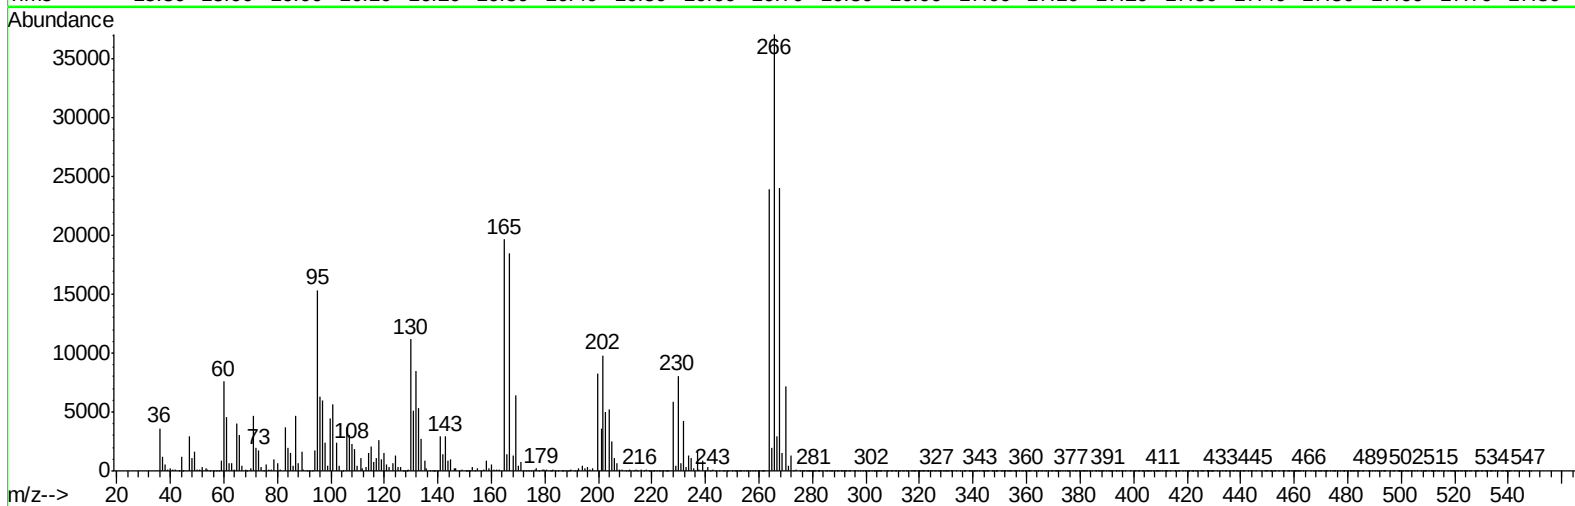


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121619\  
Data File : BE100929.D  
Acq On : 16 Dec 2019 21:20  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 08:29:53 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE120419.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 13 10:42:38 2019  
Response via : Initial Calibration

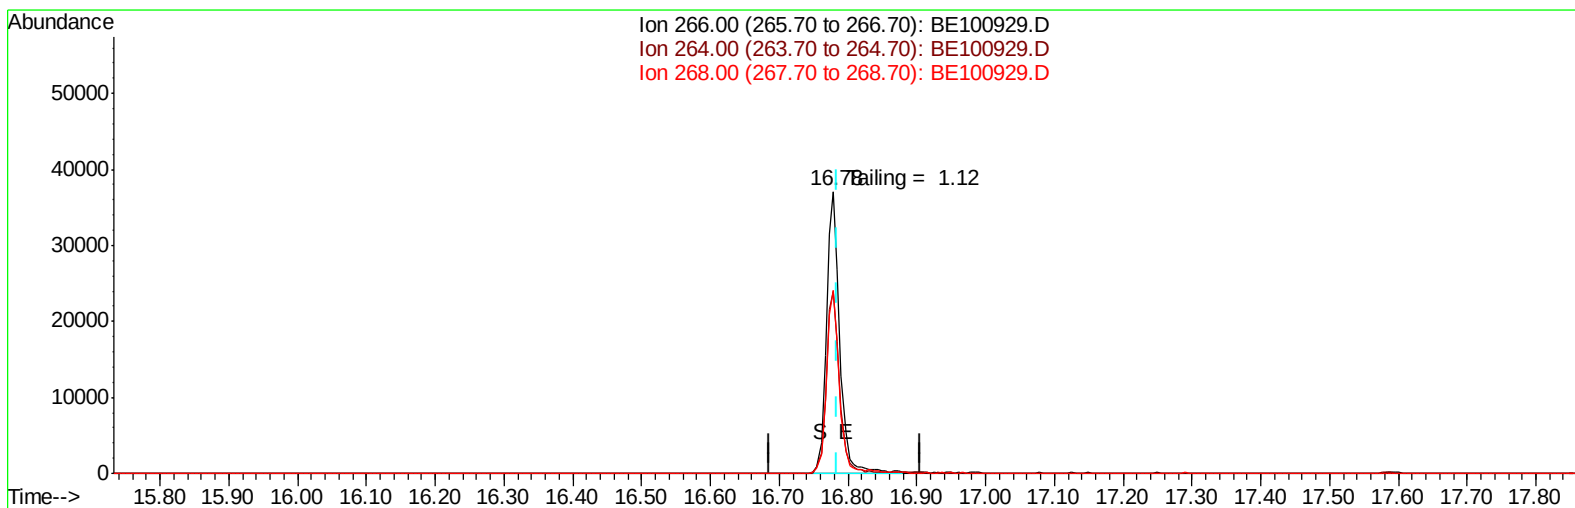

TIC: BE100929.D

(22) Pentachlorophenol

16.779min (-0.007) 38680.98ng

response 49912

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 266.00 | 100   | 100   |
| 264.00 | 68.90 | 64.44 |
| 268.00 | 63.40 | 69.03 |
| 0.00   | 0.00  | 0.00  |