


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE121619\
Data File : BE100914.D
Acq On : 16 Dec 2019 9:22
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE120419.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 13 10:42:38 2019

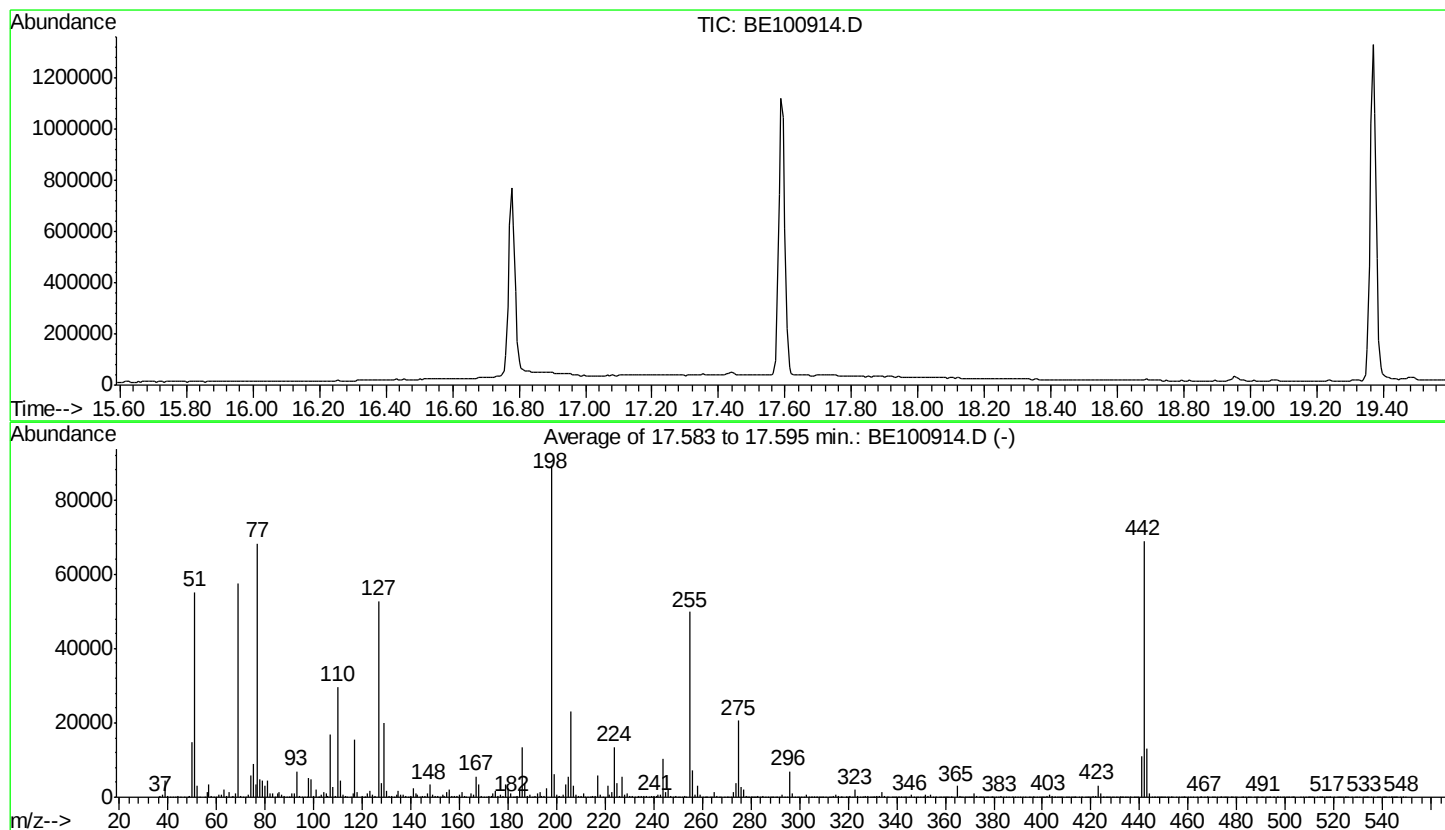

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2545

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.8	55098	PASS
68	69	0.00	2	1.8	1052	PASS
69	198	0.00	100	64.4	57381	PASS
70	69	0.00	2	0.5	280	PASS
127	198	10	80	59.2	52776	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89158	PASS
199	198	5	9	7.0	6216	PASS
275	198	10	60	23.2	20651	PASS
365	198	1	100	3.3	2977	PASS
441	198	0.01	100	12.4	11086	PASS
442	198	50	100	77.4	68985	PASS
443	442	15	24	19.2	13229	PASS