


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE121619\
 Data File : BE100929.D
 Acq On : 16 Dec 2019 21:20
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE120419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 13 10:42:38 2019

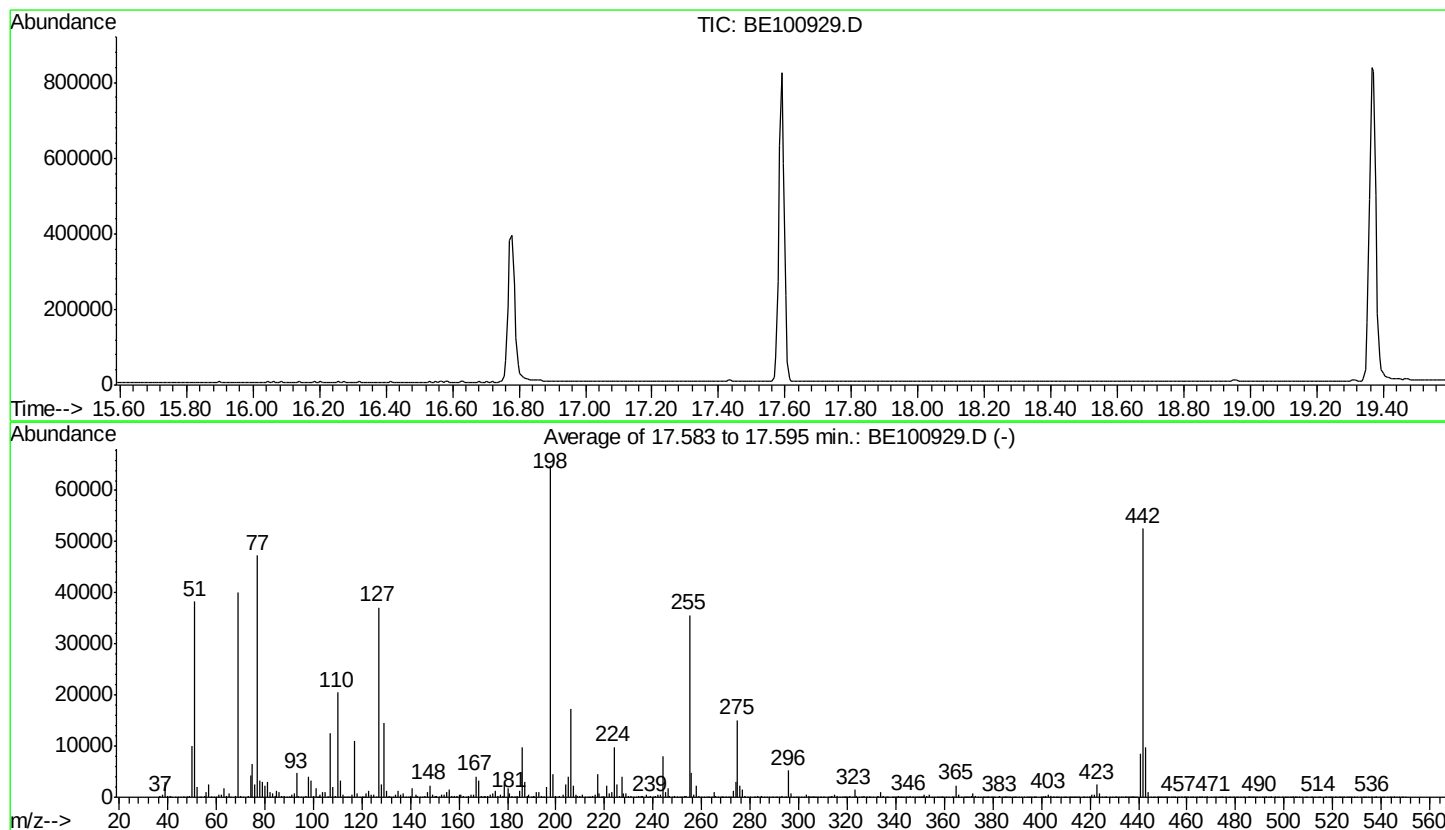

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.9	38233	PASS
68	69	0.00	2	0.8	314	PASS
69	198	0.00	100	61.7	40007	PASS
70	69	0.00	2	0.4	151	PASS
127	198	10	80	57.2	37132	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64889	PASS
199	198	5	9	7.1	4629	PASS
275	198	10	60	23.3	15103	PASS
365	198	1	100	3.5	2295	PASS
441	198	0.01	100	13.2	8550	PASS
442	198	50	100	81.0	52548	PASS
443	442	15	24	18.7	9802	PASS