


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE121918\
 Data File : BE098521.D
 Acq On : 19 Dec 2018 9:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

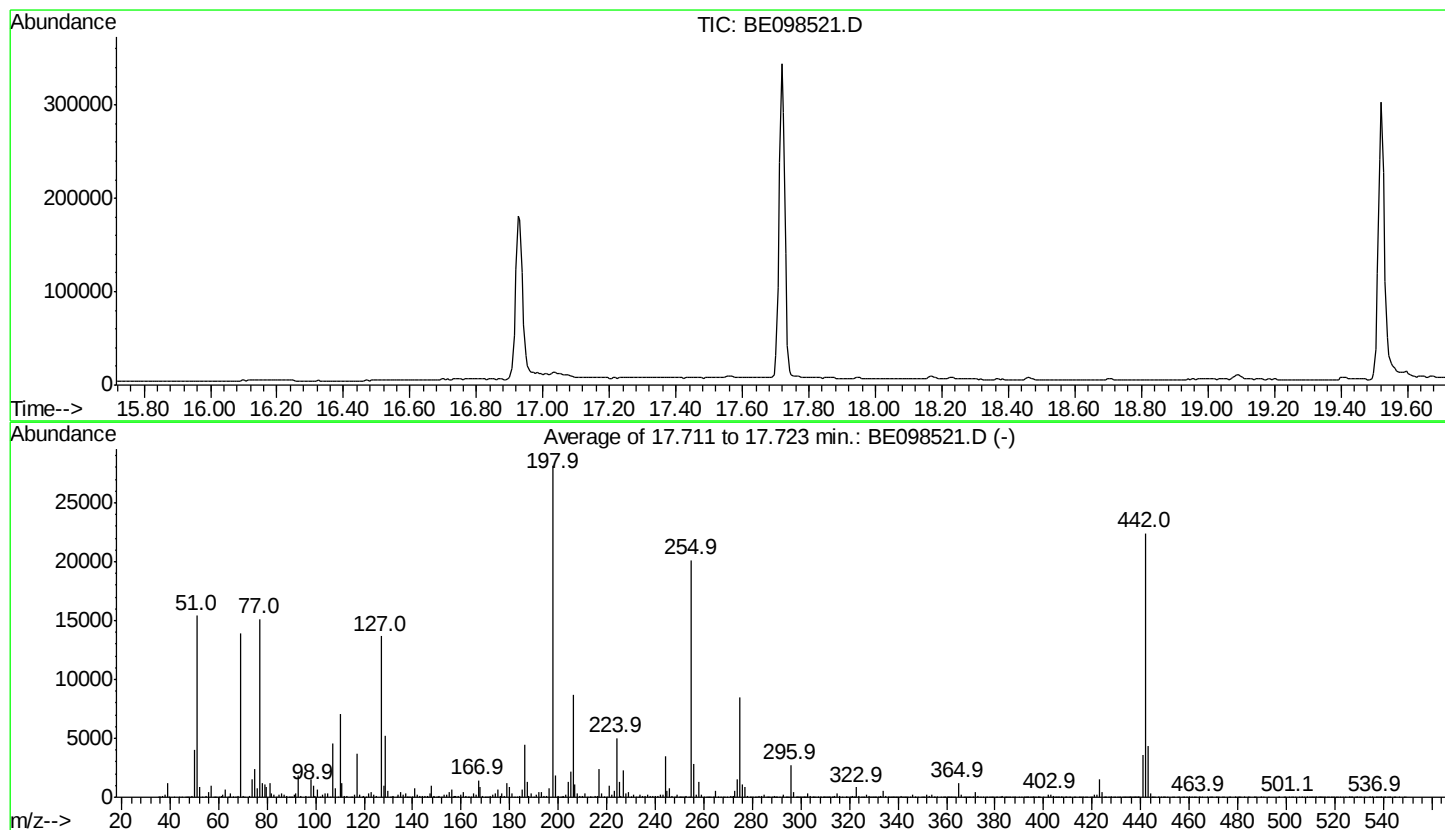

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.7	15405	PASS
68	69	0.00	2	0.4	58	PASS
69	198	0.00	100	49.5	13937	PASS
70	69	0.00	2	0.9	122	PASS
127	198	10	80	48.6	13680	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28165	PASS
199	198	5	9	6.6	1852	PASS
275	198	10	60	30.2	8510	PASS
365	198	1	100	4.3	1222	PASS
441	198	0.01	100	12.8	3615	PASS
442	198	50	100	79.6	22416	PASS
443	442	15	24	19.4	4355	PASS