


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121919\
 Data File : BE100950.D
 Acq On : 19 Dec 2019 15:48
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 20 01:12:26 2019

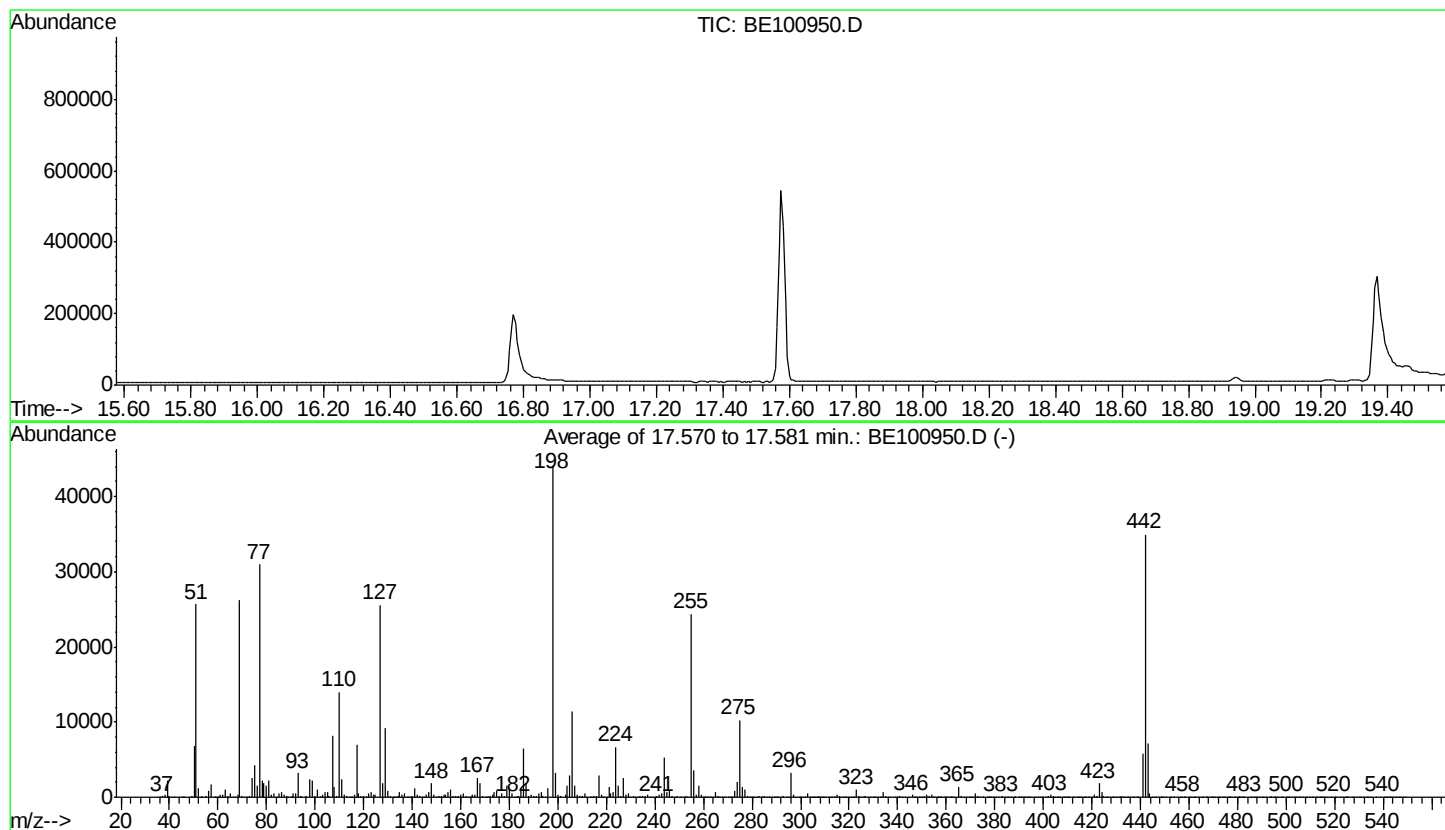

AutoFind: Scans 2550, 2551, 2552; Background Corrected with Scan 2543

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.1	25655	PASS
68	69	0.00	2	1.1	301	PASS
69	198	0.00	100	59.5	26239	PASS
70	69	0.00	2	0.5	130	PASS
127	198	10	80	58.0	25597	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44130	PASS
199	198	5	9	7.2	3171	PASS
275	198	10	60	23.2	10252	PASS
365	198	1	100	3.3	1447	PASS
441	198	0.01	100	13.3	5855	PASS
442	198	50	100	79.3	34999	PASS
443	442	15	24	20.3	7088	PASS