


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE122018\
 Data File : BE098531.D
 Acq On : 20 Dec 2018 8:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

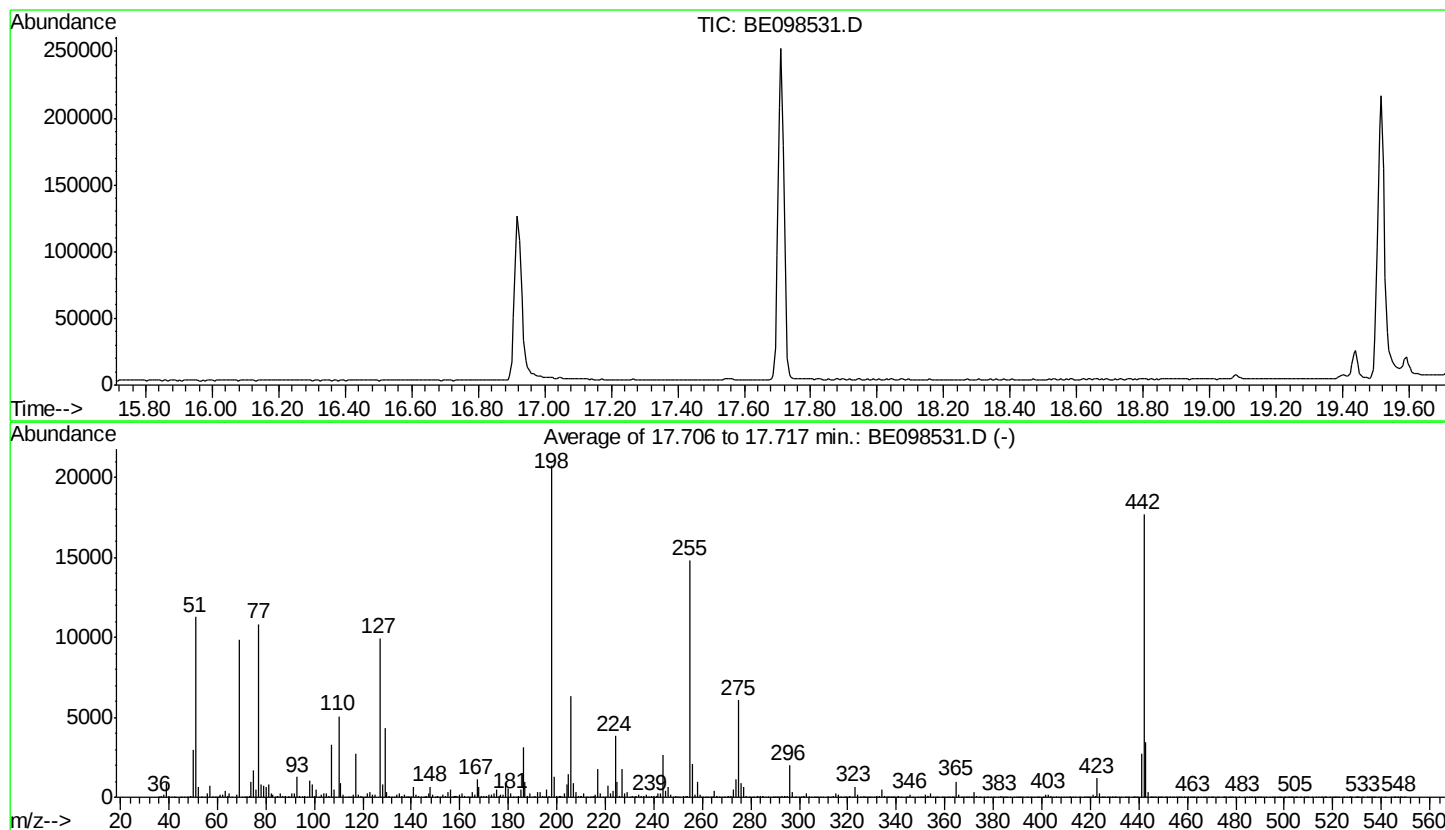

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.4	11290	PASS
68	69	0.00	2	1.3	127	PASS
69	198	0.00	100	47.5	9871	PASS
70	69	0.00	2	0.4	38	PASS
127	198	10	80	47.7	9900	PASS
197	198	0.00	2	0.3	59	PASS
198	198	100	100	100.0	20760	PASS
199	198	5	9	6.1	1260	PASS
275	198	10	60	29.2	6071	PASS
365	198	1	100	4.7	974	PASS
441	198	0.01	100	13.3	2763	PASS
442	198	50	100	85.2	17680	PASS
443	442	15	24	19.3	3416	PASS