

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE122118\
 Data File : BE098555.D
 Acq On : 21 Dec 2018 17:09
 Operator : SJ/JU
 Sample : PB115910BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB115910BL

Quant Time: Dec 22 00:57:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	397	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	1666	0.40	ng	0.00
13) Acenaphthene-d10	14.51	164	1268	0.40	ng	-0.01
19) Phenanthrene-d10	17.27	188	4185	0.40	ng	-0.01
27) Chrysene-d12	21.45	240	7285	0.40	ng	-0.01
34) Perylene-d12	23.99	264	6335	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.45	112	401	0.43	ng	0.00
5) Phenol-d6	7.06	99	442	0.34	ng	0.00
8) Nitrobenzene-d5	9.07	82	337	0.22	ng	0.05
11) 2-Methylnaphthalene-d10	12.27	152	974	0.36	ng	0.00
14) 2,4,6-Tribromophenol	16.02	330	205	0.44	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	1532	0.29	ng	0.00
25) Fluoranthene-d10	19.30	212	26756	0.50	ng	-0.01
29) Terphenyl-d14	19.90	244	5540	0.31	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.35	88	21	0.031	ng	Qvalue # 12
3) n-Nitrosodimethylamine	3.67	42	30	0.049	ng	# 100
22) Pentachlorophenol	16.95	266	3	0.024	ng	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE122118\
Data File : BE098555.D
Acq On : 21 Dec 2018 17:09
Operator : SJ/JU
Sample : PB115910BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB115910BL

Quant Time: Dec 22 00:57:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

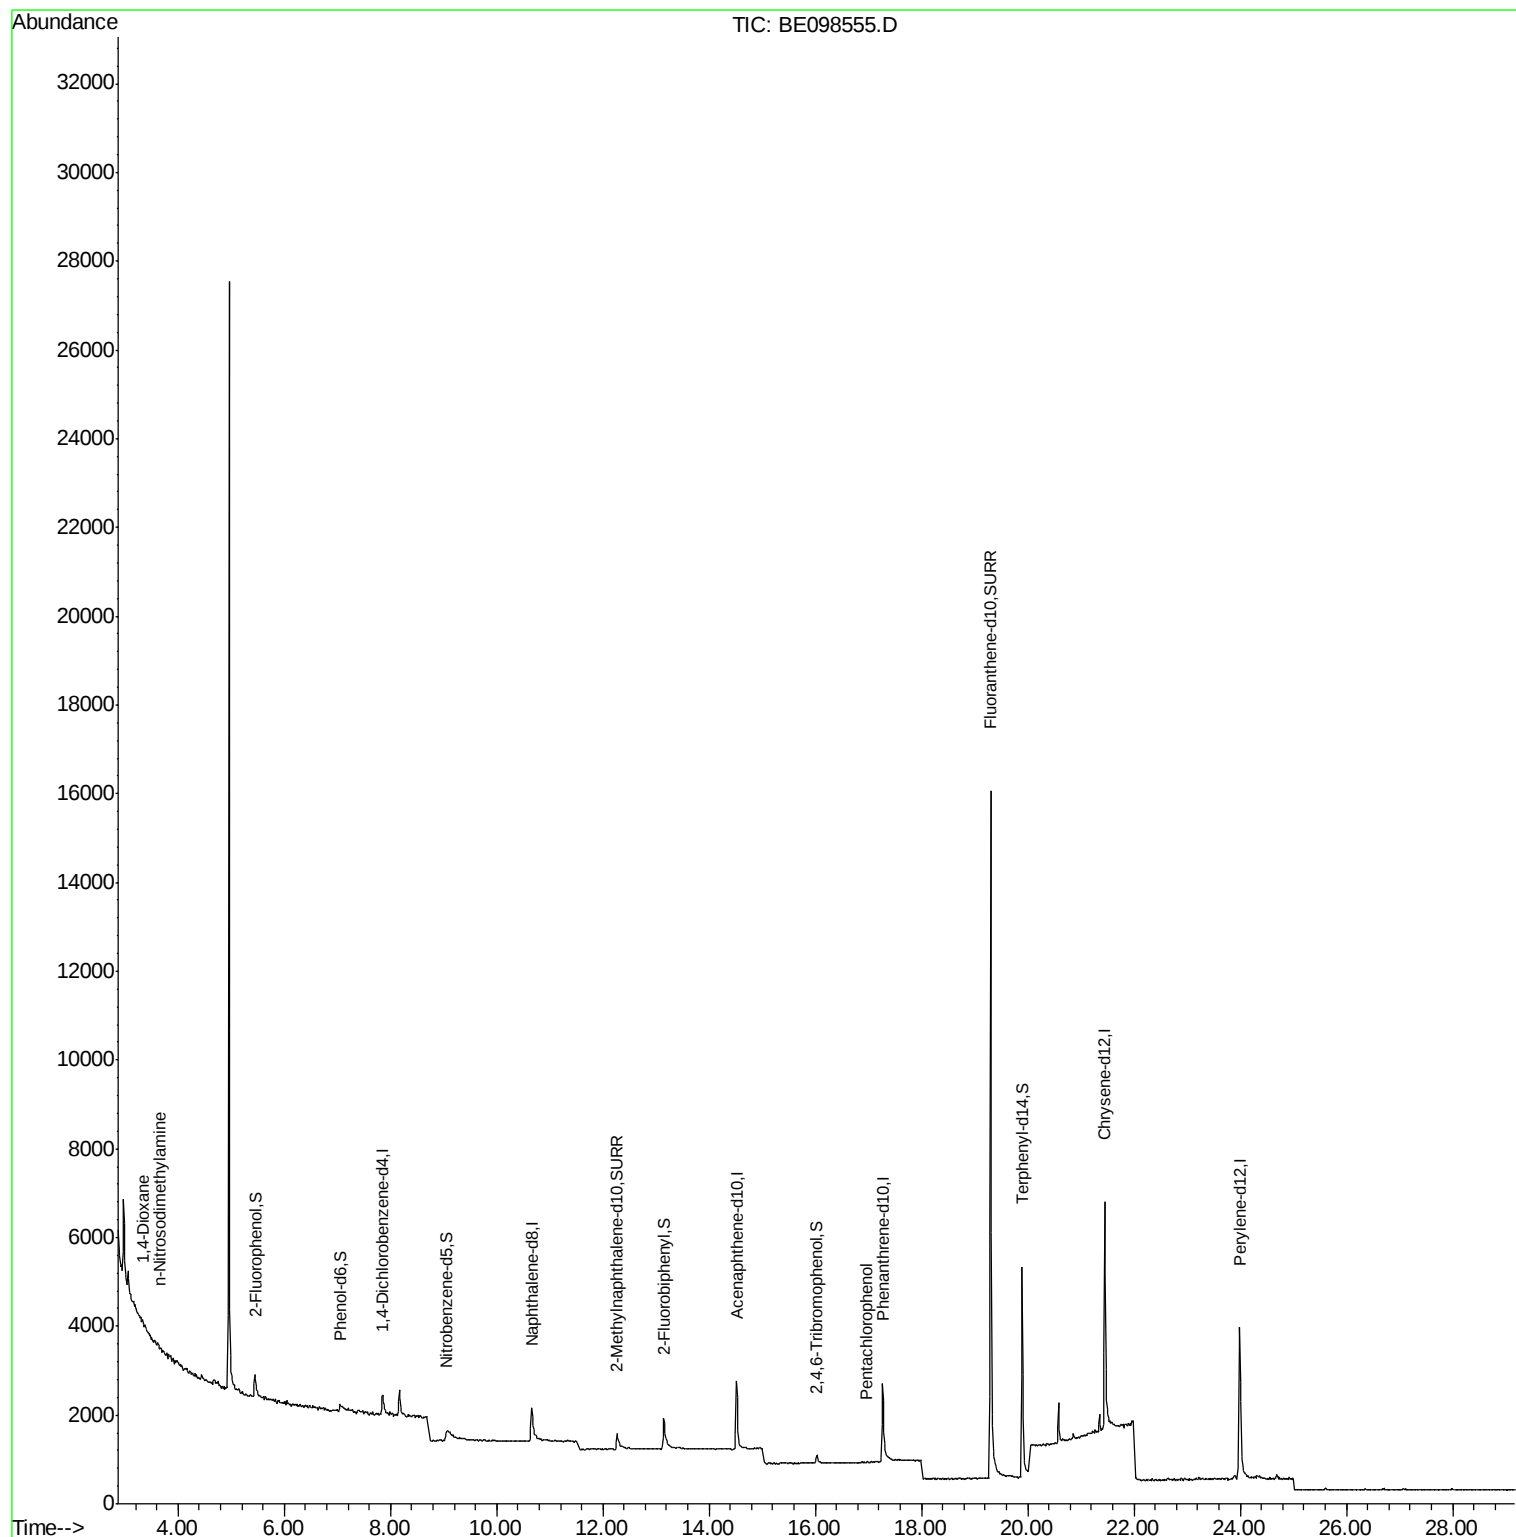

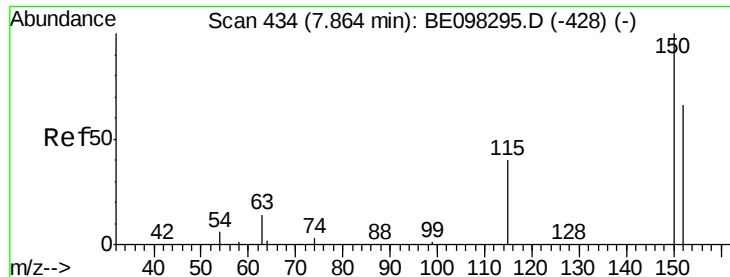


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.86 min Scan# 434
Delta R.T. -0.00 min
Lab File: BE098555.D
Acq: 21 Dec 2018 17:09

Instrument :
BNA_E
ClientSampleId :
PB115910BL

Tgt Ion: 152 Resp: 397
Ion Ratio Lower Upper
152 100
150 143.9 124.2 186.4
115 73.9 53.9 80.9

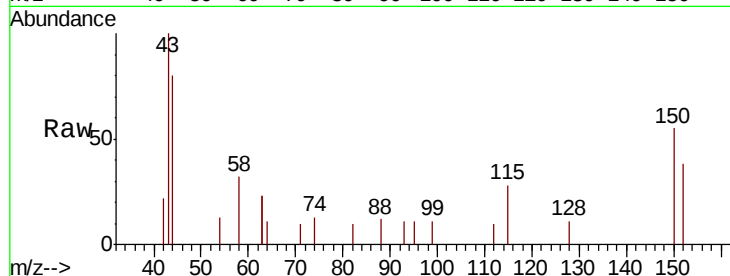


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

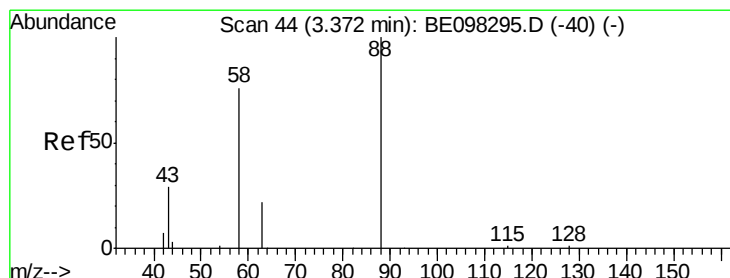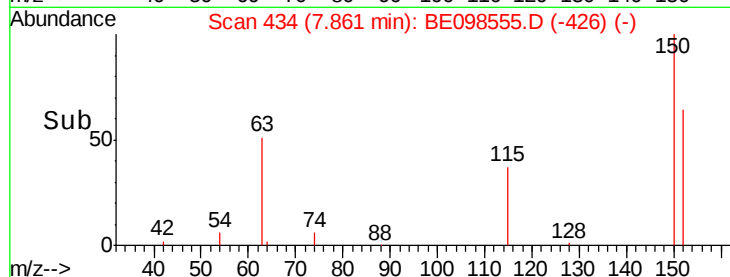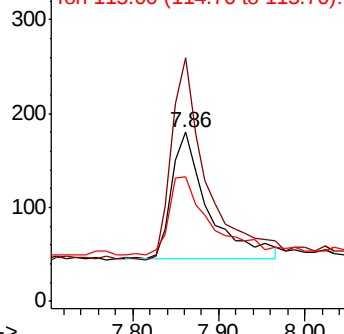



#2


1,4-Dioxane
Concen: 0.031 ng
RT: 3.35 min Scan# 42
Delta R.T. -0.03 min
Lab File: BE098555.D
Acq: 21 Dec 2018 17:09

Tgt Ion: 88 Resp: 21
Ion Ratio Lower Upper
88 100
58 0.0 75.0 112.6#
43 0.0 38.3 57.5#

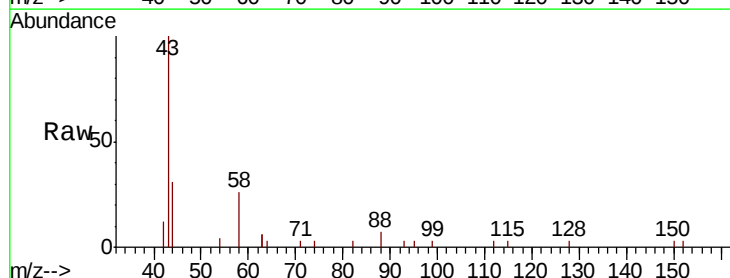

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

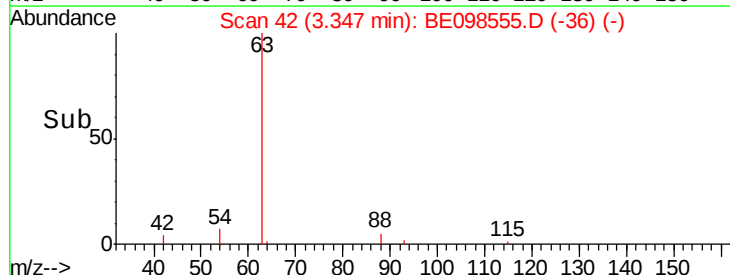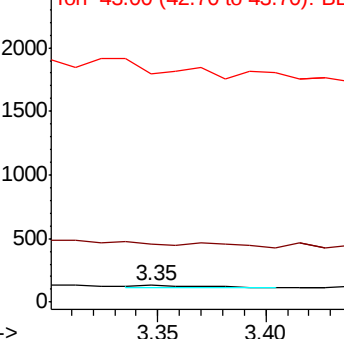

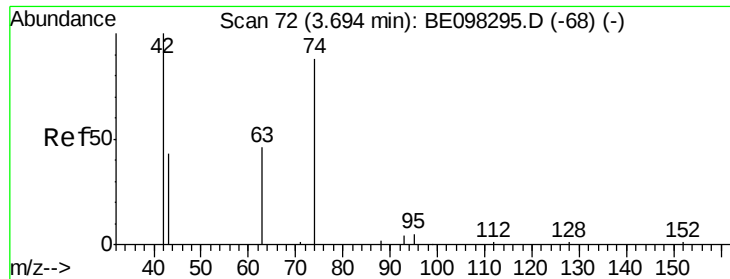

#3

n-Nitrosodimethylamine

Concen: 0.049 ng

RT: 3.67 min Scan# 70

Delta R.T. -0.03 min

Lab File: BE098555.D

Acq: 21 Dec 2018 17:09

Instrument :

BNA_E

ClientSampleId :

PB115910BL


Tgt Ion: 42 Resp: 30

Ion Ratio Lower Upper




42 100

74 0.0 0.0 0.0

44 210.0 0.0 0.0#

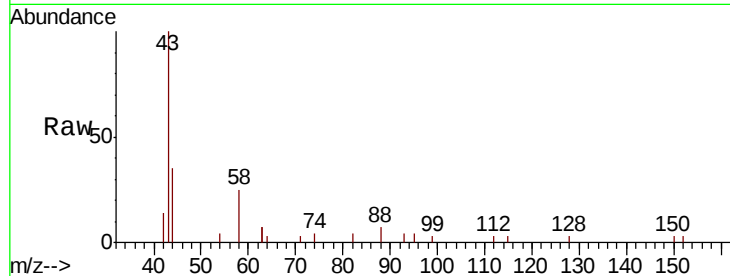

Abundance Ion 42.00 (41.70 to 42.70): BE0
Ion 74.00 (73.70 to 74.70): BE0
Ion 44.00 (43.70 to 44.70): BE0

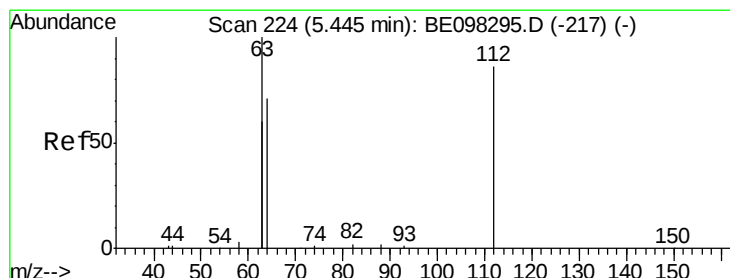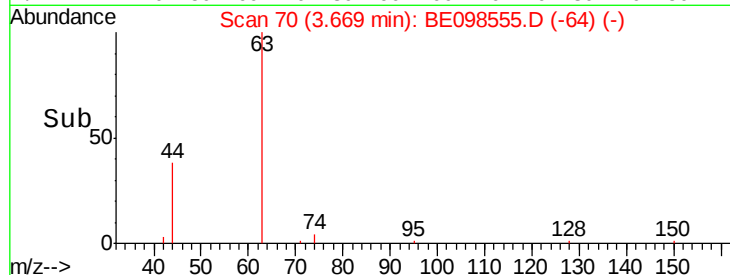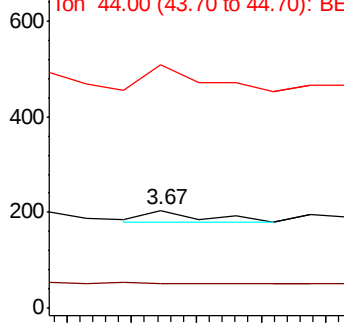

#4

2-Fluorophenol

Concen: 0.432 ng

RT: 5.45 min Scan# 225

Delta R.T. 0.01 min

Lab File: BE098555.D

Acq: 21 Dec 2018 17:09


Tgt Ion: 112 Resp: 401

Ion Ratio Lower Upper



112 100


64 84.5 59.8 89.8

63 177.6 133.7 200.5

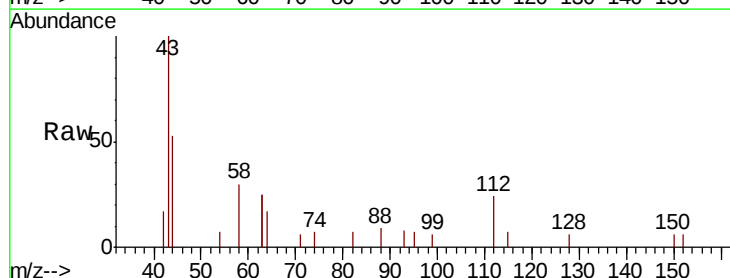

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

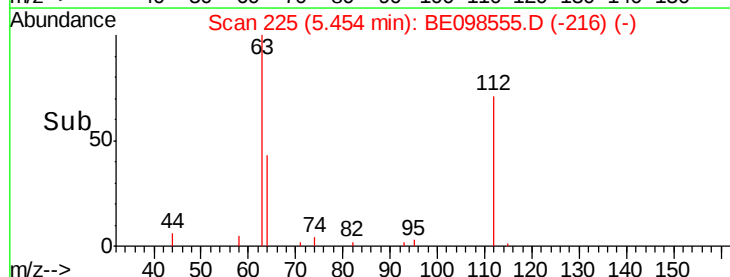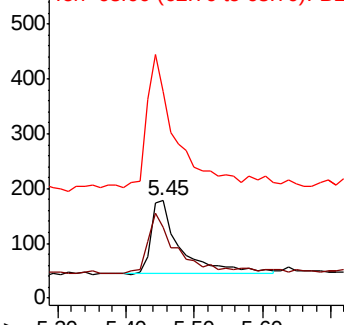

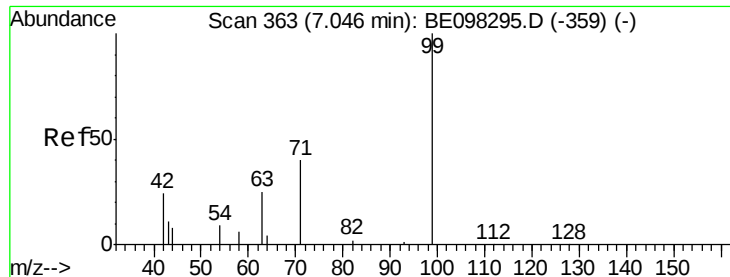

#5

Phenol-d6

Concen: 0.336 ng

RT: 7.06 min Scan# 364

Delta R.T. 0.01 min

Lab File: BE098555.D

Acq: 21 Dec 2018 17:09

Instrument :

BNA_E

ClientSampleId :

PB115910BL


Tgt Ion: 99 Resp: 442

Ion Ratio Lower Upper

99 100

42 35.1 26.3 39.5

71 44.1 33.6 50.4

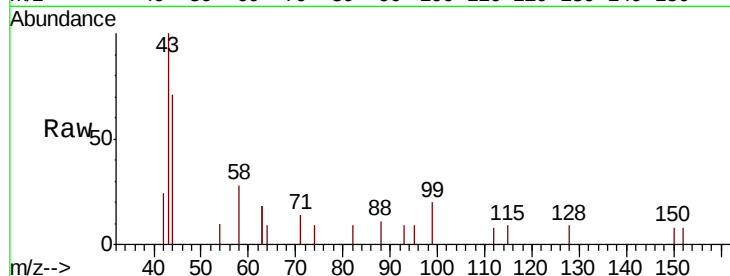


Abundance Ion 99.00 (98.70 to 99.70): BE098295.D (-359) (-)


Ion 42.00 (41.70 to 42.70): BE098295.D (-359) (-)

Ion 71.00 (70.70 to 71.70): BE098295.D (-359) (-)

Time-->

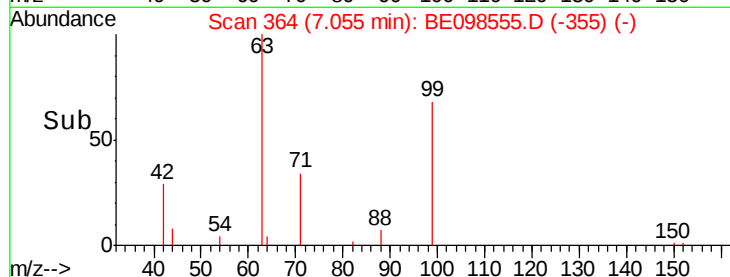

Time-->

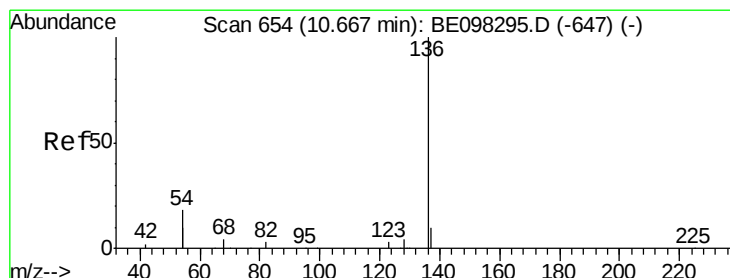

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. -0.00 min

Lab File: BE098555.D

Acq: 21 Dec 2018 17:09

Tgt Ion: 136 Resp: 1666


Ion Ratio Lower Upper

136 100

137 19.1 9.2 13.8#

54 76.1 28.4 42.6#

68 14.1 5.4 8.0#

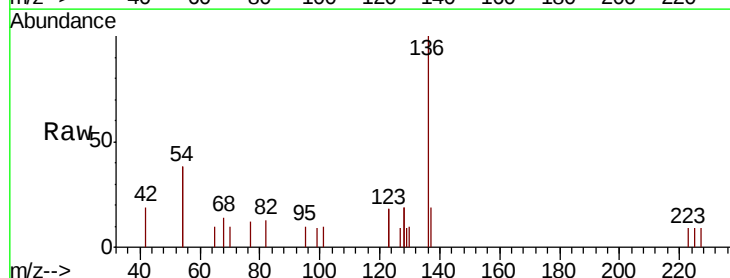


Abundance Ion 136.00 (135.70 to 136.70): BE098295.D (-647) (-)

Ion 137.00 (136.70 to 137.70): BE098295.D (-647) (-)


Ion 54.00 (53.70 to 54.70): BE098295.D (-647) (-)

Ion 68.00 (67.70 to 68.70): BE098295.D (-647) (-)

Time-->

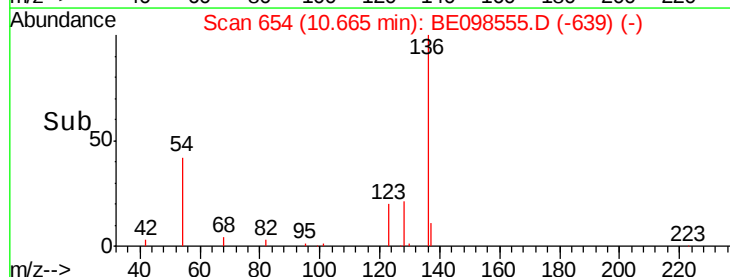





Time-->



#8
 Nitrobenzene-d5
 Concen: 0.222 ng
 RT: 9.07 min Scan# 531
 Delta R.T. 0.05 min
 Lab File: BE098555.D
 Acq: 21 Dec 2018 17:09




Instrument :
 BNA_E
 ClientSampleId :
 PB115910BL


Tgt Ion	Ratio	Lower	Upper
82	100		
128	263.0	102.4	153.6#
54	347.8	221.8	332.8#

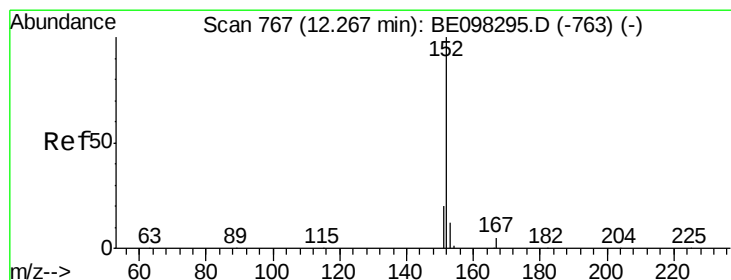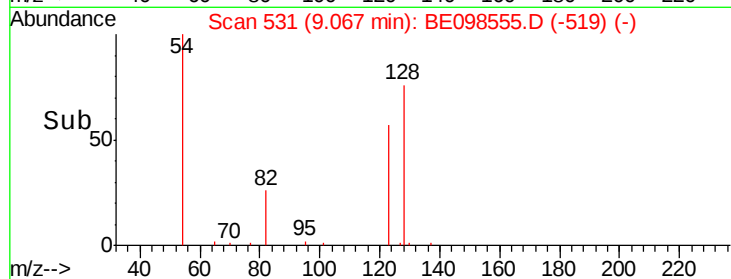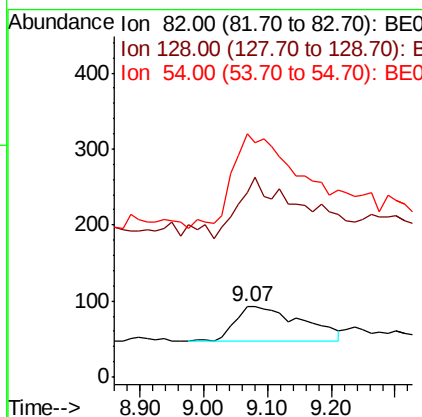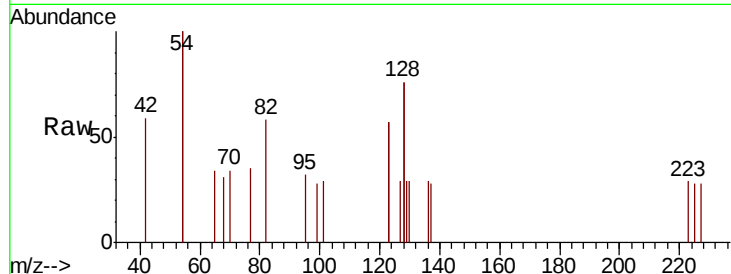

#11
 2-Methylnaphthalene-d10
 Concen: 0.360 ng
 RT: 12.27 min Scan# 767
 Delta R.T. 0.00 min
 Lab File: BE098555.D
 Acq: 21 Dec 2018 17:09

Tgt Ion	Ratio	Lower	Upper
152	100		
151	14.9	16.2	24.4#

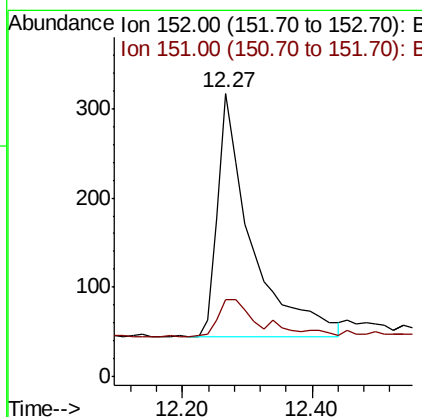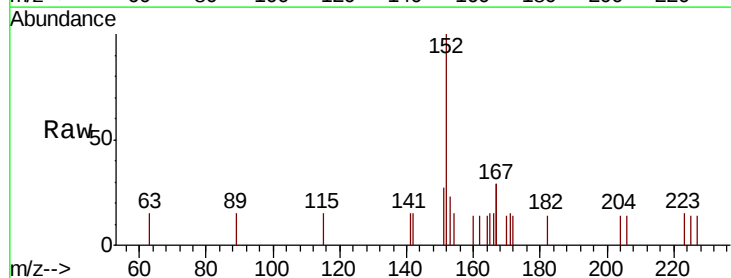


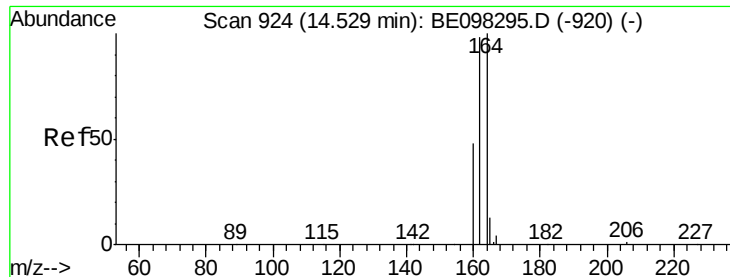




#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.51 min Scan# 923
 Delta R.T. -0.01 min
 Lab File: BE098555.D
 Acq: 21 Dec 2018 17:09

Instrument :
 BNA_E
 ClientSampleId :
 PB115910BL

Tgt Ion:164 Resp: 1268
 Ion Ratio Lower Upper
 164 100
 162 99.0 77.6 116.4
 160 52.7 36.0 54.0

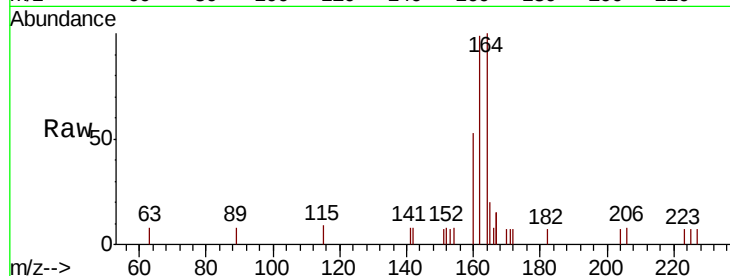


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

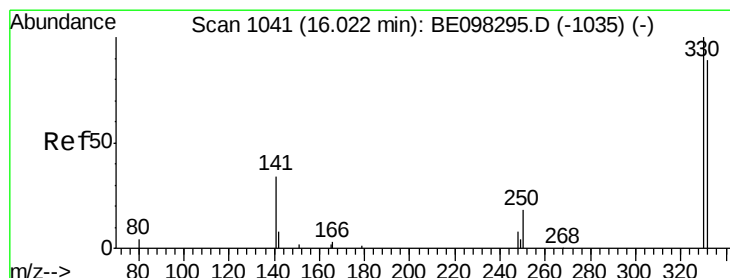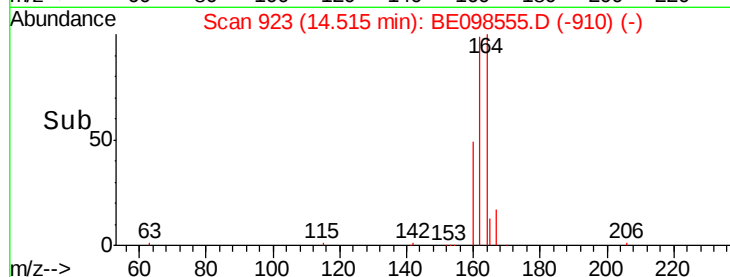
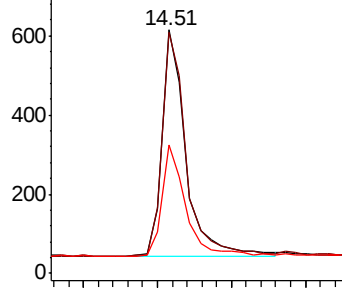



#14
 2,4,6-Tribromophenol
 Concen: 0.440 ng
 RT: 16.02 min Scan# 1041
 Delta R.T. -0.00 min
 Lab File: BE098555.D
 Acq: 21 Dec 2018 17:09

Tgt Ion:330 Resp: 205
 Ion Ratio Lower Upper
 330 100
 332 94.6 76.2 114.4
 141 49.3 39.0 58.4

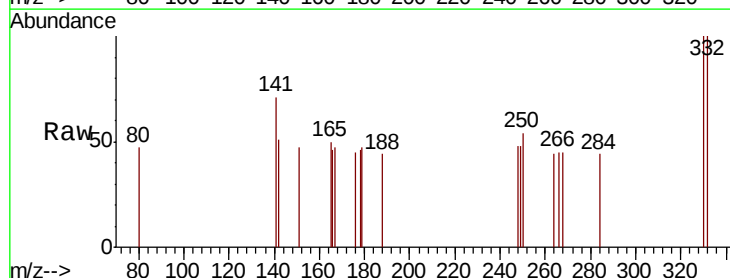

Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

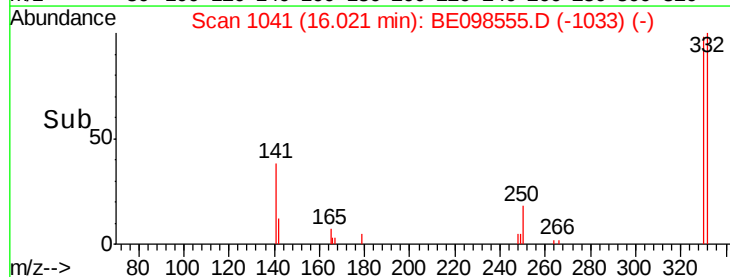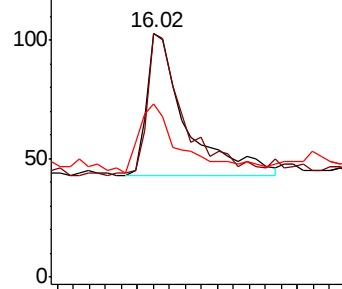


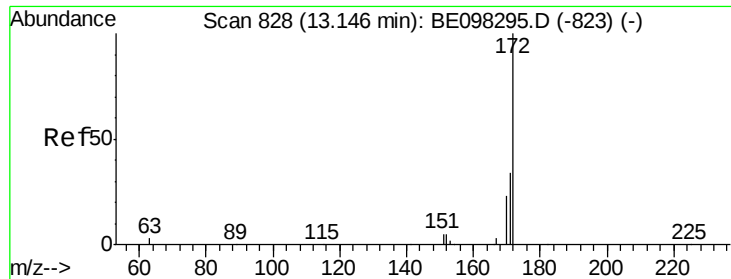




#15
2-Fluorobiphenyl
Concen: 0.286 ng
RT: 13.15 min Scan# 828
Delta R.T. 0.00 min
Lab File: BE098555.D
Acq: 21 Dec 2018 17:09

Instrument :
BNA_E
ClientSampleId :
PB115910BL

Tgt Ion:172 Resp: 1532
Ion Ratio Lower Upper
172 100
171 37.6 27.5 41.3
170 30.4 19.6 29.4#

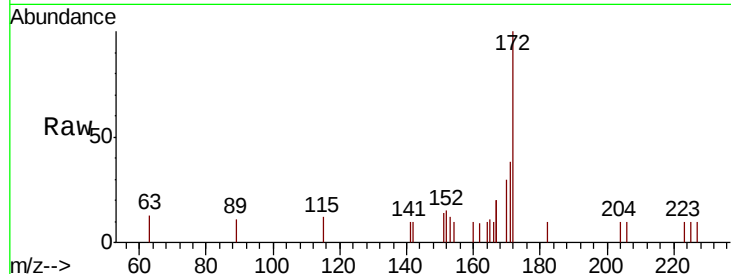


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

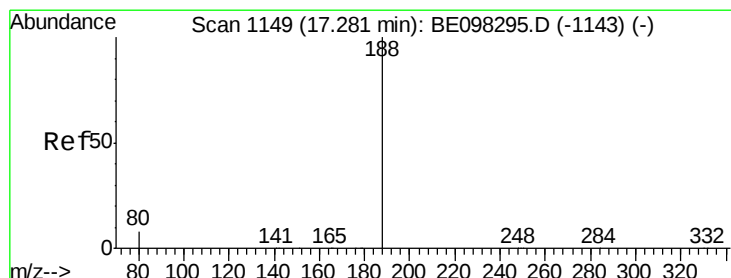
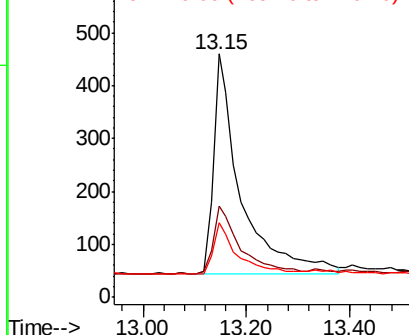



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.27 min Scan# 1148
Delta R.T. -0.01 min
Lab File: BE098555.D
Acq: 21 Dec 2018 17:09

Tgt Ion:188 Resp: 4185
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.7 7.2 10.8#

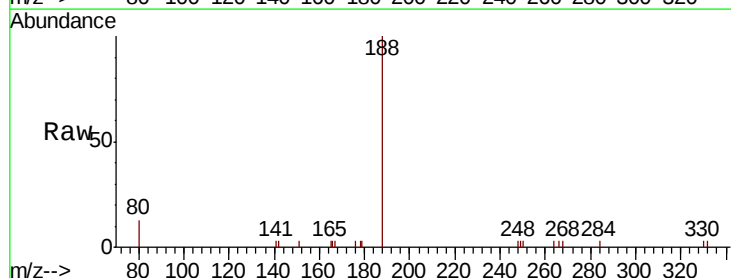

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0




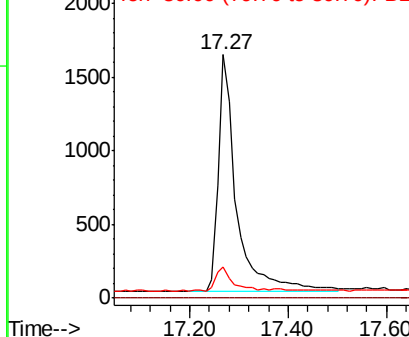




#22
 Pentachlorophenol
 Concen: 0.024 ng
 RT: 16.95 min Scan# 1121
 Delta R.T. 0.01 min
 Lab File: BE098555.D
 Acq: 21 Dec 2018 17:09




Instrument :
 BNA_E
 ClientSampleId :
 PB115910BL


Tgt Ion: 266 Resp: 3
 Ion Ratio Lower Upper
 266 100
 264 95.7 59.0 88.4#
 268 100.0 55.1 82.7#

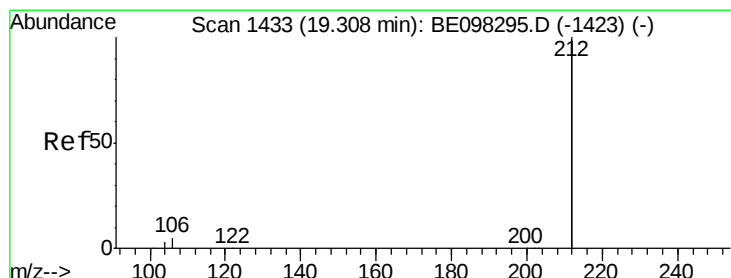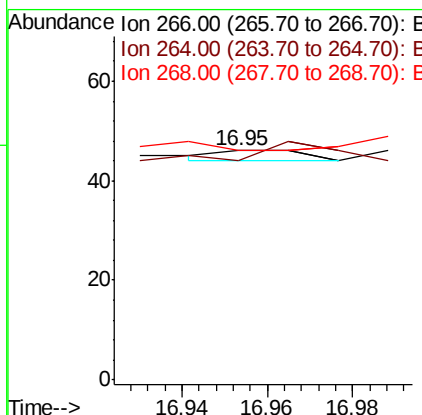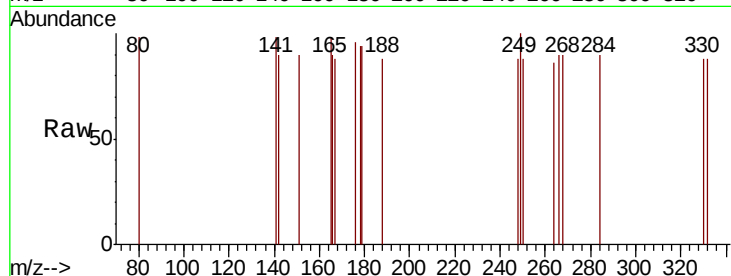

#25
 Fluoranthene-d10
 Concen: 0.498 ng
 RT: 19.30 min Scan# 1431
 Delta R.T. -0.01 min
 Lab File: BE098555.D
 Acq: 21 Dec 2018 17:09

Tgt Ion: 212 Resp: 26756
 Ion Ratio Lower Upper
 212 100
 106 2.2 2.2 3.2
 104 1.4 1.3 1.9



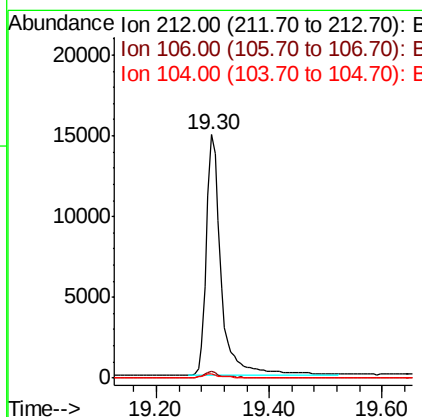
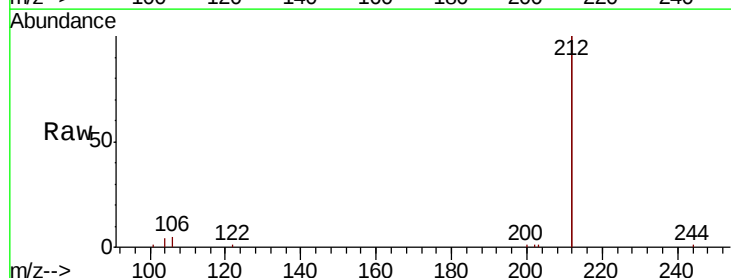




#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.45 min Scan# 1670
Delta R.T. -0.01 min
Lab File: BE098555.D
Acq: 21 Dec 2018 17:09




Instrument :
BNA_E
ClientSampleId :
PB115910BL




Tgt Ion:240 Resp: 7285
Ion Ratio Lower Upper
240 100
120 9.3 9.5 14.3#
236 26.9 22.7 34.1

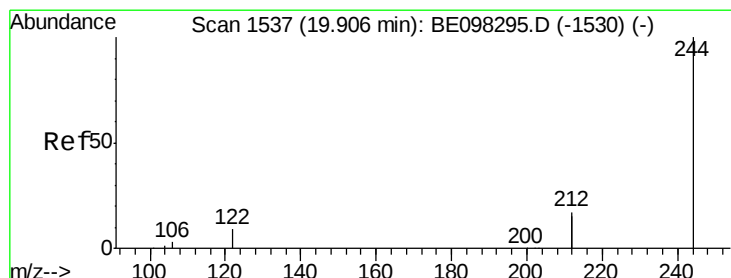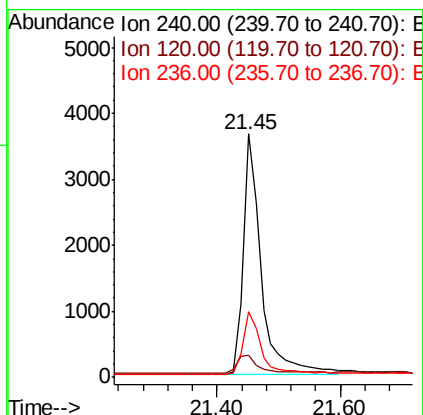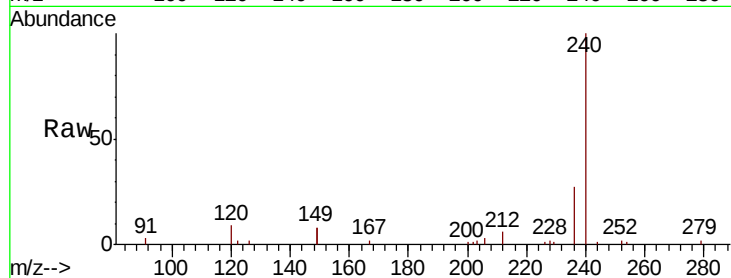

#29
Terphenyl-d14
Concen: 0.313 ng
RT: 19.90 min Scan# 1535
Delta R.T. -0.01 min
Lab File: BE098555.D
Acq: 21 Dec 2018 17:09

Tgt Ion:244 Resp: 5540
Ion Ratio Lower Upper
244 100
212 36.7 27.4 41.0
122 9.7 8.3 12.5

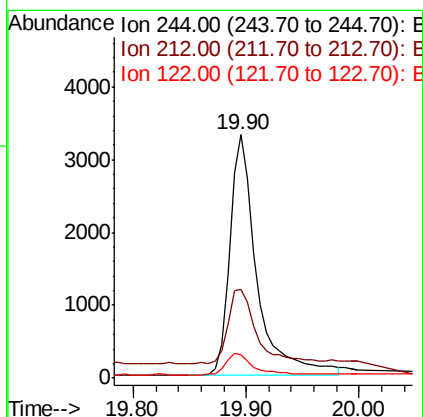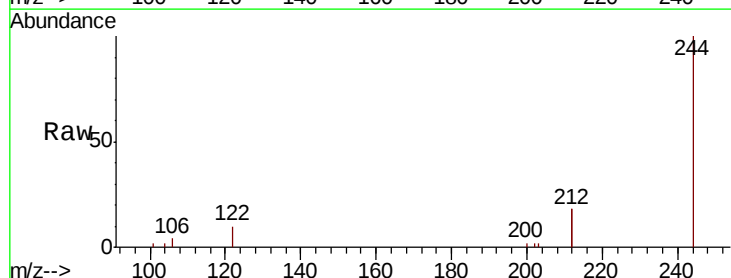

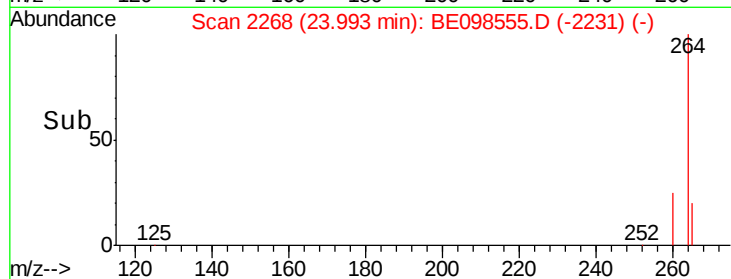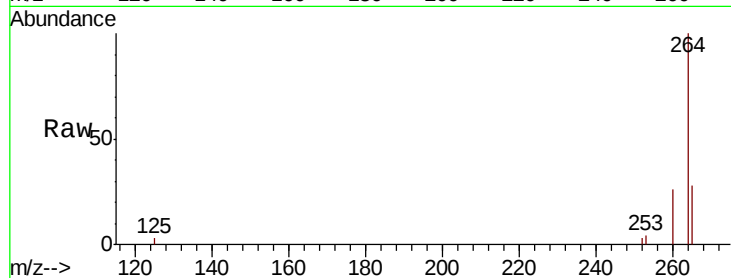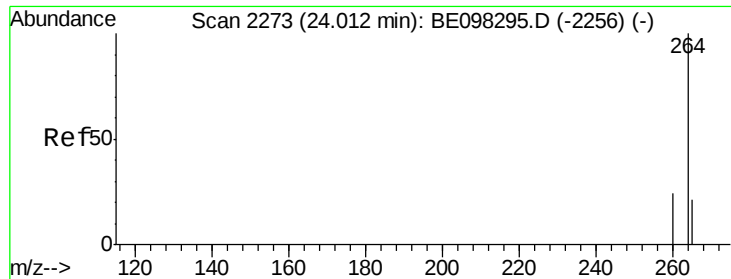

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.99 min Scan# 2268

Delta R.T. -0.02 min

Lab File: BE098555.D

Acq: 21 Dec 2018 17:09

Instrument :

BNA_E

ClientSampleId :

PB115910BL

Tgt Ion: 264 Resp: 6335

Ion Ratio Lower Upper

264 100

260 26.1 20.2 30.2

265 28.4 25.2 37.8

