

Data File : BE098573.D
Acq On : 28 Dec 2018 14:21
Operator : SJ/JU
Sample : PB115945BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK45

Quant Time: Dec 29 00:16:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	1045	0.40	ng/ul	0.00
2) Naphthalene-d8	10.61	136	4689	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	3268	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.33	188	703989	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.93	264	13878	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	2670	0.35	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.47	166	1104	0.084	ng/ul#	14
23) Benzo(a)pyrene	23.76	252	3215	0.078	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE098573.D
Acq On : 28 Dec 2018 14:21
Operator : SJ/JU
Sample : PB115945BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK45

Quant Time: Dec 29 00:16:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration




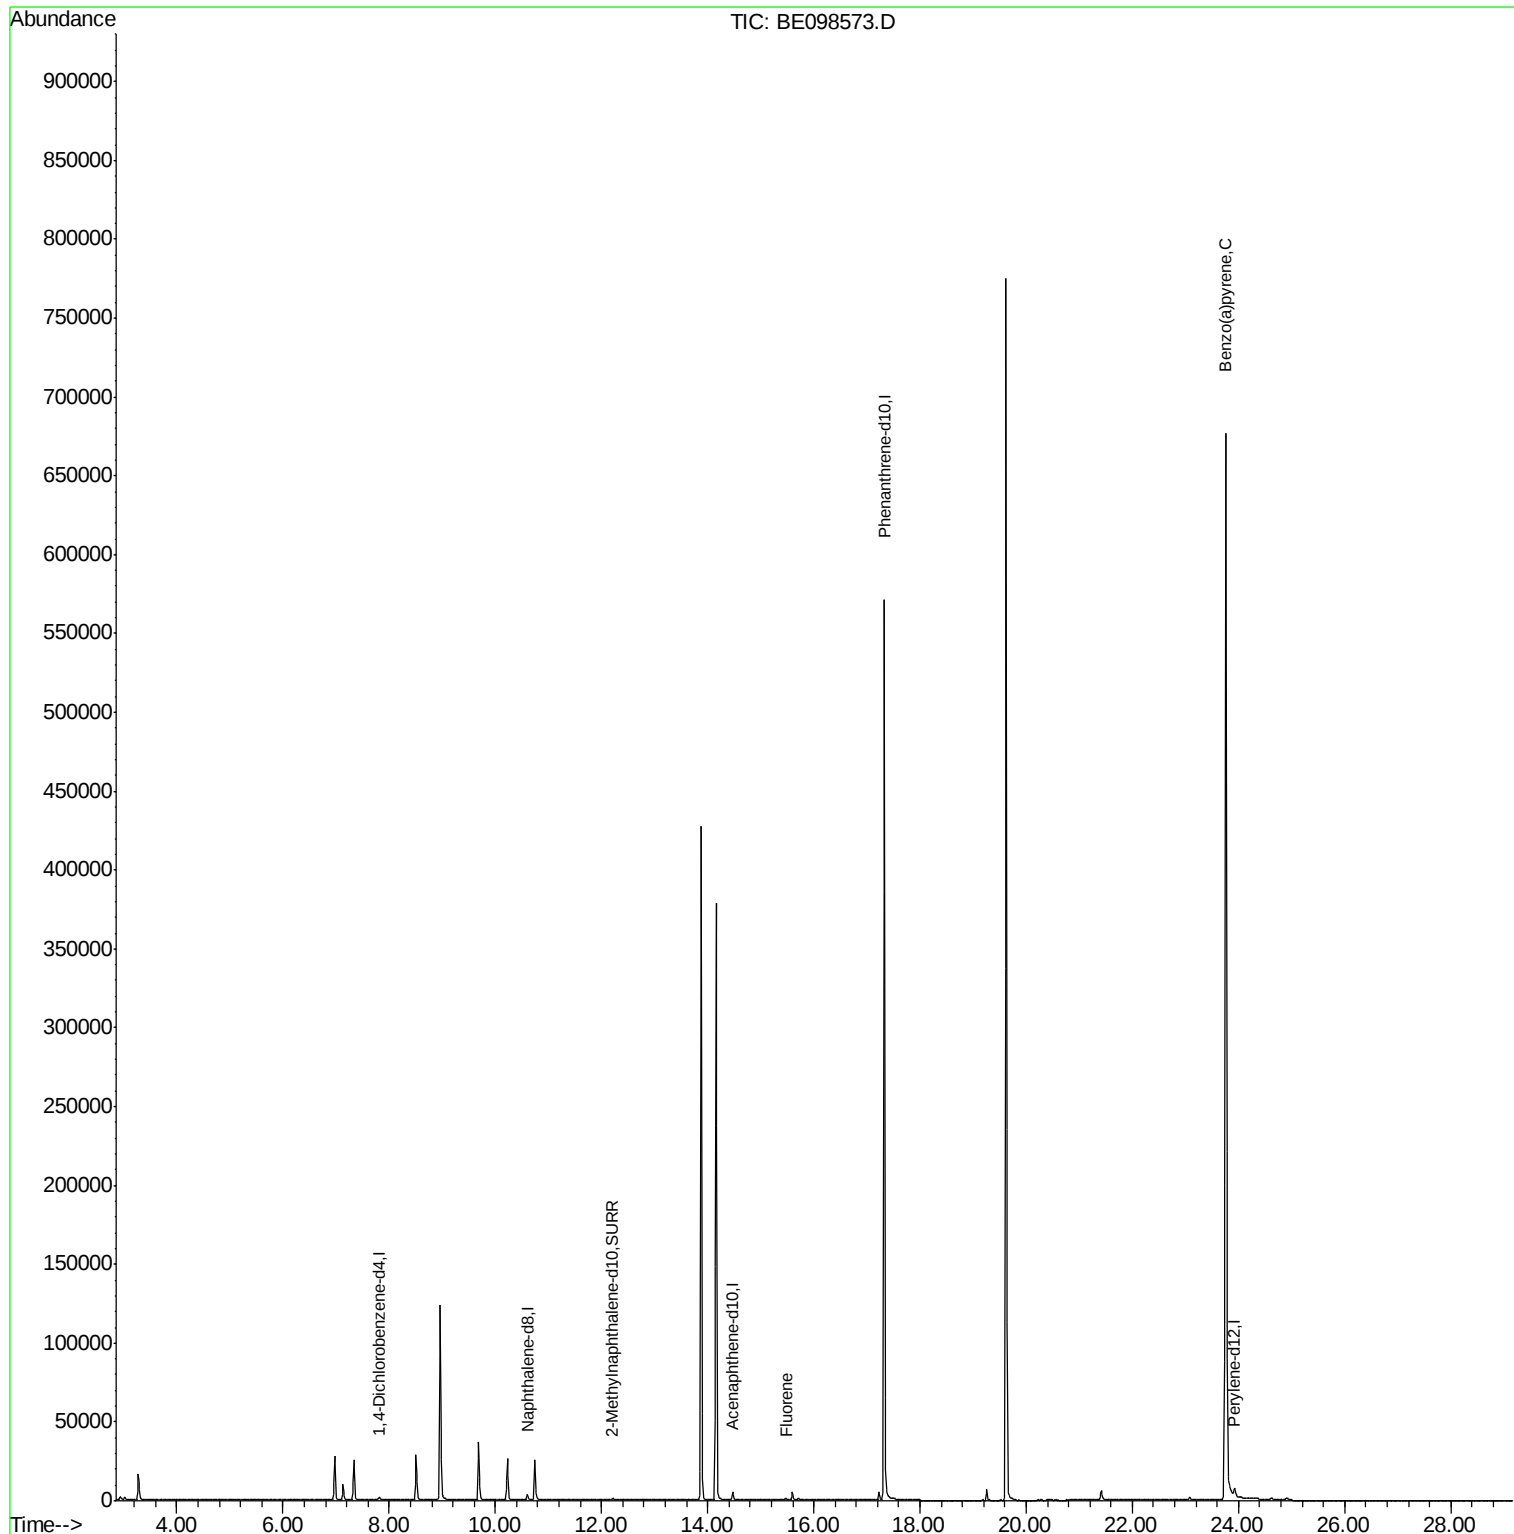


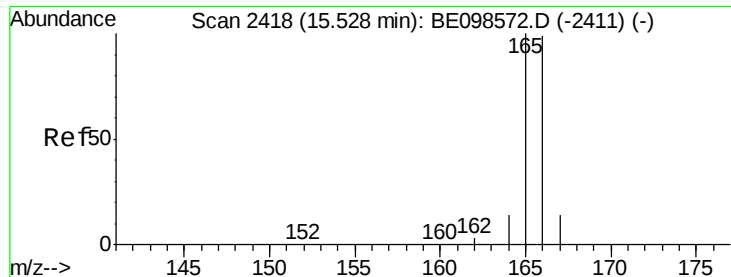

#9
Fluorene
 Concen: 0.084 ng/ul
 RT: 15.47 min Scan# 2410
 Delta R.T. -0.06 min
 Lab File: BE098573.D
 Acq: 28 Dec 2018 14:21

Instrument :
 BNA_E
 ClientSampleId :
 SBLK45

Tgt Ion:166 Resp: 1104
 Ion Ratio Lower Upper
 166 100
 165 9.5 80.2 120.4#
 167 37.0 12.0 18.0#

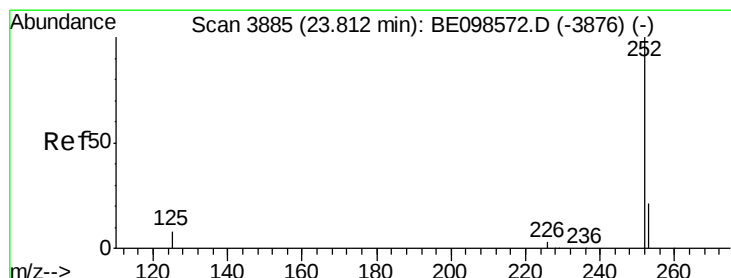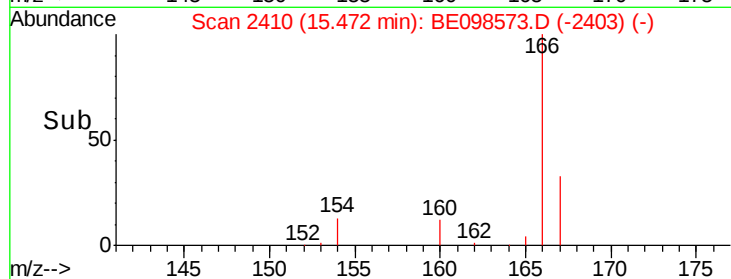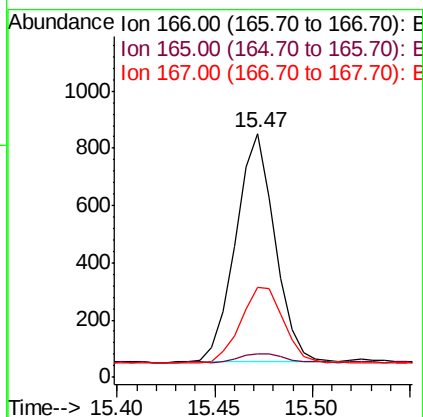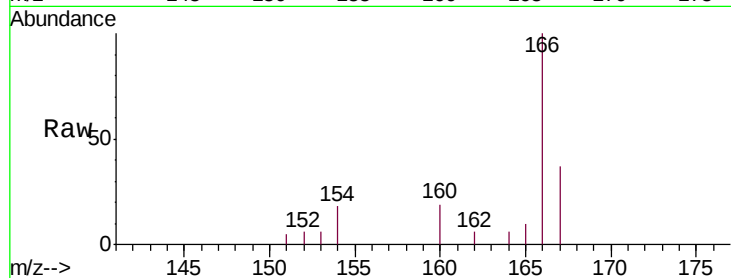

#23
Benzo(a)pyrene
 Concen: 0.078 ng/ul
 RT: 23.76 min Scan# 3880
 Delta R.T. -0.05 min
 Lab File: BE098573.D
 Acq: 28 Dec 2018 14:21

Tgt Ion:252 Resp: 3215
 Ion Ratio Lower Upper
 252 100
 253 31.5 19.4 29.2#
 125 20.0 7.8 11.8#

