

Data File : BE098575.D
Acq On : 28 Dec 2018 15:35
Operator : SJ/JU
Sample : PB115951BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK51

Quant Time: Dec 29 00:17:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	1100	0.40	ng/ul	0.00
2) Naphthalene-d8	10.60	136	4845	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	3437	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	718422	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.93	264	14263	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	2908	0.37	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.47	166	1165	0.085	ng/ul#	14
23) Benzo(a)pyrene	23.76	252	3425	0.081	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE098575.D
Acq On : 28 Dec 2018 15:35
Operator : SJ/JU
Sample : PB115951BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK51

Quant Time: Dec 29 00:17:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration




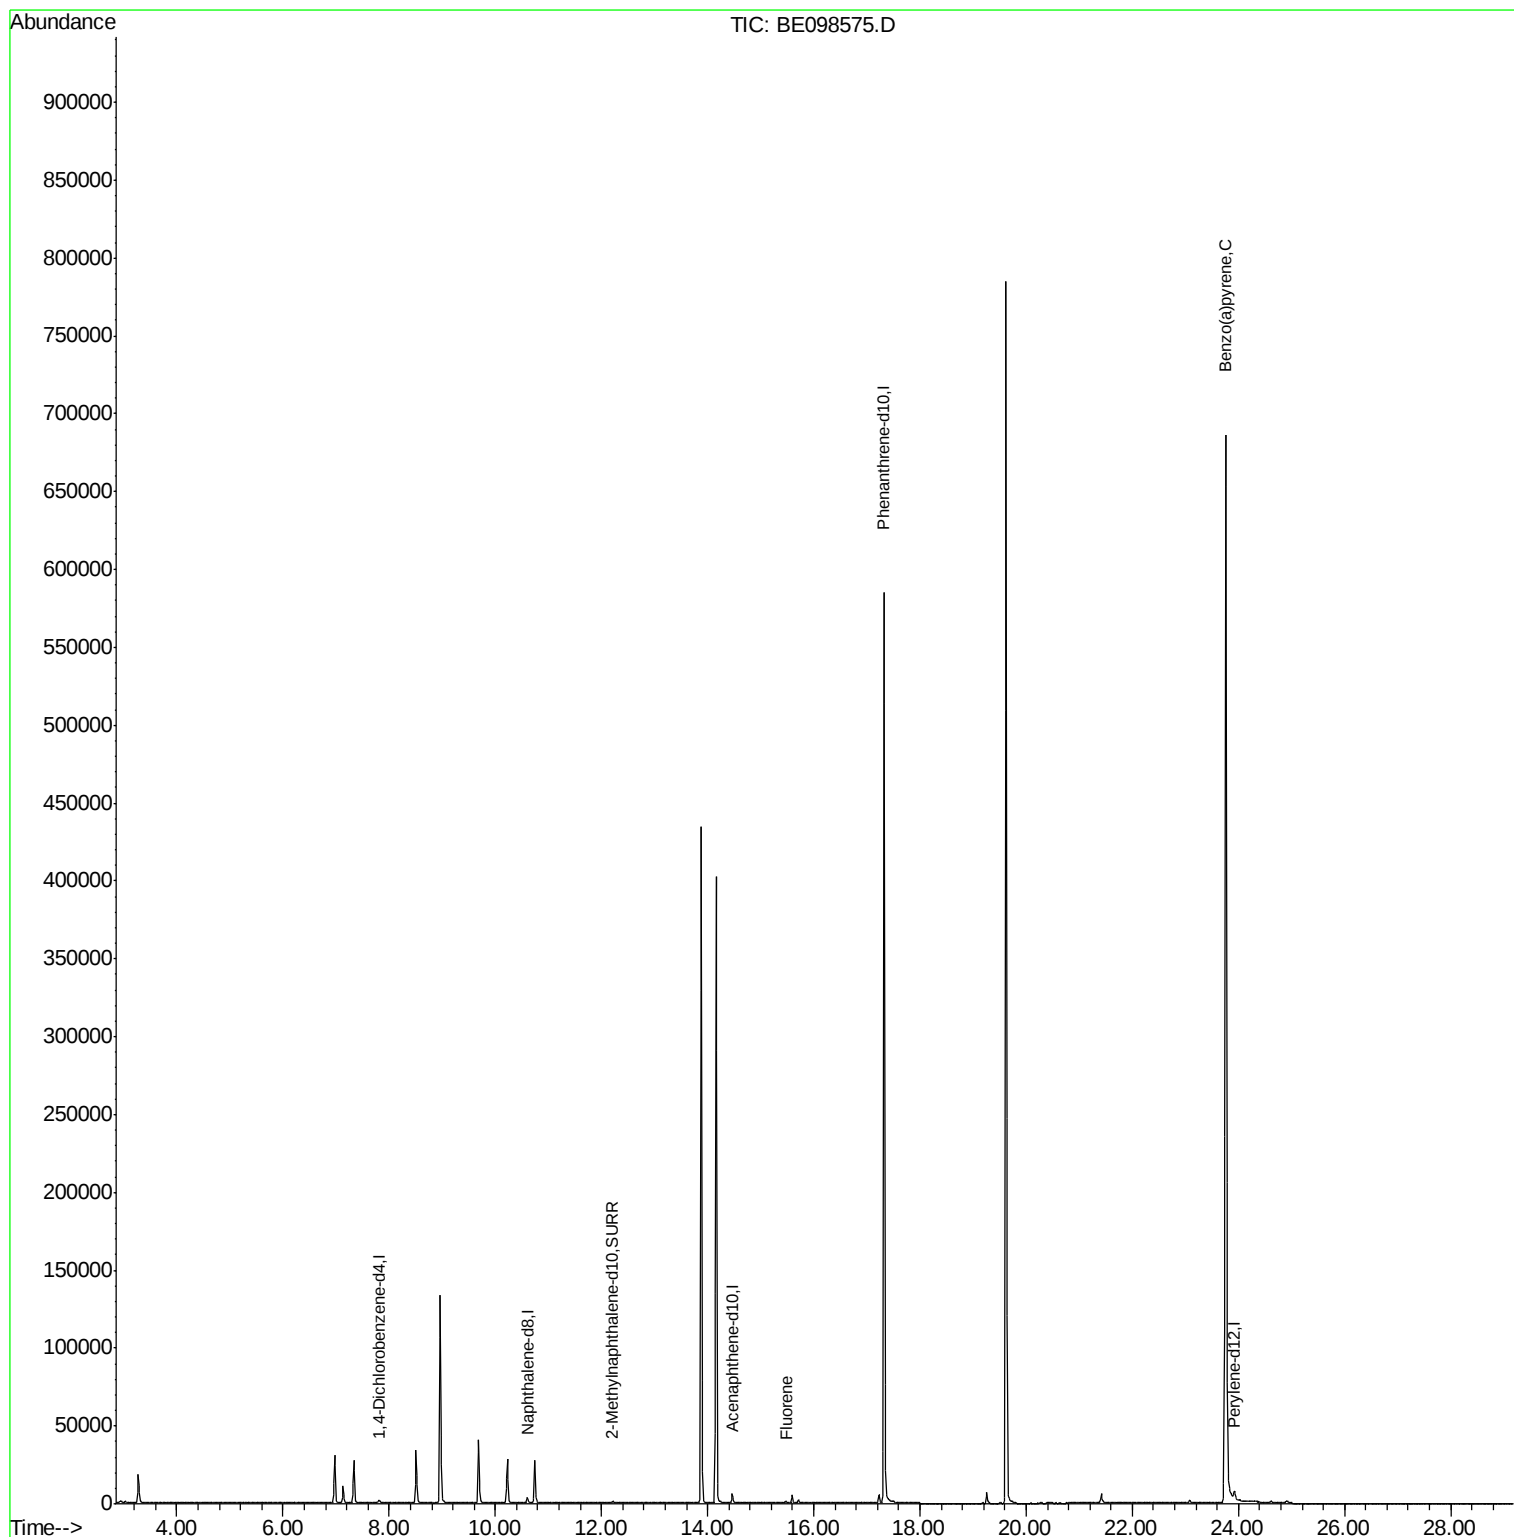


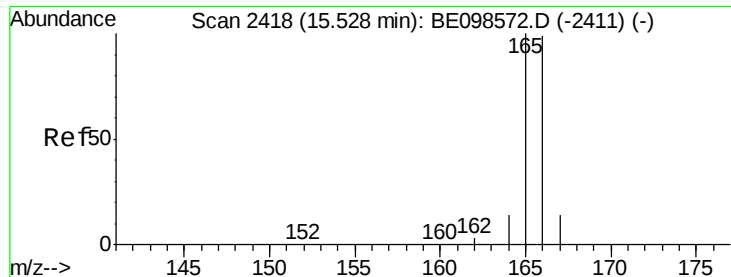

#9
Fluorene
 Concen: 0.085 ng/ul
 RT: 15.47 min Scan# 2409
 Delta R.T. -0.06 min
 Lab File: BE098575.D
 Acq: 28 Dec 2018 15:35

Instrument :
 BNA_E
 ClientSampleId :
 SBLK51

Tgt Ion:166 Resp: 1165
 Ion Ratio Lower Upper
 166 100
 165 9.9 80.2 120.4#
 167 38.3 12.0 18.0#

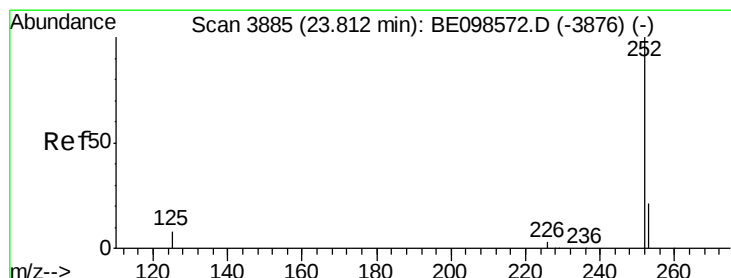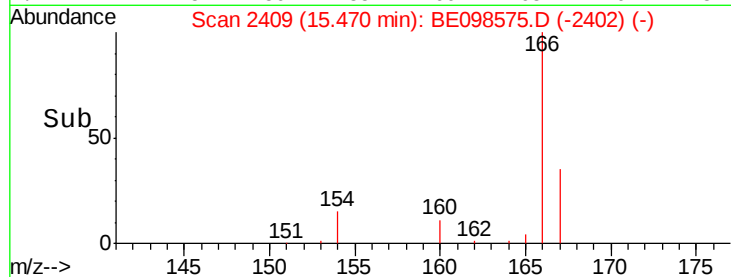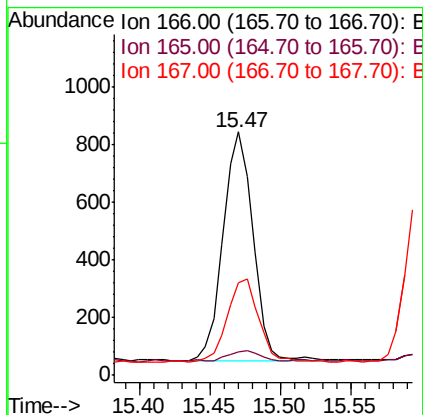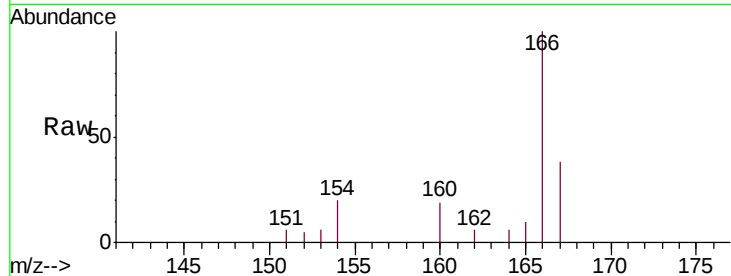

#23
Benzo(a)pyrene
 Concen: 0.081 ng/ul
 RT: 23.76 min Scan# 3880
 Delta R.T. -0.05 min
 Lab File: BE098575.D
 Acq: 28 Dec 2018 15:35

Tgt Ion:252 Resp: 3425
 Ion Ratio Lower Upper
 252 100
 253 31.7 19.4 29.2#
 125 21.4 7.8 11.8#

