

Data File : BE098578.D
Acq On : 28 Dec 2018 17:26
Operator : SJ/JU
Sample : J6489-18
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F9F60

Quant Time: Dec 29 00:17:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	1090	0.40	ng/ul	0.00
2) Naphthalene-d8	10.61	136	4789	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	3440	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	652159	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.92	264	14372	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	2577	0.33	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.47	166	1055	0.077	ng/ul#	15
23) Benzo(a)pyrene	23.76	252	2962	0.069	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE098578.D
Acq On : 28 Dec 2018 17:26
Operator : SJ/JU
Sample : J6489-18
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F9F60

Quant Time: Dec 29 00:17:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration

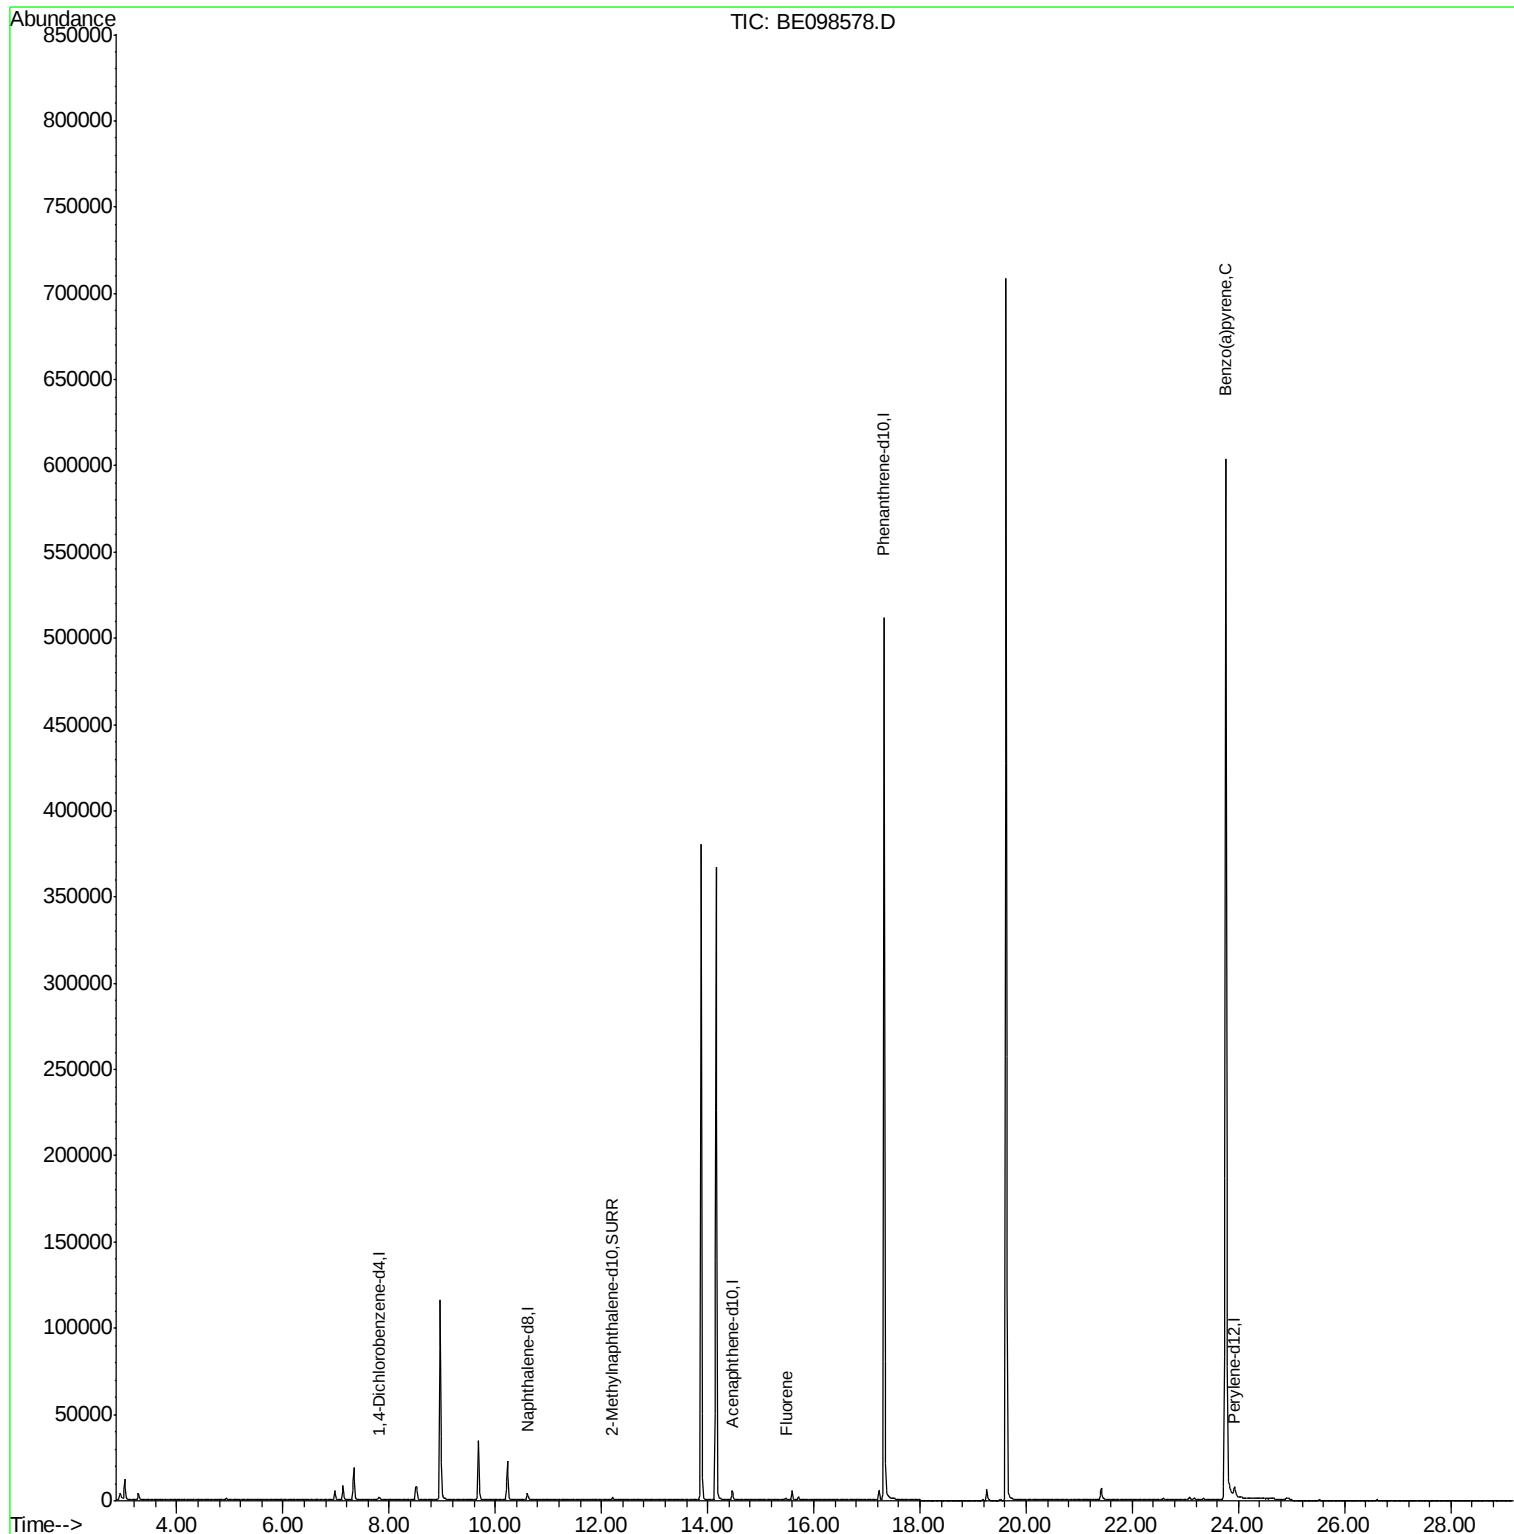

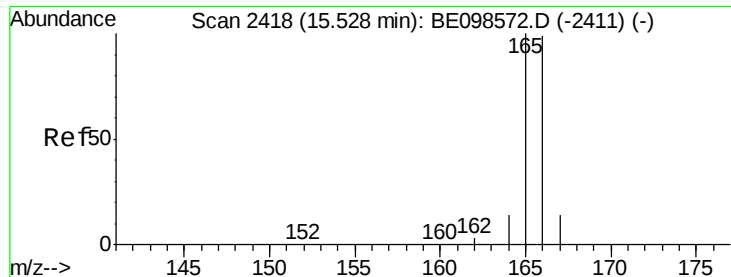

#9

Fluorene

Concen: 0.077 ng/ul

RT: 15.47 min Scan# 2409

Delta R.T. -0.06 min

Lab File: BE098578.D

Acq: 28 Dec 2018 17:26

Instrument :

BNA_E

ClientSampled :

F9F60





Tgt Ion:166 Resp: 1055

Ion Ratio Lower Upper

166 100

165 9.6 80.2 120.4#

167 36.6 12.0 18.0#

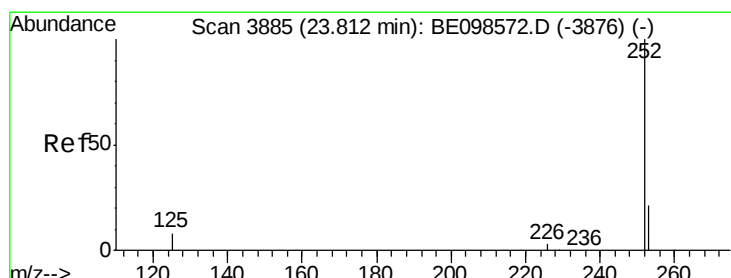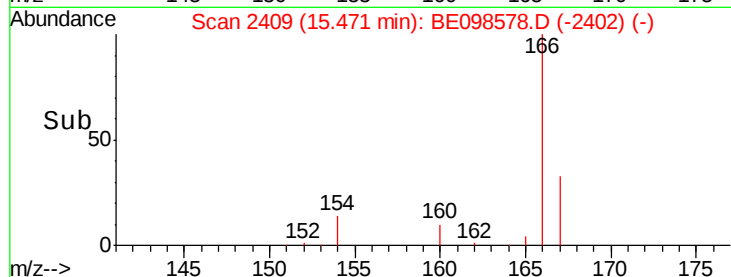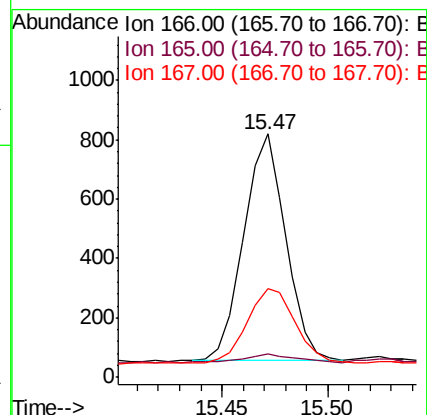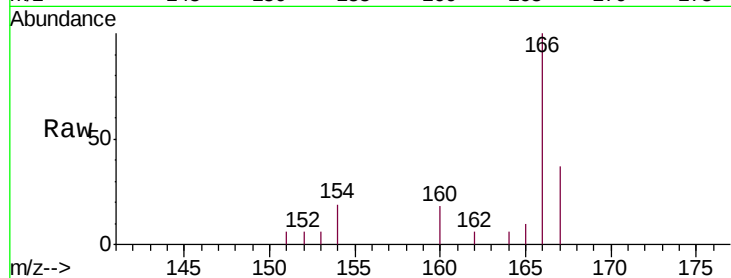

#23

Benzo(a)pyrene

Concen: 0.069 ng/ul

RT: 23.76 min Scan# 3879

Delta R.T. -0.05 min

Lab File: BE098578.D

Acq: 28 Dec 2018 17:26

Tgt Ion:252 Resp: 2962

Ion Ratio Lower Upper

252 100

253 32.4 19.4 29.2#

125 21.5 7.8 11.8#

