

Data File : BE098579.D
Acq On : 28 Dec 2018 18:05
Operator : SJ/JU
Sample : J6489-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F9F88

Quant Time: Dec 29 00:17:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	1052	0.40	ng/ul	0.00
2) Naphthalene-d8	10.60	136	4783	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	3481	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	618626	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.92	264	14039	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	2460	0.32	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.47	166	989	0.071	ng/ul#	16
23) Benzo(a)pyrene	23.76	252	2823	0.067	ng/ul#	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE098579.D

Acq On : 28 Dec 2018 18:05

Operator : SJ/JU

Sample : J6489-19

Misc :

ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F9F88


Quant Time: Dec 29 00:17:32 2018


Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Dec 29 00:05:35 2018

Response via : Initial Calibration




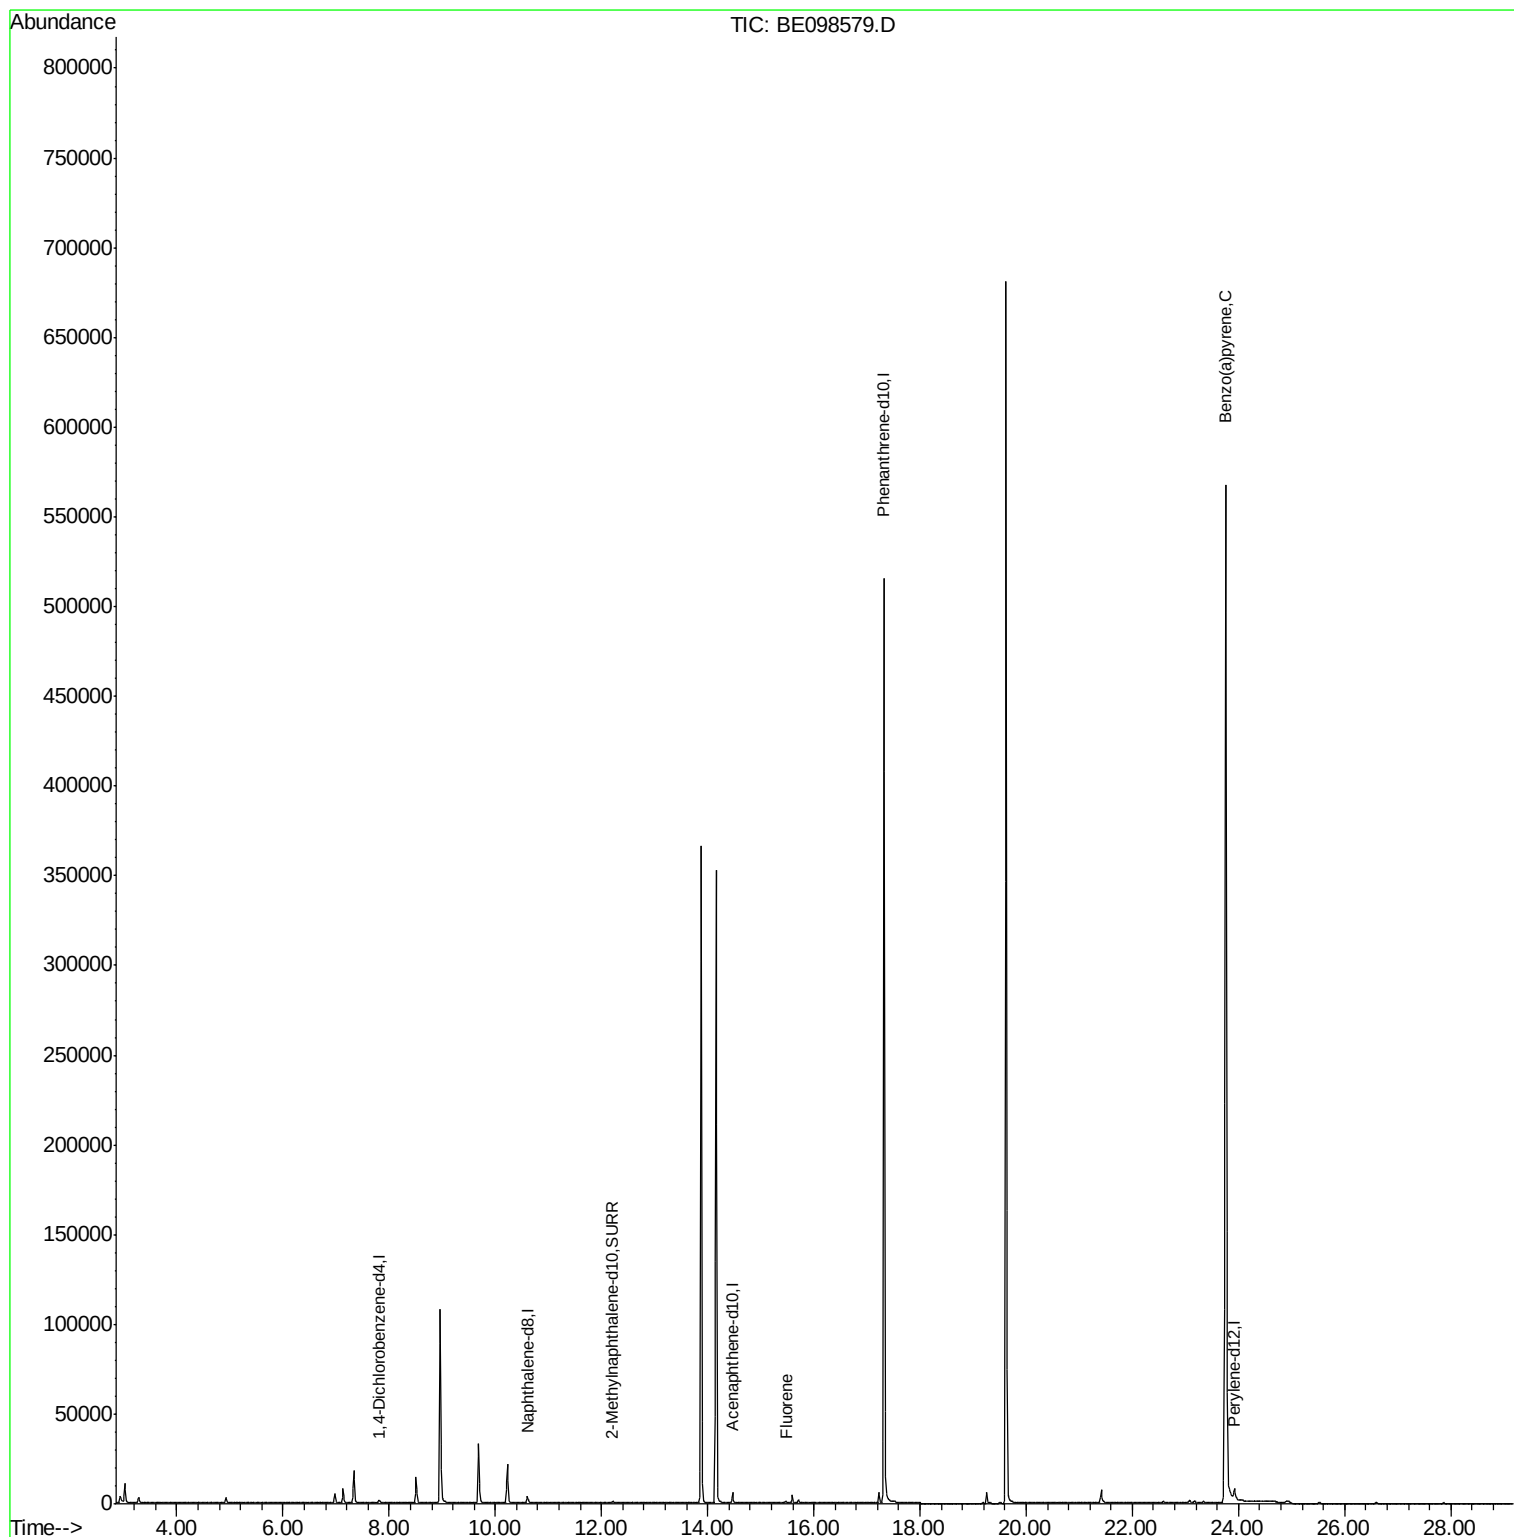


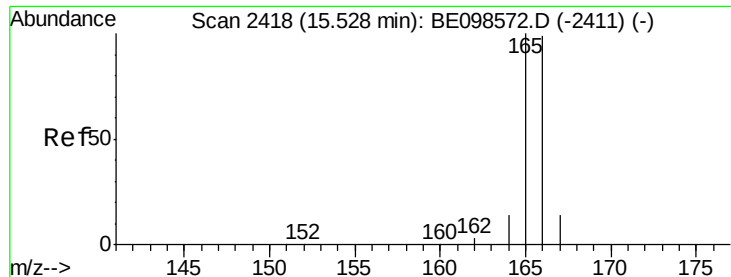

#9
Fluorene
 Concen: 0.071 ng/ul
 RT: 15.47 min Scan# 2409
 Delta R.T. -0.06 min
 Lab File: BE098579.D
 Acq: 28 Dec 2018 18:05

Instrument :
 BNA_E
 ClientSampleId :
 F9F88

Tgt Ion:166 Resp: 989
 Ion Ratio Lower Upper
 166 100
 165 12.8 80.2 120.4#
 167 39.6 12.0 18.0#

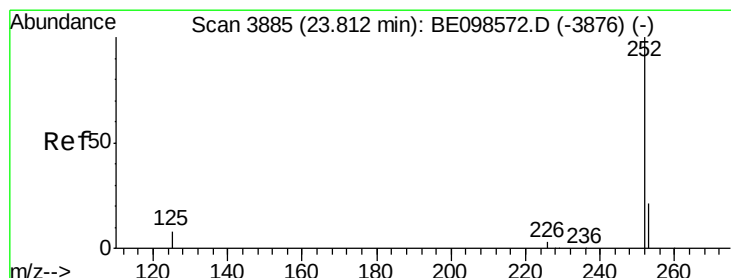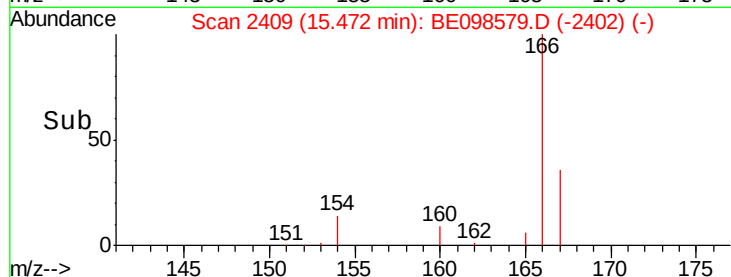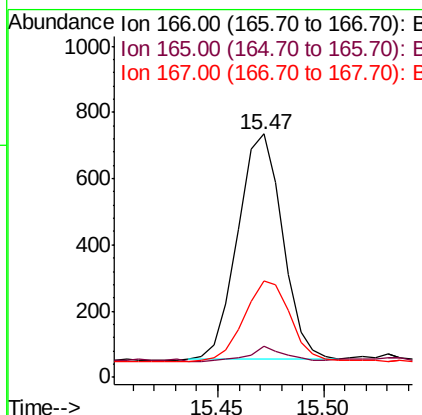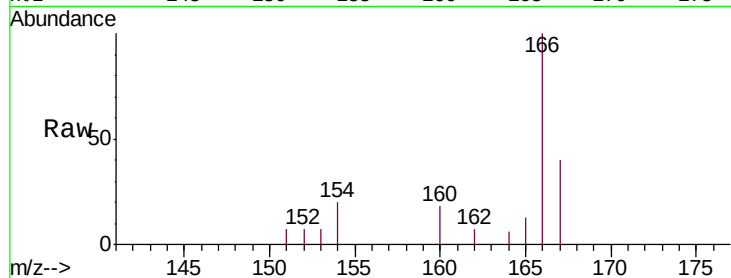

#23
Benzo(a)pyrene
 Concen: 0.067 ng/ul
 RT: 23.76 min Scan# 3879
 Delta R.T. -0.05 min
 Lab File: BE098579.D
 Acq: 28 Dec 2018 18:05

Tgt Ion:252 Resp: 2823
 Ion Ratio Lower Upper
 252 100
 253 33.6 19.4 29.2#
 125 21.7 7.8 11.8#

