

Data File : BE098582.D
Acq On : 28 Dec 2018 19:55
Operator : SJ/JU
Sample : J6489-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F9F56

Quant Time: Dec 29 00:17:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	1147	0.40	ng/ul	0.00
2) Naphthalene-d8	10.60	136	4972	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	3548	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.33	188	472679	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.92	264	12363	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.20	152	2078	0.26	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.65	128	739	0.055	ng/ul#	70
5) 2-Methylnaphthalene	12.28	142	644	0.075	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE098582.D
Acq On : 28 Dec 2018 19:55
Operator : SJ/JU
Sample : J6489-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F9F56

Quant Time: Dec 29 00:17:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration

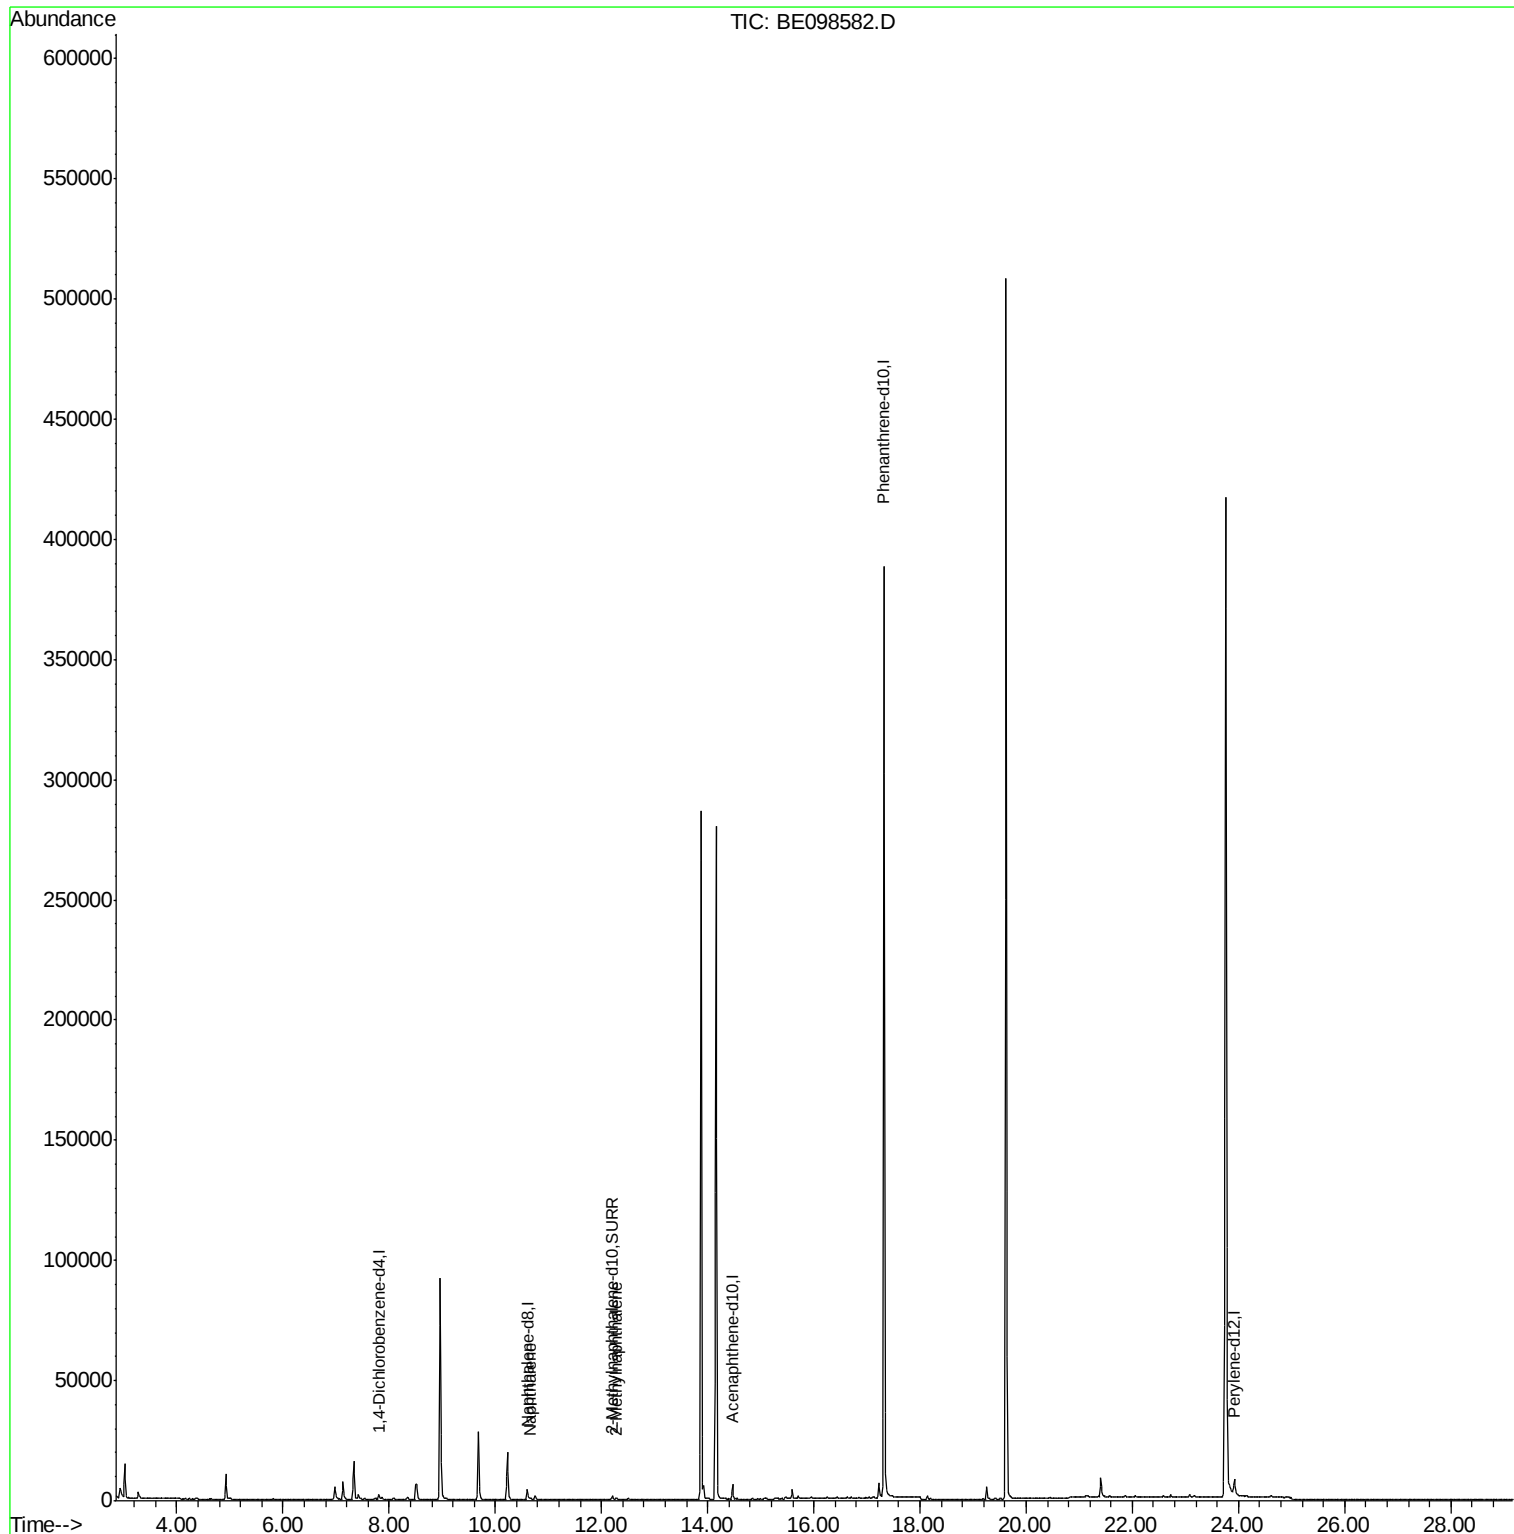

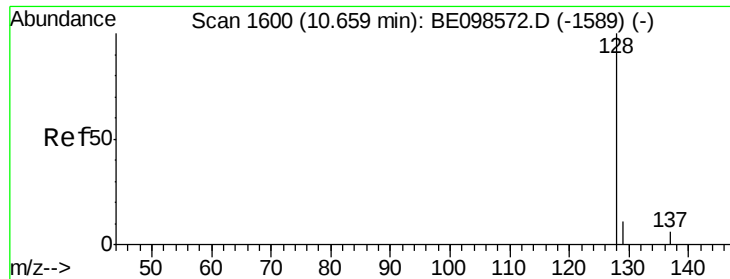

#3

Naphthalene

Concen: 0.055 ng/ul

RT: 10.65 min Scan# 1599

Delta R.T. -0.00 min

Lab File: BE098582.D

Acq: 28 Dec 2018 19:55

Instrument :

BNA_E

ClientSampleId :

F9F56


Tgt Ion:128 Resp: 739

Ion Ratio Lower Upper

128 100

129 25.0 10.5 15.7#




127 0.0 0.0 0.0

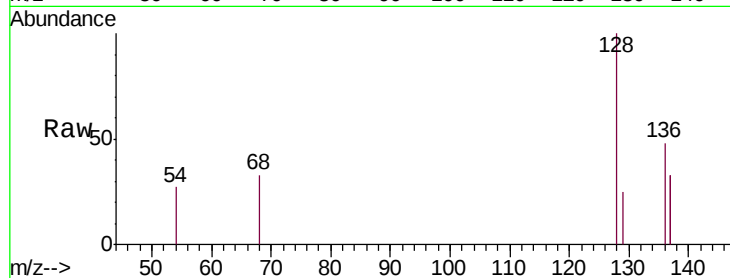

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

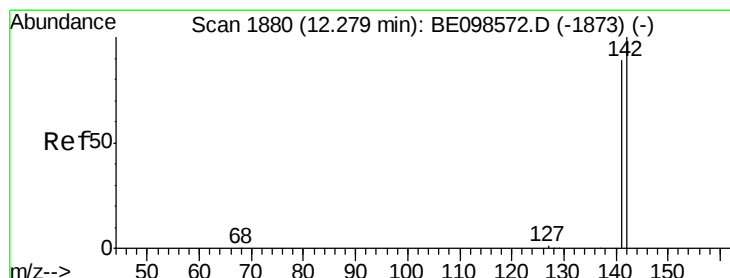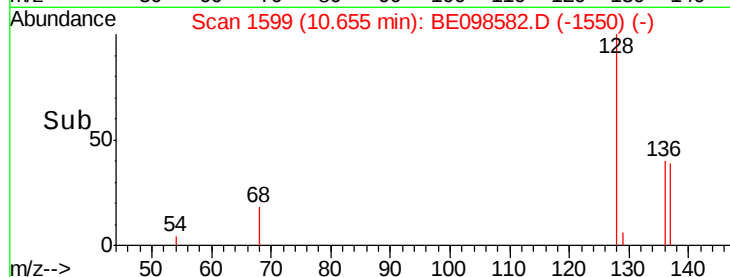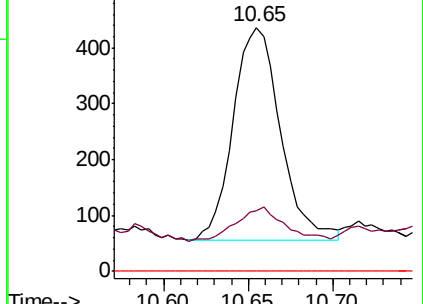

#5

2-Methylnaphthalene

Concen: 0.075 ng/ul

RT: 12.28 min Scan# 1880

Delta R.T. 0.00 min

Lab File: BE098582.D


Acq: 28 Dec 2018 19:55

Tgt Ion:142 Resp: 644

Ion Ratio Lower Upper

142 100

141 93.5 72.5 108.7

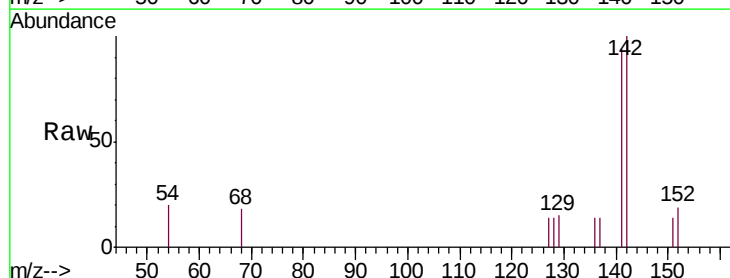

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

