

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE122818\
Quantitation Report (Not Reviewed)

Data File : BE098584.D
Acq On : 28 Dec 2018 21:07
Operator : SJ/JU
Sample : J6489-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F9F57

Quant Time: Dec 29 00:18:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	1214	0.40	ng/ul	0.00
2) Naphthalene-d8	10.61	136	5351	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	3807	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	634683	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.92	264	14036	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.20	152	2612	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.76	252	2879	0.069	ng/ul#	Qvalue 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE098584.D
Acq On : 28 Dec 2018 21:07
Operator : SJ/JU
Sample : J6489-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F9F57

Quant Time: Dec 29 00:18:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 29 00:05:35 2018
Response via : Initial Calibration

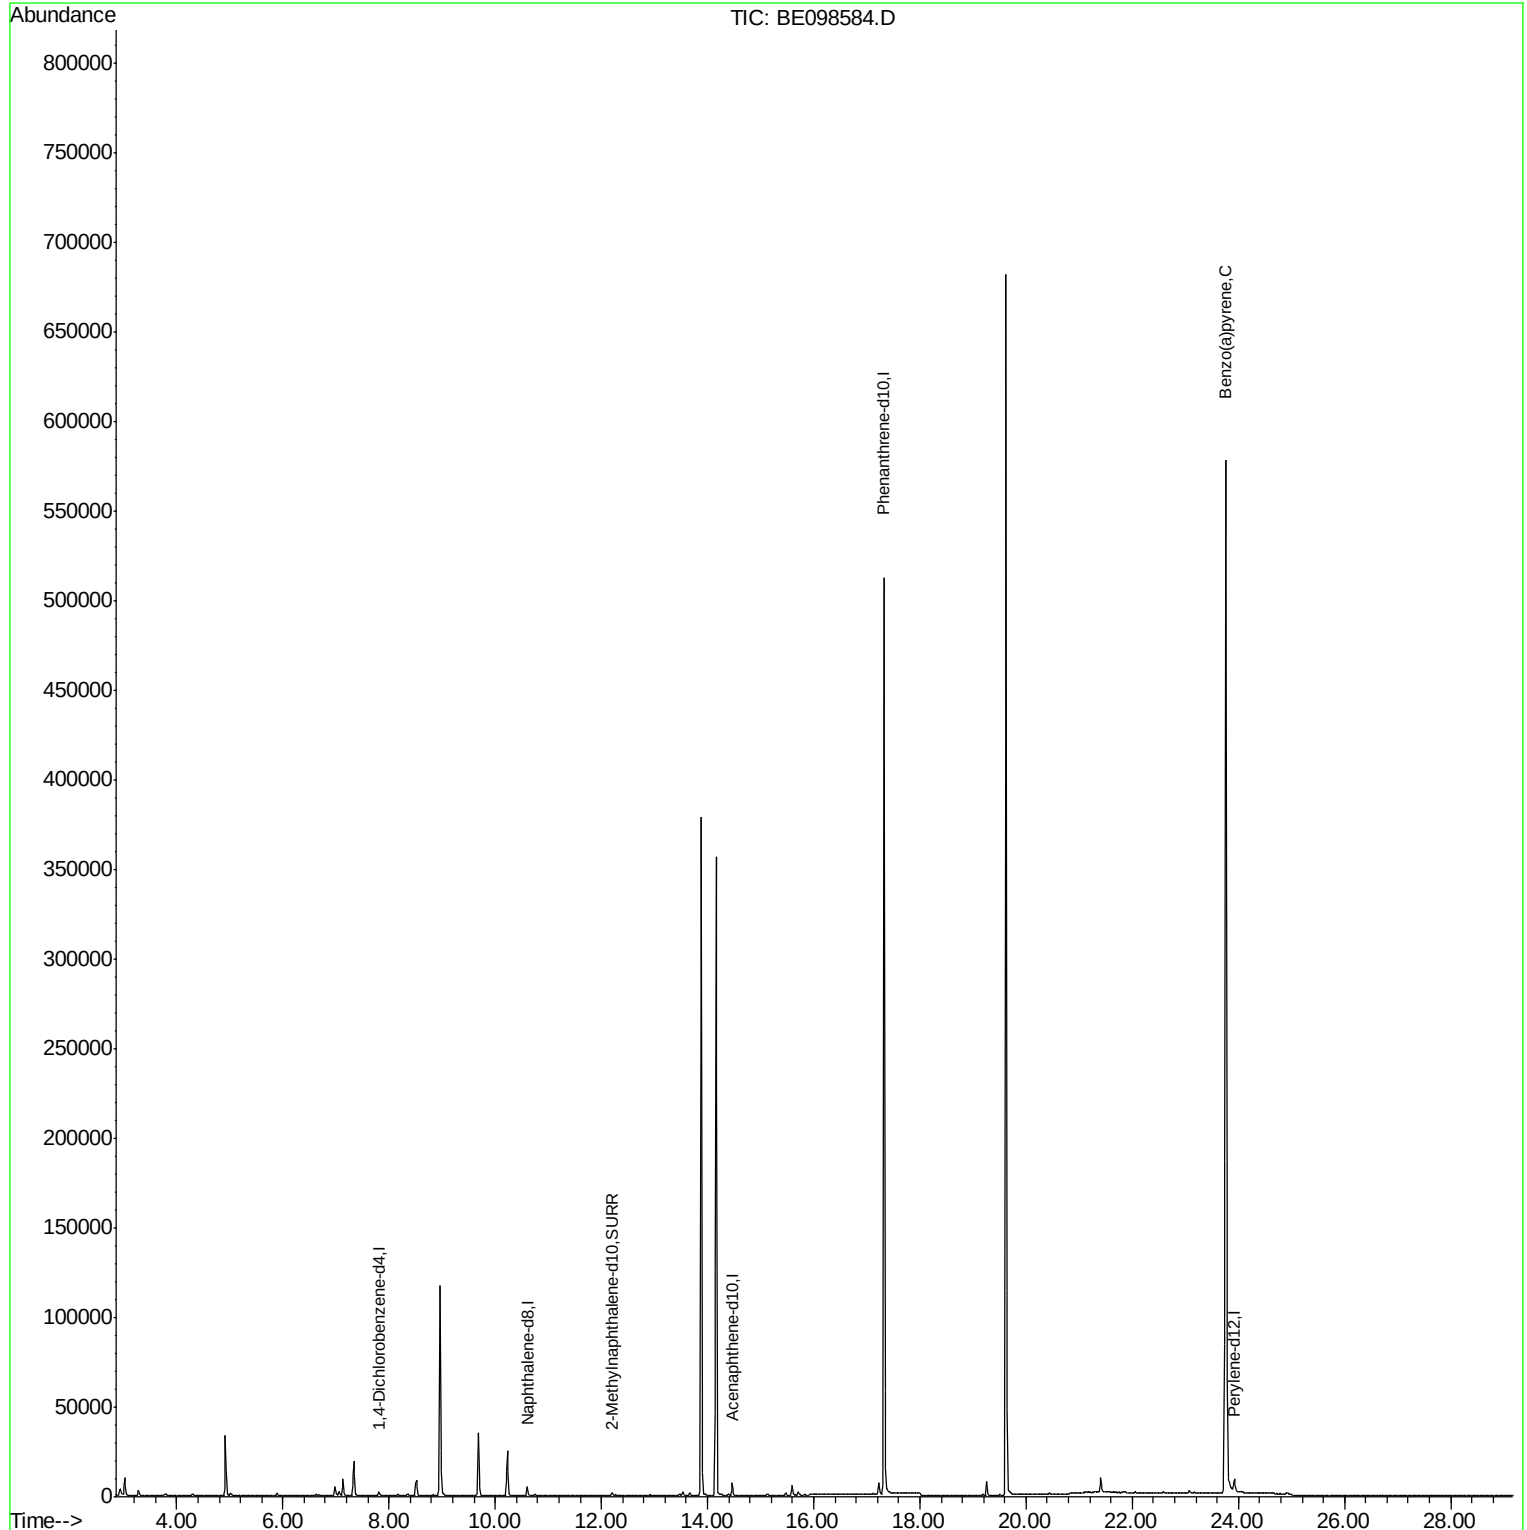

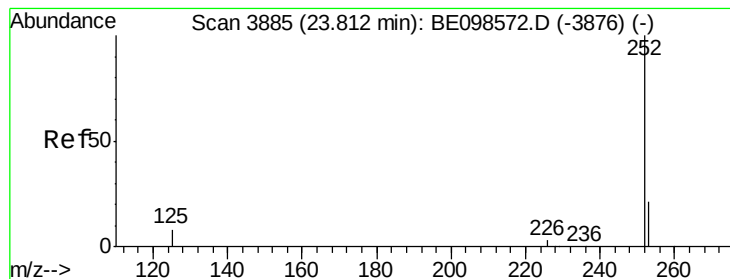

#23

Benzo(a)pyrene

Concen: 0.069 ng/ul

RT: 23.76 min Scan# 3880

Delta R.T. -0.05 min

Lab File: BE098584.D


Acq: 28 Dec 2018 21:07

Instrument :

BNA_E

ClientSampleId :

F9F57

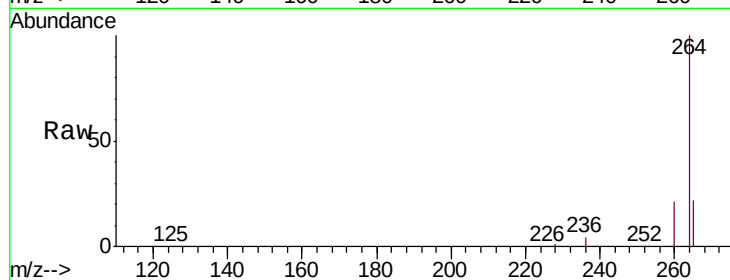

Tgt Ion: 252 Resp: 2879

Ion Ratio Lower Upper

252 100

253 38.1 19.4 29.2#

125 24.7 7.8 11.8#

