

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE122818\  
Quantitation Report (QT Reviewed)


Data File : BE098578.D  
Acq On : 28 Dec 2018 17:26  
Operator : SJ/JU  
Sample : J6489-18  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F9F60

Manual Integrations  
APPROVED

Sohil  
1/2/2019 3:56:46 PM

Quant Time: Dec 29 00:39:17 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE122818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 29 00:05:35 2018  
Response via : Initial Calibration

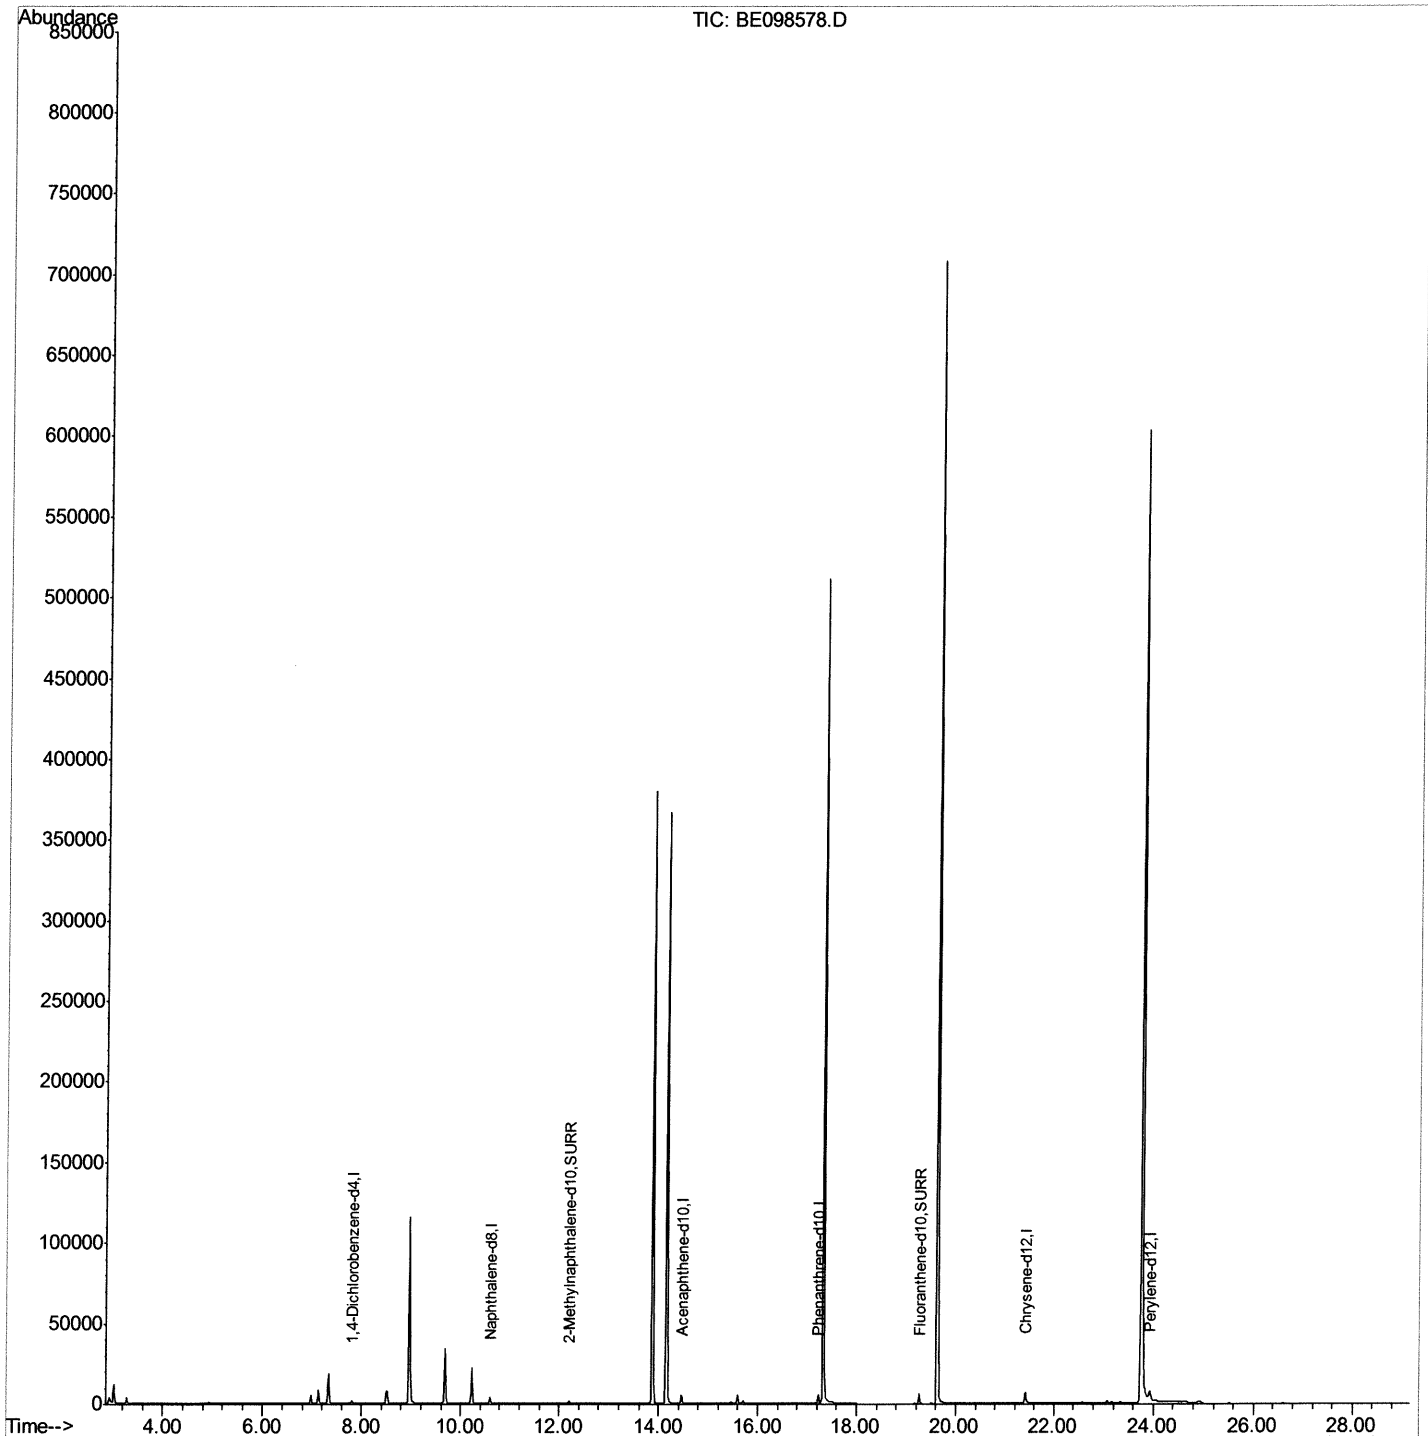

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE122818\  
Quantitation Report (Qedit)




Data File : BE098578.D  
Acq On : 28 Dec 2018 17:26  
Operator : SJ/JU  
Sample : J6489-18  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F9F60

Manual Integrations  
APPROVED

Sohil  
1/2/2019 3:56:46 PM

Quant Time: Dec 29 00:17:26 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE122818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 29 00:05:35 2018  
Response via : Initial Calibration

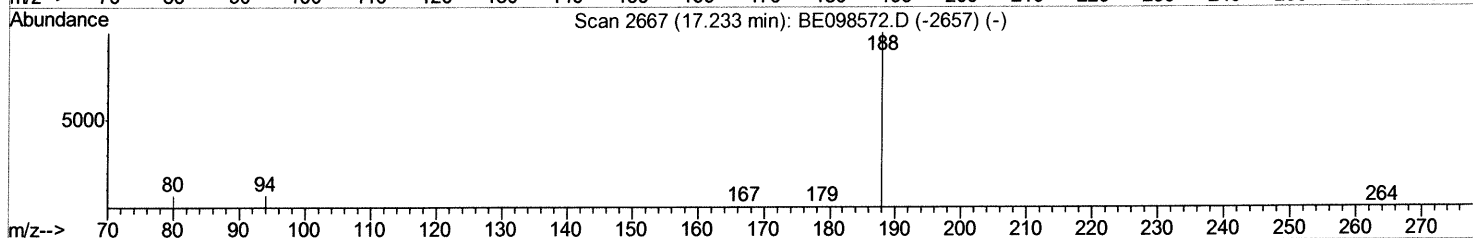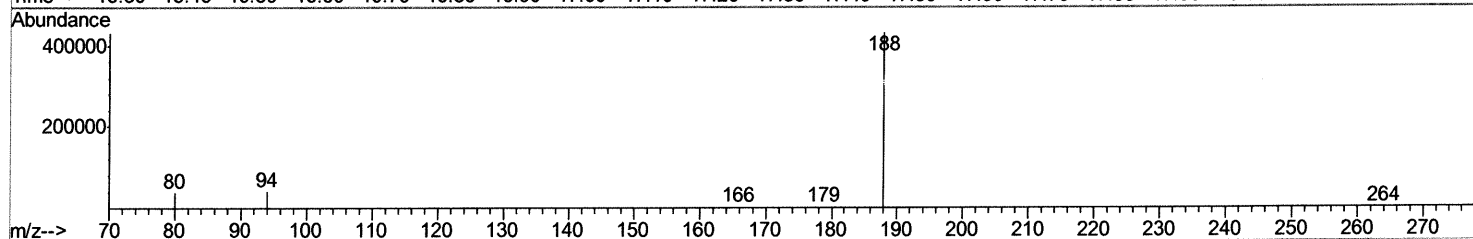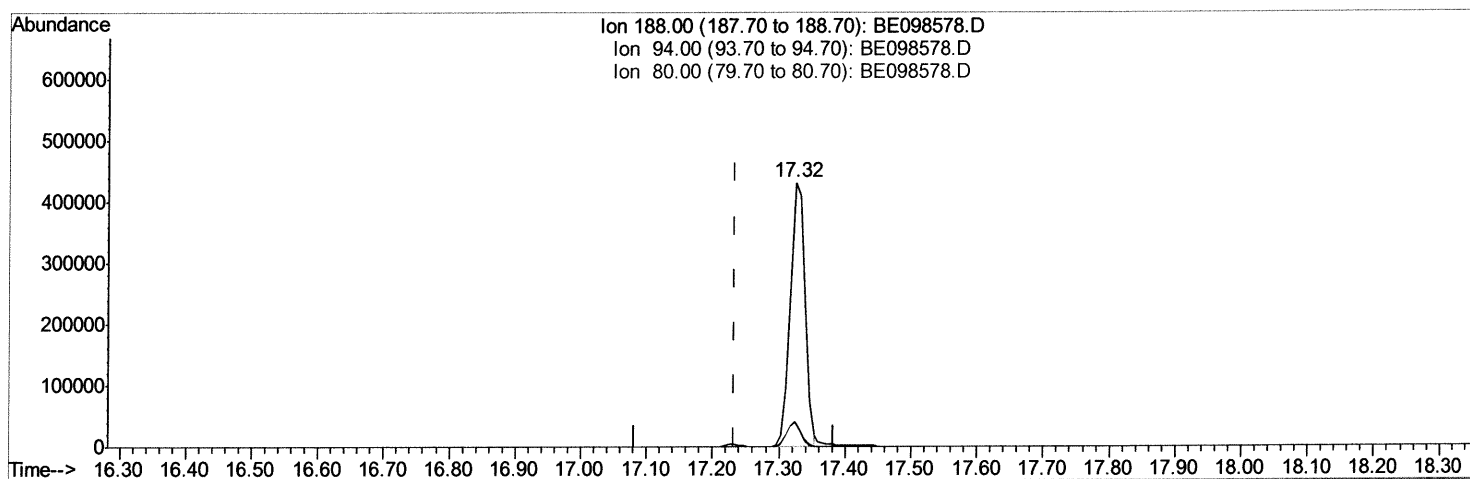

TIC: BE098578.D

(10) Phenanthrene-d10 (I)

17.324min (+0.092) 0.40ng/ul

response 652159

| Ion    | Exp% | Act%  |
|--------|------|-------|
| 188.00 | 100  | 100   |
| 94.00  | 7.30 | 9.38# |
| 80.00  | 8.50 | 8.90  |
| 0.00   | 0.00 | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE122818\  
Quantitation Report (Qedit)




Data File : BE098578.D  
Acq On : 28 Dec 2018 17:26  
Operator : SJ/JU  
Sample : J6489-18  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F9F60

Manual Integrations  
APPROVED

Sohil  
1/2/2019 3:56:46 PM

Quant Time: Dec 29 00:17:26 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE122818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 29 00:05:35 2018  
Response via : Initial Calibration

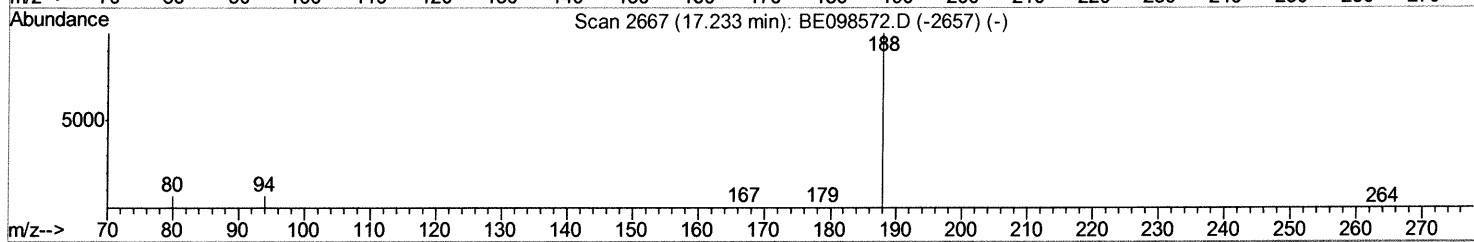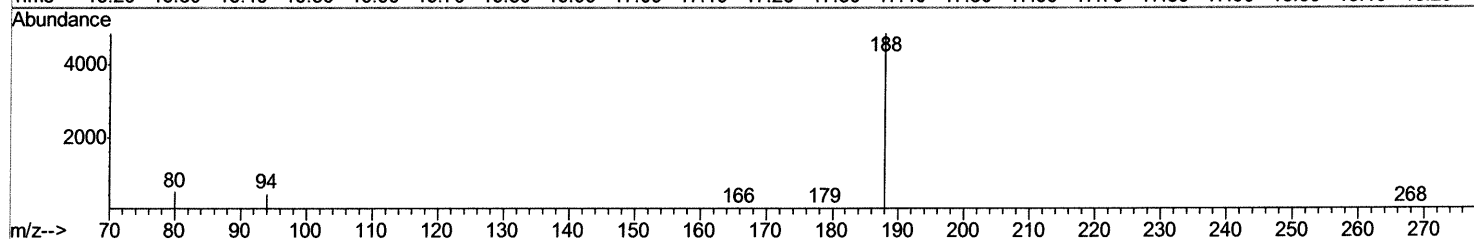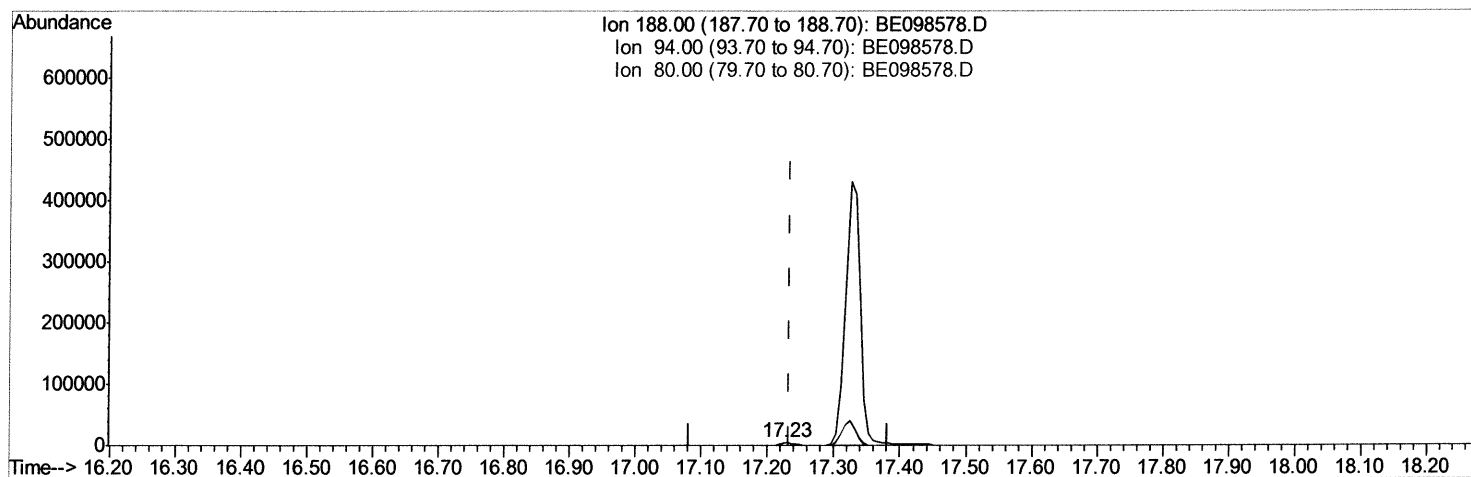

TIC: BE098578.D

(10) Phenanthrene-d10 (I)

17.226min (-0.007) 0.40ng/ul m

SJ 1/2/19

response 7856

| Ion    | Exp% | Act%   |
|--------|------|--------|
| 188.00 | 100  | 100    |
| 94.00  | 7.30 | 9.32#  |
| 80.00  | 8.50 | 10.41# |
| 0.00   | 0.00 | 0.00   |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE122818\  
Quantitation Report (Qedit)




Data File : BE098578.D  
Acq On : 28 Dec 2018 17:26  
Operator : SJ/JU  
Sample : J6489-18  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F9F60

Manual Integrations  
APPROVED

Sohil  
1/2/2019 3:56:46 PM

Quant Time: Dec 29 00:36:46 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE122818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 29 00:05:35 2018  
Response via : Initial Calibration

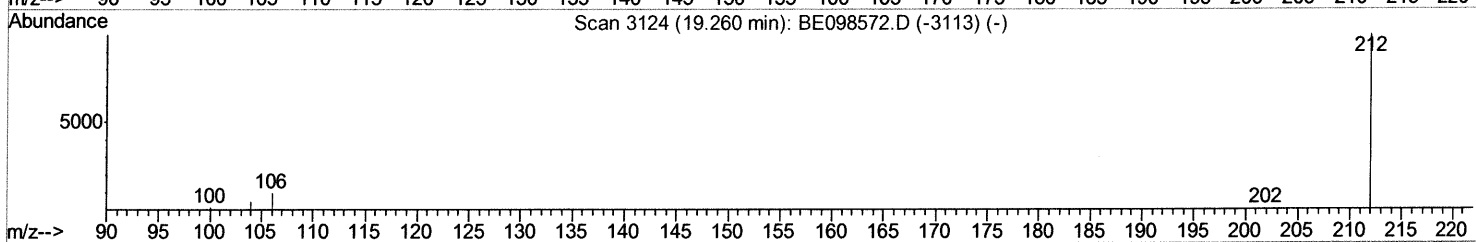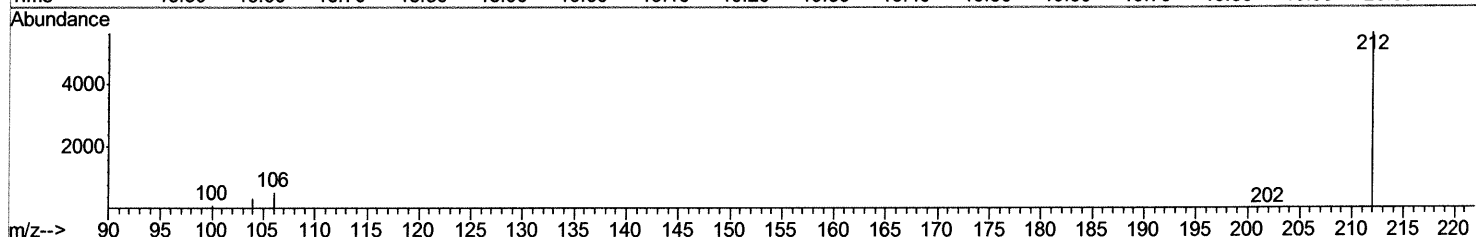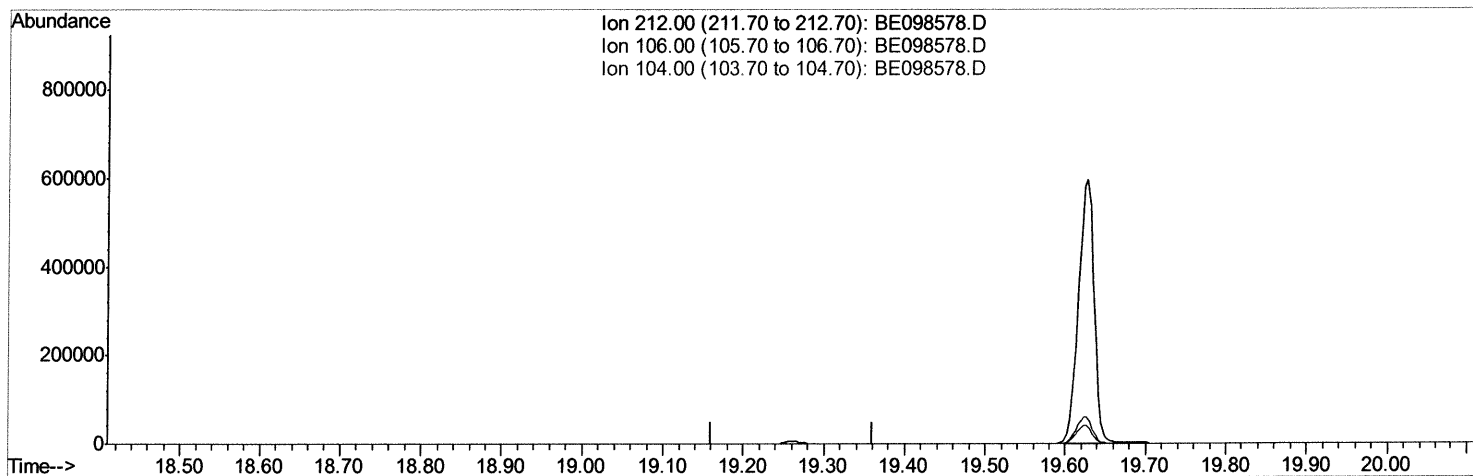

TIC: BE098578.D

(14) Fluoranthene-d10 (SURR)

19.260min (-19.260) 0.00ng/ul

response 0

| Ion    | Exp% | Act%  |
|--------|------|-------|
| 212.00 | 100  | 0.00  |
| 106.00 | 7.20 | 0.00# |
| 104.00 | 4.20 | 0.00# |
| 0.00   | 0.00 | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE122818\  
Quantitation Report (Qedit)




Data File : BE098578.D  
Acq On : 28 Dec 2018 17:26  
Operator : SJ/JU  
Sample : J6489-18  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F9F60

Manual Integrations  
APPROVED

Sohil  
1/2/2019 3:56:46 PM

Quant Time: Dec 29 00:36:46 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE122818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 29 00:05:35 2018  
Response via : Initial Calibration

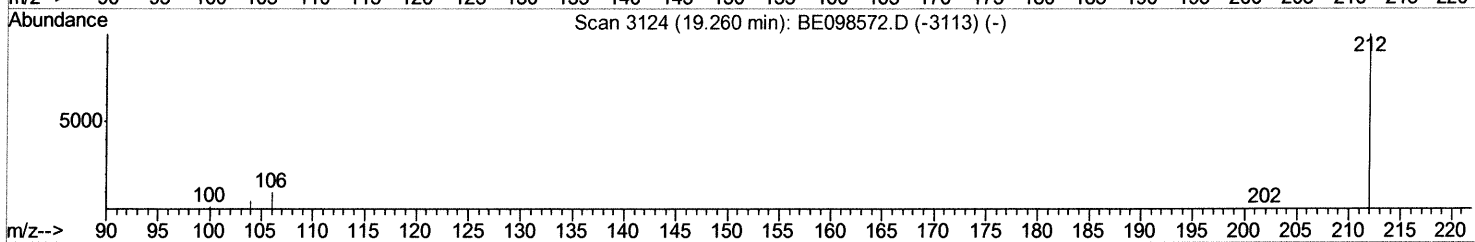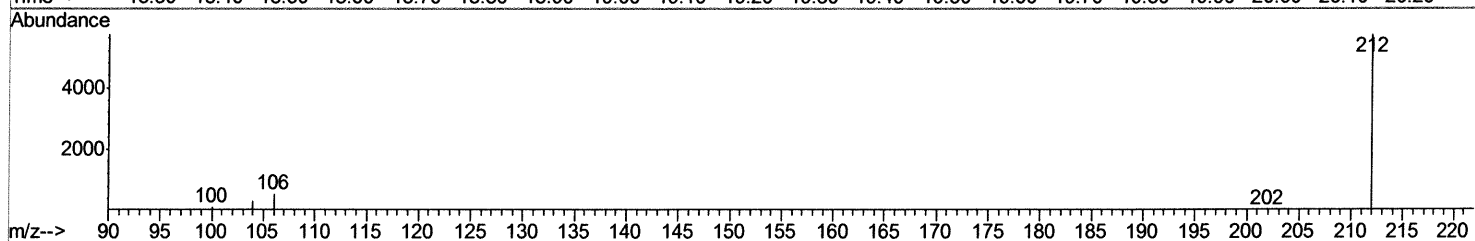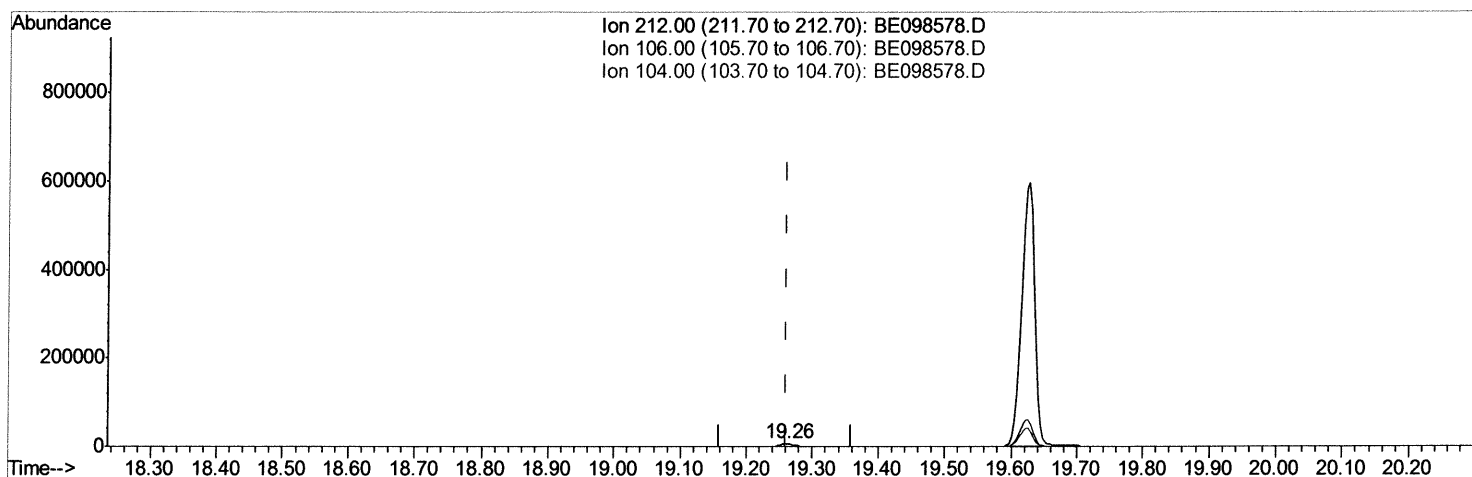

TIC: BE098578.D

(14) Fluoranthene-d10 (SURR)

19.263min (+0.003) 0.34ng/ul m

SJ 1/2/19

response 8439

| Ion    | Exp% | Act%  |
|--------|------|-------|
| 212.00 | 100  | 100   |
| 106.00 | 7.20 | 0.00# |
| 104.00 | 4.20 | 0.00# |
| 0.00   | 0.00 | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE122818\  
Quantitation Report (Qedit)




Data File : BE098578.D  
Acq On : 28 Dec 2018 17:26  
Operator : SJ/JU  
Sample : J6489-18  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F9F60

Manual Integrations  
APPROVED

Sohil  
1/2/2019 3:56:46 PM

Quant Time: Dec 29 00:36:46 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE122818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 29 00:05:35 2018  
Response via : Initial Calibration

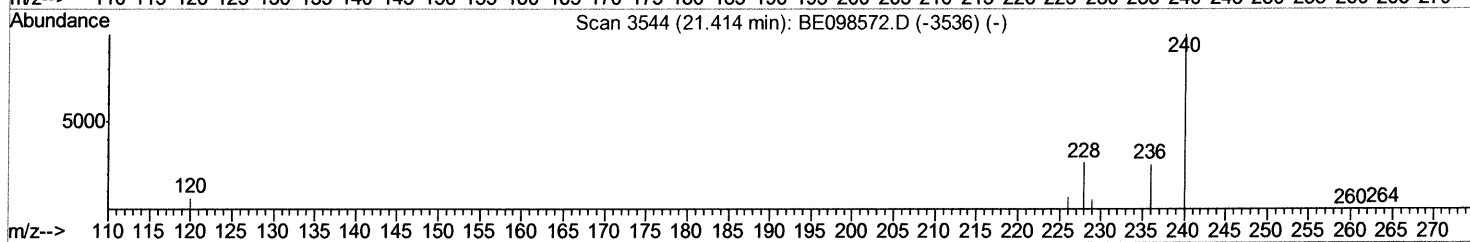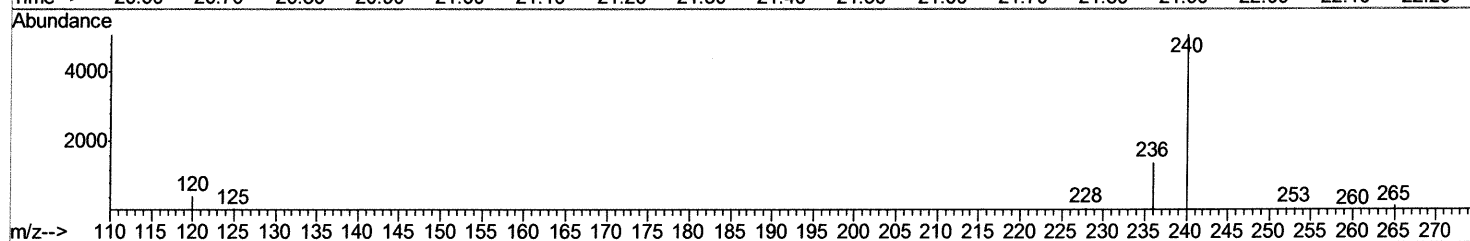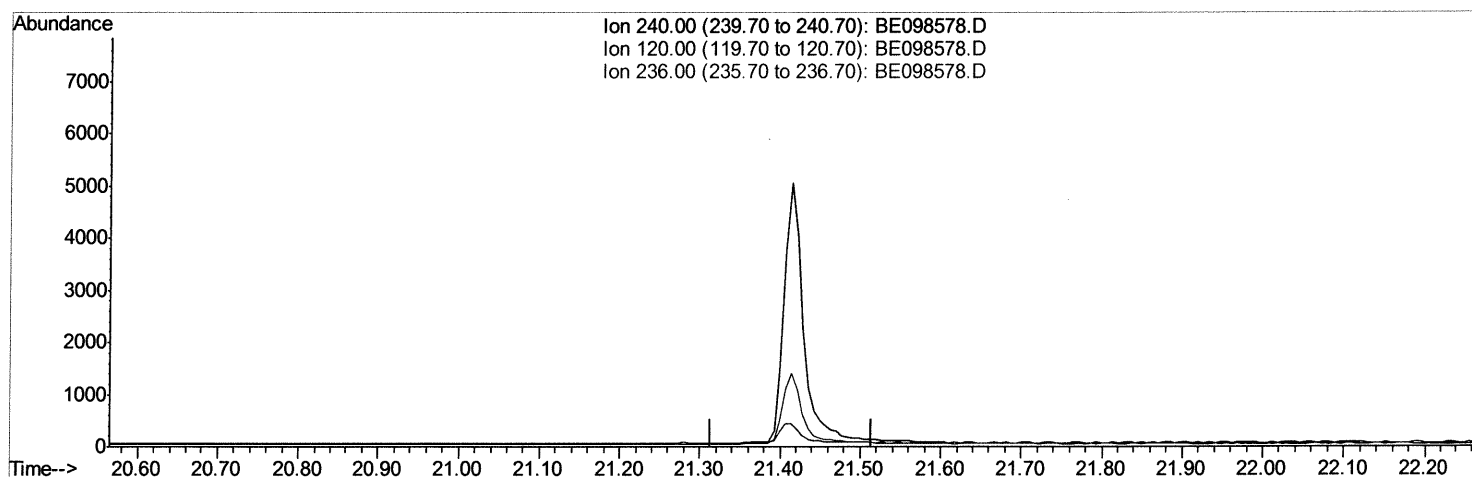

TIC: BE098578.D

(16) Chrysene-d12 (I)

21.414min (-21.414) 0.00ng/ul

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 240.00 | 100   | 0.00  |
| 120.00 | 7.50  | 0.00# |
| 236.00 | 26.20 | 0.00# |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE122818\  
Quantitation Report (Qedit)




Data File : BE098578.D  
Acq On : 28 Dec 2018 17:26  
Operator : SJ/JU  
Sample : J6489-18  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F9F60

Manual Integrations  
APPROVED

Sohil  
1/2/2019 3:56:46 PM

Quant Time: Dec 29 00:36:46 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE122818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 29 00:05:35 2018  
Response via : Initial Calibration

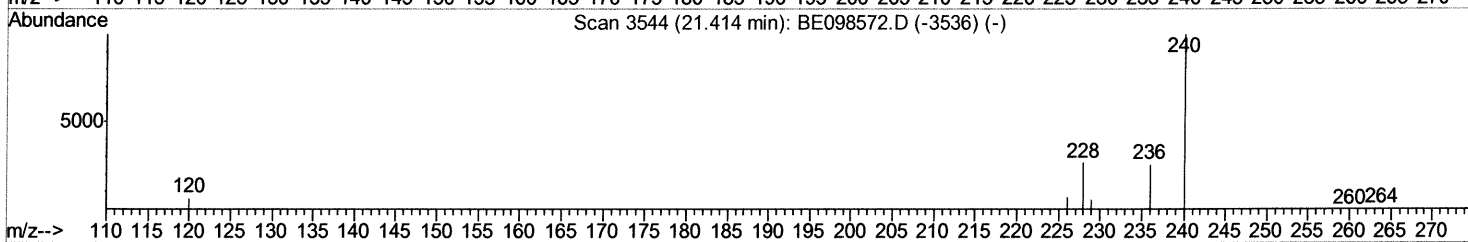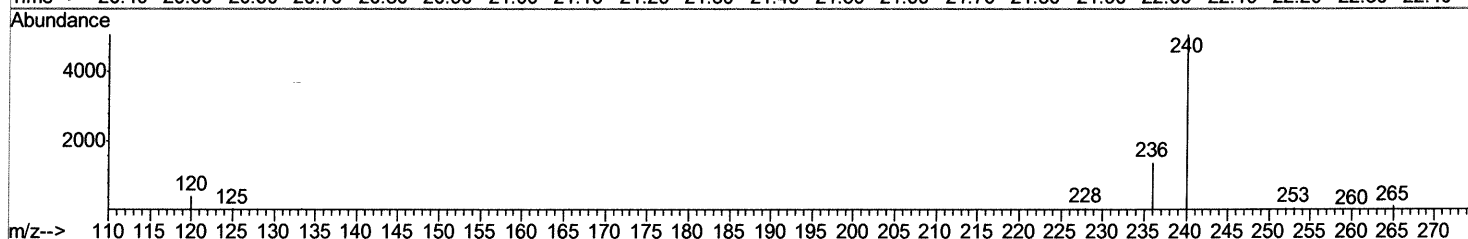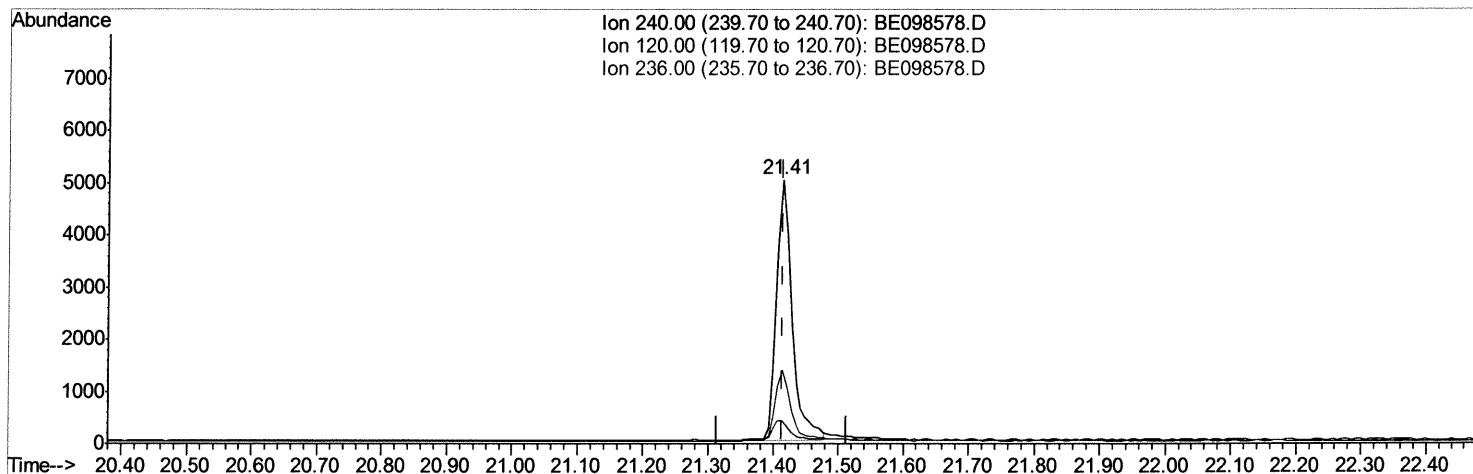

TIC: BE098578.D

(16) Chrysene-d12 (I)

21.414min (-0.000) 0.40ng/ul m

SJ 1/2/19

response 8187

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 240.00 | 100   | 100   |
| 120.00 | 7.50  | 8.71  |
| 236.00 | 26.20 | 27.71 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE122818\  
Quantitation Report (Qedit)




Data File : BE098578.D  
Acq On : 28 Dec 2018 17:26  
Operator : SJ/JU  
Sample : J6489-18  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F9F60

Manual Integrations  
APPROVED

Sohil  
1/2/2019 3:56:46 PM

Quant Time: Dec 29 00:38:23 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE122818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 29 00:05:35 2018  
Response via : Initial Calibration

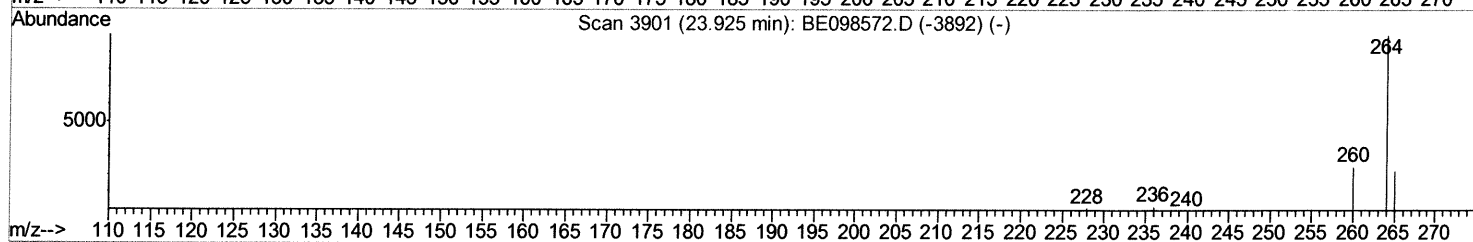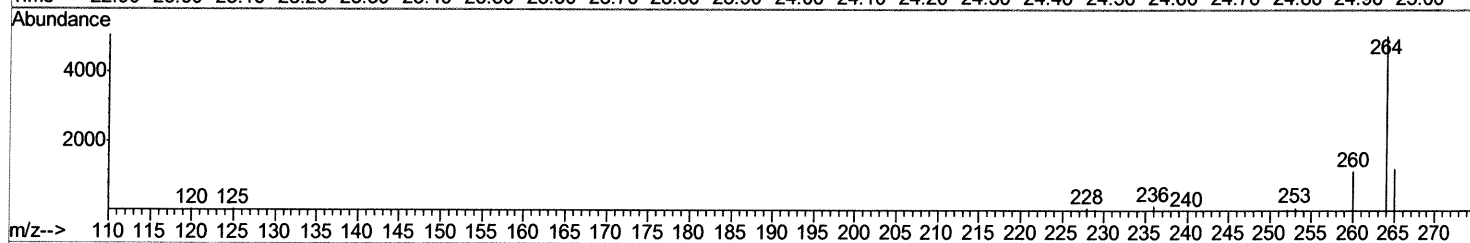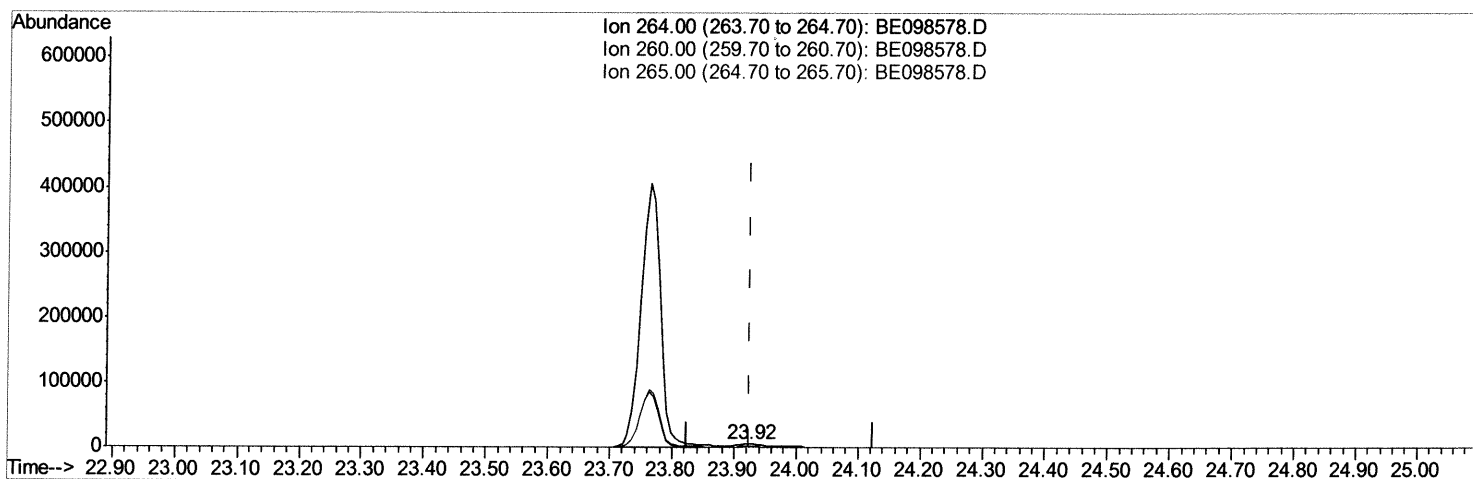

TIC: BE098578.D

(20) Perylene-d12 (I)

23.924min (-0.000) 0.40ng/ul

response 14372

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 264.00 | 100   | 100   |
| 260.00 | 25.20 | 23.24 |
| 265.00 | 28.00 | 25.02 |
| 0.00   | 0.00  | 0.00  |



Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE122818\  
Quantitation Report (Qedit)




Data File : BE098578.D  
Acq On : 28 Dec 2018 17:26  
Operator : SJ/JU  
Sample : J6489-18  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F9F60

Manual Integrations  
APPROVED

Sohil  
1/2/2019 3:56:46 PM

Quant Time: Dec 29 00:38:23 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE122818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 29 00:05:35 2018  
Response via : Initial Calibration

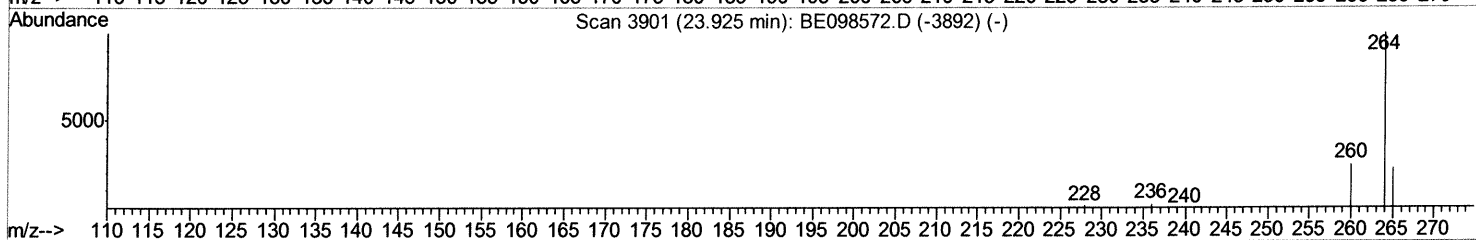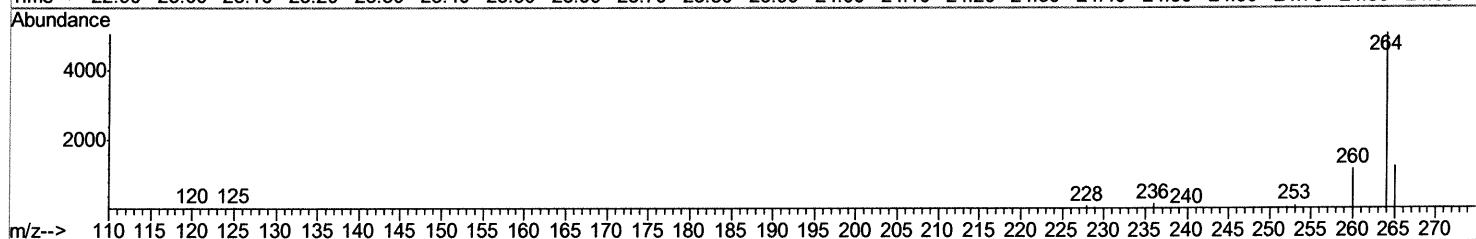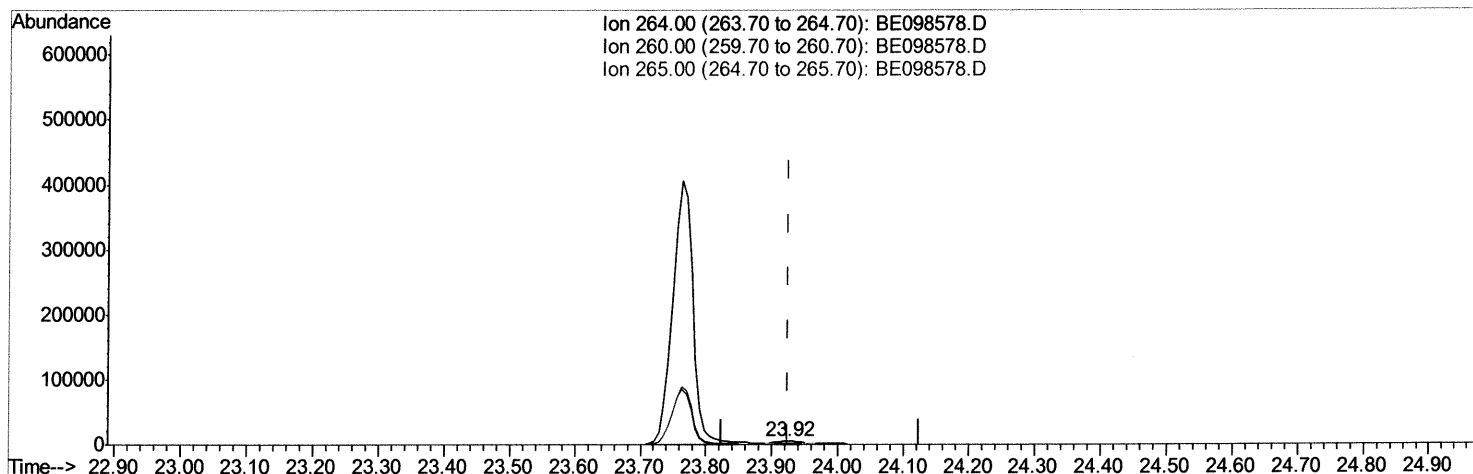

TIC: BE098578.D

(20) Perylene-d12 (I)

23.924min (-0.000) 0.40ng/ul m

SJ 1/2/19

response 7170

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 264.00 | 100   | 100   |
| 260.00 | 25.20 | 23.24 |
| 265.00 | 28.00 | 25.02 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE122818\  
Quantitation Report (QT Reviewed)

Data File : BE098578.D  
Acq On : 28 Dec 2018 17:26  
Operator : SJ/JU  
Sample : J6489-18  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F9F60

Manual Integrations  
APPROVED

Sohil  
1/2/2019 3:56:46 PM

Quant Time: Dec 29 00:39:17 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE122818.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 29 00:05:35 2018  
Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|-----------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 7.81  | 152  | 1090     | 0.40 | ng/ul | 0.00     |
| 2) Naphthalene-d8           | 10.61 | 136  | 4789     | 0.40 | ng/ul | 0.00     |
| 6) Acenaphthene-d10         | 14.47 | 164  | 3440     | 0.40 | ng/ul | 0.00     |
| 10) Phenanthrene-d10        | 17.23 | 188  | 7856m    | 0.40 | ng/ul | 0.00     |
| 16) Chrysene-d12            | 21.41 | 240  | 8187m    | 0.40 | ng/ul | 0.00     |
| 20) Perylene-d12            | 23.92 | 264  | 7170m    | 0.40 | ng/ul | 0.00     |
| System Monitoring Compounds |       |      |          |      |       |          |
| 4) 2-Methylnaphthalene-d10  | 12.21 | 152  | 2577     | 0.33 | ng/ul | 0.00     |
| 14) Fluoranthene-d10        | 19.26 | 212  | 8439m    | 0.34 | ng/ul | 0.00     |

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ  
1/2/19