

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE122818\
 Data File : BE098580.D
 Acq On : 28 Dec 2018 18:40
 Operator : SJ/JU
 Sample : J6489-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
ClientSampleId :
 F9F77

Manual Integrations
APPROVED
 Sohil
 1/2/2019 3:56:52 PM

Quant Time: Dec 29 00:54:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE122818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 29 00:05:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	1065	0.40	ng/ul	0.00
2) Naphthalene-d8	10.60	136	4635	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	3324	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.23	188	7722m	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	8287m	0.40	ng/ul	0.00
20) Perylene-d12	23.93	264	7026m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	2071	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.26	212	7530m	0.31	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.55	153	642	0.057	ng/ul#	Ovalue 33


(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE122818\
 Data File : BE098580.D
 Acq On : 28 Dec 2018 18:40
 Operator : SJ/JU
 Sample : J6489-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F9F77

Manual Integrations
 APPROVED
 Sohil
 1/2/2019 3:56:52 PM

Quant Time: Dec 29 00:54:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE122818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 29 00:05:35 2018
 Response via : Initial Calibration

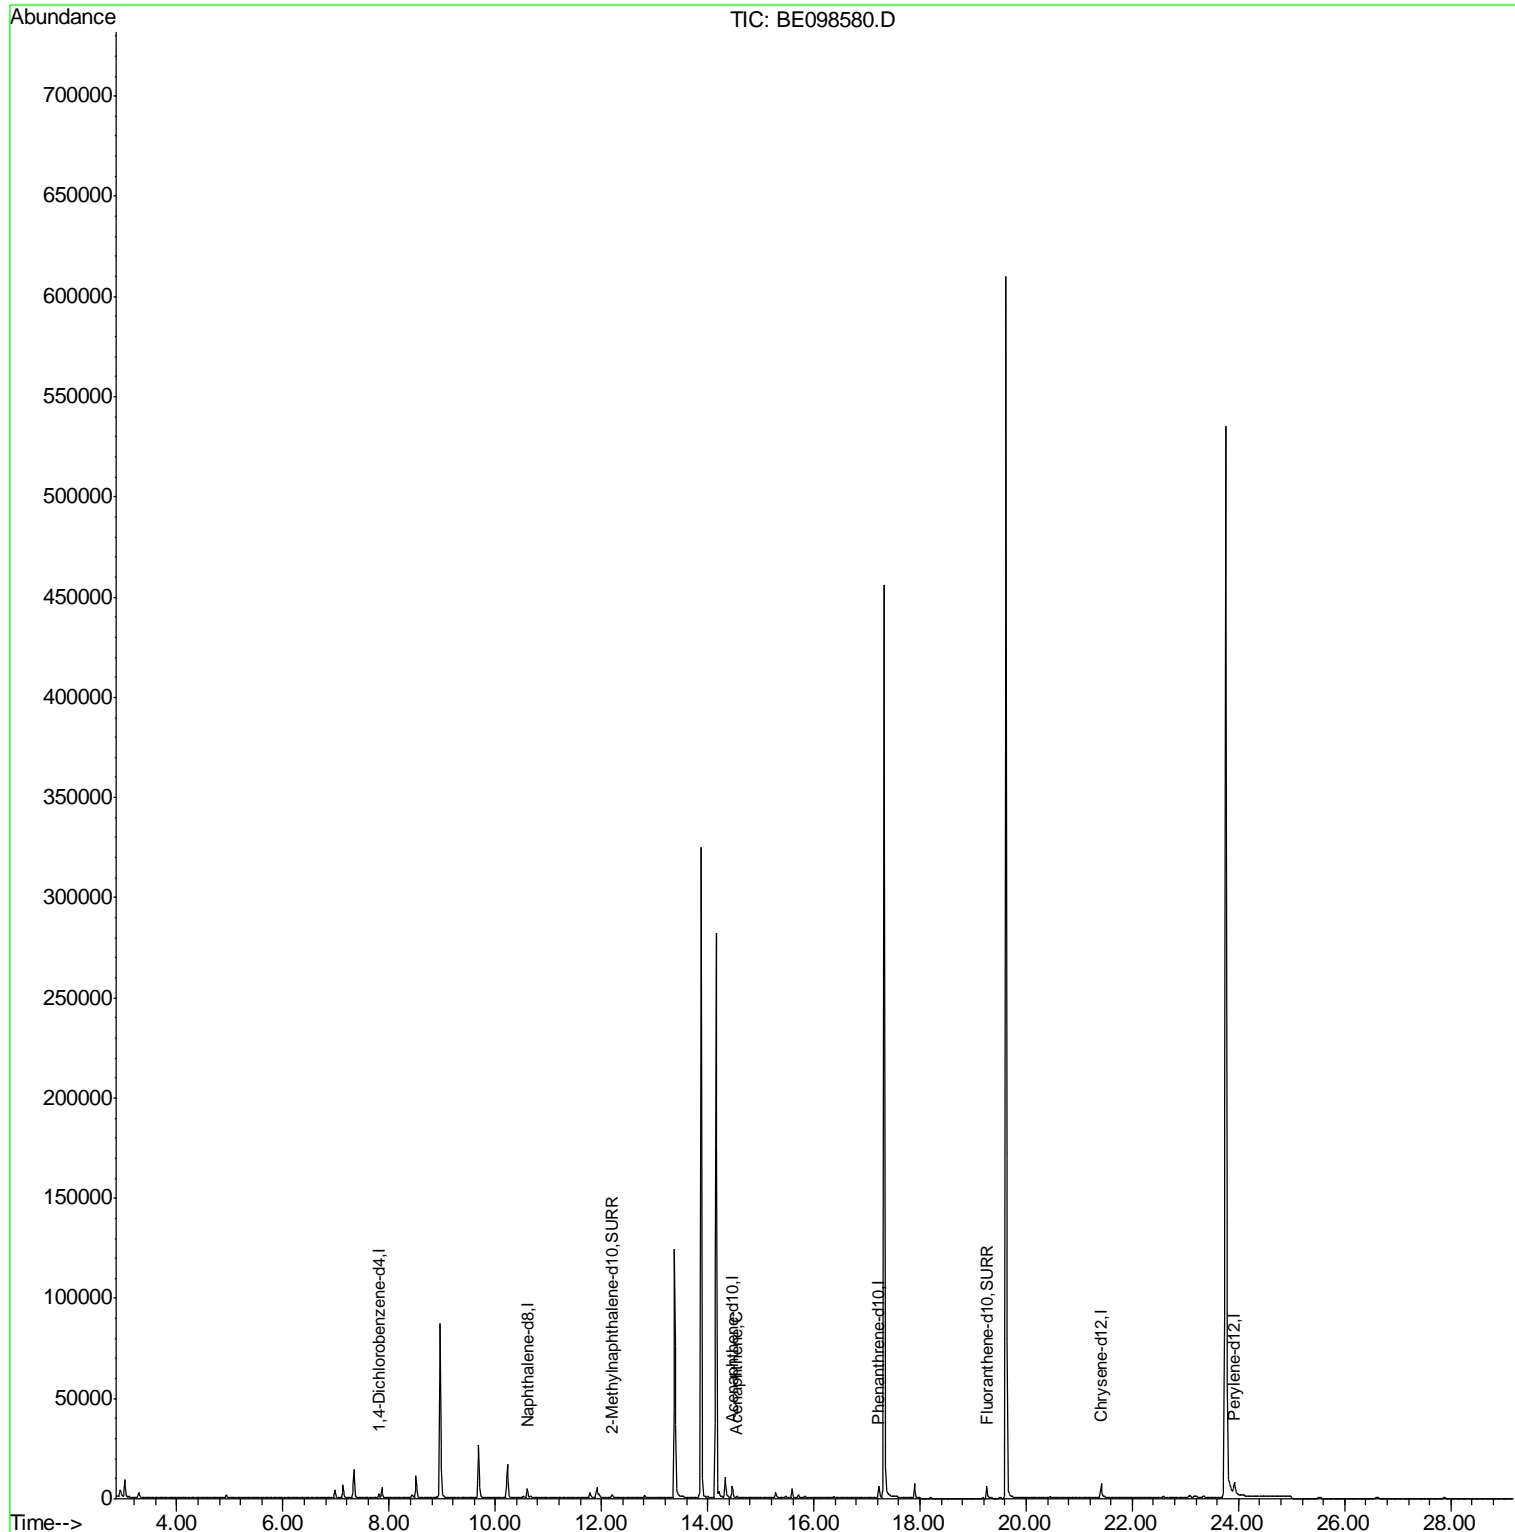

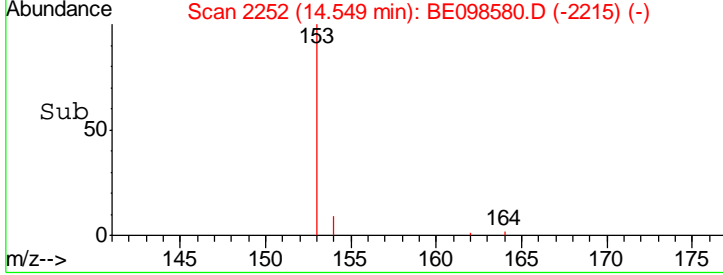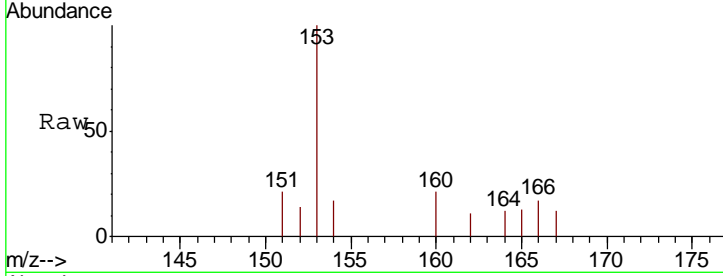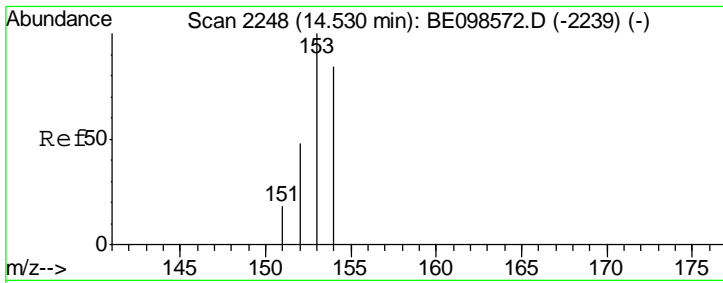

#8
 Acenaphthene
 Concen: 0.057 ng/ul
 RT: 14.55 min Scan# 2252
 Delta R.T. 0.02 min
 Lab File: BE098580.D
 Acq: 28 Dec 2018 18:40

Tot Ion: 153 Resp: 642

Ion	Ratio	Lower	Upper
153	100		
152	13.8	39.4	59.0#
154	17.2	70.5	105.7#

Instrument :
 BNA_E
 ClientSampled :
 F9F77

Manual Integrations
 APPROVED
 Sohil
 1/2/2019 3:56:52 PM

