

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE032421\
 Data File : BE101150.D
 Acq On : 24 Mar 2021 15:05
 Operator : CG/JU
 Sample : SSTDIC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDIC5.0

Quant Time: Mar 24 15:50:51 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE032421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 24 13:22:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.853	152	5496	0.40	ng	0.00
7) Naphthalene-d8	10.628	136	21368	0.40	ng	#-0.01
13) Acenaphthene-d10	14.458	164	14654	0.40	ng	-0.01
19) Phenanthrene-d10	17.226	188	34110	0.40	ng	0.00
29) Chrysene-d12	21.378	240	46243	0.40	ng	0.00
36) Perylene-d12	23.860	264	36533	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.434	112	59949	4.48	ng	0.00
5) Phenol-d6	7.001	99	96754	4.65	ng	0.00
8) Nitrobenzene-d5	8.992	82	73872	6.52	ng	0.00
11) 2-Methylnaphthalene-d10	12.210	152	176464	5.14	ng	0.00
14) 2,4,6-Tribromophenol	15.971	330	15619	5.93	ng	0.00
15) 2-Fluorobiphenyl	13.089	172	240215	4.30	ng	-0.01
27) Fluoranthene-d10	19.232	212	2205230	4.96	ng	0.00
31) Terphenyl-d14	19.830	244	478403	4.74	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.384	88	36154	4.00	ng	95
3) n-Nitrosodimethylamine	3.672	42	43995	4.52	ng	# 98
6) bis(2-Chloroethyl)ether	7.277	93	75787	4.51	ng	100
9) Naphthalene	10.680	128	1039005	4.78	ng	100
10) Hexachlorobutadiene	10.979	225	45953	4.66	ng	99
12) 2-Methylnaphthalene	12.282	142	189692	5.11	ng	99
16) Acenaphthylene	14.184	152	297494	5.23	ng	99
17) Acenaphthene	14.530	154	198343	4.87	ng	96
18) Fluorene	15.517	166	258397	4.86	ng	99
21) 4-Bromophenyl-phenylether	16.424	248	74408	4.54	ng	94
22) Hexachlorobenzene	16.530	284	80634	4.78	ng	99
24) Pentachlorophenol	16.863	266	31573	8.36	ng	98
25) Phenanthrene	17.256	178	465369	4.89	ng	99
26) Anthracene	17.347	178	443313	5.40	ng	98
28) Fluoranthene	19.261	202	611936	4.91	ng	98
30) Pyrene	19.623	202	628395	4.81	ng	98
32) Benzo(a)anthracene	21.354	228	612219	5.19	ng	98
33) Chrysene	21.415	228	660240	4.73	ng	99
35) Indeno(1,2,3-cd)pyrene	26.488	276	537157	6.03	ng	99
37) Benzo(b)fluoranthene	23.101	252	541423	5.72	ng	99
38) Benzo(k)fluoranthene	23.151	252	630754	4.94	ng	99
39) Benzo(a)pyrene	23.749	252	513079	5.73	ng	98
40) Dibenzo(a,h)anthracene	26.516	278	460547	6.49	ng	98
41) Benzo(g,h,i)perylene	27.294	276	500642	5.50	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE032421\
Data File : BE101150.D
Acq On : 24 Mar 2021 15:05
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0

Quant Time: Mar 24 15:50:51 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE032421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 13:22:06 2021
Response via : Initial Calibration




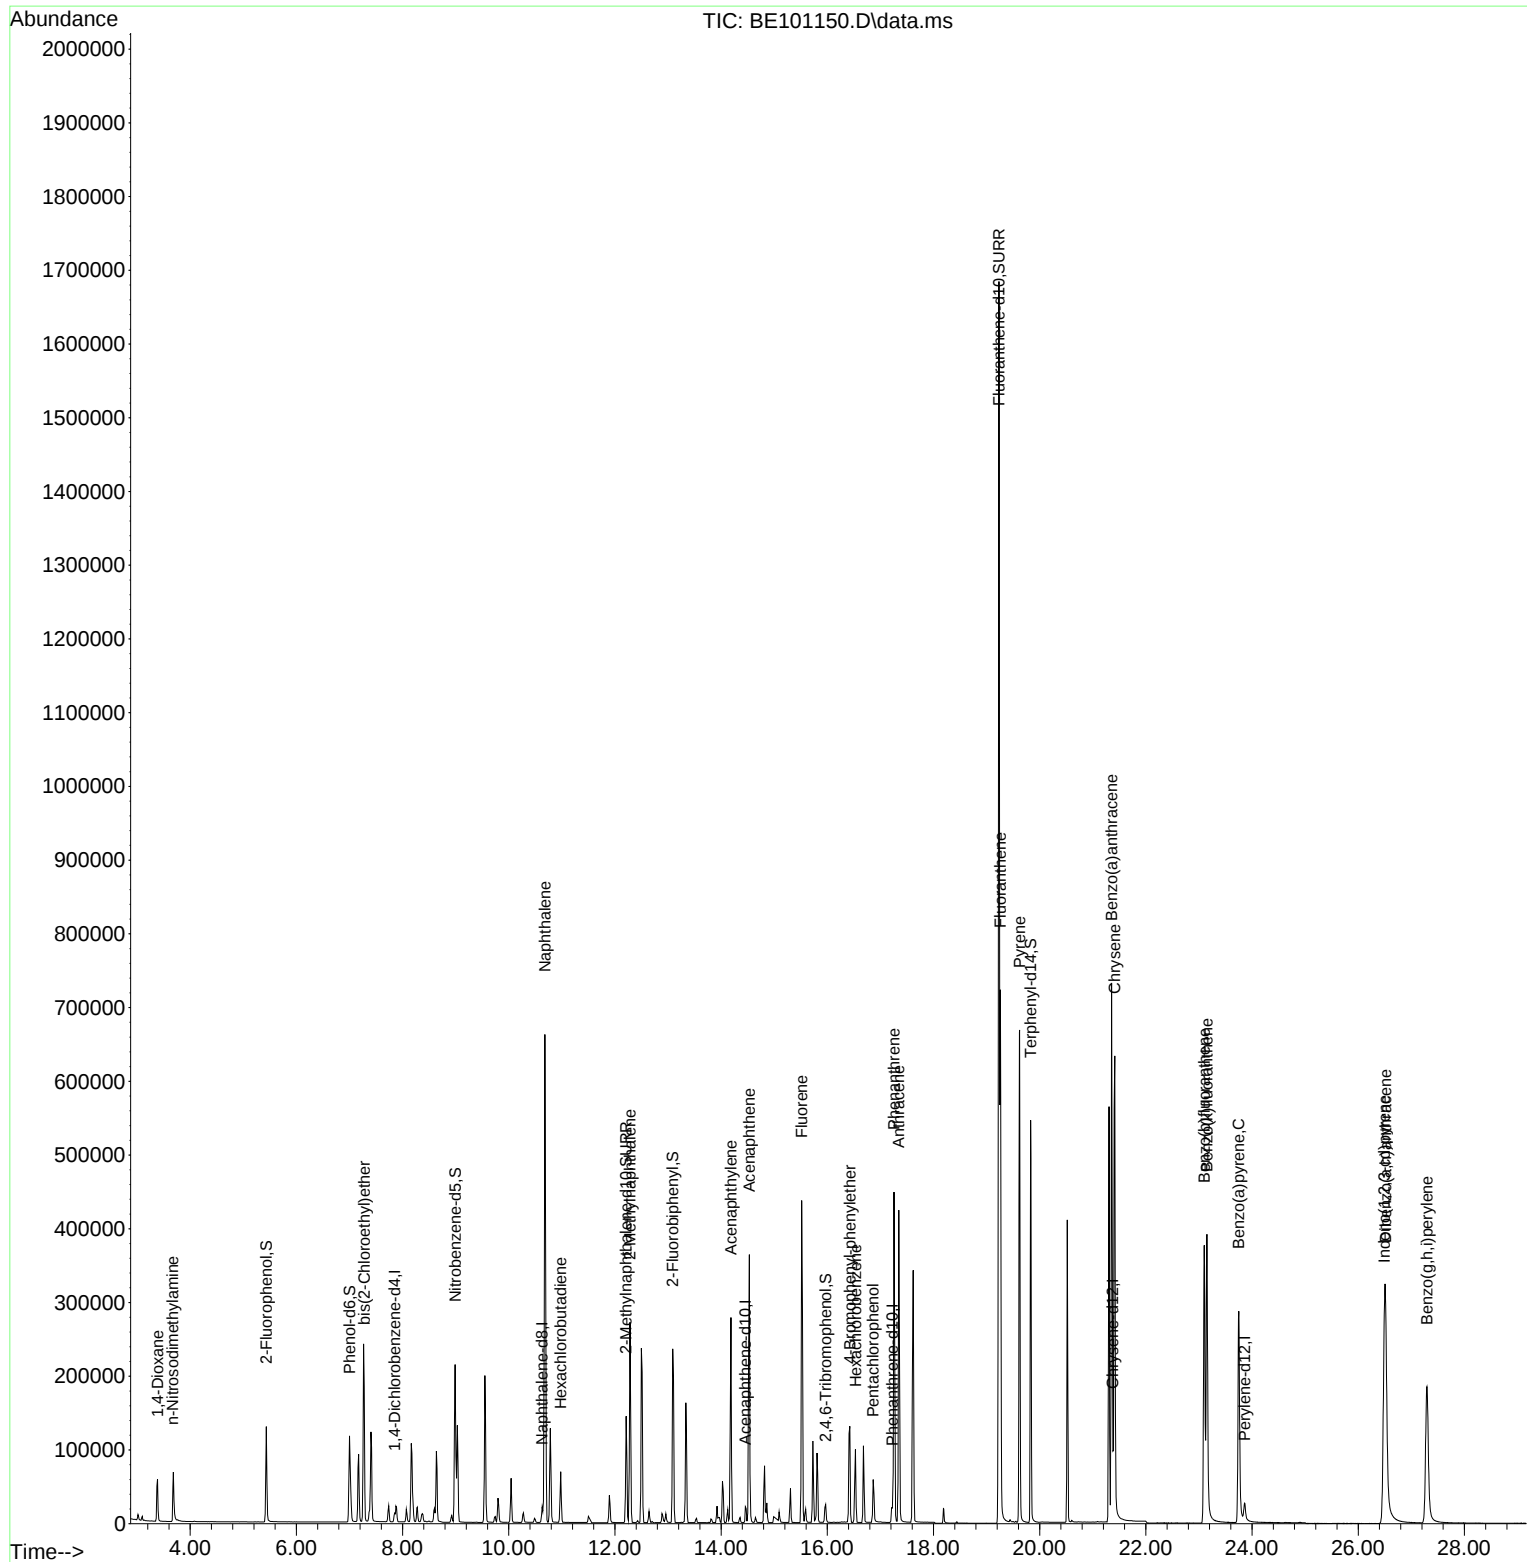


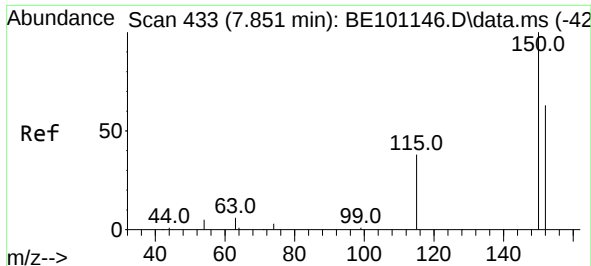

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.853 min Scan# 433
 Delta R.T. 0.002 min
 Lab File: BE101150.D
 Acq: 24 Mar 2021 15:05




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 5496
 Ion Ratio Lower Upper
 152 100
 150 148.4 126.3 189.5
 115 58.1 48.9 73.3

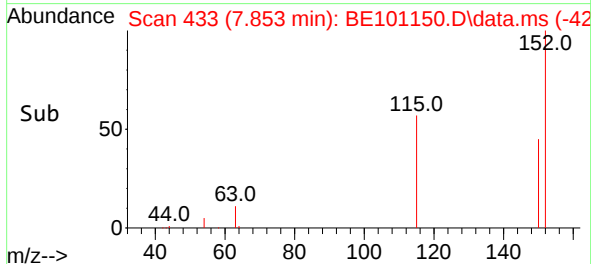

#2
 1,4-Dioxane
 Concen: 4.00 ng
 RT: 3.384 min Scan# 45
 Delta R.T. 0.002 min
 Lab File: BE101150.D
 Acq: 24 Mar 2021 15:05

Tgt Ion: 88 Resp: 36154
 Ion Ratio Lower Upper
 88 100
 58 90.9 68.5 102.7
 43 34.8 27.2 40.8


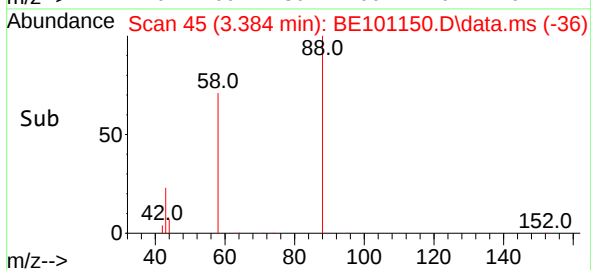

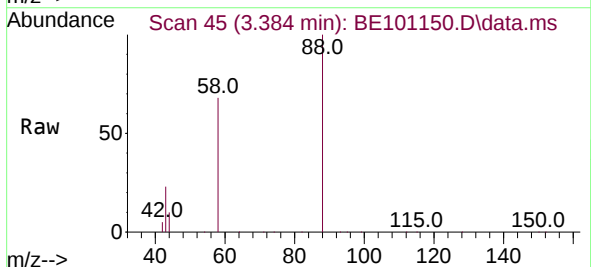


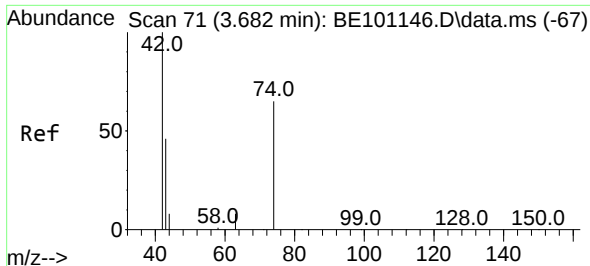

#3
n-Nitrosodimethylamine
Concen: 4.52 ng
RT: 3.672 min Scan# 70
Delta R.T. -0.010 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 43995
Ion Ratio Lower Upper
42 100
74 110.7 87.0 130.6
44 8.0 8.3 12.5#

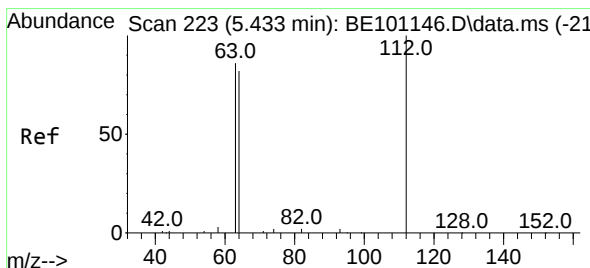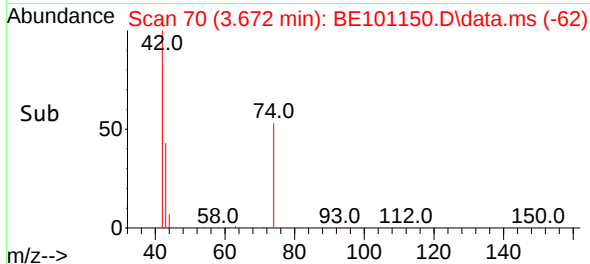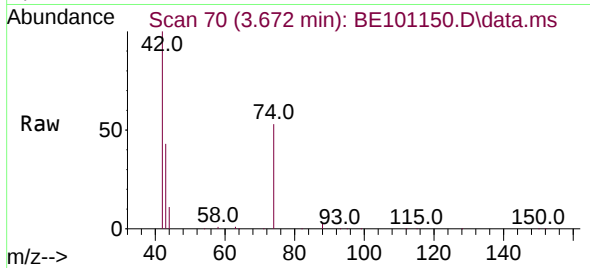

#4
2-Fluorophenol
Concen: 4.48 ng
RT: 5.434 min Scan# 223
Delta R.T. 0.002 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion: 112 Resp: 59949
Ion Ratio Lower Upper
112 100
64 75.5 60.8 91.2
63 148.6 119.4 179.0


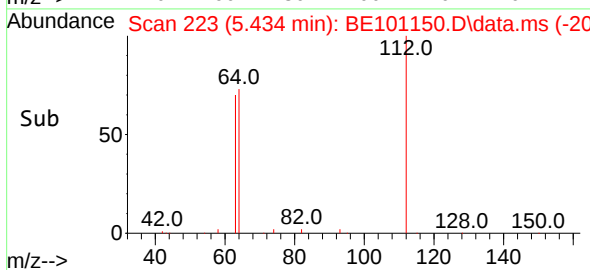

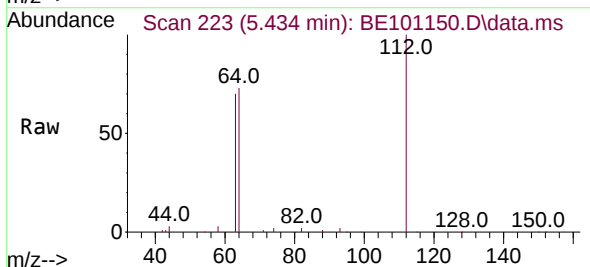


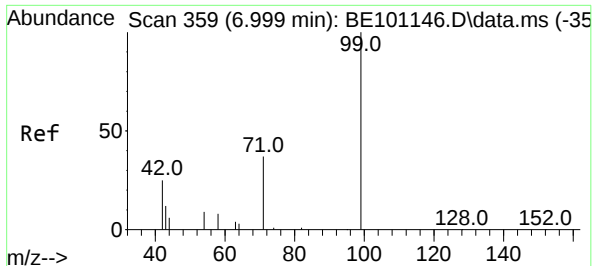

#5
Phenol-d6
Concen: 4.65 ng
RT: 7.001 min Scan# 359
Delta R.T. 0.002 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 96754
Ion Ratio Lower Upper
99 100
42 23.9 18.8 28.2
71 33.6 26.3 39.5

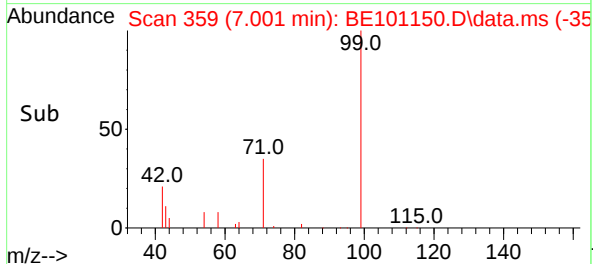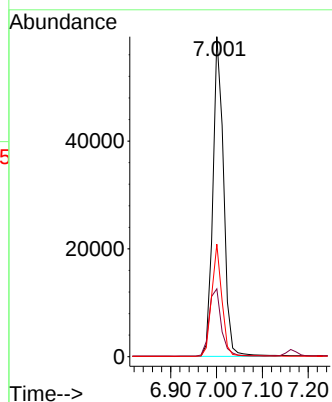

#6
bis(2-Chloroethyl)ether
Concen: 4.51 ng
RT: 7.277 min Scan# 383
Delta R.T. 0.002 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion: 93 Resp: 75787
Ion Ratio Lower Upper
93 100
63 365.0 292.5 438.7
95 32.3 25.8 38.6


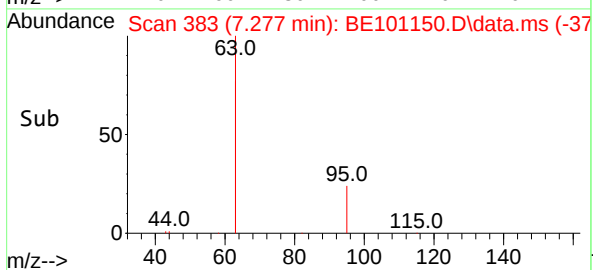
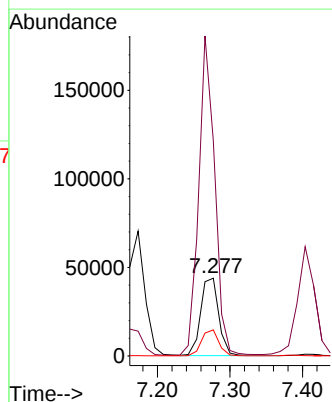
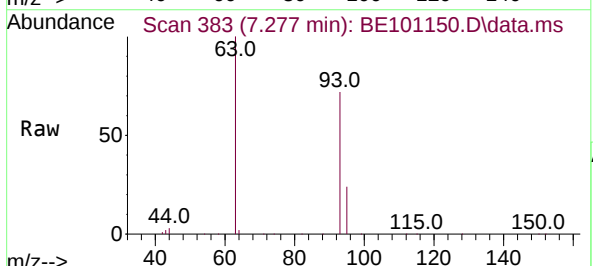




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.628 min Scan# 651
Delta R.T. -0.012 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	21368
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	56.1	20.2	30.4#
68	10.1	4.0	6.0#

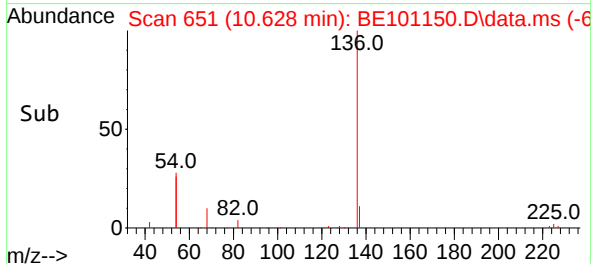

#8
Nitrobenzene-d5
Concen: 6.52 ng
RT: 8.992 min Scan# 525
Delta R.T. 0.001 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:	82	Resp:	73872
Ion	Ratio	Lower	Upper
82	100		
128	136.7	101.5	152.3
54	217.4	189.8	284.6


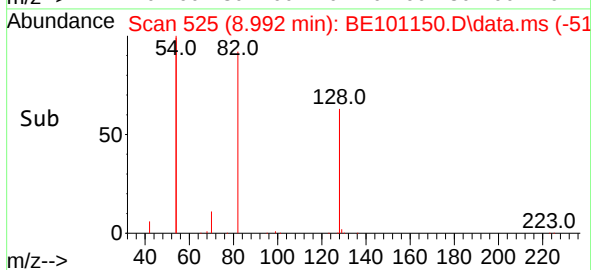

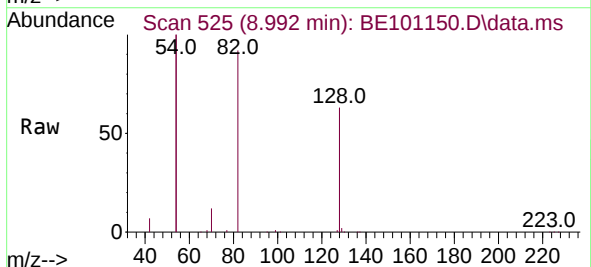


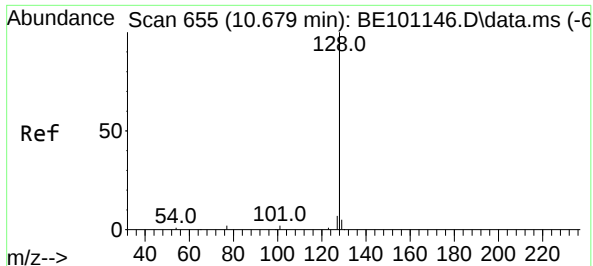

#9
Naphthalene
Concen: 4.78 ng
RT: 10.680 min Scan# 655
Delta R.T. 0.001 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 1039005
Ion Ratio Lower Upper
128 100
129 2.8 2.2 3.2
127 3.3 2.7 4.1

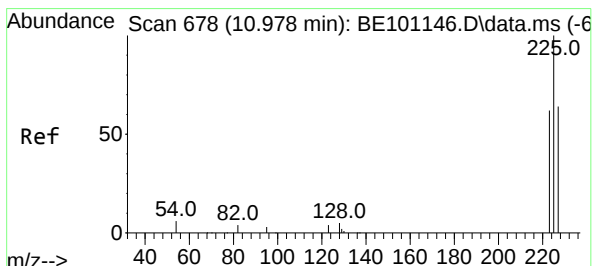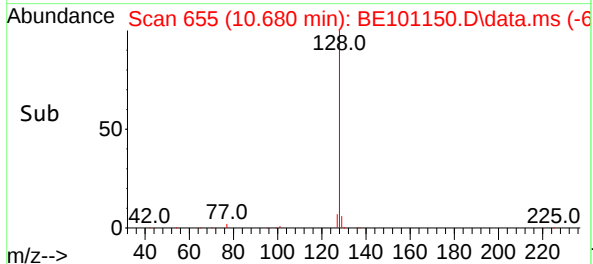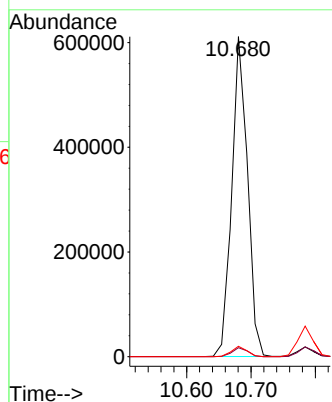

#10
Hexachlorobutadiene
Concen: 4.66 ng
RT: 10.979 min Scan# 678
Delta R.T. 0.001 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:225 Resp: 45953
Ion Ratio Lower Upper
225 100
223 63.0 50.1 75.1
227 63.8 51.7 77.5


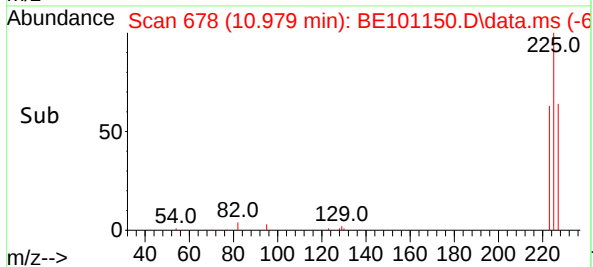
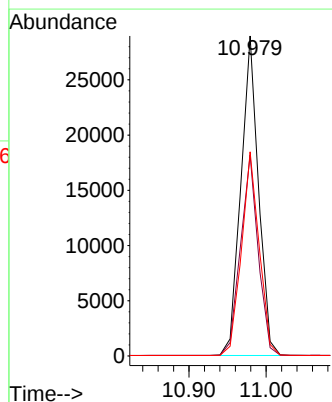
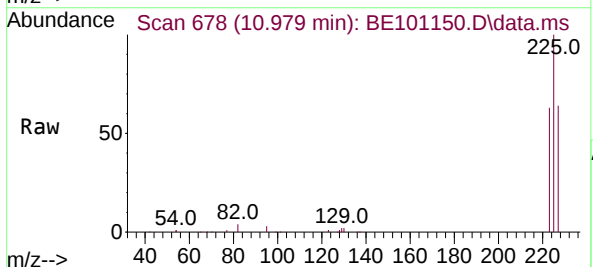


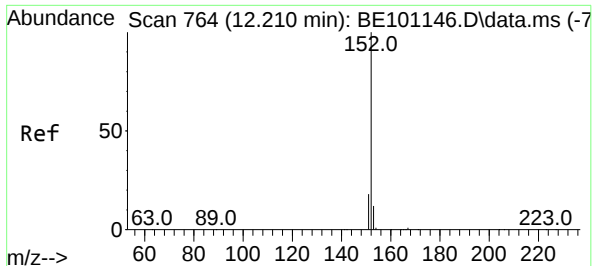

#11
2-Methylnaphthalene-d10
Concen: 5.14 ng
RT: 12.210 min Scan# 764
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 176464
Ion Ratio Lower Upper
152 100
151 20.3 16.6 24.8

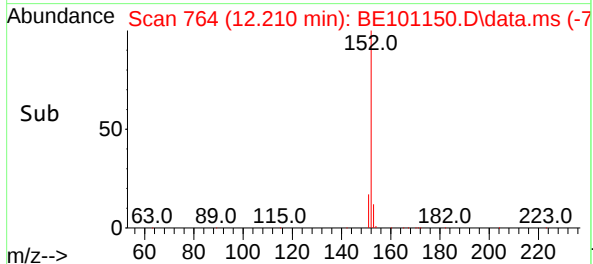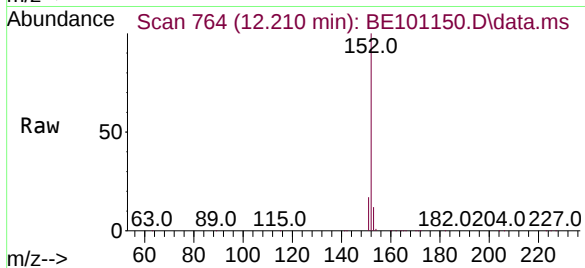

#12
2-Methylnaphthalene
Concen: 5.11 ng
RT: 12.282 min Scan# 769
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05


Tgt Ion:142 Resp: 189692
Ion Ratio Lower Upper
142 100
141 90.4 71.8 107.6
115 34.6 27.8 41.6

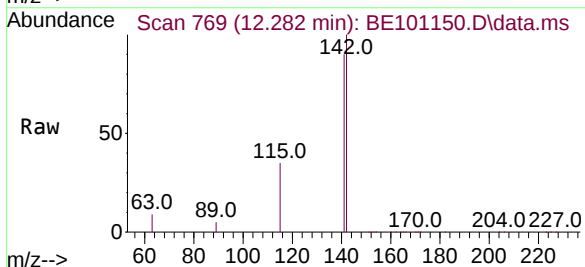



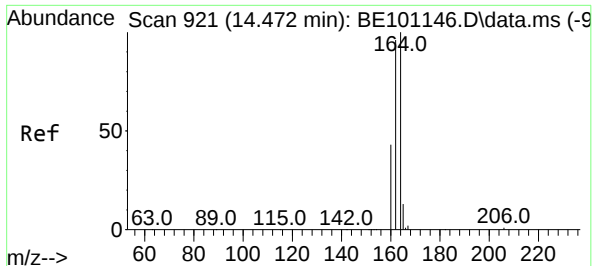


#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.458 min Scan# 920
Delta R.T. -0.014 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0



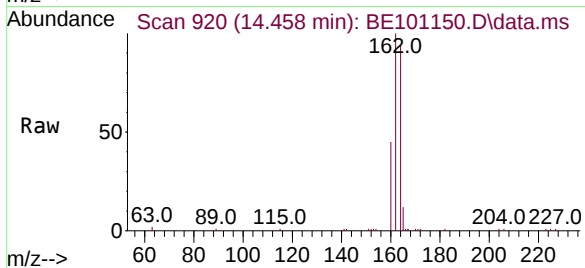



Tgt Ion:164 Resp: 14654
Ion Ratio Lower Upper
164 100
162 106.4 76.6 115.0
160 48.2 34.5 51.7

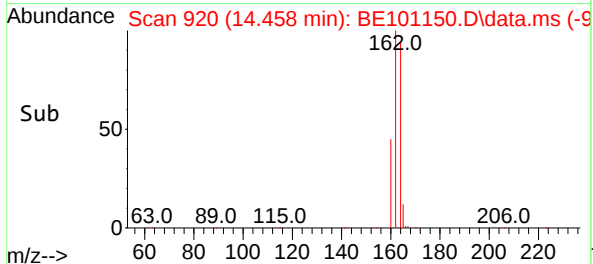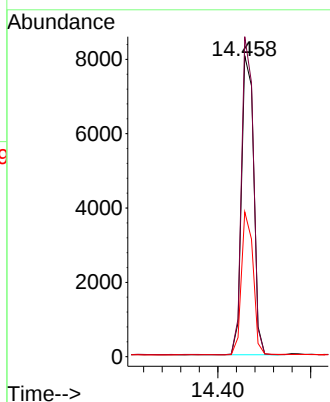

#14
2,4,6-Tribromophenol
Concen: 5.93 ng
RT: 15.971 min Scan# 1017
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:330 Resp: 15619
Ion Ratio Lower Upper
330 100
332 97.9 69.1 103.7
141 41.1 30.6 45.8


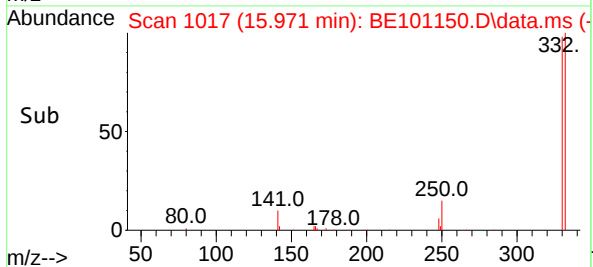

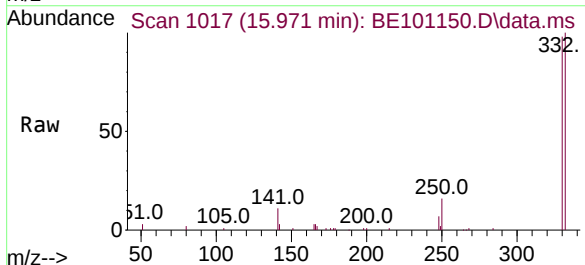




#15
2-Fluorobiphenyl
Concen: 4.30 ng
RT: 13.089 min Scan# 825
Delta R.T. -0.014 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:	172	Resp:	240215
Ion Ratio	Lower	Upper	
172	100		
171	35.8	26.4	39.6
170	24.9	17.4	26.0

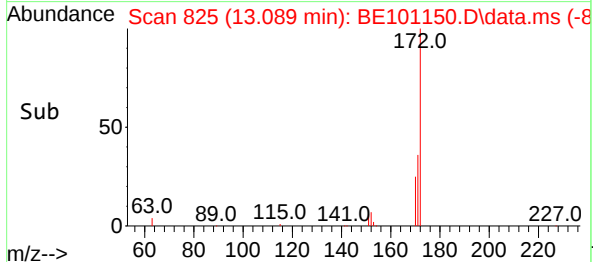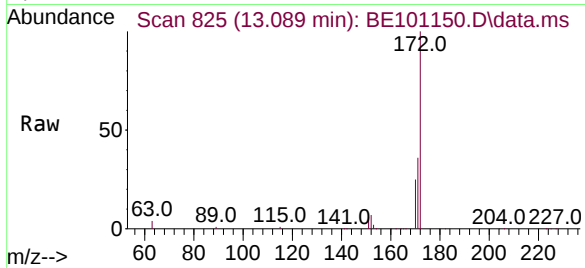

#16
Acenaphthylene
Concen: 5.23 ng
RT: 14.184 min Scan# 901
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:	152	Resp:	297494
Ion Ratio	Lower	Upper	
152	100		
151	19.4	15.4	23.0
153	13.4	10.3	15.5


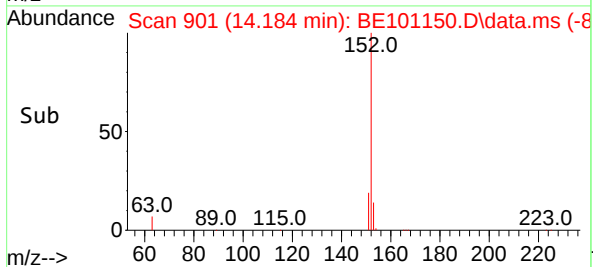

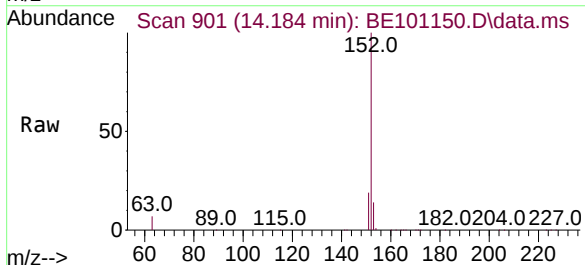




#17
Acenaphthene
Concen: 4.87 ng
RT: 14.530 min Scan# 925
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 198343
Ion Ratio Lower Upper
154 100
153 105.7 86.7 130.1
152 52.5 46.1 69.1

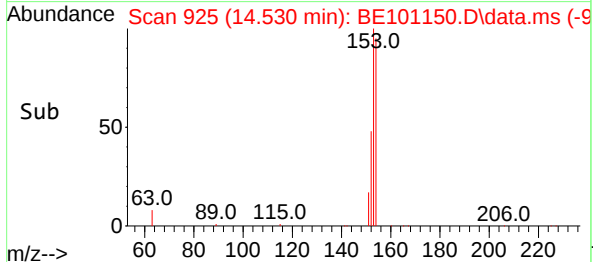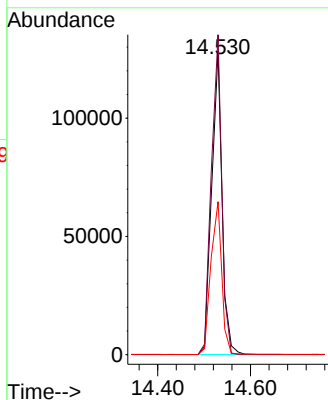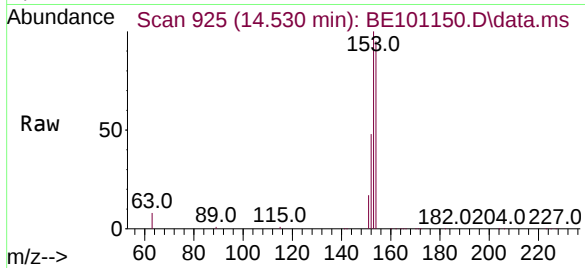

#18
Fluorene
Concen: 4.86 ng
RT: 15.517 min Scan# 987
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:166 Resp: 258397
Ion Ratio Lower Upper
166 100
165 97.6 78.9 118.3
167 13.9 10.7 16.1


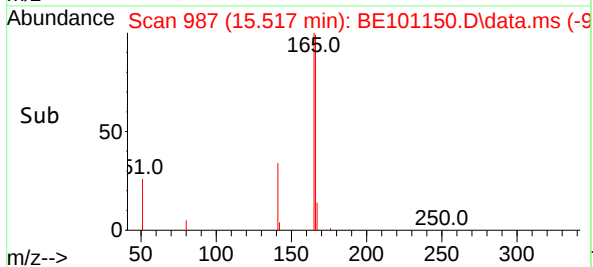
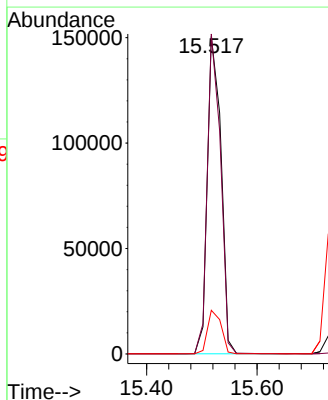
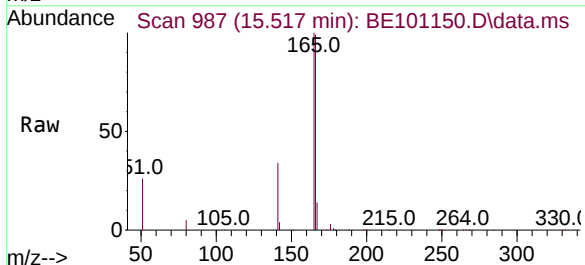


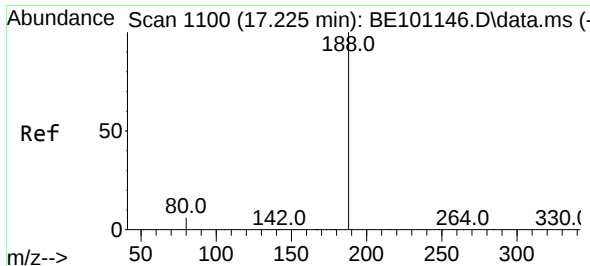

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.226 min Scan# 1100
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:	188	Resp:	34110
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	5.8	4.8	7.2

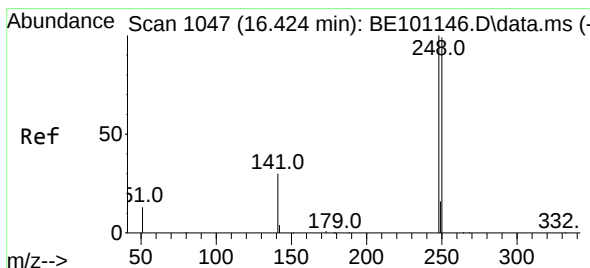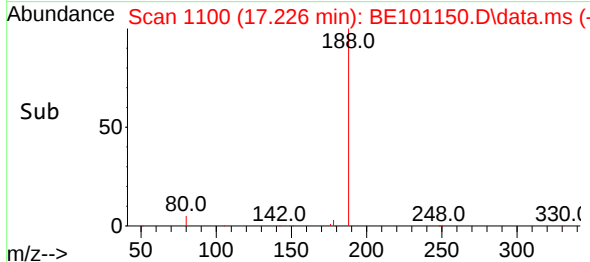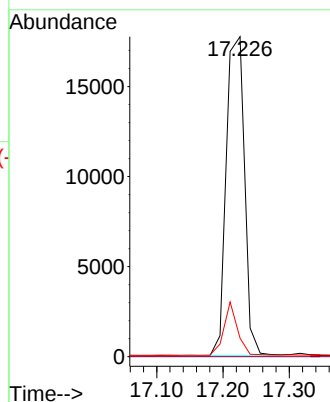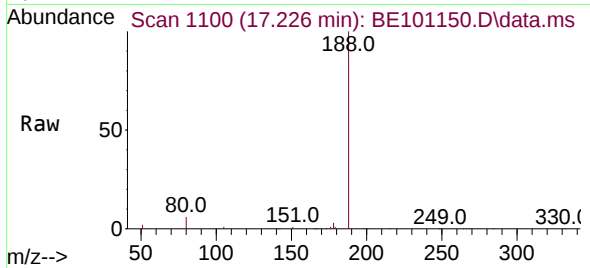

#21
4-Bromophenyl-phenylether
Concen: 4.54 ng
RT: 16.424 min Scan# 1047
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:	248	Resp:	74408
Ion Ratio	Lower	Upper	
248	100		
250	103.4	79.0	118.6
141	26.3	24.9	37.3


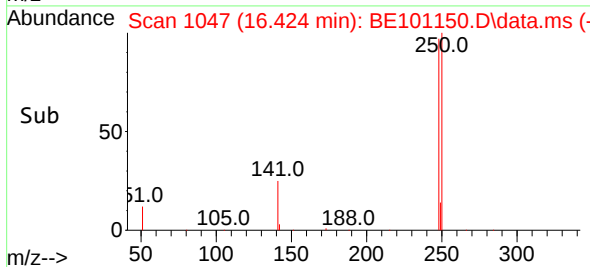

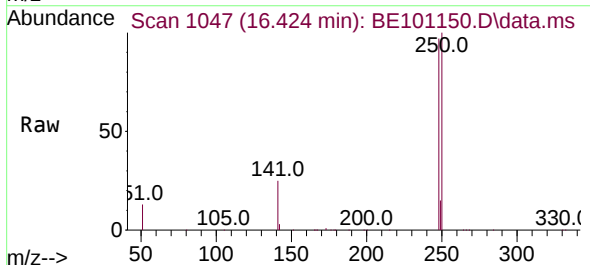




#22
Hexachlorobenzene
Concen: 4.78 ng
RT: 16.530 min Scan# 1054
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:284 Resp: 80634
Ion Ratio Lower Upper
284 100
142 34.4 28.3 42.5
249 34.1 27.1 40.7

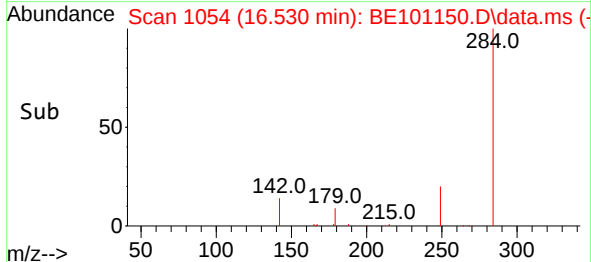

#24
Pentachlorophenol
Concen: 8.36 ng
RT: 16.863 min Scan# 1076
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:266 Resp: 31573
Ion Ratio Lower Upper
266 100
264 62.8 51.4 77.0
268 64.5 49.9 74.9


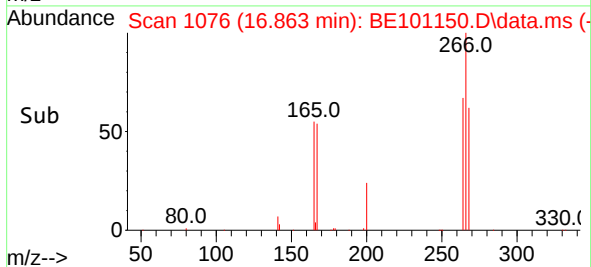

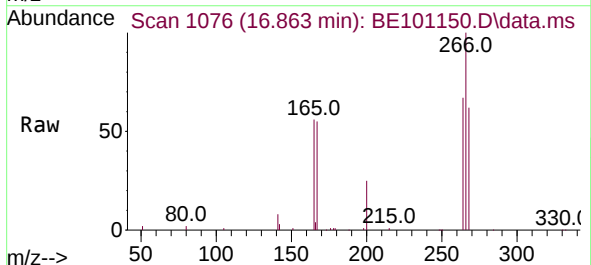


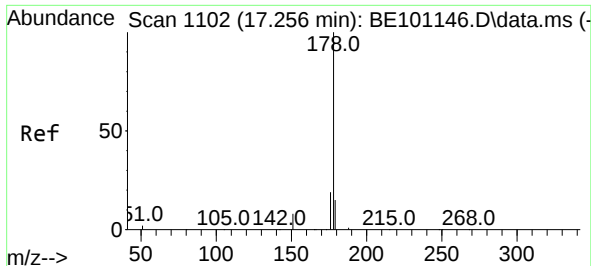

#25
Phenanthrene
Concen: 4.89 ng
RT: 17.256 min Scan# 1102
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 465369
Ion Ratio Lower Upper
178 100
176 19.1 14.7 22.1
179 15.7 12.4 18.6

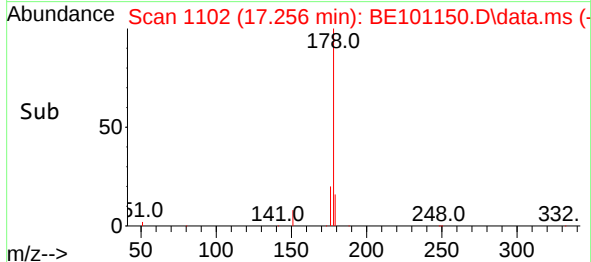

#26
Anthracene
Concen: 5.40 ng
RT: 17.347 min Scan# 1108
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:178 Resp: 443313
Ion Ratio Lower Upper
178 100
176 18.7 14.4 21.6
179 15.9 12.2 18.4


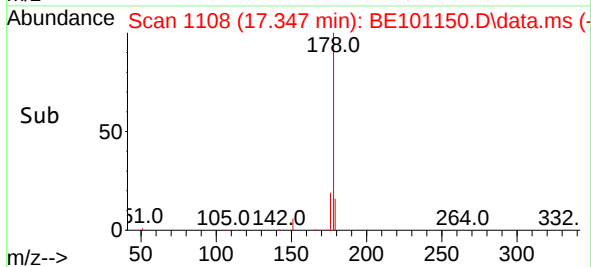

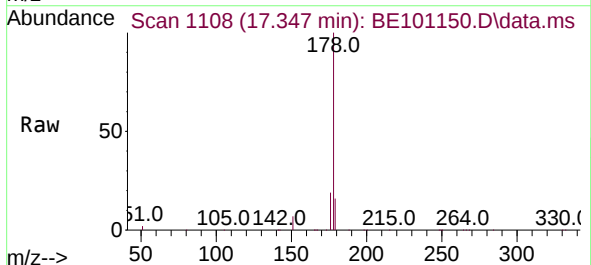




#27
Fluoranthene-d10
Concen: 4.96 ng
RT: 19.232 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 2205230
Ion Ratio Lower Upper
212 100
106 3.4 2.6 3.8
104 1.9 1.4 2.2

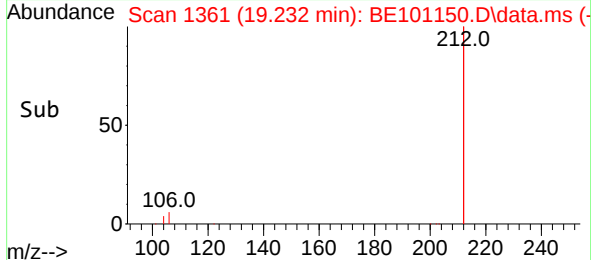

#28
Fluoranthene
Concen: 4.91 ng
RT: 19.261 min Scan# 1366
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:202 Resp: 611936
Ion Ratio Lower Upper
202 100
101 11.7 8.9 13.3
203 18.1 13.8 20.6


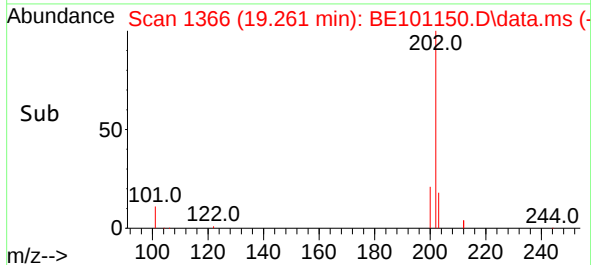

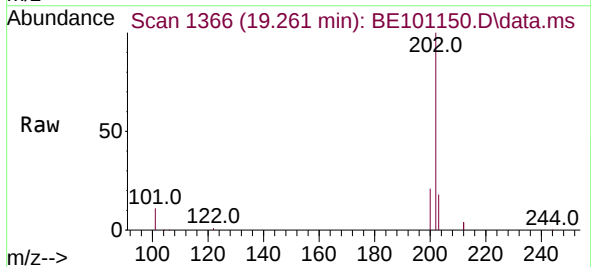


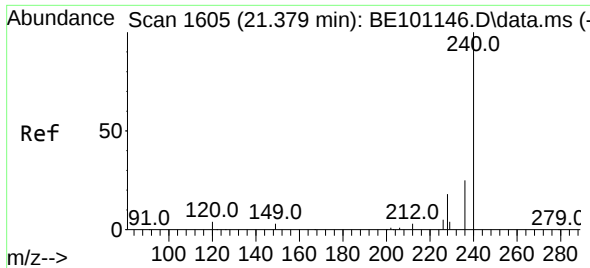

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.378 min Scan# 1605
Delta R.T. -0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:240	Resp:	46243
Ion Ratio	Lower	Upper
240	100	
120	4.7	4.1 6.1
236	25.2	20.3 30.5

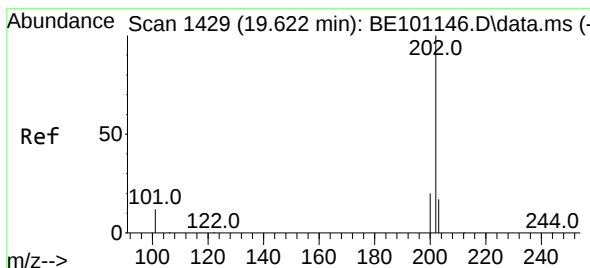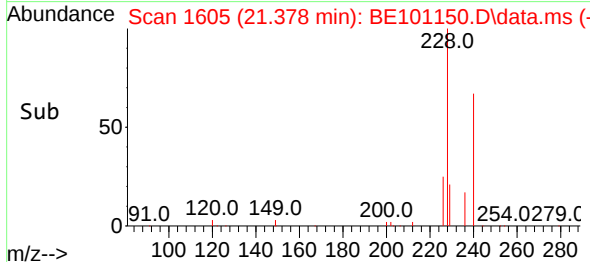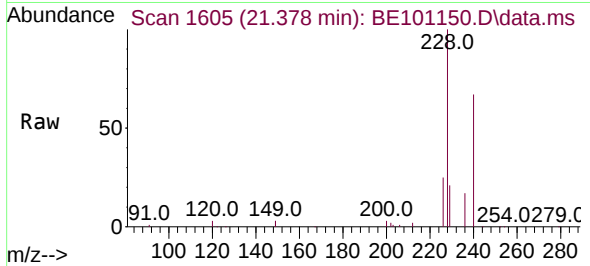

#30
Pyrene
Concen: 4.81 ng
RT: 19.623 min Scan# 1429
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:202	Resp:	628395
Ion Ratio	Lower	Upper
202	100	
200	21.2	16.2 24.2
203	18.1	13.9 20.9


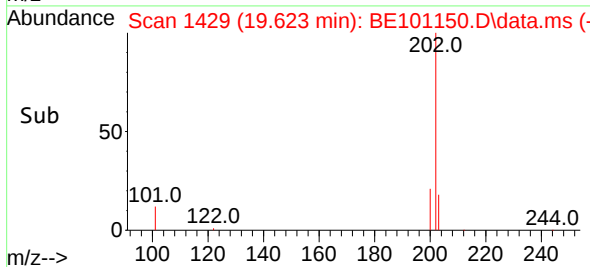

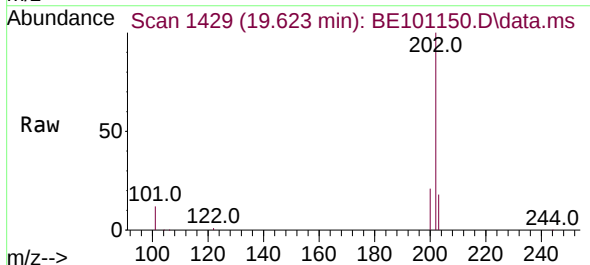


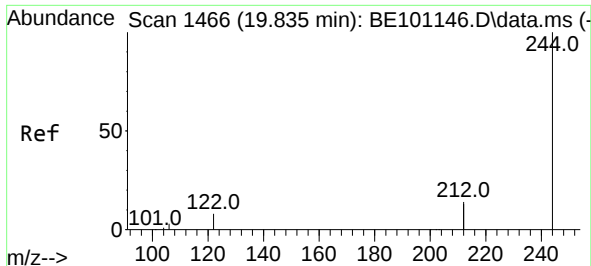

#31
 Terphenyl-d14
 Concen: 4.74 ng
 RT: 19.830 min Scan# 1465
 Delta R.T. -0.005 min
 Lab File: BE101150.D
 Acq: 24 Mar 2021 15:05




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:244 Resp: 478403
 Ion Ratio Lower Upper
 244 100
 212 30.0 21.7 32.5
 122 11.5 6.6 10.0#

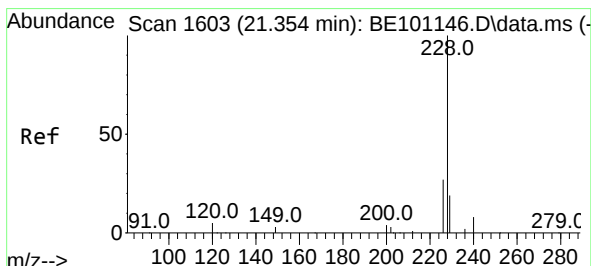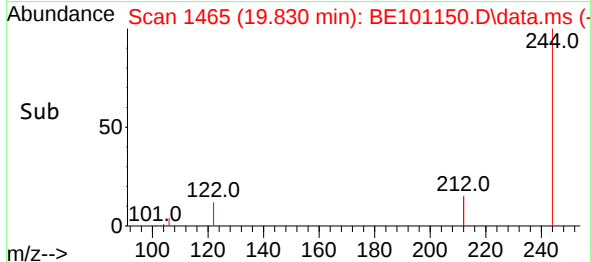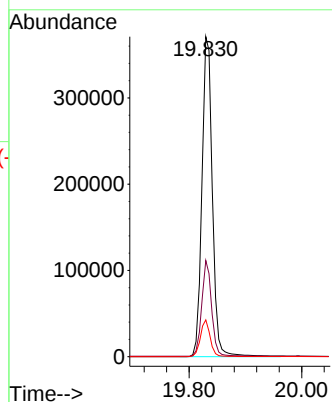

#32
 Benzo(a)anthracene
 Concen: 5.19 ng
 RT: 21.354 min Scan# 1603
 Delta R.T. -0.000 min
 Lab File: BE101150.D
 Acq: 24 Mar 2021 15:05

Tgt Ion:228 Resp: 612219
 Ion Ratio Lower Upper
 228 100
 226 28.2 21.8 32.8
 229 20.2 15.4 23.0


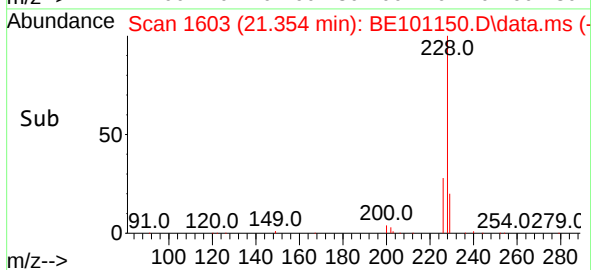
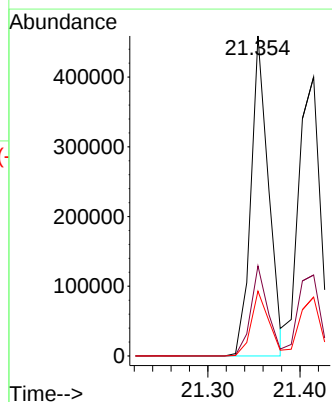
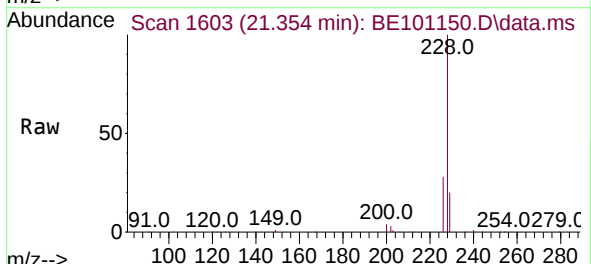


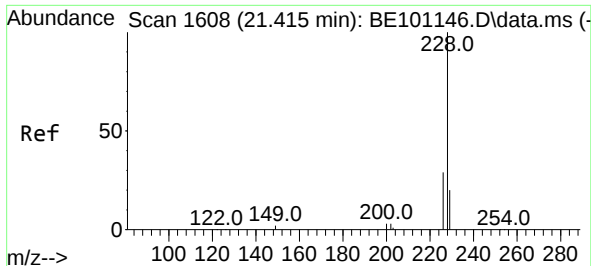

#33
Chrysene
Concen: 4.73 ng
RT: 21.415 min Scan# 1608
Delta R.T. -0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05




Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 660240
Ion Ratio Lower Upper
228 100
226 29.0 22.8 34.2
229 21.1 16.2 24.2

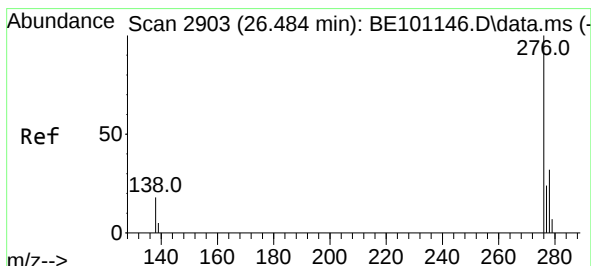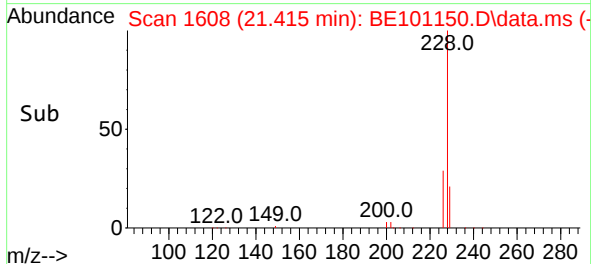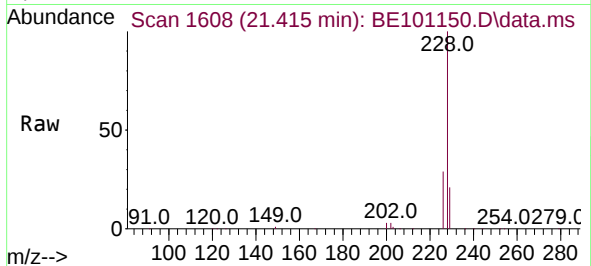

#35
Indeno(1,2,3-cd)pyrene
Concen: 6.03 ng
RT: 26.488 min Scan# 2904
Delta R.T. 0.004 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:276 Resp: 537157
Ion Ratio Lower Upper
276 100
138 21.9 17.1 25.7
277 25.2 19.8 29.8


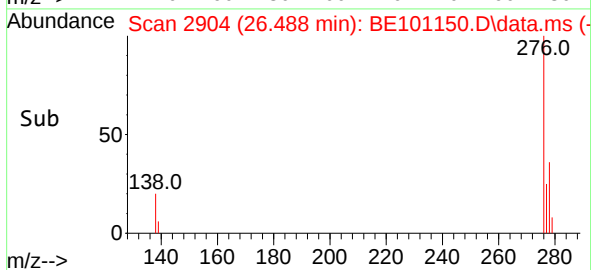

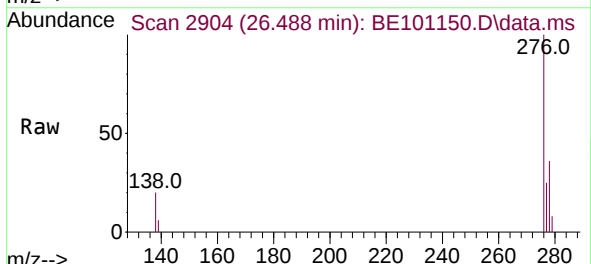




#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.860 min Scan# 2171
 Delta R.T. -0.003 min
 Lab File: BE101150.D
 Acq: 24 Mar 2021 15:05




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:264	Resp:	36533
Ion Ratio	Lower	Upper
264	100	
260	25.2	20.5 30.7
265	24.8	20.6 30.8

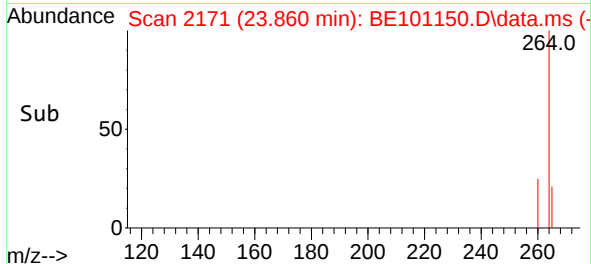

#37
 Benzo(b)fluoranthene
 Concen: 5.72 ng
 RT: 23.101 min Scan# 1958
 Delta R.T. 0.000 min
 Lab File: BE101150.D
 Acq: 24 Mar 2021 15:05


Tgt Ion:252	Resp:	541423
Ion Ratio	Lower	Upper
252	100	
253	22.4	17.8 26.8
125	8.8	7.5 11.3

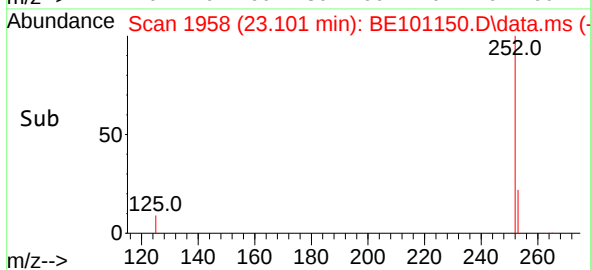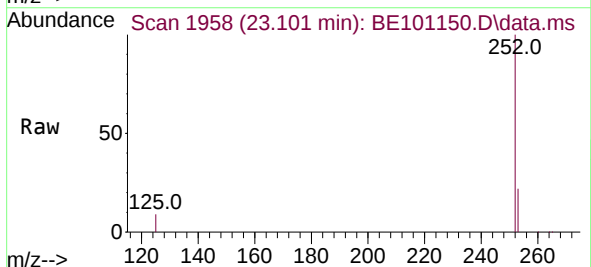


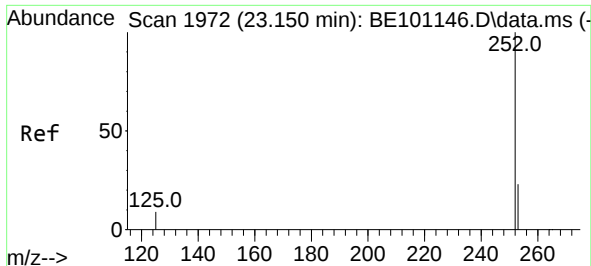


#38
Benzo(k)fluoranthene
Concen: 4.94 ng
RT: 23.151 min Scan# 1972
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0







Tgt Ion:252 Resp: 630754
Ion Ratio Lower Upper
252 100
253 22.6 18.2 27.4
125 8.7 7.5 11.3



#39
Benzo(a)pyrene
Concen: 5.73 ng
RT: 23.749 min Scan# 2140
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:252 Resp: 513079
Ion Ratio Lower Upper
252 100
253 22.4 18.6 28.0
125 9.8 8.3 12.5


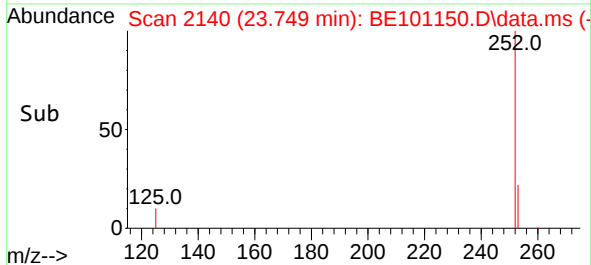

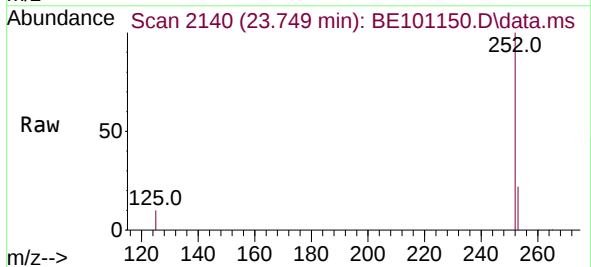


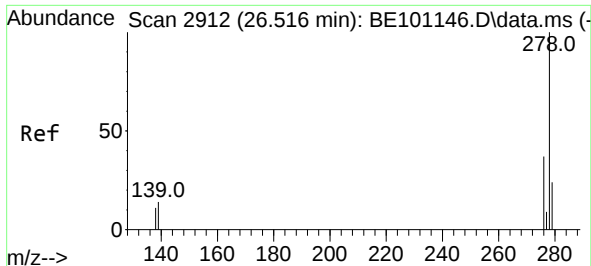

#40
Dibenzo(a,h)anthracene
Concen: 6.49 ng
RT: 26.516 min Scan# 2912
Delta R.T. 0.000 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Instrument :
BNA_E
ClientSampleId :
SSTDICC5.0

Tgt Ion:278 Resp: 460547
Ion Ratio Lower Upper
278 100
139 14.5 12.0 18.0
279 23.9 20.2 30.4

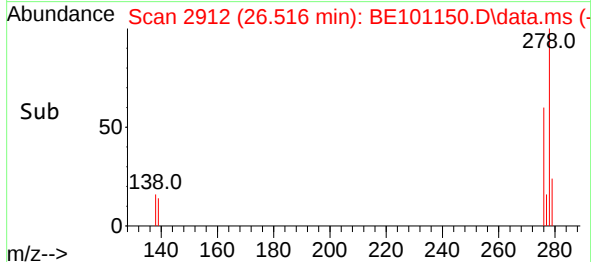

#41
Benzo(g,h,i)perylene
Concen: 5.50 ng
RT: 27.294 min Scan# 3130
Delta R.T. 0.004 min
Lab File: BE101150.D
Acq: 24 Mar 2021 15:05

Tgt Ion:276 Resp: 500642
Ion Ratio Lower Upper
276 100
277 24.4 19.7 29.5
138 19.3 15.3 22.9

