

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE032421\
 Data File : BE101151.D
 Acq On : 24 Mar 2021 17:26
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 ICVBE032421

Quant Time: Mar 24 18:12:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE032421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 24 16:00:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.850	152	4124	0.40	ng	0.00
7) Naphthalene-d8	10.641	136	17099	0.40	ng	0.00
13) Acenaphthene-d10	14.472	164	10870	0.40	ng	0.00
19) Phenanthrene-d10	17.225	188	28627	0.40	ng	0.00
29) Chrysene-d12	21.378	240	30446	0.40	ng	0.00
36) Perylene-d12	23.863	264	28796	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.431	112	4489	0.46	ng	0.00
5) Phenol-d6	6.997	99	6887	0.46	ng	0.00
8) Nitrobenzene-d5	8.991	82	4912	0.48	ng	0.00
11) 2-Methylnaphthalene-d10	12.210	152	11893	0.43	ng	0.00
14) 2,4,6-Tribromophenol	15.970	330	640	0.33	ng	0.00
15) 2-Fluorobiphenyl	13.103	172	17565	0.43	ng	0.00
27) Fluoranthene-d10	19.232	212	150733	0.42	ng	0.00
31) Terphenyl-d14	19.835	244	32408	0.47	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.381	88	3085	0.46	ng	97
3) n-Nitrosodimethylamine	3.681	42	3432	0.49	ng	# 94
6) bis(2-Chloroethyl)ether	7.274	93	5744	0.45	ng	98
9) Naphthalene	10.680	128	78341	0.45	ng	100
10) Hexachlorobutadiene	10.979	225	3487	0.44	ng	100
12) 2-Methylnaphthalene	12.282	142	13043	0.44	ng	99
16) Acenaphthylene	14.184	152	16755	0.40	ng	100
17) Acenaphthene	14.530	154	12390	0.41	ng	100
18) Fluorene	15.532	166	16138	0.41	ng	100
20) 4,6-Dinitro-2-methylph...	15.592	198	680	0.47	ng	# 85
21) 4-Bromophenyl-phenylether	16.424	248	4463	0.35	ng	98
22) Hexachlorobenzene	16.530	284	5805	0.41	ng	98
23) Atrazine	16.681	200	3247	0.40	ng	98
24) Pentachlorophenol	16.877	266	1233	0.50	ng	96
25) Phenanthrene	17.255	178	34462	0.43	ng	99
26) Anthracene	17.346	178	28857	0.42	ng	100
28) Fluoranthene	19.261	202	42361	0.42	ng	100
30) Pyrene	19.623	202	42151	0.47	ng	100
32) Benzo(a)anthracene	21.354	228	35913	0.46	ng	99
33) Chrysene	21.415	228	42128	0.45	ng	100
34) Bis(2-ethylhexyl)phtha...	21.306	149	21176	0.41	ng	100
35) Indeno(1,2,3-cd)pyrene	26.487	276	28604	0.47	ng	100
37) Benzo(b)fluoranthene	23.100	252	30462	0.40	ng	99
38) Benzo(k)fluoranthene	23.150	252	40878	0.42	ng	99
39) Benzo(a)pyrene	23.749	252	26659	0.38	ng	99
40) Dibenzo(a,h)anthracene	26.520	278	23389	0.42	ng	99
41) Benzo(g,h,i)perylene	27.293	276	30483	0.42	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE032421\
Data File : BE101151.D
Acq On : 24 Mar 2021 17:26
Operator : CG/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
ICVBE032421

Quant Time: Mar 24 18:12:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE032421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 16:00:06 2021
Response via : Initial Calibration







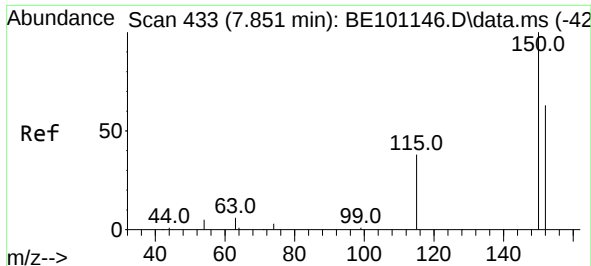

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.850 min Scan# 433
 Delta R.T. -0.001 min
 Lab File: BE101151.D
 Acq: 24 Mar 2021 17:26




Instrument :
 BNA_E
 ClientSampleId :
 ICVBE032421


Tgt Ion:152 Resp: 4124
 Ion Ratio Lower Upper
 152 100
 150 155.5 126.3 189.5
 115 60.5 48.9 73.3



#2
 1,4-Dioxane
 Concen: 0.46 ng
 RT: 3.381 min Scan# 45
 Delta R.T. -0.002 min
 Lab File: BE101151.D
 Acq: 24 Mar 2021 17:26

Tgt Ion: 88 Resp: 3085
 Ion Ratio Lower Upper
 88 100
 58 89.0 68.5 102.7
 43 35.5 27.2 40.8







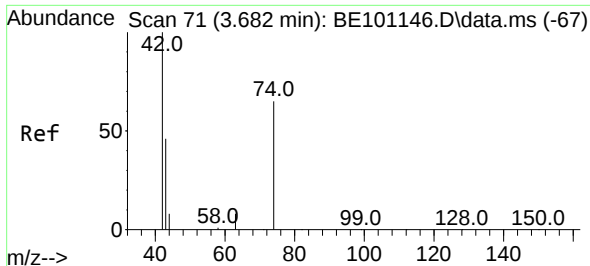

#3
n-Nitrosodimethylamine
Concen: 0.49 ng
RT: 3.681 min Scan# 71
Delta R.T. -0.002 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion: 42 Resp: 3432
Ion Ratio Lower Upper
42 100
74 102.8 87.0 130.6
44 14.7 8.3 12.5#

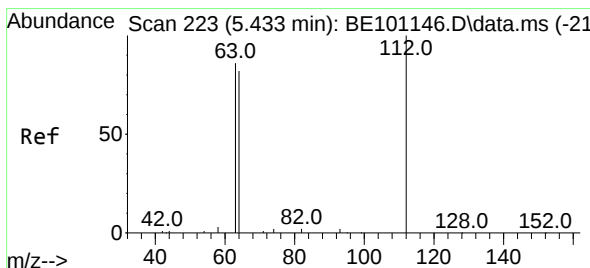

#4
2-Fluorophenol
Concen: 0.46 ng
RT: 5.431 min Scan# 223
Delta R.T. -0.002 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion: 112 Resp: 4489
Ion Ratio Lower Upper
112 100
64 74.9 60.8 91.2
63 151.1 119.4 179.0









#5
Phenol-d6
Concen: 0.46 ng
RT: 6.997 min Scan# 359
Delta R.T. -0.002 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:	99	Resp:	6887
Ion	Ratio	Lower	Upper
99	100		
42	24.5	18.8	28.2
71	33.1	26.3	39.5



#6
bis(2-Chloroethyl)ether
Concen: 0.45 ng
RT: 7.274 min Scan# 383
Delta R.T. -0.002 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:	93	Resp:	5744
Ion	Ratio	Lower	Upper
93	100		
63	370.5	292.5	438.7
95	32.9	25.8	38.6









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.641 min Scan# 652
Delta R.T. 0.001 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:	136	Resp:	17099
Ion Ratio	Lower	Upper	
136	100		
137	11.8	8.9	13.3
54	24.0	20.2	30.4
68	5.7	4.0	6.0



#8
Nitrobenzene-d5
Concen: 0.48 ng
RT: 8.991 min Scan# 525
Delta R.T. 0.001 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:	82	Resp:	4912
Ion Ratio	Lower	Upper	
82	100		
128	130.8	101.5	152.3
54	221.1	189.8	284.6









#9
Naphthalene
Concen: 0.45 ng
RT: 10.680 min Scan# 655
Delta R.T. 0.001 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:	128	Resp:	78341
Ion	Ratio	Lower	Upper
128	100		
129	2.9	2.2	3.2
127	3.3	2.7	4.1

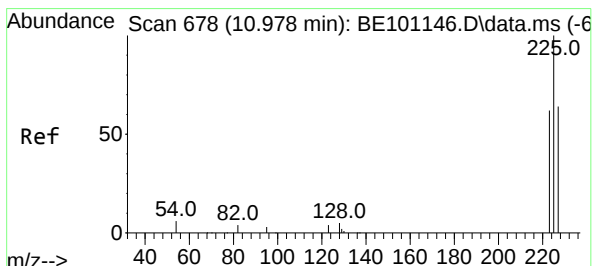

#10
Hexachlorobutadiene
Concen: 0.44 ng
RT: 10.979 min Scan# 678
Delta R.T. 0.001 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:	225	Resp:	3487
Ion	Ratio	Lower	Upper
225	100		
223	62.8	50.1	75.1
227	64.7	51.7	77.5









#11
2-Methylnaphthalene-d10
Concen: 0.43 ng
RT: 12.210 min Scan# 764
Delta R.T. 0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:152 Resp: 11893
Ion Ratio Lower Upper
152 100
151 20.8 16.6 24.8



#12
2-Methylnaphthalene
Concen: 0.44 ng
RT: 12.282 min Scan# 769
Delta R.T. 0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:142 Resp: 13043
Ion Ratio Lower Upper
142 100
141 90.5 71.8 107.6
115 34.3 27.8 41.6







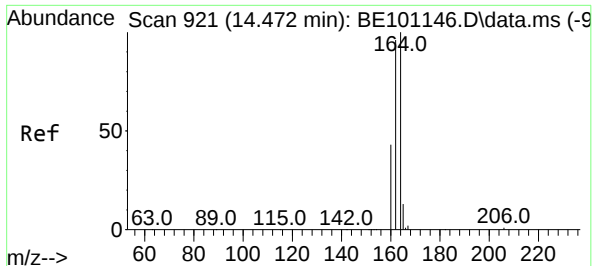

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.472 min Scan# 921
Delta R.T. 0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:164	Resp:	10870
Ion Ratio	Lower	Upper
164	100	
162	98.5	76.6 115.0
160	43.3	34.5 51.7



#14
2,4,6-Tribromophenol
Concen: 0.33 ng
RT: 15.970 min Scan# 1017
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:330	Resp:	640
Ion Ratio	Lower	Upper
330	100	
332	99.8	69.1 103.7
141	41.7	30.6 45.8









#15
2-Fluorobiphenyl
Concen: 0.43 ng
RT: 13.103 min Scan# 826
Delta R.T. 0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:	172	Resp:	17565
Ion Ratio	Lower	Upper	
172	100		
171	33.2	26.4	39.6
170	21.8	17.4	26.0



#16
Acenaphthylene
Concen: 0.40 ng
RT: 14.184 min Scan# 901
Delta R.T. 0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:	152	Resp:	16755
Ion Ratio	Lower	Upper	
152	100		
151	19.1	15.4	23.0
153	13.1	10.3	15.5









#17
Acenaphthene
Concen: 0.41 ng
RT: 14.530 min Scan# 925
Delta R.T. 0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:154 Resp: 12390
Ion Ratio Lower Upper
154 100
153 108.2 86.7 130.1
152 56.9 46.1 69.1



#18
Fluorene
Concen: 0.41 ng
RT: 15.532 min Scan# 988
Delta R.T. 0.015 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:166 Resp: 16138
Ion Ratio Lower Upper
166 100
165 98.8 78.9 118.3
167 13.4 10.7 16.1







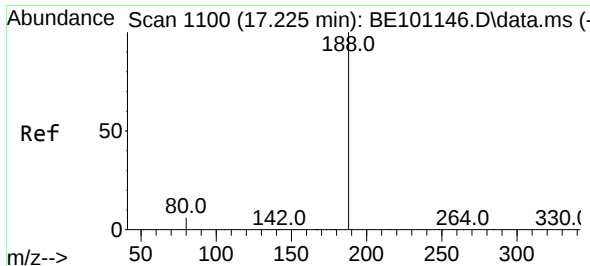

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.225 min Scan# 1100
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	6.1	4.8	7.2



#20
4,6-Dinitro-2-methylphenol
Concen: 0.47 ng
RT: 15.592 min Scan# 992
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion	Ratio	Lower	Upper
198	100		
51	65.9	68.8	103.2#
105	40.2	32.7	49.1









#21
4-Bromophenyl-phenylether
Concen: 0.35 ng
RT: 16.424 min Scan# 1047
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:248 Resp: 4463
Ion Ratio Lower Upper
248 100
250 98.7 79.0 118.6
141 35.8 24.9 37.3



#22
Hexachlorobenzene
Concen: 0.41 ng
RT: 16.530 min Scan# 1054
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:284 Resp: 5805
Ion Ratio Lower Upper
284 100
142 33.7 28.3 42.5
249 35.0 27.1 40.7









#23
Atrazine
Concen: 0.40 ng
RT: 16.681 min Scan# 1064
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:	200	Resp:	3247
Ion Ratio	Lower	Upper	
200	100		
173	31.8	23.9	35.9
215	51.5	40.6	61.0



#24
Pentachlorophenol
Concen: 0.50 ng
RT: 16.877 min Scan# 1077
Delta R.T. 0.014 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:	266	Resp:	1233
Ion Ratio	Lower	Upper	
266	100		
264	60.8	51.4	77.0
268	64.6	49.9	74.9









#25
Phenanthrene
Concen: 0.43 ng
RT: 17.255 min Scan# 1102
Delta R.T. -0.001 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:178 Resp: 34462
Ion Ratio Lower Upper
178 100
176 18.7 14.7 22.1
179 15.0 12.4 18.6



#26
Anthracene
Concen: 0.42 ng
RT: 17.346 min Scan# 1108
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:178 Resp: 28857
Ion Ratio Lower Upper
178 100
176 18.2 14.4 21.6
179 15.3 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.42 ng
RT: 19.232 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:212 Resp: 150733
Ion Ratio Lower Upper
212 100
106 3.1 2.6 3.8
104 1.8 1.4 2.2



#28
Fluoranthene
Concen: 0.42 ng
RT: 19.261 min Scan# 1366
Delta R.T. 0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:202 Resp: 42361
Ion Ratio Lower Upper
202 100
101 11.0 8.9 13.3
203 17.3 13.8 20.6









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.378 min Scan# 1605
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:240	Resp:	30446
Ion Ratio	Lower	Upper
240	100	
120	5.1	4.1 6.1
236	25.9	20.3 30.5



#30
Pyrene
Concen: 0.47 ng
RT: 19.623 min Scan# 1429
Delta R.T. 0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:202	Resp:	42151
Ion Ratio	Lower	Upper
202	100	
200	20.4	16.2 24.2
203	17.5	13.9 20.9









#31
 Terphenyl-d14
 Concen: 0.47 ng
 RT: 19.835 min Scan# 1466
 Delta R.T. 0.000 min
 Lab File: BE101151.D
 Acq: 24 Mar 2021 17:26




Instrument :
 BNA_E
 ClientSampleId :
 ICVBE032421


Tgt Ion:244	Resp:	32408
Ion Ratio	Lower	Upper
244	100	
212	26.5	21.7 32.5
122	8.6	6.6 10.0



#32
 Benzo(a)anthracene
 Concen: 0.46 ng
 RT: 21.354 min Scan# 1603
 Delta R.T. -0.000 min
 Lab File: BE101151.D
 Acq: 24 Mar 2021 17:26

Tgt Ion:228	Resp:	35913
Ion Ratio	Lower	Upper
228	100	
226	26.8	21.8 32.8
229	19.4	15.4 23.0









#33
Chrysene
Concen: 0.45 ng
RT: 21.415 min Scan# 1608
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:	228	Resp:	42128
Ion Ratio	Lower	Upper	
228	100		
226	28.5	22.8	34.2
229	20.1	16.2	24.2



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.41 ng
RT: 21.306 min Scan# 1599
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:	149	Resp:	21176
Ion Ratio	Lower	Upper	
149	100		
167	6.9	5.4	8.2
279	1.2	0.9	1.3









#35
Indeno(1,2,3-cd)pyrene
Concen: 0.47 ng
RT: 26.487 min Scan# 2904
Delta R.T. 0.004 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:	276	Resp:	28604
Ion Ratio	Lower	Upper	
276	100		
138	21.3	17.1	25.7
277	24.5	19.8	29.8



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.863 min Scan# 2172
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:	264	Resp:	28796
Ion Ratio	Lower	Upper	
264	100		
260	24.9	20.5	30.7
265	25.8	20.6	30.8









#37
Benzo(b)fluoranthene
Concen: 0.40 ng
RT: 23.100 min Scan# 1958
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26




Instrument :
BNA_E
ClientSampleId :
ICVBE032421


Tgt Ion:252 Resp: 30462
Ion Ratio Lower Upper
252 100
253 22.7 17.8 26.8
125 9.3 7.5 11.3



#38
Benzo(k)fluoranthene
Concen: 0.42 ng
RT: 23.150 min Scan# 1972
Delta R.T. -0.000 min
Lab File: BE101151.D
Acq: 24 Mar 2021 17:26

Tgt Ion:252 Resp: 40878
Ion Ratio Lower Upper
252 100
253 22.2 18.2 27.4
125 9.6 7.5 11.3





#39

Benzo(a)pyrene

Concen: 0.38 ng

RT: 23.749 min Scan# 2140

Delta R.T. -0.000 min

Lab File: BE101151.D

Acq: 24 Mar 2021 17:26





Tgt Ion:	252	Resp:	26659
Ion Ratio	Lower	Upper	
252	100		
253	22.6	18.6	28.0
125	10.9	8.3	12.5

Instrument :

BNA_E

ClientSampleId :

ICVBE032421



#40

Dibenzo(a,h)anthracene

Concen: 0.42 ng




RT: 26.520 min Scan# 2913


Delta R.T. 0.004 min

Lab File: BE101151.D

Acq: 24 Mar 2021 17:26

Tgt Ion:	278	Resp:	23389
Ion Ratio	Lower	Upper	
278	100		
139	15.5	12.0	18.0
279	24.9	20.2	30.4





#41
 Benzo(g,h,i)perylene
 Concen: 0.42 ng
 RT: 27.293 min Scan# 3130
 Delta R.T. 0.004 min
 Lab File: BE101151.D
 Acq: 24 Mar 2021 17:26

Instrument :
 BNA_E
 ClientSampleId :
 ICVBE032421

Tgt Ion:	276	Resp:	30483
Ion Ratio	Lower	Upper	
276	100		
277	25.6	19.7	29.5
138	19.3	15.3	22.9

