
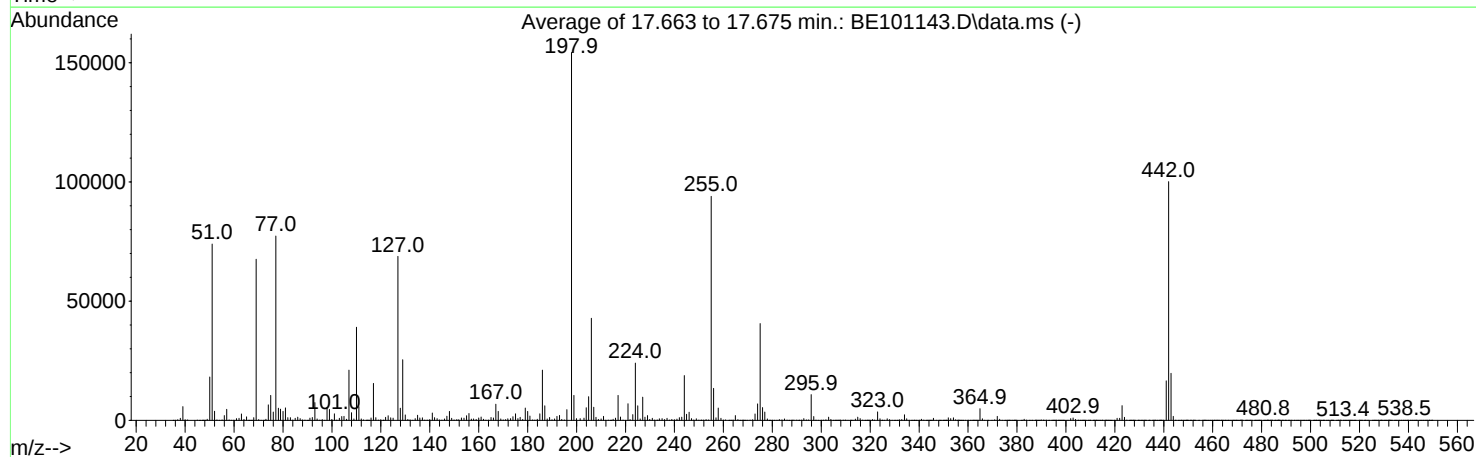


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE032421\
 Data File : BE101143.D
 Acq On : 24 Mar 2021 10:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE032421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 24 16:00:06 2021

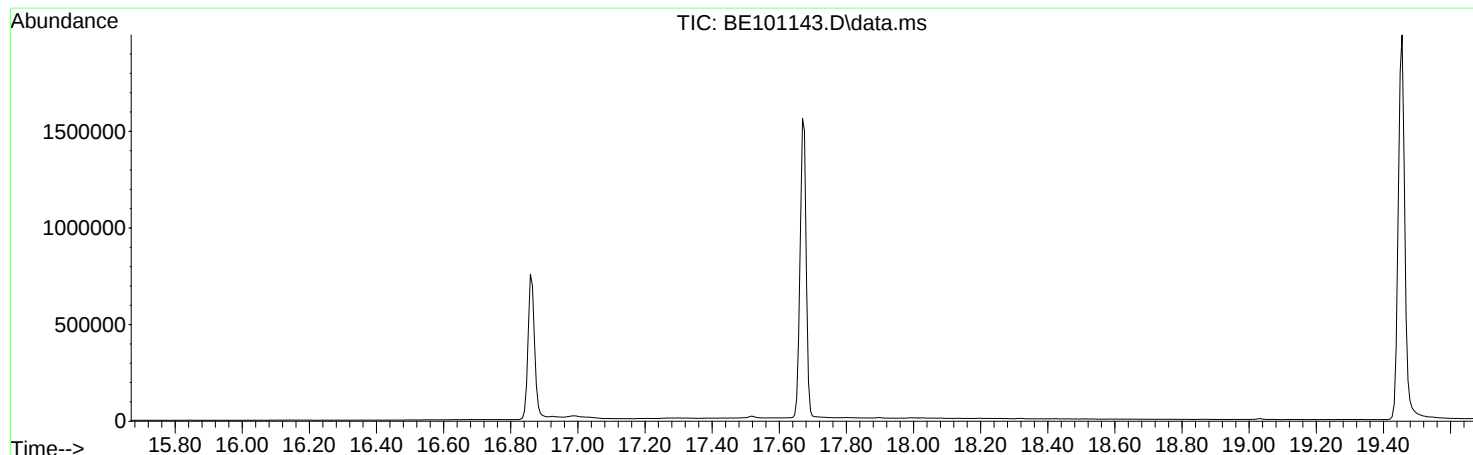




AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	73926	PASS
68	69	0.00	2	1.7	1169	PASS
69	198	0.00	100	43.8	67547	PASS
70	69	0.00	2	0.5	368	PASS
127	198	10	80	44.6	68768	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	154285	PASS
199	198	5	9	6.8	10488	PASS
275	198	10	60	26.3	40611	PASS
365	198	1	100	3.2	4916	PASS
441	198	0.01	100	10.7	16581	PASS
442	442	50	100	100.0	100156	PASS
443	442	15	24	19.7	19728	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE032421\
 Data File : BE101143.D
 Acq On : 24 Mar 2021 10:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Mar 25 02:47:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 25 02:47:17 2021
 Response via : Initial Calibration

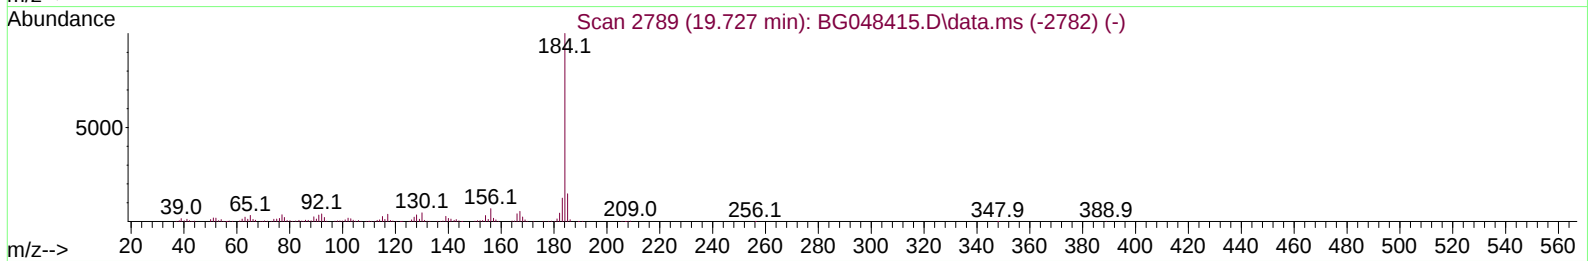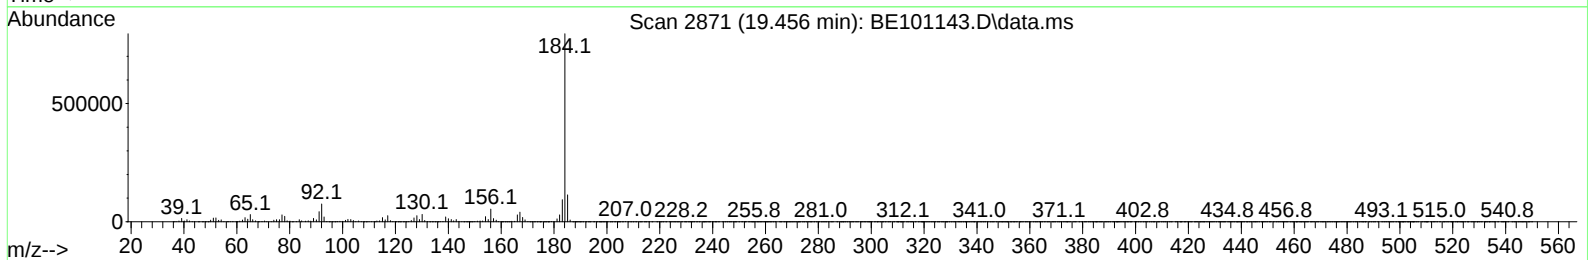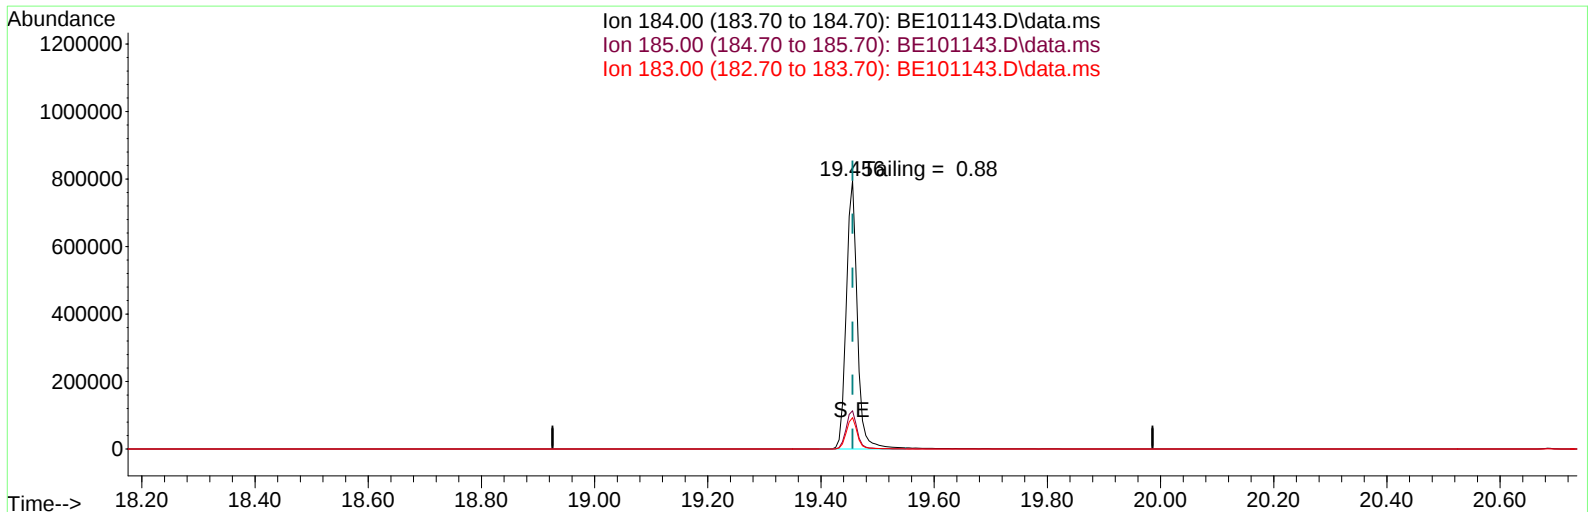

TIC: BE101143.D\data.ms

(77) Benzidine

19.456min (0.000) 1210641.28 ng




response 1087936

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	11.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE032421\
 Data File : BE101143.D
 Acq On : 24 Mar 2021 10:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Mar 25 02:41:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE032421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 24 16:00:06 2021
 Response via : Initial Calibration

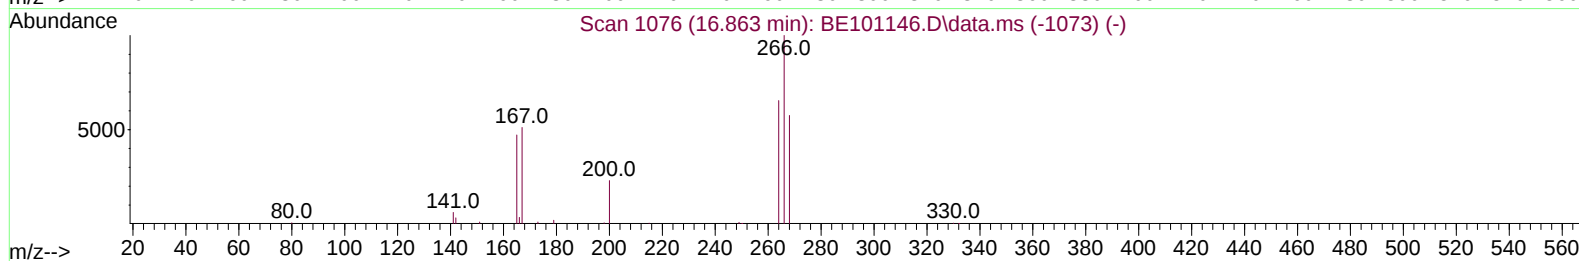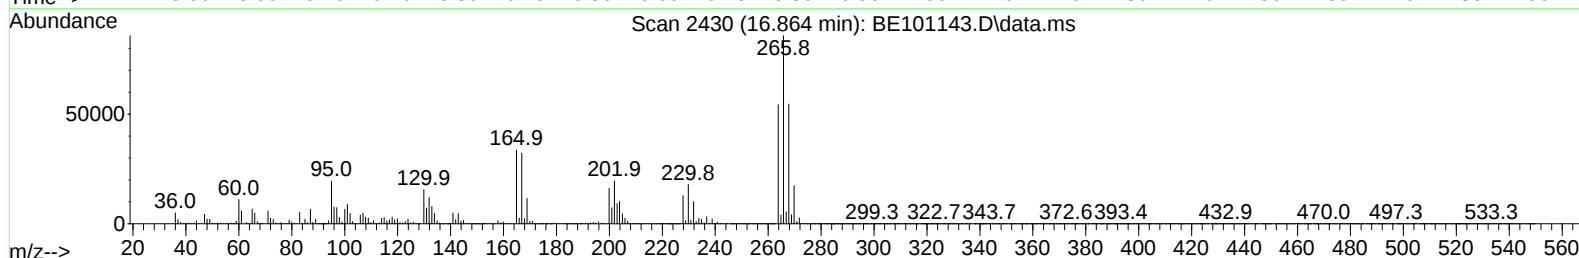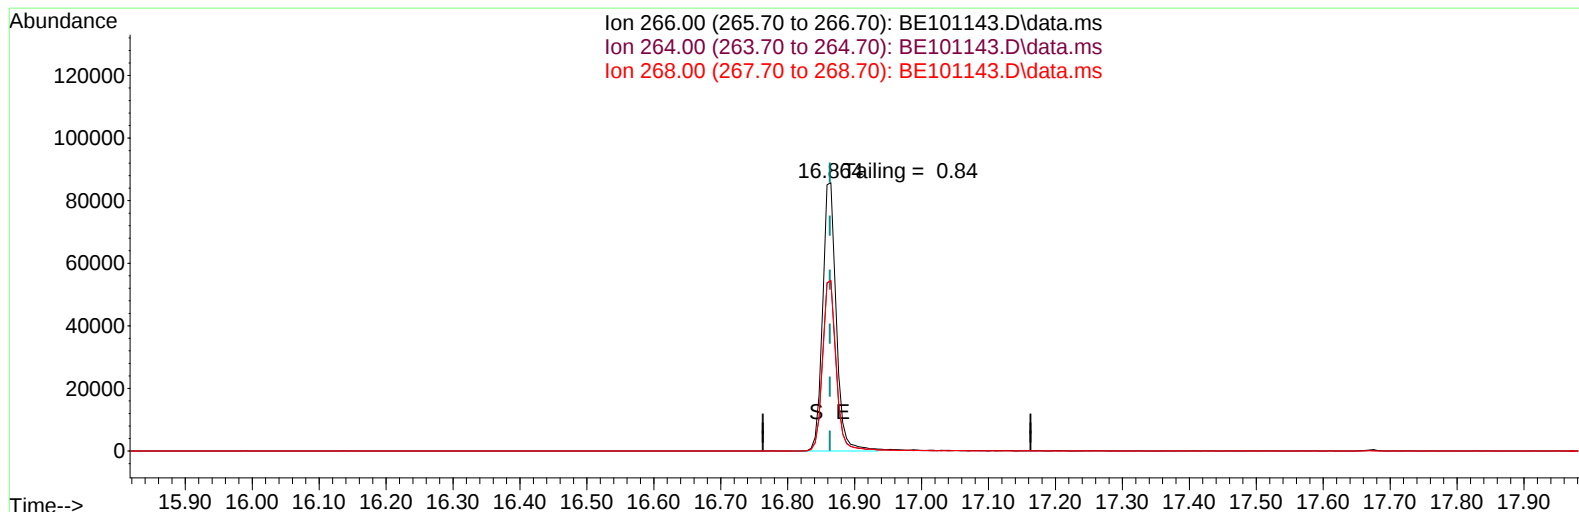

TIC: BE101143.D\data.ms

(24) Pentachlorophenol

16.864min (+ 0.001) 36088.04 ng

response 122536

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.20	63.46
268.00	62.40	63.12
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_E
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/24/2021	BNA_E	BE101143.D
Compound Name	Response	Retention Time
DDT	195742	20.69
DDD	459	20.24
DDE	658	19.74
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1117	196859	0.57