

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032919\
 Data File : BE099256.D
 Acq On : 29 Mar 2019 15:51
 Operator : JU/SJ
 Sample : K1982-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 EXT-027-SW013-032519

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:45:08 PM

Quant Time: Mar 29 23:20:16 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Mar 26 07:02:06 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	3461	0.40	ng	-0.01
7) Naphthalene-d8	10.63	136	14780	0.40	ng	0.00
13) Acenaphthene-d10	14.47	164	11238	0.40	ng	-0.01
19) Phenanthrene-d10	17.20	188	32214	0.40	ng	-0.01
27) Chrysene-d12	21.38	240	39904	0.40	ng	-0.01
34) Perylene-d12	23.89	264	38995	0.40	ng	0.00

System Monitoring Compounds

4) 2-Fluorophenol	5.41	112	1657	0.16	ng	0.00
5) Phenol-d6	6.99	99	2492	0.16	ng	0.00
8) Nitrobenzene-d5	8.99	82	1942	0.16	ng	0.00
11) 2-Methylnaphthalene-d10	12.21	152	4624	0.16	ng	-0.01
14) 2,4,6-Tribromophenol	15.96	330	713	0.34	ng	0.00
15) 2-Fluorobiphenyl	13.10	172	6748	0.15	ng	0.00
25) Fluoranthene-d10	19.23	212	60162	0.15	ng	-0.01
29) Terphenyl-d14	19.83	244	10305	0.12	ng	0.00

Target Compounds

						Qvalue
9) Naphthalene	10.67	128	17734	0.102	ng	98
12) 2-Methylnaphthalene	12.30	142	2536	0.081	ng	97
16) Acenaphthylene	14.20	152	1974	0.034	ng	# 95
17) Acenaphthene	14.53	154	11492	0.335	ng	98
18) Fluorene	15.50	166	11871	0.246	ng	# 97
23) Phenanthrene	17.24	178	281750	2.978	ng	100
24) Anthracene	17.34	178	56510	0.661	ng	# 93
26) Fluoranthene	19.26	202	391622	3.244	ng	99
28) Pyrene	19.63	202	341740	2.578	ng	# 95
30) Benzo(a)anthracene	21.37	228	213309	1.620	ng	98
31) Chrysene	21.41	228	167231	1.188	ng	96
32) Bis(2-ethylhexyl)phthalate	21.28	149	17044	0.109	ng	100
33) Indeno(1,2,3-cd)pyrene	26.53	276	64264	0.483	ng	97
35) Benzo(b)fluoranthene	23.11	252	179322	1.397	ng	98
36) Benzo(k)fluoranthene	23.16	252	80074m	0.590	ng	
37) Benzo(a)pyrene	23.77	252	128001	1.068	ng	98
38) Dibenzo(a,h)anthracene	26.56	278	17560	0.165	ng	# 92
39) Benzo(g,h,i)perylene	27.35	276	60439	0.566	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032919\
Data File : BE099256.D
Acq On : 29 Mar 2019 15:51
Operator : JU/SJ
Sample : K1982-10
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
EXT-027-SW013-032519

Manual Integrations
APPROVED

Sohil
4/1/2019 5:45:08 PM

Quant Time: Mar 29 23:20:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 07:02:06 2019
Response via : Initial Calibration





#1


1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.83 min Scan# 431
Delta R.T. -0.01 min
Lab File: BE099256.D
Acq: 29 Mar 2019 15:51

Instrument :
BNA_E
ClientSampleId :
EXT-027-SW013-032519

Tgt Ion	Ratio	Lower	Upper
152	100		
150	143.7	112.8	169.2
115	63.9	45.1	67.7

Manual Integrations
APPROVED

Sohil
4/1/2019 5:45:08 PM






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E



#4

2-Fluorophenol
Concen: 0.160 ng
RT: 5.41 min Scan# 221
Delta R.T. -0.00 min
Lab File: BE099256.D
Acq: 29 Mar 2019 15:51

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.7	46.2	69.2
63	114.4	89.9	134.9






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0





#5

Phenol-d6

Concen: 0.158 ng

RT: 6.99 min Scan# 358

Delta R.T. -0.00 min

Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Instrument :

BNA_E





ClientSampleId :

EXT-027-SW013-032519

Tgt Ion:	99	Resp:	2492
Ion	Ratio	Lower	Upper
99	100		
42	17.1	12.4	18.6
71	37.2	28.4	42.6

Manual Integrations
APPROVED

Sohil
4/1/2019 5:45:08 PM



#7

Naphthalene-d8

Concen: 0.400 ng




RT: 10.63 min Scan# 651

Delta R.T. 0.00 min

Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Tgt Ion:	136	Resp:	14780
Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.7	13.1
54	17.0	18.7	28.1#
68	4.7	5.2	7.8#





#8

Nitrobenzene-d5

Concen: 0.161 ng

RT: 8.99 min Scan# 525

Delta R.T. 0.00 min

Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Instrument :

BNA_E


ClientSampleId :

EXT-027-SW013-032519




Tgt Ion:	82	Resp:	1942
Ion Ratio	Lower	Upper	
82	100		
128	154.2	107.5	161.3
54	132.6	106.3	159.5

Manual Integrations
APPROVED

Sohil
4/1/2019 5:45:08 PM



Abundance Ion 82.00 (81.70 to 82.70): BE0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BE0



#9

Naphthalene

Concen: 0.102 ng

RT: 10.67 min Scan# 654




Delta R.T. -0.01 min


Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Tgt Ion:	128	Resp:	17734
Ion Ratio	Lower	Upper	
128	100		
129	3.4	2.3	3.5
127	3.8	2.6	3.8

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E



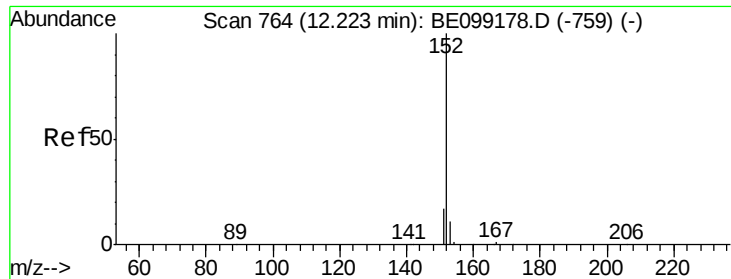





#11
 2-Methylnaphthalene-d10
 Concen: 0.162 ng
 RT: 12.21 min Scan# 763
 Delta R.T. -0.01 min
 Lab File: BE099256.D
 Acq: 29 Mar 2019 15:51

Instrument :
 BNA_E
 ClientSampleId :
 EXT-027-SW013-032519

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.5	15.0	22.6




Manual Integrations
 APPROVED


Sohil
 4/1/2019 5:45:08 PM



#12
 2-Methylnaphthalene
 Concen: 0.081 ng
 RT: 12.30 min Scan# 769
 Delta R.T. 0.00 min
 Lab File: BE099256.D
 Acq: 29 Mar 2019 15:51

Tgt Ion	Ratio	Lower	Upper
142	100		
141	88.5	71.3	106.9
115	42.8	30.4	45.6





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.47 min Scan# 920

Delta R.T. -0.01 min

Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Instrument :

BNA_E


ClientSampleId :

EXT-027-SW013-032519




Tgt Ion:	164	Resp:	11238
Ion Ratio	Lower	Upper	
164	100		
162	98.0	79.2	118.8
160	46.4	36.7	55.1

Manual Integrations
APPROVED

Sohil
4/1/2019 5:45:08 PM



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E



#14

2,4,6-Tribromophenol

Concen: 0.342 ng

RT: 15.96 min Scan# 1025




Delta R.T. 0.00 min


Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Tgt Ion:	330	Resp:	713
Ion Ratio	Lower	Upper	
330	100		
332	99.6	71.3	106.9
141	41.7	21.7	32.5#

Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E









#15
2-Fluorobiphenyl
Concen: 0.147 ng
RT: 13.10 min Scan# 825
Delta R.T. 0.00 min
Lab File: BE099256.D
Acq: 29 Mar 2019 15:51

Instrument :
BNA_E
ClientSampleId :
EXT-027-SW013-032519

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.2	27.4	41.0
170	22.2	19.1	28.7




Manual Integrations
APPROVED


Sohil
4/1/2019 5:45:08 PM



#16
Acenaphthylene
Concen: 0.034 ng
RT: 14.20 min Scan# 901
Delta R.T. 0.00 min
Lab File: BE099256.D
Acq: 29 Mar 2019 15:51

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.8	15.7	23.5
153	18.2	10.6	15.8





#17

Acenaphthene

Concen: 0.335 ng

RT: 14.53 min Scan# 924

Delta R.T. -0.01 min

Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Instrument :

BNA_E


ClientSampleId :

EXT-027-SW013-032519




Tgt Ion:	154	Resp:	11492
Ion Ratio	Lower	Upper	
154	100		
153	118.9	93.4	140.0
152	57.4	46.6	69.8

Manual Integrations
APPROVED

Sohil
4/1/2019 5:45:08 PM



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E



#18

Fluorene

Concen: 0.246 ng

RT: 15.50 min Scan# 991




Delta R.T. -0.01 min


Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Tgt Ion:	166	Resp:	11871
Ion Ratio	Lower	Upper	
166	100		
165	100.7	78.9	118.3
167	17.4	10.9	16.3#

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.20 min Scan# 1118

Delta R.T. -0.01 min

Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Instrument :

BNA_E


ClientSampleId :

EXT-027-SW013-032519

Tgt Ion:	188	Resp:	32214
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	8.6	4.5	6.7#

Manual Integrations
APPROVED




Sohil
4/1/2019 5:45:08 PM



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0



#23

Phenanthrene

Concen: 2.978 ng

RT: 17.24 min Scan# 1121

Delta R.T. -0.01 min

Lab File: BE099256.D




Acq: 29 Mar 2019 15:51


Tgt Ion:	178	Resp:	281750
Ion Ratio	Lower	Upper	
178	100		
176	19.5	15.4	23.2
179	15.4	12.3	18.5

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E





#24

Anthracene

Concen: 0.661 ng

RT: 17.34 min Scan# 1128

Delta R.T. 0.00 min

Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Instrument :

BNA_E





ClientSampleId :

EXT-027-SW013-032519

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.5	15.1	22.7
179	21.9	12.4	18.6

Manual Integrations
APPROVED

Sohil
4/1/2019 5:45:08 PM



#25

Fluoranthene-d10

Concen: 0.154 ng




RT: 19.23 min Scan# 1386


Delta R.T. -0.01 min

Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Tgt Ion	Ratio	Lower	Upper
212	100		
106	2.4	1.8	2.8
104	1.3	1.1	1.7






#26
 Fluoranthene
 Concen: 3.244 ng
 RT: 19.26 min Scan# 1392
 Delta R.T. -0.01 min
 Lab File: BE099256.D
 Acq: 29 Mar 2019 15:51

Instrument :
 BNA_E
 ClientSampleId :
 EXT-027-SW013-032519




Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	7.9	7.0	10.4
203	17.6	13.8	20.6

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:45:08 PM






Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 203.00 (202.70 to 203.70): E




#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.38 min Scan# 1631
 Delta R.T. -0.01 min
 Lab File: BE099256.D
 Acq: 29 Mar 2019 15:51

Tgt Ion	Ratio	Resp Lower	Resp Upper
240	100		
120	5.8	2.6	3.8#
236	26.6	20.9	31.3

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E









#28
 Pyrene
 Concen: 2.578 ng
 RT: 19.63 min Scan# 1455
 Delta R.T. -0.01 min
 Lab File: BE099256.D
 Acq: 29 Mar 2019 15:51

Instrument :
 BNA_E
 ClientSampleId :
 EXT-027-SW013-032519

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
200	20.0	15.8	23.8
203	22.4	14.1	21.1#




Manual Integrations
 APPROVED


Sohil
 4/1/2019 5:45:08 PM



#29
 Terphenyl-d14
 Concen: 0.119 ng
 RT: 19.83 min Scan# 1490
 Delta R.T. -0.01 min
 Lab File: BE099256.D
 Acq: 29 Mar 2019 15:51

Tgt Ion	Ratio	Resp Lower	Resp Upper
244	100		
212	34.7	22.7	34.1#
122	7.6	5.8	8.6









#30
Benzo(a)anthracene
Concen: 1.620 ng
RT: 21.37 min Scan# 1630
Delta R.T. -0.00 min
Lab File: BE099256.D
Acq: 29 Mar 2019 15:51

Instrument :
BNA_E
ClientSampleId :
EXT-027-SW013-032519

Tgt Ion	Ratio	Lower	Upper
228	100		
226	26.7	21.7	32.5
229	21.6	15.9	23.9




Manual Integrations
APPROVED


Sohil
4/1/2019 5:45:08 PM



#31
Chrysene
Concen: 1.188 ng
RT: 21.41 min Scan# 1634
Delta R.T. -0.00 min
Lab File: BE099256.D
Acq: 29 Mar 2019 15:51

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.3	24.8	37.2
229	22.8	15.4	23.0





#32

Bis(2-ethylhexyl)phthalate

Concen: 0.109 ng

RT: 21.28 min Scan# 1623

Delta R.T. -0.01 min

Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Instrument :

BNA_E


ClientSampleId :

EXT-027-SW013-032519




Tgt Ion:	149	Resp:	17044
Ion Ratio	Lower	Upper	
149	100		
167	7.5	5.9	8.9
279	1.4	1.0	1.6

Manual Integrations
APPROVED

Sohil
4/1/2019 5:45:08 PM



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E



#33

Indeno(1,2,3-cd)pyrene

Concen: 0.483 ng

RT: 26.53 min Scan# 2941




Delta R.T. -0.03 min


Lab File: BE099256.D

Acq: 29 Mar 2019 15:51

Tgt Ion:	276	Resp:	64264
Ion Ratio	Lower	Upper	
276	100		
138	13.0	12.9	19.3
277	22.9	18.3	27.5

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E









#34
Perylene-d12
 Concen: 0.400 ng
 RT: 23.89 min Scan# 2205
 Delta R.T. -0.01 min
 Lab File: BE099256.D
 Acq: 29 Mar 2019 15:51

Instrument :
 BNA_E
 ClientSampleId :
 EXT-027-SW013-032519

Tgt Ion	Ratio	Lower	Upper
264	100		
260	25.4	18.2	27.2
265	27.5	21.8	32.8




Manual Integrations
 APPROVED


Sohil
 4/1/2019 5:45:08 PM



#35
Benzo(b)fluoranthene
 Concen: 1.397 ng
 RT: 23.11 min Scan# 1988
 Delta R.T. -0.01 min
 Lab File: BE099256.D
 Acq: 29 Mar 2019 15:51

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.8	26.8
125	7.7	6.1	9.1









#36
Benzo(k)fluoranthene
Concen: 0.590 ng m
RT: 23.16 min Scan# 2001
Delta R.T. -0.01 min
Lab File: BE099256.D
Acq: 29 Mar 2019 15:51

Instrument :
BNA_E
ClientSampleId :
EXT-027-SW013-032519

Tgt Ion: 252 Resp: 80074
Ion Ratio Lower Upper
252 100
253 23.9 17.8 26.6
125 7.0 5.9 8.9




Manual Integrations
APPROVED


Sohil
4/1/2019 5:45:08 PM



#37
Benzo(a)pyrene
Concen: 1.068 ng
RT: 23.77 min Scan# 2173
Delta R.T. -0.01 min
Lab File: BE099256.D
Acq: 29 Mar 2019 15:51

Tgt Ion: 252 Resp: 128001
Ion Ratio Lower Upper
252 100
253 23.4 18.1 27.1
125 7.8 6.8 10.2









#38
Dibenzo(a,h)anthracene
Concen: 0.165 ng
RT: 26.56 min Scan# 2949
Delta R.T. -0.03 min
Lab File: BE099256.D
Acq: 29 Mar 2019 15:51

Instrument :
BNA_E
ClientSampleId :
EXT-027-SW013-032519

Tgt Ion	Ratio	Lower	Upper
278	100		
139	12.2	9.5	14.3
279	29.5	19.1	28.7

Manual Integrations
APPROVED

Sohil
4/1/2019 5:45:08 PM



#39
Benzo(g,h,i)perylene
Concen: 0.566 ng
RT: 27.35 min Scan# 3172
Delta R.T. -0.03 min
Lab File: BE099256.D
Acq: 29 Mar 2019 15:51

Tgt Ion	Ratio	Lower	Upper
276	100		
277	24.6	19.0	28.4
138	13.7	11.1	16.7

