


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE032919\
 Data File : BE099247.D
 Acq On : 29 Mar 2019 9:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 07:02:06 2019

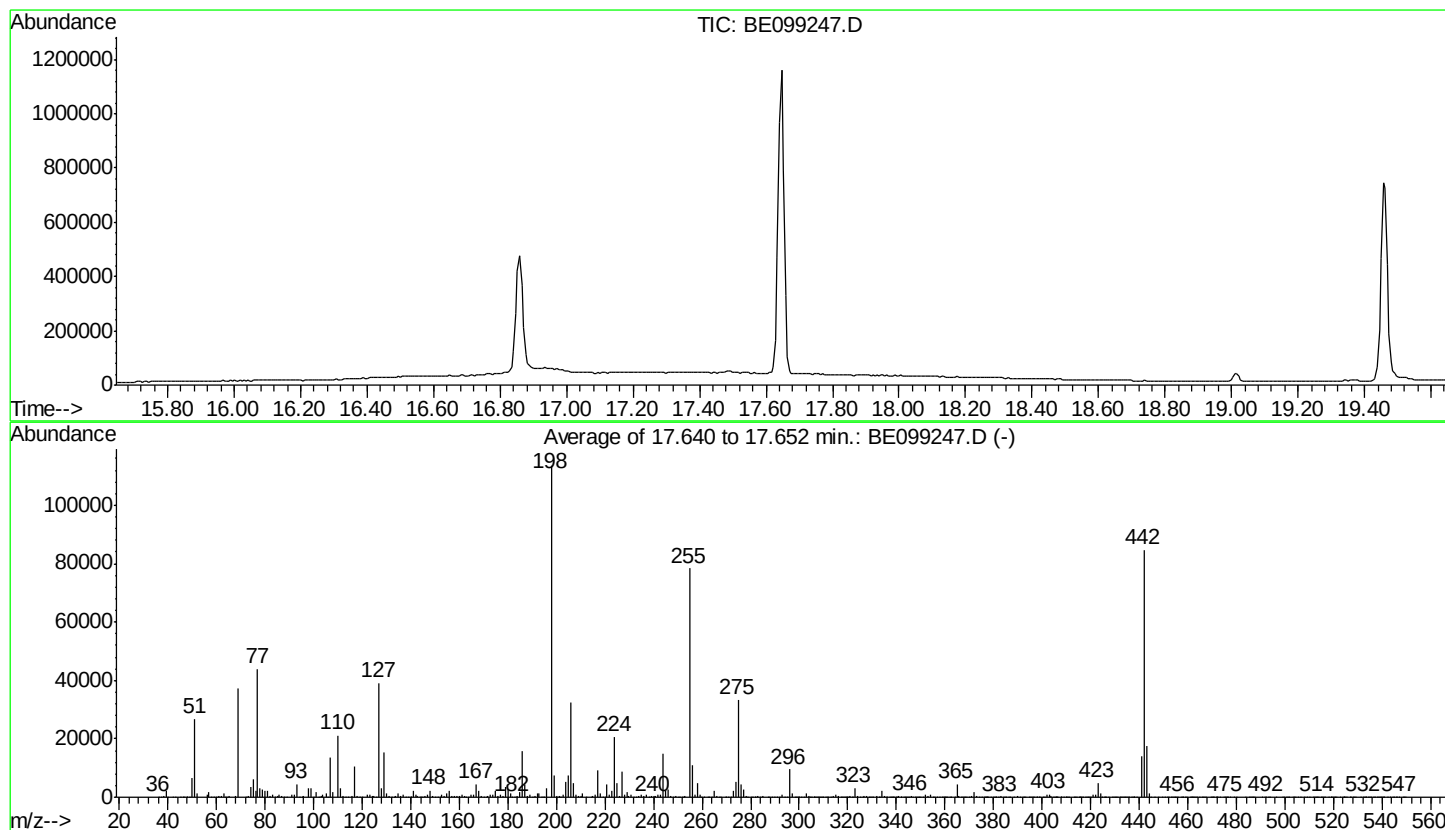

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.6	26790	PASS
68	69	0.00	2	1.6	612	PASS
69	198	0.00	100	32.7	37187	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.5	39227	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	113554	PASS
199	198	5	9	6.4	7320	PASS
275	198	10	60	29.5	33464	PASS
365	198	1	100	4.0	4568	PASS
441	198	0.01	100	12.2	13842	PASS
442	198	50	100	74.5	84624	PASS
443	442	15	24	20.6	17392	PASS