


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE032919\
 Data File : BE099264.D
 Acq On : 29 Mar 2019 21:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 07:02:06 2019

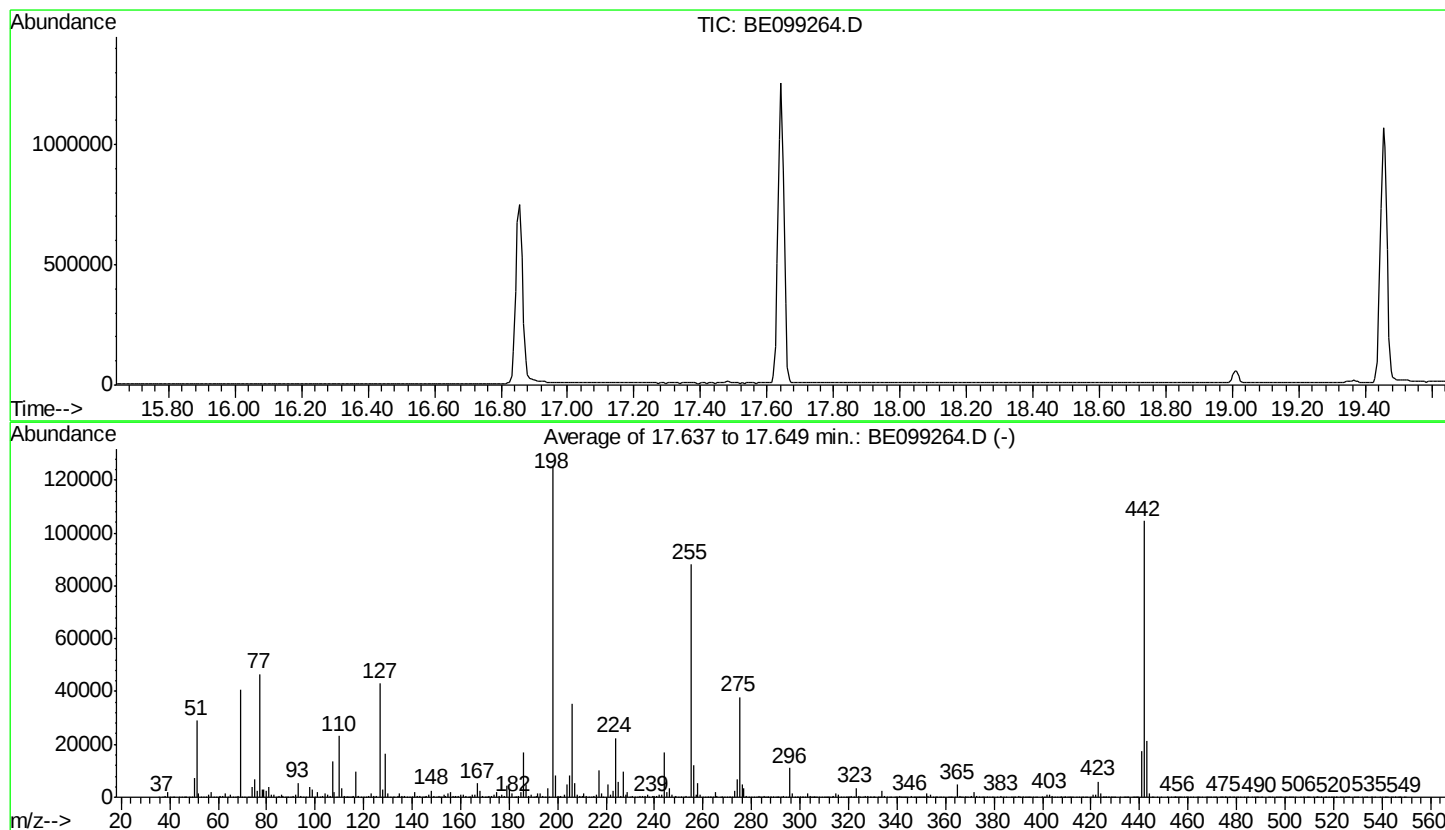

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.1	28992	PASS
68	69	0.00	2	1.8	724	PASS
69	198	0.00	100	32.4	40683	PASS
70	69	0.00	2	0.5	193	PASS
127	198	10	80	34.2	42955	PASS
197	198	0.00	2	0.1	111	PASS
198	198	100	100	100.0	125497	PASS
199	198	5	9	6.5	8213	PASS
275	198	10	60	30.2	37851	PASS
365	198	1	100	3.8	4797	PASS
441	198	0.01	100	14.1	17639	PASS
442	198	50	100	83.2	104438	PASS
443	442	15	24	20.4	21264	PASS