

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040821\
 Data File : BE101252.D
 Acq On : 8 Apr 2021 18:37
 Operator : CG/JU
 Sample : M1966-06MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 MW-123RMS

Quant Time: Apr 09 01:30:05 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 07 10:22:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.838	152	2049	0.40	ng	0.00
7) Naphthalene-d8	10.615	136	8679	0.40	ng	# 0.00
13) Acenaphthene-d10	14.443	164	8018	0.40	ng	0.00
19) Phenanthrene-d10	17.195	188	12048	0.40	ng	#-0.01
29) Chrysene-d12	21.354	240	12619	0.40	ng	# 0.00
36) Perylene-d12	23.838	264	11528	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.420	112	1598	0.33	ng	0.00
5) Phenol-d6	6.998	99	1014	0.13	ng	0.00
8) Nitrobenzene-d5	8.978	82	3030	0.47	ng	0.00
11) 2-Methylnaphthalene-d10	12.196	152	6192	0.31	ng	0.00
14) 2,4,6-Tribromophenol	15.955	330	855	0.40	ng	0.00
15) 2-Fluorobiphenyl	13.075	172	7768	0.27	ng	0.00
27) Fluoranthene-d10	19.238	212	56296	0.27	ng	0.02
31) Terphenyl-d14	19.812	244	15137	0.45	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.370	88	1061	0.34	ng	# 78
3) n-Nitrosodimethylamine	3.669	42	1284	0.39	ng	# 42
6) bis(2-Chloroethyl)ether	7.251	93	2636	0.38	ng	78
9) Naphthalene	10.667	128	188971	2.00	ng	100
10) Hexachlorobutadiene	10.953	225	1265	0.30	ng	99
12) 2-Methylnaphthalene	12.268	142	8375	0.49	ng	96
16) Acenaphthylene	14.169	152	73084	2.34	ng	97
17) Acenaphthene	14.515	154	29913	1.28	ng	97
18) Fluorene	15.502	166	37360	1.19	ng	99
20) 4,6-Dinitro-2-methylph...	15.577	198	612	0.51	ng	# 1
21) 4-Bromophenyl-phenylether	16.394	248	2466	0.41	ng	# 32
22) Hexachlorobenzene	16.515	284	2126	0.35	ng	99
23) Atrazine	16.681	200	2350	0.58	ng	# 71
24) Pentachlorophenol	16.863	266	1397	0.63	ng	95
25) Phenanthrene	17.241	178	110423	3.09	ng	99
26) Anthracene	17.331	178	30522	1.00	ng	# 94
28) Fluoranthene	19.261	202	50186	1.08	ng	99
30) Pyrene	19.611	202	42562	0.93	ng	97
32) Benzo(a)anthracene	21.342	228	17791	0.50	ng	# 91
33) Chrysene	21.390	228	17190	0.41	ng	# 90
34) Bis(2-ethylhexyl)phtha...	21.281	149	37760	1.47	ng	99
35) Indeno(1,2,3-cd)pyrene	26.444	276	15402	0.50	ng	100
37) Benzo(b)fluoranthene	23.075	252	15295	0.41	ng	# 87
38) Benzo(k)fluoranthene	23.125	252	14806	0.35	ng	# 86
39) Benzo(a)pyrene	23.724	252	13250	0.41	ng	# 85
40) Dibenzo(a,h)anthracene	26.469	278	12033	0.39	ng	# 89
41) Benzo(g,h,i)perylene	27.240	276	13515	0.40	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040821\
Data File : BE101252.D
Acq On : 8 Apr 2021 18:37
Operator : CG/JU
Sample : M1966-06MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
MW-123RMS

Quant Time: Apr 09 01:30:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:22:45 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.838 min Scan# 432
 Delta R.T. 0.008 min
 Lab File: BE101252.D
 Acq: 8 Apr 2021 18:37




Instrument :
 BNA_E
 ClientSampleId :
 MW-123RMS


Tgt Ion:152 Resp: 2049
 Ion Ratio Lower Upper
 152 100
 150 149.2 116.9 175.3
 115 64.8 44.5 66.7



#2
 1,4-Dioxane
 Concen: 0.34 ng
 RT: 3.370 min Scan# 44
 Delta R.T. 0.009 min
 Lab File: BE101252.D
 Acq: 8 Apr 2021 18:37

Tgt Ion: 88 Resp: 1061
 Ion Ratio Lower Upper
 88 100
 58 99.0 73.6 110.4
 43 0.0 27.6 41.4#









#3
n-Nitrosodimethylamine
Concen: 0.39 ng
RT: 3.669 min Scan# 70
Delta R.T. -0.003 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion: 42 Resp: 1284
Ion Ratio Lower Upper
42 100
74 52.9 92.7 139.1#
44 38.1 10.7 16.1#



#4
2-Fluorophenol
Concen: 0.33 ng
RT: 5.420 min Scan# 222
Delta R.T. -0.003 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion: 112 Resp: 1598
Ion Ratio Lower Upper
112 100
64 78.2 62.3 93.5
63 116.8 117.3 175.9#









#5
Phenol-d6
Concen: 0.13 ng
RT: 6.998 min Scan# 359
Delta R.T. 0.009 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion: 99 Resp: 1014
Ion Ratio Lower Upper
99 100
42 415.6 18.5 27.7#
71 0.0 26.5 39.7#



#6
bis(2-Chloroethyl)ether
Concen: 0.38 ng
RT: 7.251 min Scan# 381
Delta R.T. -0.003 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion: 93 Resp: 2636
Ion Ratio Lower Upper
93 100
63 313.1 292.5 438.7
95 30.4 25.7 38.5









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.615 min Scan# 650
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:	136	Resp:	8679
Ion	Ratio	Lower	Upper
136	100		
137	12.8	8.6	13.0
54	56.5	34.7	52.1#
68	13.3	7.0	10.4#



#8
Nitrobenzene-d5
Concen: 0.47 ng
RT: 8.978 min Scan# 524
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:	82	Resp:	3030
Ion	Ratio	Lower	Upper
82	100		
128	163.7	118.7	178.1
54	215.8	164.4	246.6









#9
Naphthalene
Concen: 2.00 ng
RT: 10.667 min Scan# 654
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:	128	Resp:	188971
Ion Ratio	Lower	Upper	
128	100		
129	2.8	2.2	3.4
127	3.3	2.6	3.8



#10
Hexachlorobutadiene
Concen: 0.30 ng
RT: 10.953 min Scan# 676
Delta R.T. -0.013 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:	225	Resp:	1265
Ion Ratio	Lower	Upper	
225	100		
223	63.0	50.4	75.6
227	64.1	50.1	75.1









#11
2-Methylnaphthalene-d10
Concen: 0.31 ng
RT: 12.196 min Scan# 763
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:152 Resp: 6192
Ion Ratio Lower Upper
152 100
151 20.1 16.5 24.7



#12
2-Methylnaphthalene
Concen: 0.49 ng
RT: 12.268 min Scan# 768
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:142 Resp: 8375
Ion Ratio Lower Upper
142 100
141 88.2 73.0 109.6
115 37.7 27.8 41.8







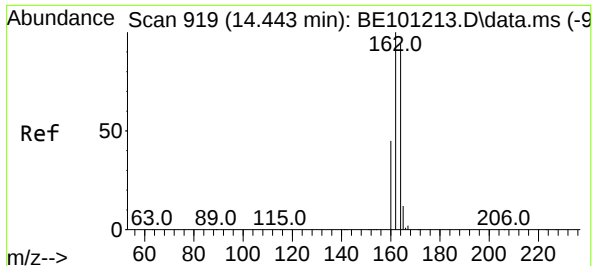

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.443 min Scan# 919
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:164 Resp: 8018
Ion Ratio Lower Upper
164 100
162 90.7 85.3 127.9
160 42.2 39.1 58.7



#14
2,4,6-Tribromophenol
Concen: 0.40 ng
RT: 15.955 min Scan# 1016
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:330 Resp: 855
Ion Ratio Lower Upper
330 100
332 100.5 77.8 116.6
141 66.8 30.4 45.6#







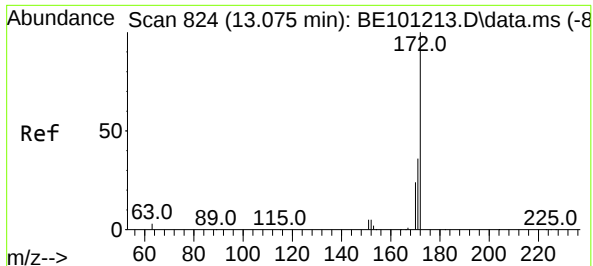

#15
2-Fluorobiphenyl
Concen: 0.27 ng
RT: 13.075 min Scan# 824
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:	172	Resp:	7768
Ion Ratio	Lower	Upper	
172	100		
171	36.1	28.7	43.1
170	24.6	19.3	28.9



#16
Acenaphthylene
Concen: 2.34 ng
RT: 14.169 min Scan# 900
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:	152	Resp:	73084
Ion Ratio	Lower	Upper	
152	100		
151	19.9	15.4	23.2
153	14.2	10.0	15.0







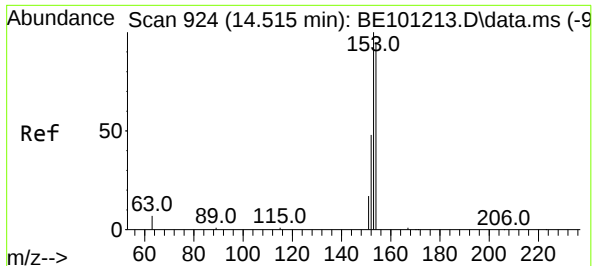

#17
Acenaphthene
Concen: 1.28 ng
RT: 14.515 min Scan# 924
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:154 Resp: 29913
Ion Ratio Lower Upper
154 100
153 104.0 84.9 127.3
152 49.7 42.7 64.1



#18
Fluorene
Concen: 1.19 ng
RT: 15.502 min Scan# 986
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:166 Resp: 37360
Ion Ratio Lower Upper
166 100
165 98.0 79.0 118.4
167 13.9 11.0 16.4









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.195 min Scan# 1098
Delta R.T. -0.015 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:188 Resp: 12048
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 35.2 4.6 6.8#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.51 ng
RT: 15.577 min Scan# 991
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:198 Resp: 612
Ion Ratio Lower Upper
198 100
51 288.7 55.9 83.9#
105 362.8 33.6 50.4#









#21
4-Bromophenyl-phenylether
Concen: 0.41 ng
RT: 16.394 min Scan# 1045
Delta R.T. -0.015 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:248 Resp: 2466
Ion Ratio Lower Upper
248 100
250 85.1 84.5 126.7
141 160.1 19.8 29.8#



#22
Hexachlorobenzene
Concen: 0.35 ng
RT: 16.515 min Scan# 1053
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:284 Resp: 2126
Ion Ratio Lower Upper
284 100
142 33.6 27.4 41.0
249 33.3 26.5 39.7









#23
Atrazine
Concen: 0.58 ng
RT: 16.681 min Scan# 1064
Delta R.T. 0.015 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:200 Resp: 2350
Ion Ratio Lower Upper
200 100
173 65.3 21.9 32.9#
215 50.6 38.6 57.8



#24
Pentachlorophenol
Concen: 0.63 ng
RT: 16.863 min Scan# 1076
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:266 Resp: 1397
Ion Ratio Lower Upper
266 100
264 66.9 49.1 73.7
268 66.1 50.6 76.0









#25
Phenanthrene
Concen: 3.09 ng
RT: 17.241 min Scan# 1101
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:178 Resp: 110423
Ion Ratio Lower Upper
178 100
176 18.9 15.0 22.6
179 16.0 12.2 18.4



#26
Anthracene
Concen: 1.00 ng
RT: 17.331 min Scan# 1107
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:178 Resp: 30522
Ion Ratio Lower Upper
178 100
176 19.8 14.4 21.6
179 18.6 11.8 17.8#









#27
Fluoranthene-d10
Concen: 0.27 ng
RT: 19.238 min Scan# 1362
Delta R.T. 0.023 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:212 Resp: 56296
Ion Ratio Lower Upper
212 100
106 3.7 2.6 4.0
104 2.3 1.4 2.2#



#28
Fluoranthene
Concen: 1.08 ng
RT: 19.261 min Scan# 1366
Delta R.T. 0.017 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:202 Resp: 50186
Ion Ratio Lower Upper
202 100
101 11.8 9.1 13.7
203 17.6 13.6 20.4









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.354 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:240 Resp: 12619
Ion Ratio Lower Upper
240 100
120 22.5 10.2 15.4#
236 31.1 21.7 32.5



#30
Pyrene
Concen: 0.93 ng
RT: 19.611 min Scan# 1427
Delta R.T. 0.006 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:202 Resp: 42562
Ion Ratio Lower Upper
202 100
200 21.6 16.6 24.8
203 19.2 13.8 20.8









#31
Terphenyl-d14
Concen: 0.45 ng
RT: 19.812 min Scan# 1462
Delta R.T. 0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:244 Resp: 15137
Ion Ratio Lower Upper
244 100
212 47.6 21.9 32.9#
122 24.1 7.3 10.9#



#32
Benzo(a)anthracene
Concen: 0.50 ng
RT: 21.342 min Scan# 1602
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:228 Resp: 17791
Ion Ratio Lower Upper
228 100
226 30.0 21.4 32.2
229 25.0 15.7 23.5#









#33
Chrysene
Concen: 0.41 ng
RT: 21.390 min Scan# 1606
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:228 Resp: 17190
Ion Ratio Lower Upper
228 100
226 34.7 24.8 37.2
229 25.5 15.2 22.8#



#34
Bis(2-ethylhexyl)phthalate
Concen: 1.47 ng
RT: 21.281 min Scan# 1597
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:149 Resp: 37760
Ion Ratio Lower Upper
149 100
167 7.2 5.5 8.3
279 1.1 1.0 1.4









#35
Indeno(1,2,3-cd)pyrene
Concen: 0.50 ng
RT: 26.444 min Scan# 2892
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:276 Resp: 15402
Ion Ratio Lower Upper
276 100
138 21.8 17.4 26.0
277 24.8 19.8 29.8



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.838 min Scan# 2165
Delta R.T. 0.003 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:264 Resp: 11528
Ion Ratio Lower Upper
264 100
260 27.3 19.3 28.9
265 40.6 22.4 33.6#









#37
Benzo(b)fluoranthene
Concen: 0.41 ng
RT: 23.075 min Scan# 1951
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:252 Resp: 15295
Ion Ratio Lower Upper
252 100
253 27.4 18.1 27.1#
125 16.6 7.6 11.4#



#38
Benzo(k)fluoranthene
Concen: 0.35 ng
RT: 23.125 min Scan# 1965
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:252 Resp: 14806
Ion Ratio Lower Upper
252 100
253 27.5 17.8 26.6#
125 16.6 7.6 11.4#









#39
Benzo(a)pyrene
Concen: 0.41 ng
RT: 23.724 min Scan# 2133
Delta R.T. -0.000 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37




Instrument :
BNA_E
ClientSampleId :
MW-123RMS


Tgt Ion:252 Resp: 13250
Ion Ratio Lower Upper
252 100
253 27.9 18.0 27.0#
125 18.3 8.0 12.0#



#40
Dibenzo(a,h)anthracene
Concen: 0.39 ng
RT: 26.469 min Scan# 2899
Delta R.T. -0.004 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Tgt Ion:278 Resp: 12033
Ion Ratio Lower Upper
278 100
139 22.0 12.2 18.2#
279 28.0 19.3 28.9





#41
Benzo(g,h,i)perylene
Concen: 0.40 ng
RT: 27.240 min Scan# 3115
Delta R.T. -0.004 min
Lab File: BE101252.D
Acq: 8 Apr 2021 18:37

Instrument :
BNA_E
ClientSampleId :
MW-123RMS

Tgt Ion:276 Resp: 13515
Ion Ratio Lower Upper
276 100
277 26.3 19.4 29.0
138 24.4 15.2 22.8#

