
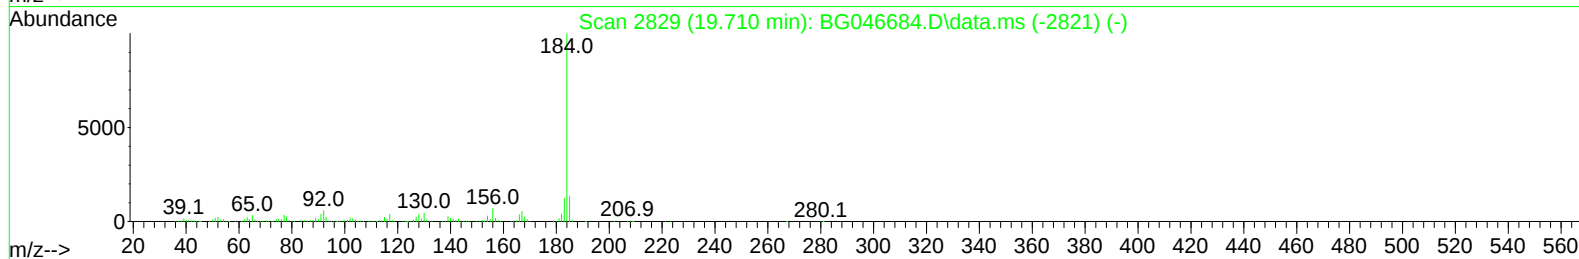
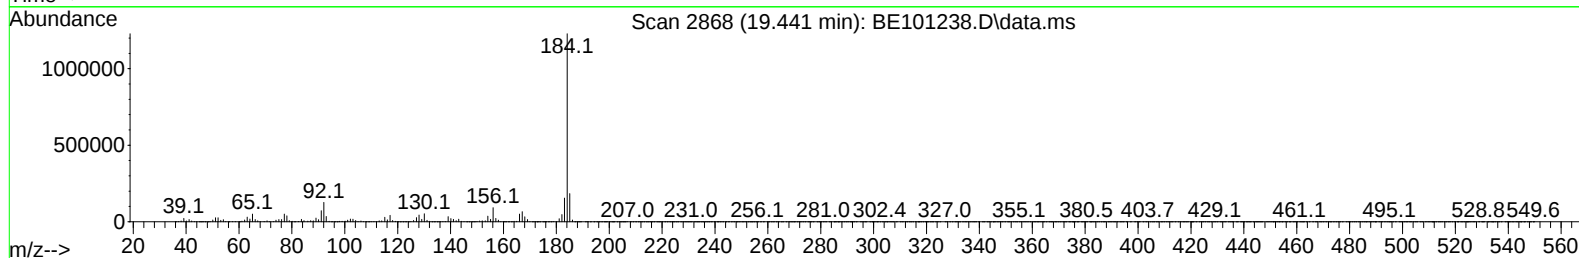


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040821\
 Data File : BE101238.D
 Acq On : 8 Apr 2021 8:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 11:26:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

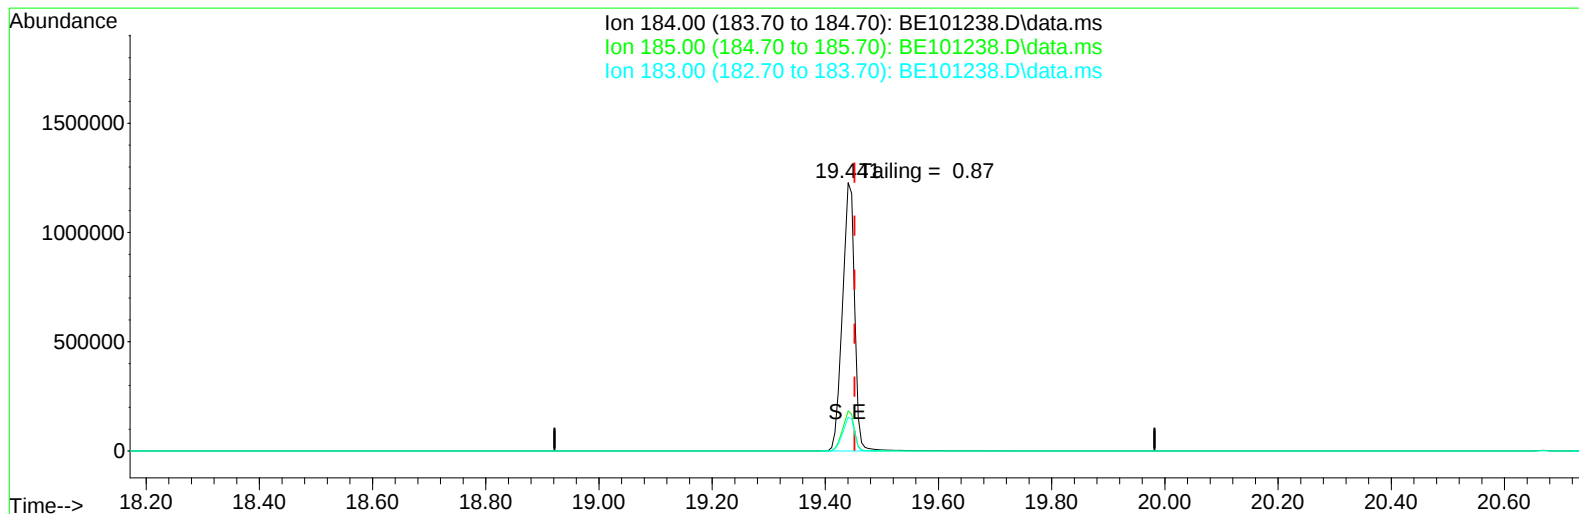




TIC: BE101238.D\data.ms

(77) Benzidine**19.441min (-0.011) 4116.90 ng****response 1831620**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.97
183.00	13.20	12.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040821\
 Data File : BE101238.D
 Acq On : 8 Apr 2021 8:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 11:26:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

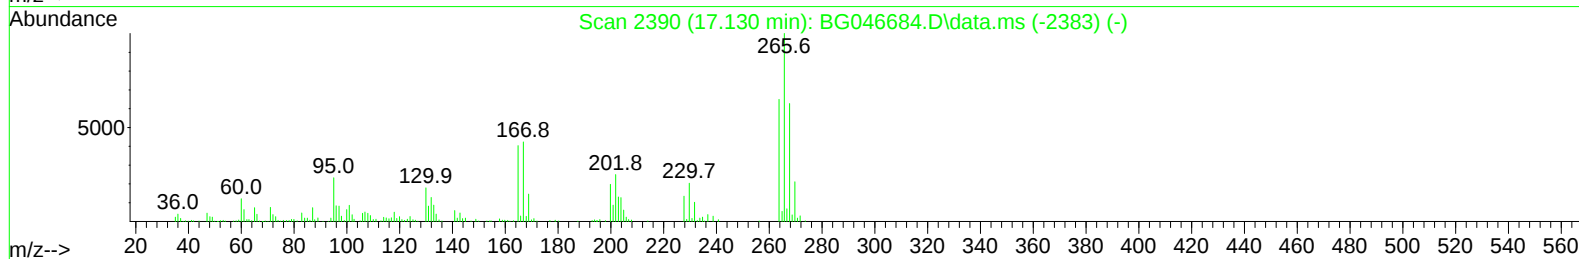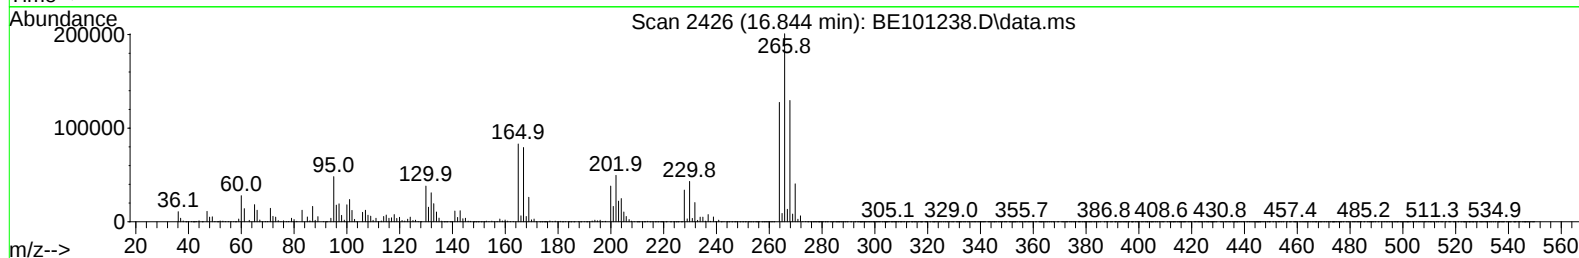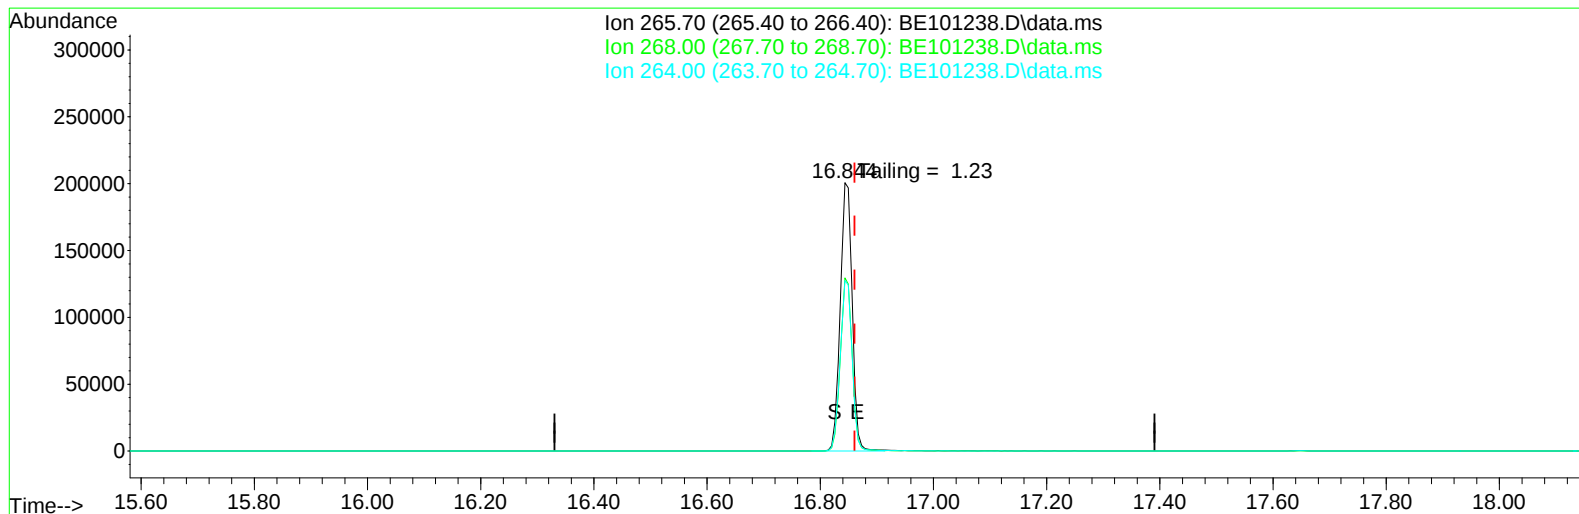

TIC: BE101238.D\data.ms

(70) Pentachlorophenol (C)

16.844min (-0.017) 6230258.48 ng

response 293361

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.50
264.00	61.60	63.48
0.00	0.00	0.00