
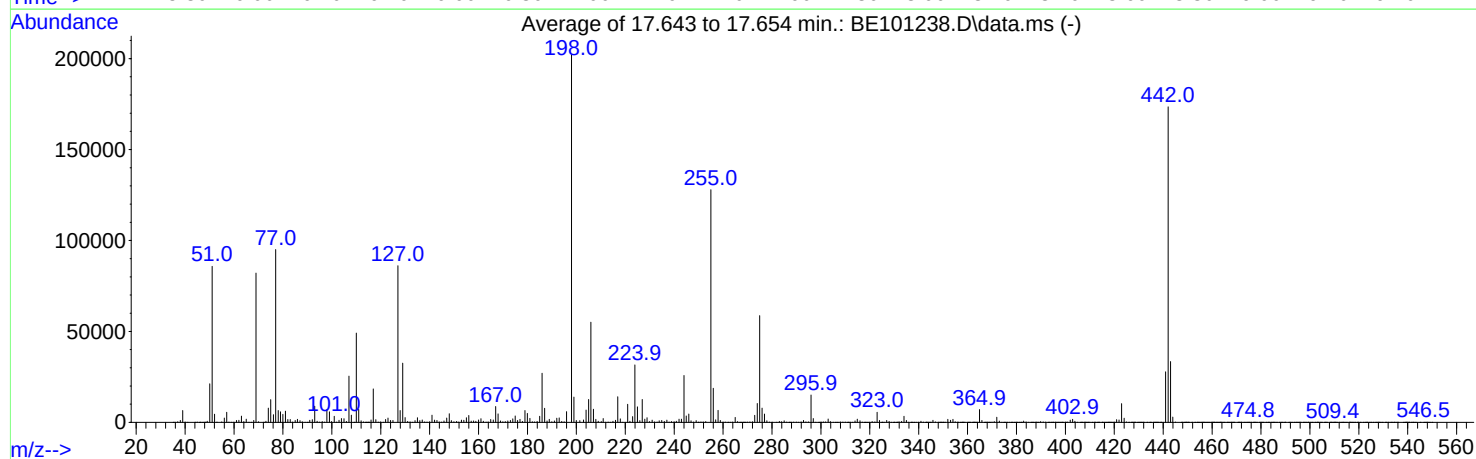


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040821\
 Data File : BE101238.D
 Acq On : 8 Apr 2021 8:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 07 10:22:45 2021

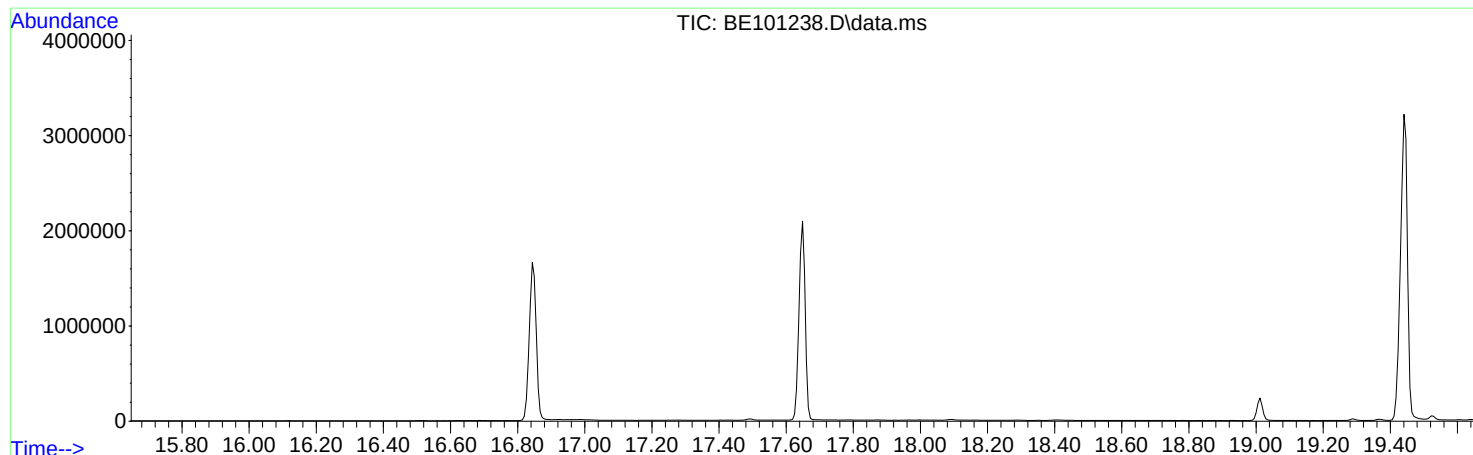




AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2548

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	85820	PASS
68	69	0.00	2	1.3	1086	PASS
69	198	0.00	100	40.6	82113	PASS
70	69	0.00	2	0.5	390	PASS
127	198	10	80	42.6	86097	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	202257	PASS
199	198	5	9	6.9	13868	PASS
275	198	10	60	29.0	58676	PASS
365	198	1	100	3.5	7080	PASS
441	198	0.01	100	13.8	27839	PASS
442	442	50	100	100.0	173518	PASS
443	442	15	24	19.3	33432	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040821\
 Data File : BE101238.D
 Acq On : 8 Apr 2021 8:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Apr 08 11:26:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

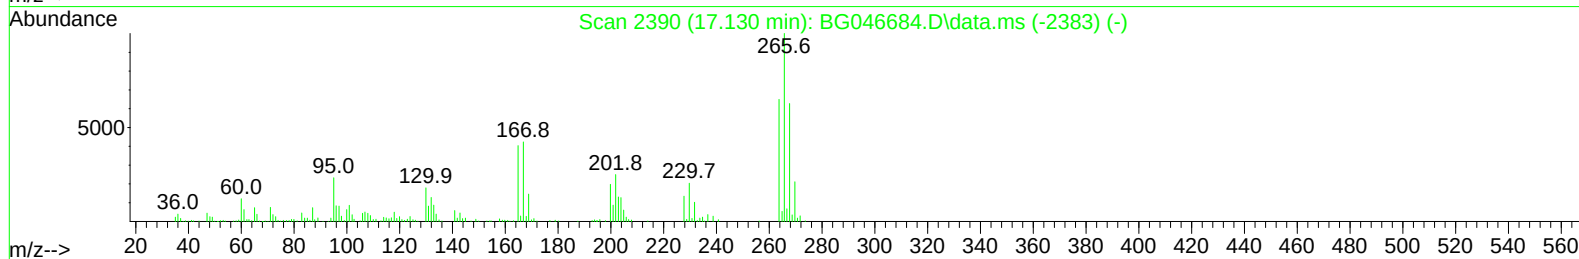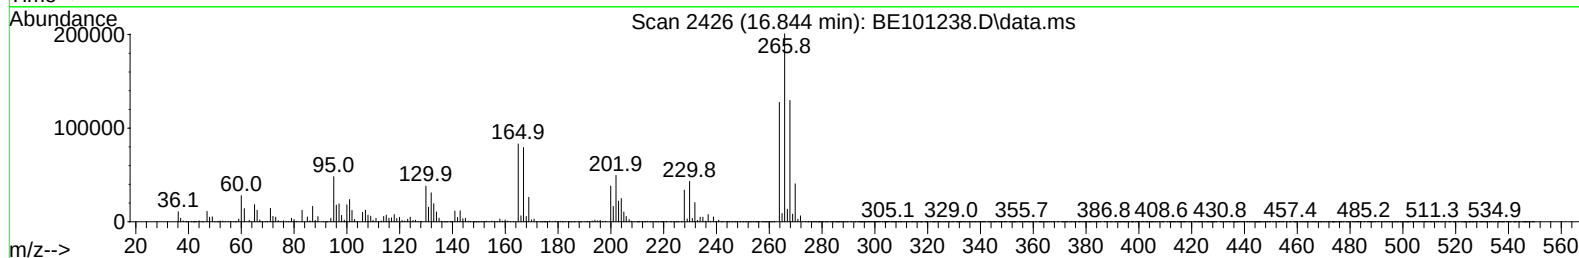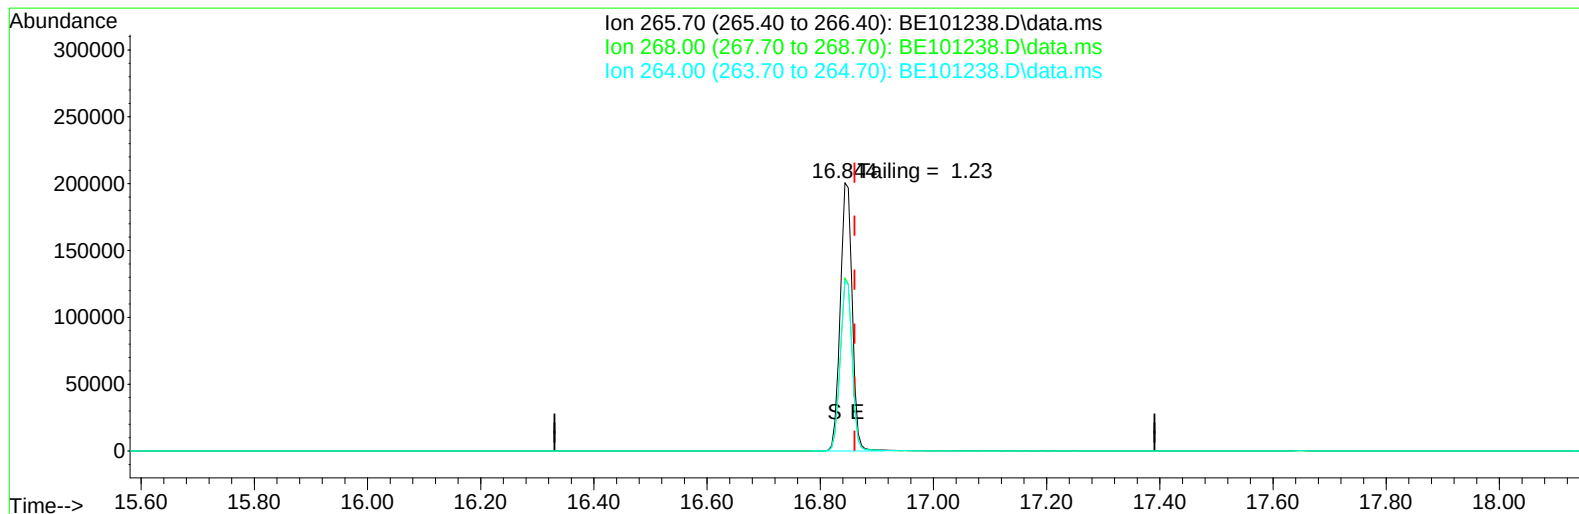

TIC: BE101238.D\data.ms

(70) Pentachlorophenol (C)

16.844min (-0.017) 6230258.48 ng

response 293361

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.50
264.00	61.60	63.48
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_E
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/9/2021	BNA_E	BE101238.D
Compound Name	Response	Retention Time
DDT	986398	20.66
DDD	23081	20.22
DDE	1330	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24411	1010809	2.41

Instrument :
BNA_E
ClientSampleId :
DFTPP