
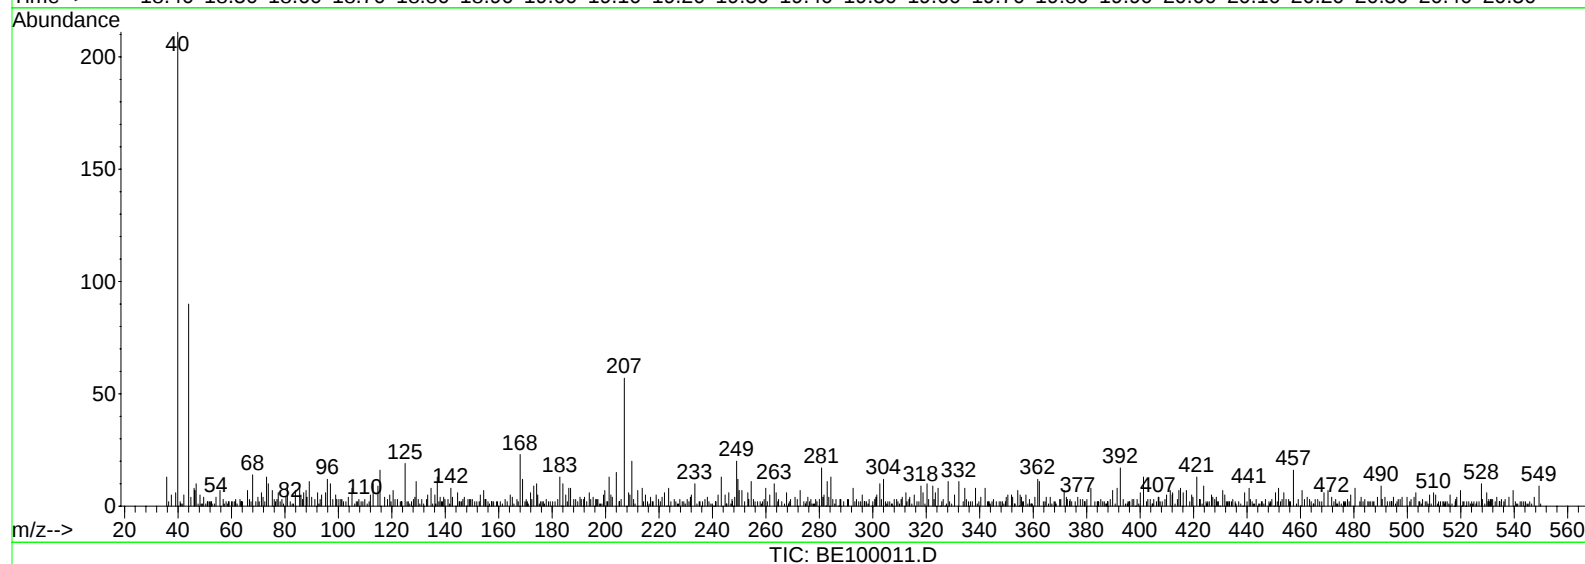


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061419\
 Data File : BE100011.D
 Acq On : 14 Jun 2019 7:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 05:51:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 01:27:44 2013
 Response via : Initial Calibration

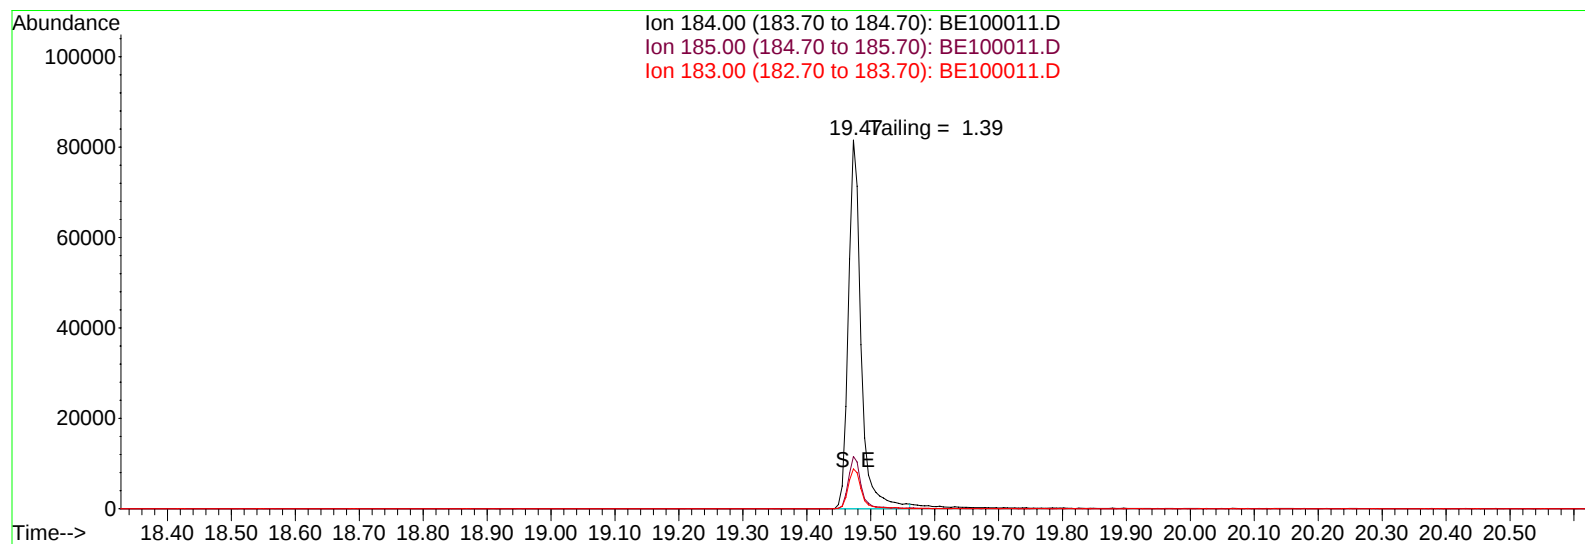

(76) Benzidine



14.596min (+0.006) 98.66ng

response 10

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	70.00#
183.00	12.20	130.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061419\
Data File : BE100011.D
Acq On : 14 Jun 2019 7:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 05:51:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

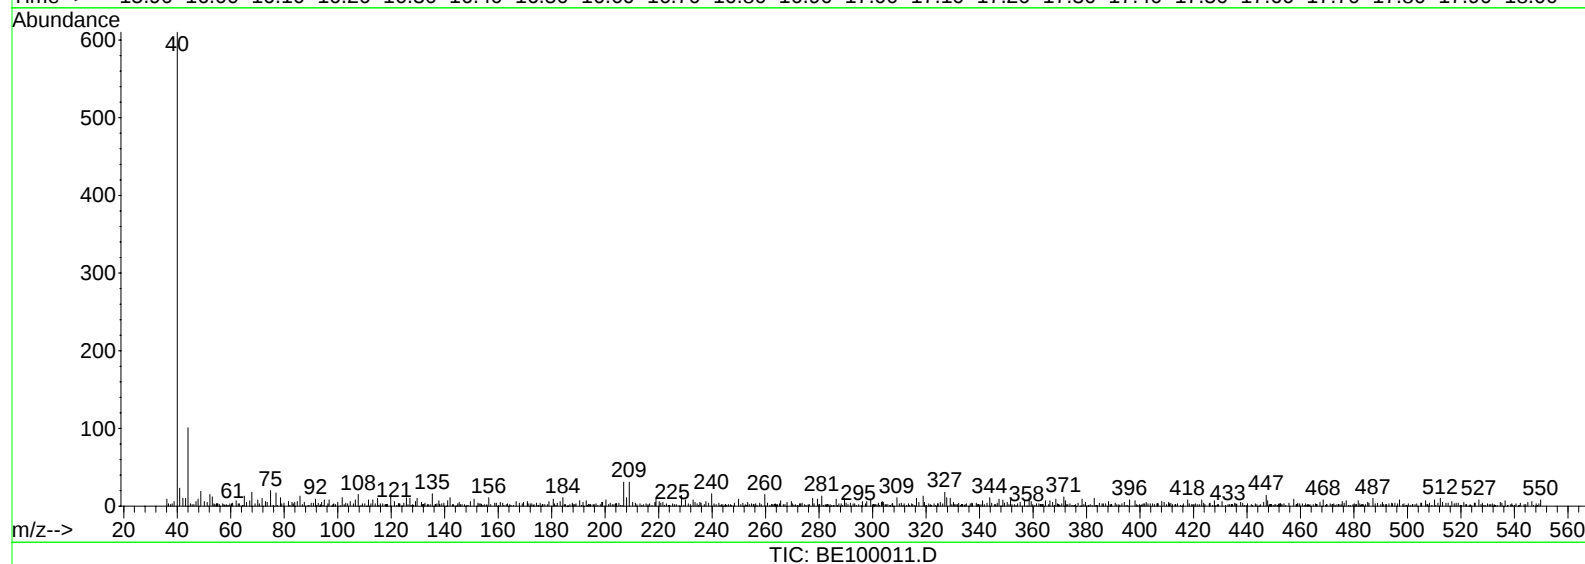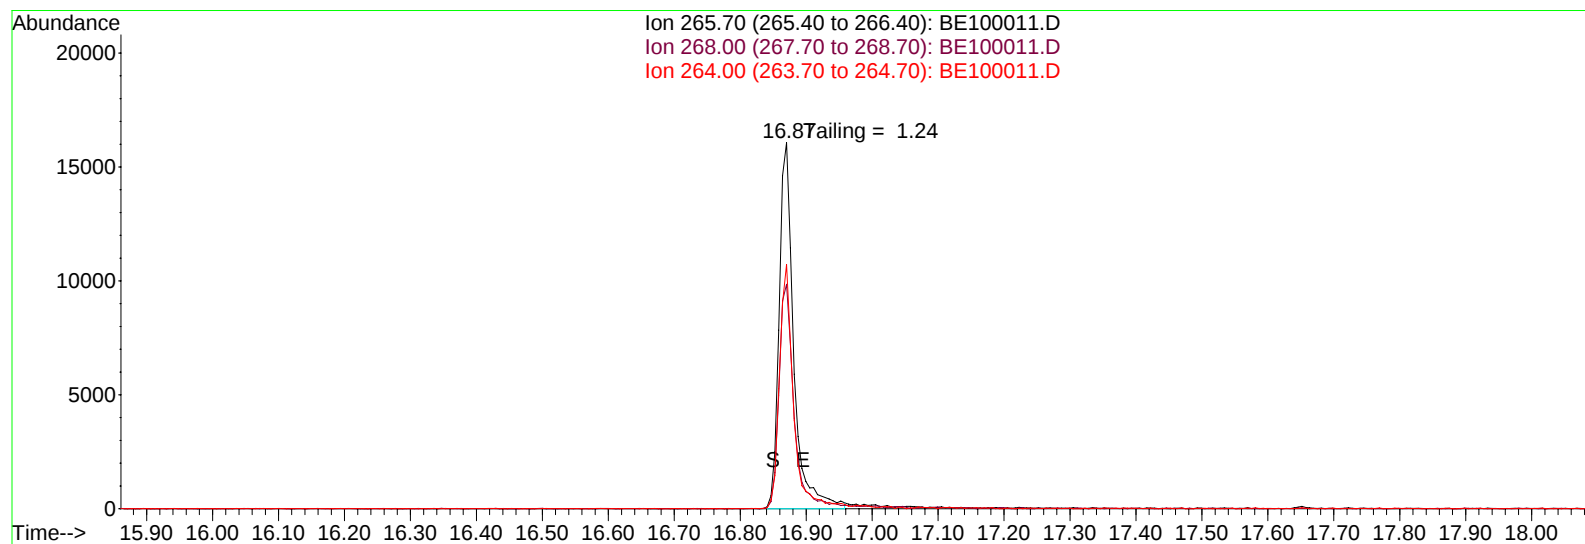

(69) Pentachlorophenol (C)

12.375min (+0.288) 85.88ng

response 5

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	71.43
264.00	65.00	71.43
0.00	0.00	0.00