
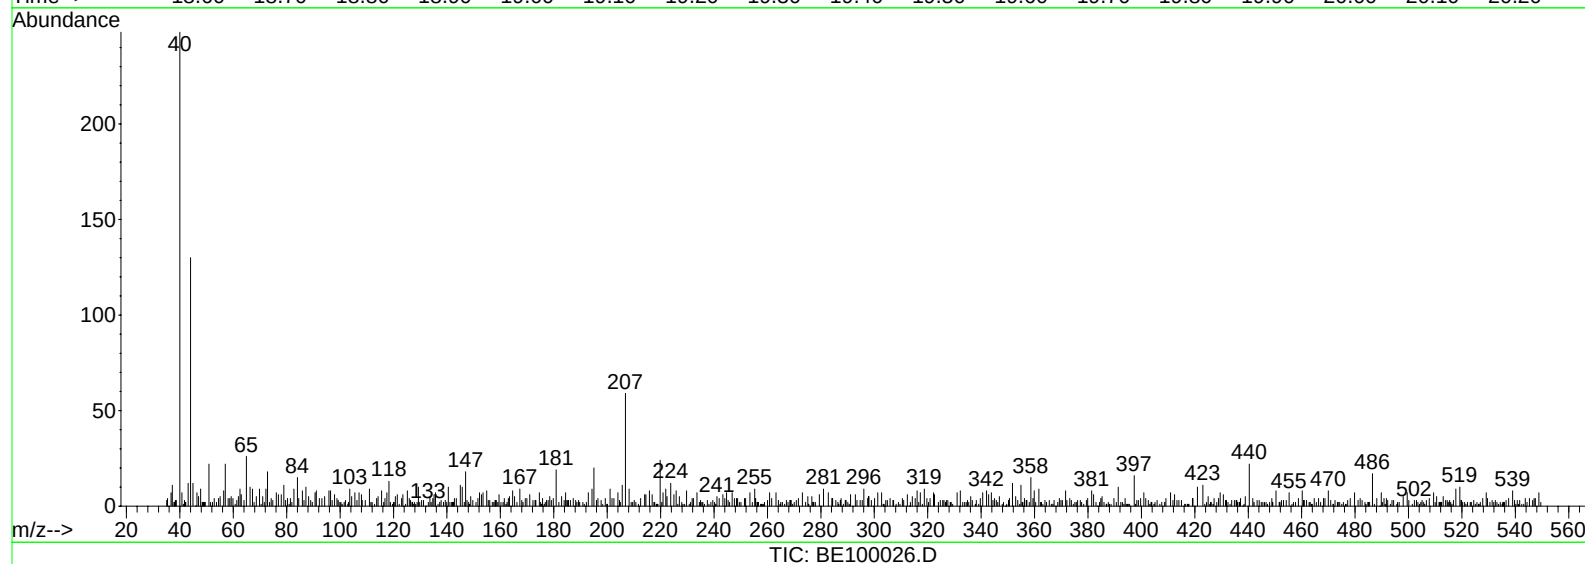


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061419\
Data File : BE100026.D
Acq On : 14 Jun 2019 16:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 05:58:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

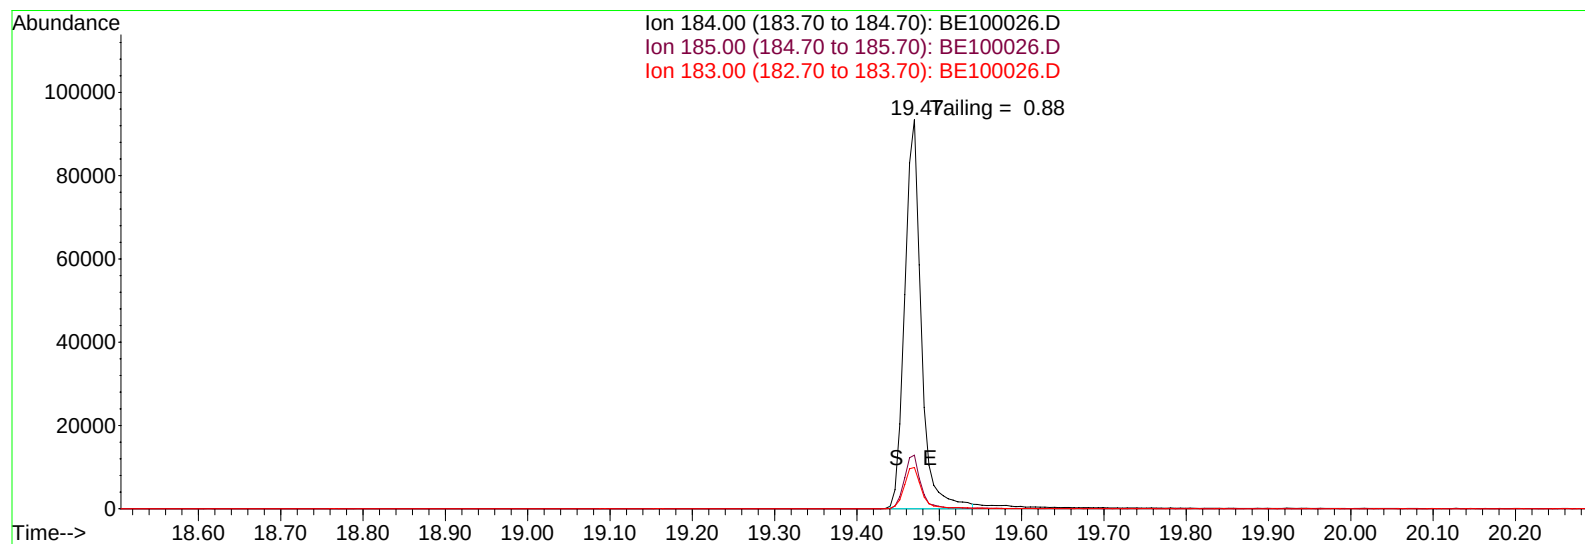

(76) Benzidine



14.440min (-0.150) 34.82ng

response 12

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	90.00#
183.00	12.20	50.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061419\
 Data File : BE100026.D
 Acq On : 14 Jun 2019 16:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 05:58:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 01:27:44 2013
 Response via : Initial Calibration

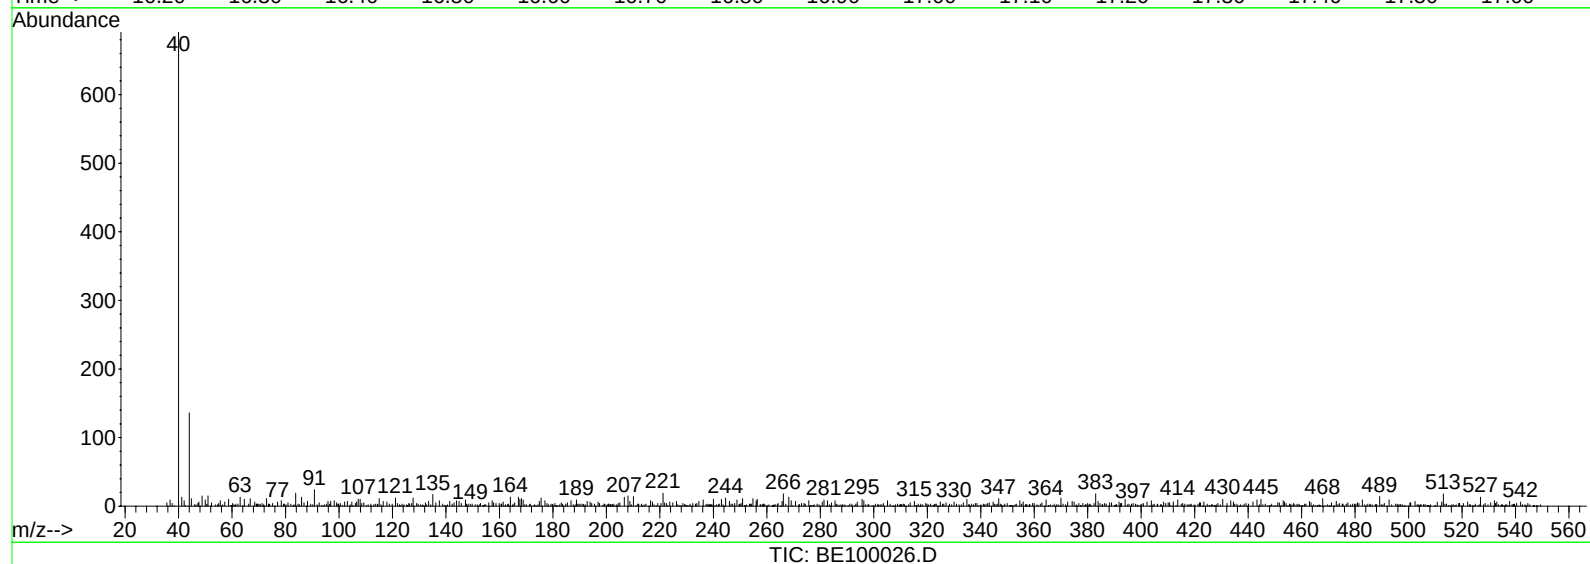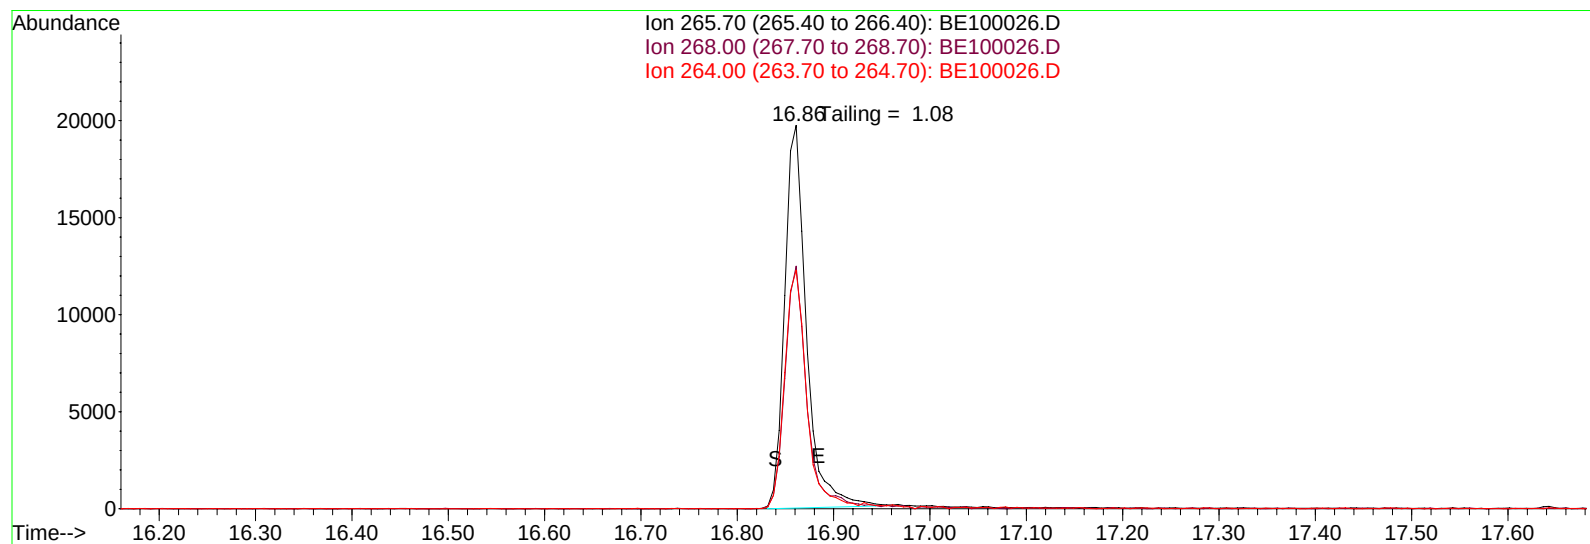

(69) Pentachlorophenol (C)

12.096min (+0.009) 480.93ng

response 16

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	52.00
264.00	65.00	24.00#
0.00	0.00	0.00