
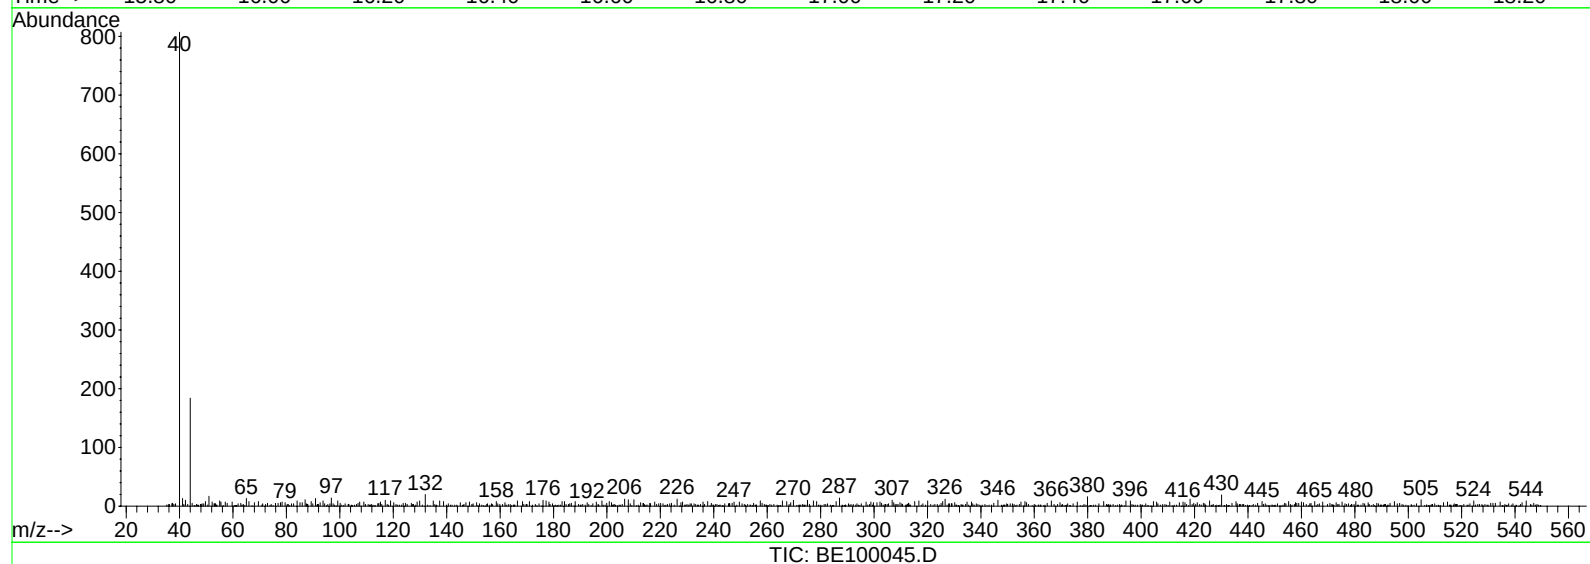


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061419\  
 Data File : BE100045.D  
 Acq On : 15 Jun 2019 5:00  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 06:07:57 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Nov 21 01:27:44 2013  
 Response via : Initial Calibration

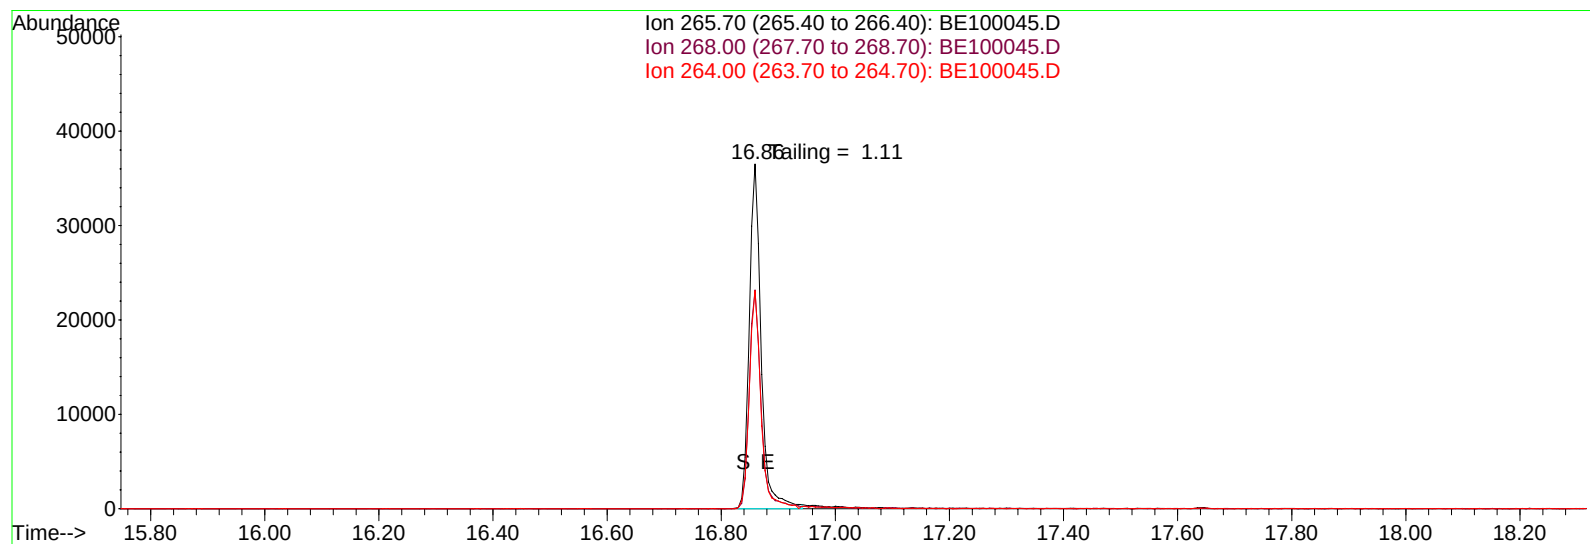

(69) Pentachlorophenol (C)



12.112min (+0.025) 45.09ng

response 3

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 265.70 | 100   | 100    |
| 268.00 | 63.30 | 33.33# |
| 264.00 | 65.00 | 44.44# |
| 0.00   | 0.00  | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061419\  
Data File : BE100045.D  
Acq On : 15 Jun 2019 5:00  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 06:07:57 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 21 01:27:44 2013  
Response via : Initial Calibration

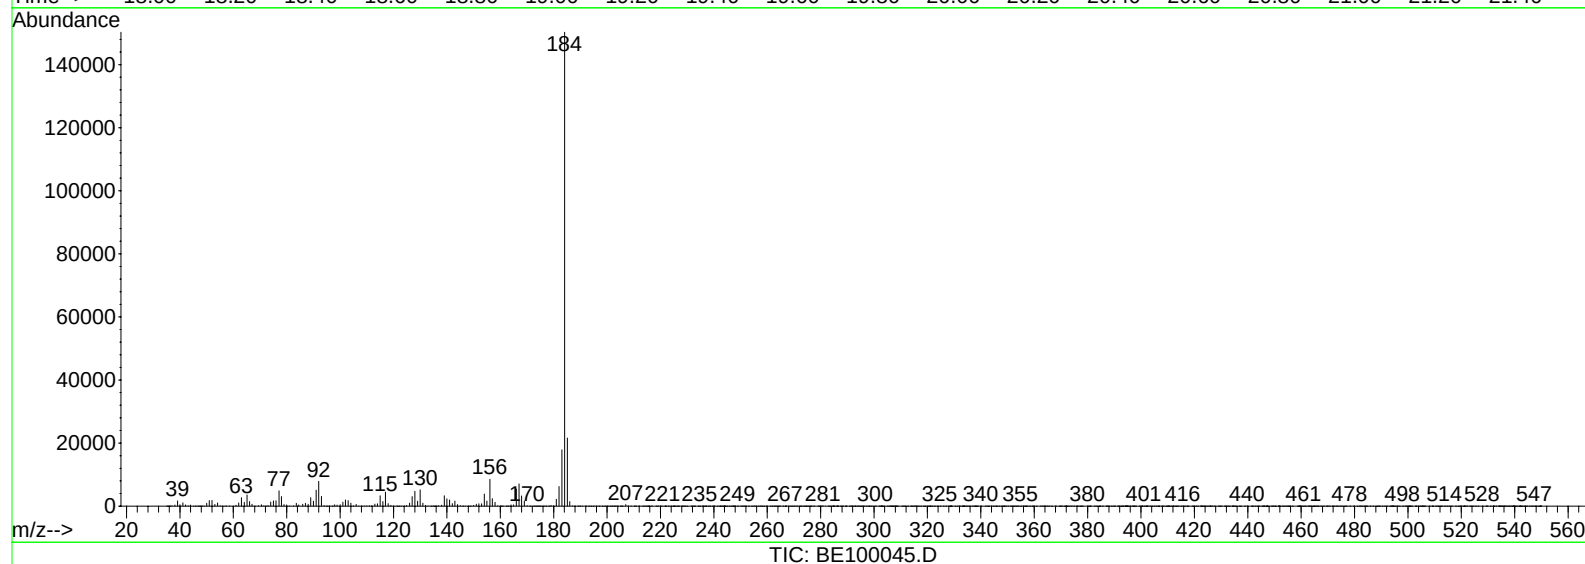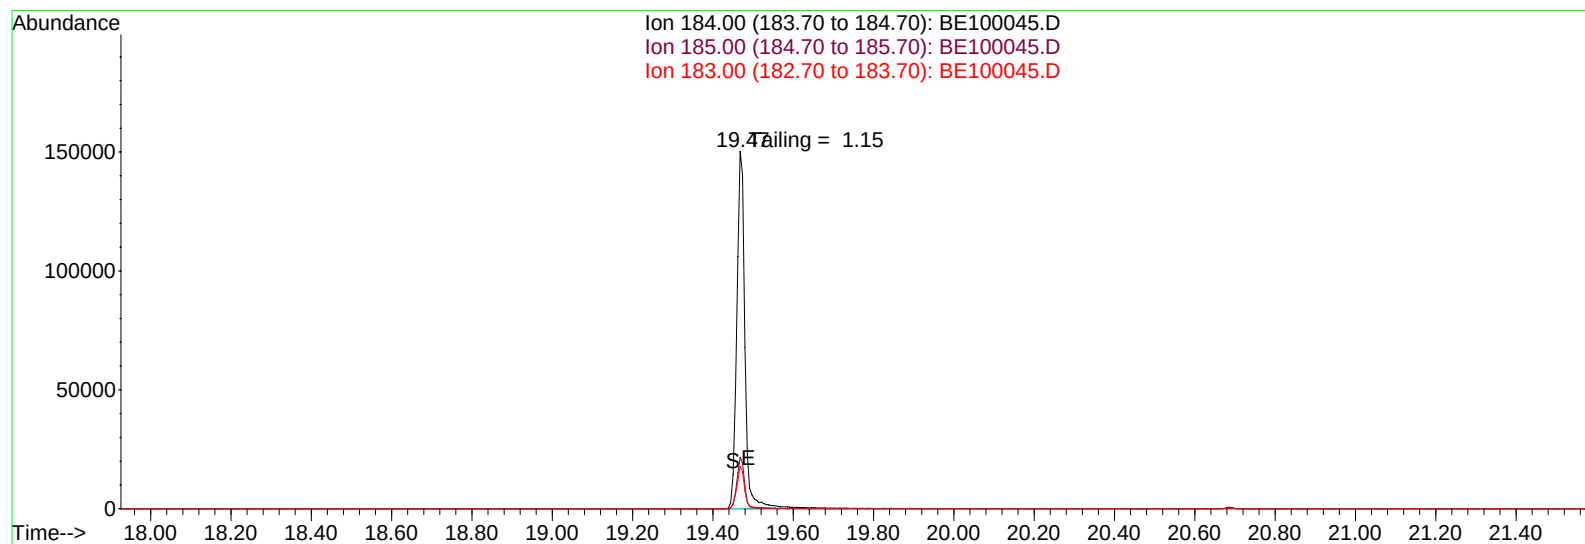

(76) Benzidine

19.468min (+4.878) 848599.60ng m

response 206429

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.90 | 14.40 |
| 183.00 | 12.20 | 11.89 |
| 0.00   | 0.00  | 0.00  |