

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061419\
 Data File : BE100029.D
 Acq On : 14 Jun 2019 18:45
 Operator : JU/SJ
 Sample : K3284-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP06-20190609

Quant Time: Jun 15 01:54:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE061019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 10 14:57:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	905	0.40	ng	0.00
7) Naphthalene-d8	10.59	136	3189	0.40	ng	-0.01
13) Acenaphthene-d10	14.46	164	2580	0.40	ng	-0.01
19) Phenanthrene-d10	17.20	188	7273	0.40	ng	-0.01
27) Chrysene-d12	21.39	240	8982	0.40	ng	-0.01
34) Perylene-d12	23.92	264	10284	0.40	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.36	112	476	0.19	ng	0.01
5) Phenol-d6	6.98	99	304	0.10	ng	0.01
8) Nitrobenzene-d5	8.96	82	1341	0.44	ng	0.00
11) 2-Methylnaphthalene-d10	12.19	152	2055	0.37	ng	-0.01
14) 2,4,6-Tribromophenol	15.96	330	823	0.43	ng	-0.01
15) 2-Fluorobiphenyl	13.07	172	4645	0.47	ng	-0.03
25) Fluoranthene-d10	19.24	212	41686	0.39	ng	0.00
29) Terphenyl-d14	19.84	244	10179	0.63	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.28	88	83	0.062	ng	# 1
9) Naphthalene	10.64	128	1398	0.041	ng	# 77
12) 2-Methylnaphthalene	12.27	142	152	0.027	ng	# 40
18) Fluorene	15.50	166	528	0.050	ng	# 82
22) Pentachlorophenol	16.87	266	76	0.337	ng	# 93
32) Bis(2-ethylhexyl)phthalate	21.29	149	1871	0.049	ng	# 77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061419\
Data File : BE100029.D
Acq On : 14 Jun 2019 18:45
Operator : JU/SJ
Sample : K3284-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-DUP06-20190609

Quant Time: Jun 15 01:54:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE061019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 10 14:57:20 2019
Response via : Initial Calibration

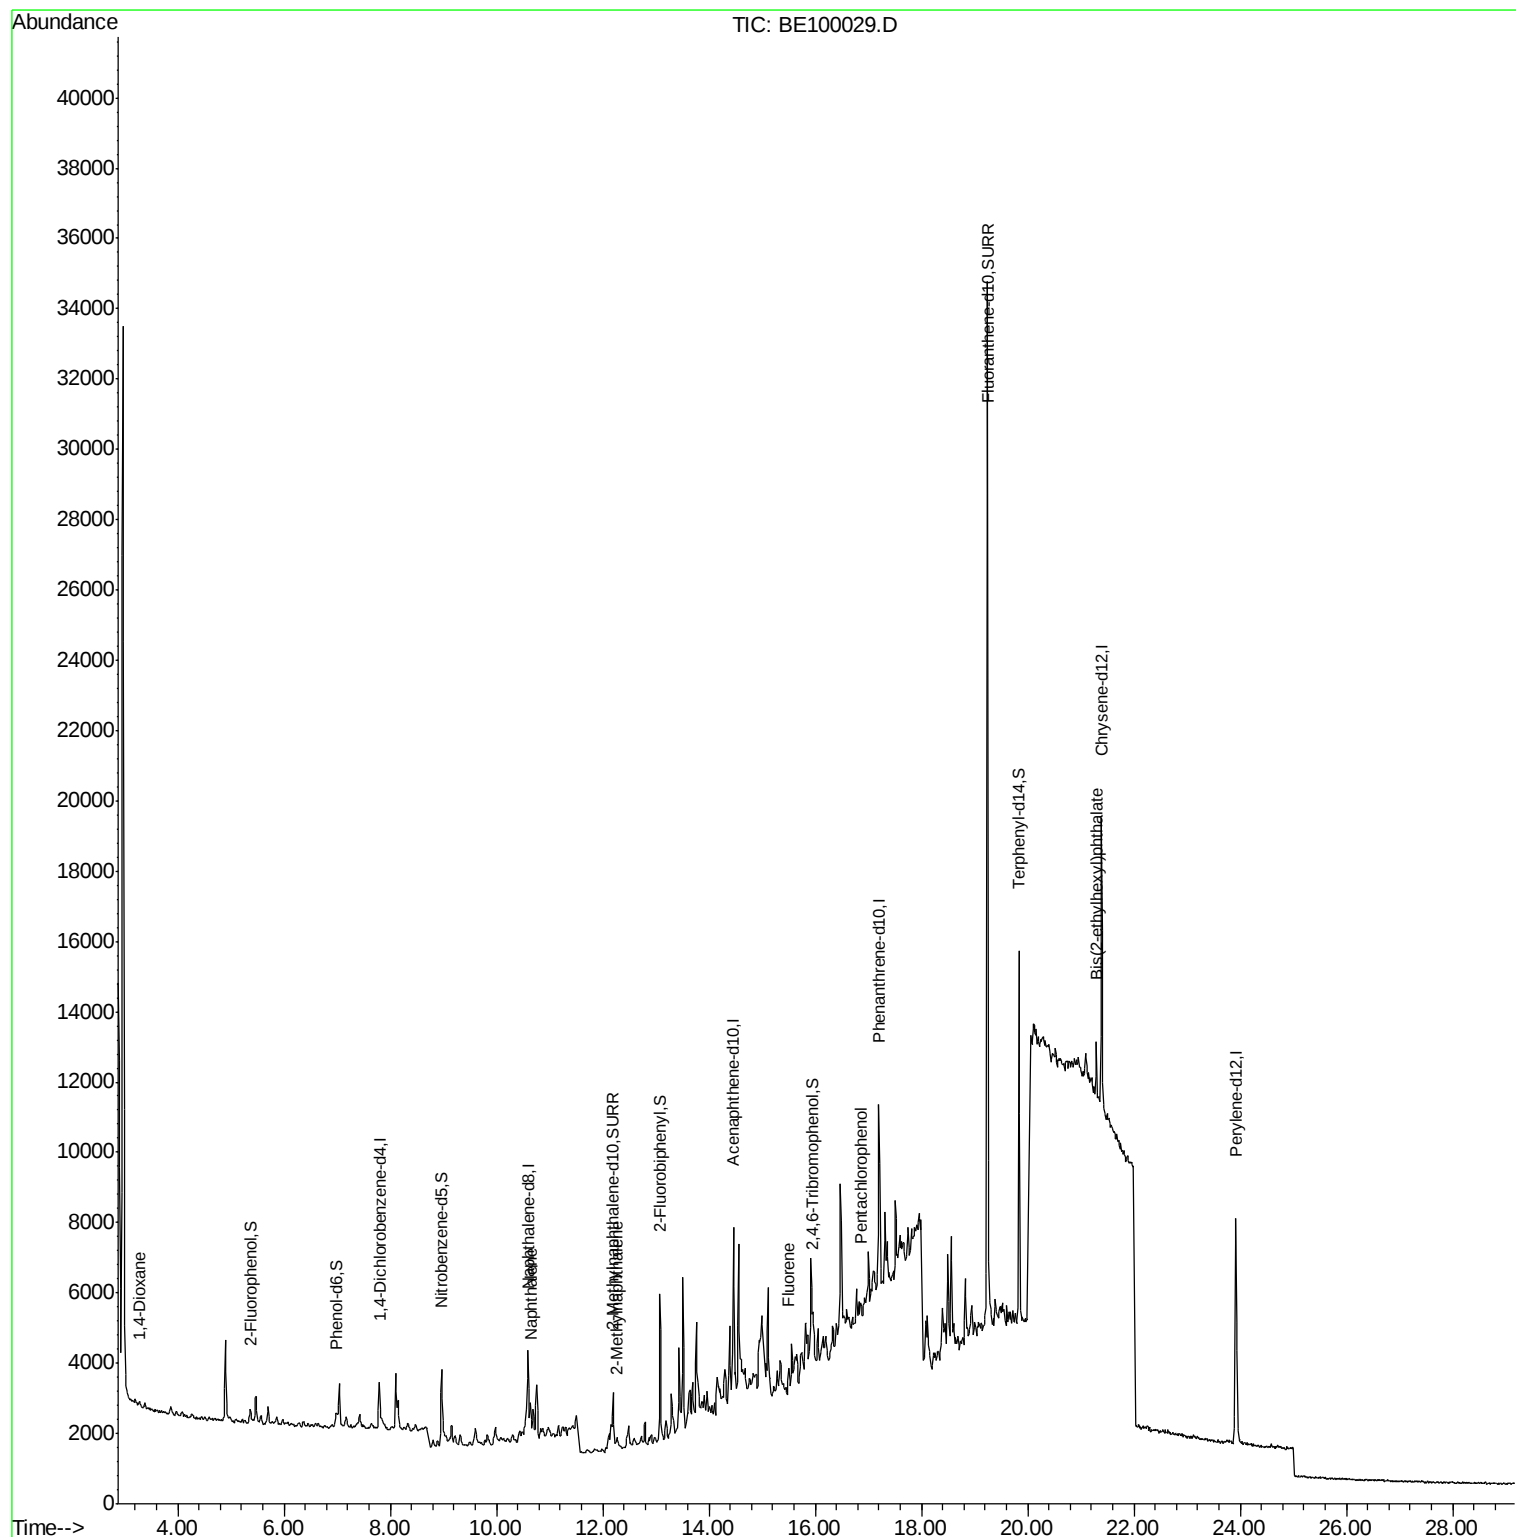







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.79 min Scan# 428
 Delta R.T. -0.00 min
 Lab File: BE100029.D
 Acq: 14 Jun 2019 18:45

Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP06-20190609

Tot Ion:152 Resp: 905
 Ion Ratio Lower Upper
 152 100
 150 132.8 111.0 166.6
 115 59.7 50.7 76.1

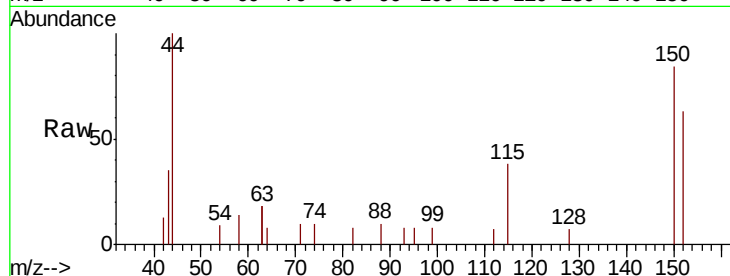


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

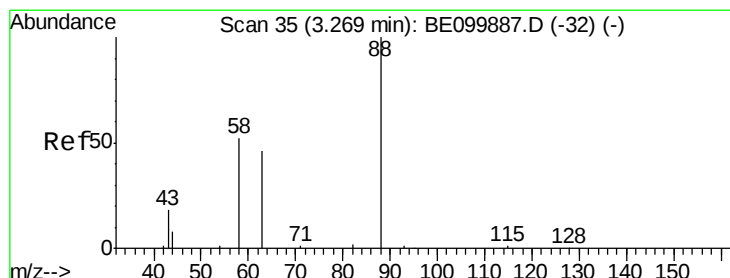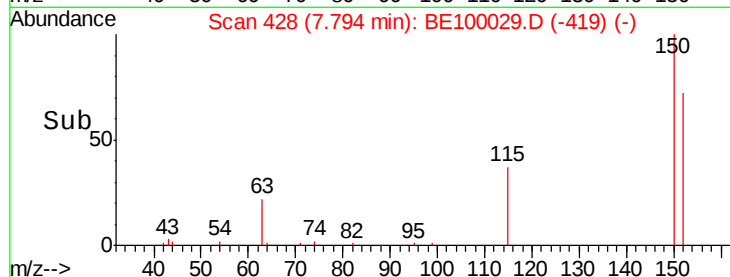
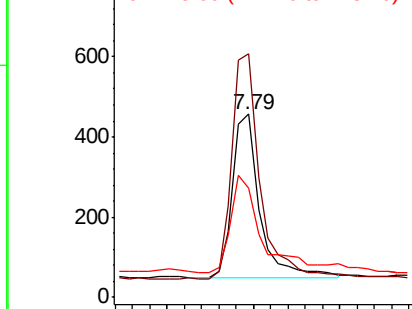


#2
 1,4-Dioxane
 Concen: 0.062 ng
 RT: 3.28 min Scan# 36
 Delta R.T. 0.01 min
 Lab File: BE100029.D
 Acq: 14 Jun 2019 18:45

Tgt Ion: 88 Resp: 83
 Ion Ratio Lower Upper
 88 100
 58 144.6 48.8 73.2#
 43 190.4 19.0 28.6#

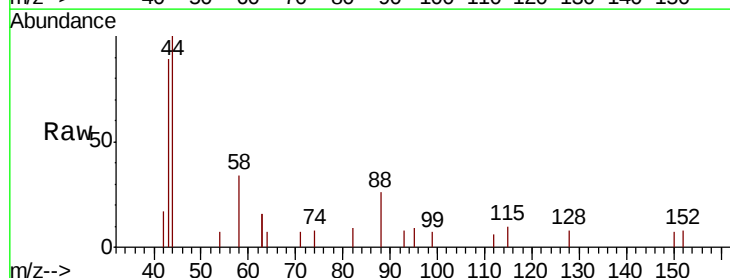

Abundance Ion 88.00 (87.70 to 88.70): BE1
 Ion 58.00 (57.70 to 58.70): BE1
 Ion 43.00 (42.70 to 43.70): BE1

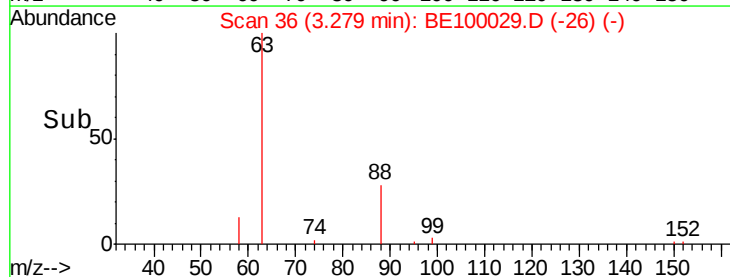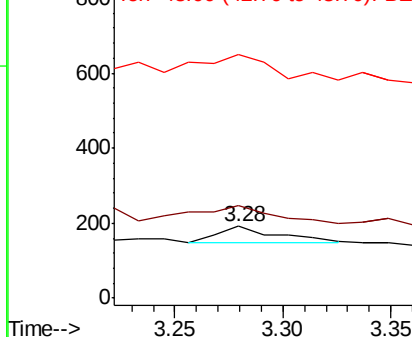



#4

2-Fluorophenol

Concen: 0.195 ng

RT: 5.36 min Scan# 217

Delta R.T. 0.01 min

Lab File: BE100029.D

Acq: 14 Jun 2019 18:45

Instrument :

BNA_E

ClientSampleId :

BP-DUP06-20190609


Tot Ion: 112 Resp: 476

Ion Ratio Lower Upper

112 100

64 38.7 44.1 66.1#



63 112.4 87.8 131.6

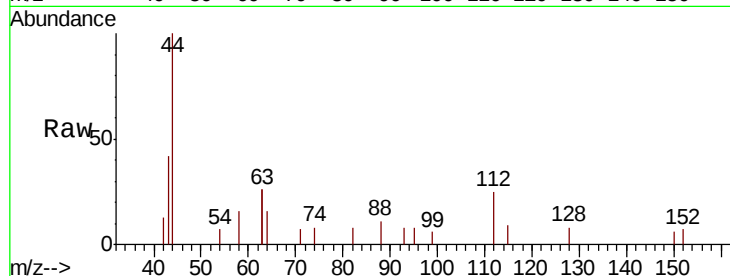

Abundance Ion 112.00 (111.70 to 112.70): BE1

Ion 64.00 (63.70 to 64.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

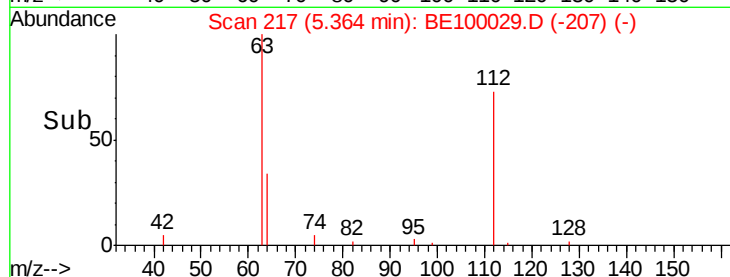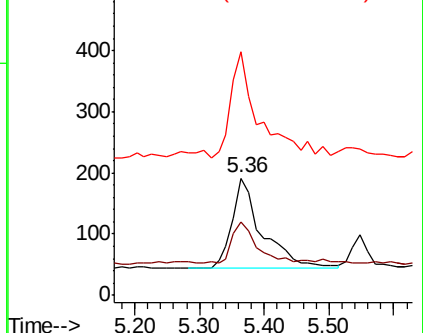

#5

Phenol-d6

Concen: 0.097 ng

RT: 6.98 min Scan# 357

Delta R.T. 0.01 min

Lab File: BE100029.D

Acq: 14 Jun 2019 18:45


Tgt Ion: 99 Resp: 304

Ion Ratio Lower Upper

99 100

42 21.7 15.9 23.9



71 67.8 34.6 52.0#

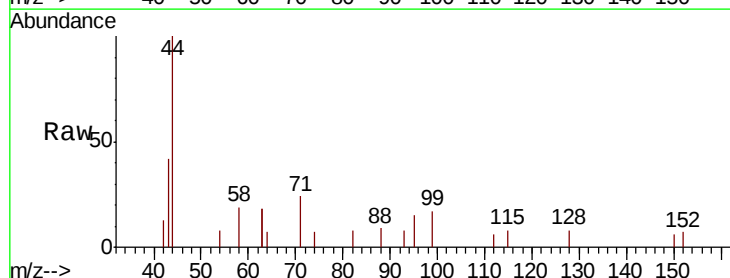

Abundance Ion 99.00 (98.70 to 99.70): BE1

Ion 42.00 (41.70 to 42.70): BE1

Ion 71.00 (70.70 to 71.70): BE1

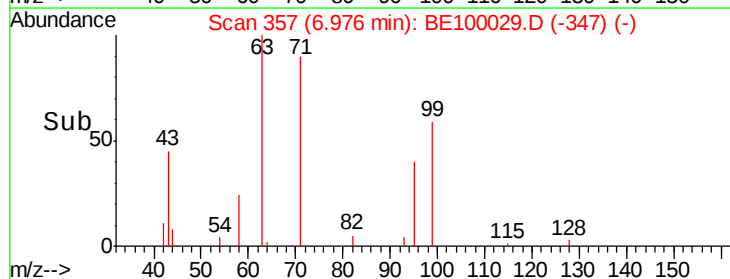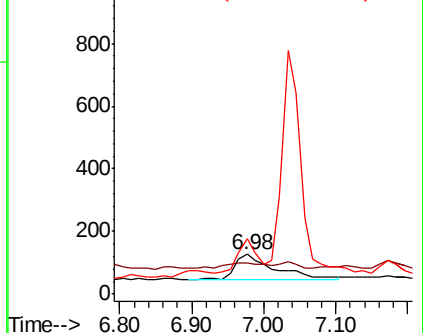



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.59 min Scan# 648

Delta R.T. -0.01 min

Lab File: BE100029.D

Acq: 14 Jun 2019 18:45

Instrument :

BNA_E

ClientSampleId :

BP-DUP06-20190609

Tot Ion:136 Resp: 3189


Ion Ratio Lower Upper

136 100

137 13.8 12.3 18.5

54 35.6 28.2 42.4

68 10.5 7.8 11.8


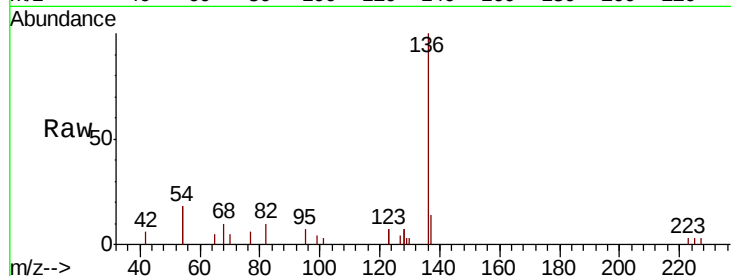


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE1

Ion 68.00 (67.70 to 68.70): BE1

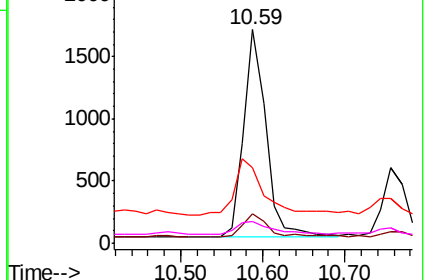

#8

Nitrobenzene-d5

Concen: 0.444 ng

RT: 8.96 min Scan# 523

Delta R.T. -0.00 min

Lab File: BE100029.D

Acq: 14 Jun 2019 18:45


Tgt Ion: 82 Resp: 1341

Ion Ratio Lower Upper

82 100

128 208.5 137.3 205.9#



54 157.6 129.7 194.5




Abundance Ion 82.00 (81.70 to 82.70): BE1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE1

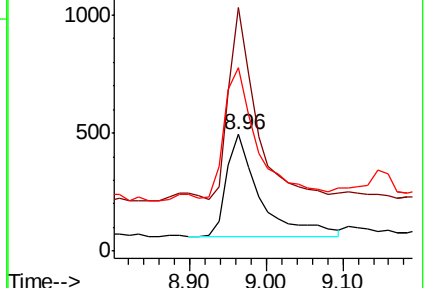



#9

Naphthalene

Concen: 0.041 ng

RT: 10.64 min Scan# 652

Delta R.T. -0.01 min

Lab File: BE100029.D

Acq: 14 Jun 2019 18:45

Instrument :

BNA_E

ClientSampleId :

BP-DUP06-20190609


Tot Ion:128 Resp: 1398

Ion Ratio Lower Upper

128 100

129 13.2 3.0 4.6#




127 10.0 3.4 5.0#

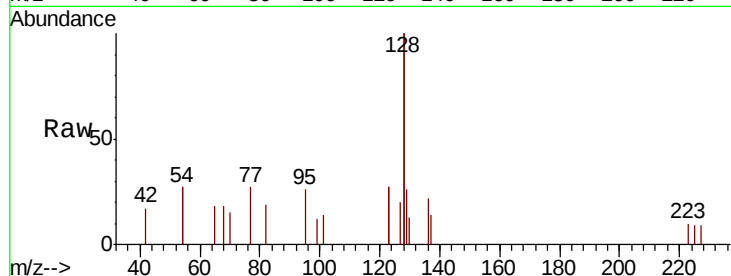

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

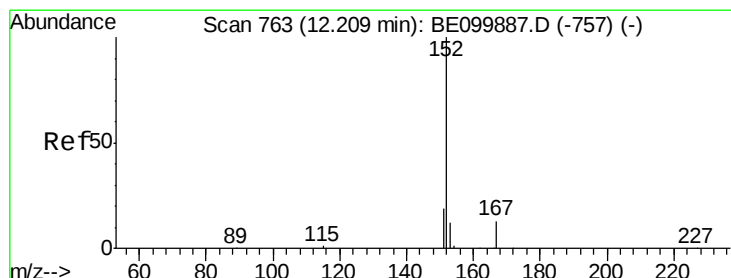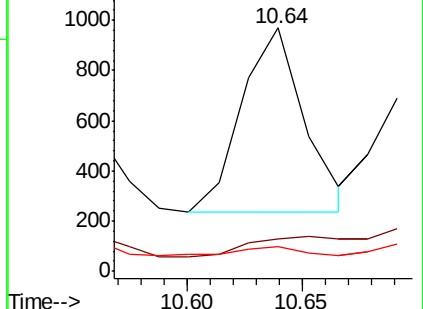

#11

2-Methylnaphthalene-d10

Concen: 0.370 ng

RT: 12.19 min Scan# 762

Delta R.T. -0.01 min

Lab File: BE100029.D


Acq: 14 Jun 2019 18:45

Tgt Ion:152 Resp: 2055

Ion Ratio Lower Upper



152 100


151 22.4 15.2 22.8



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

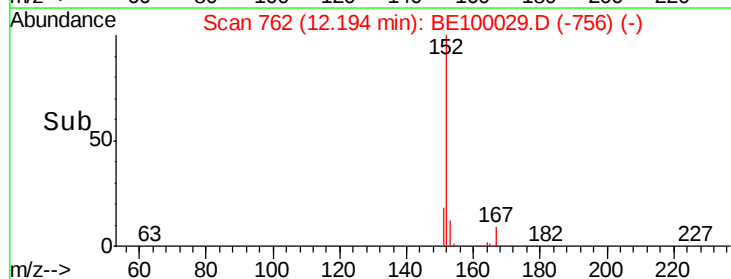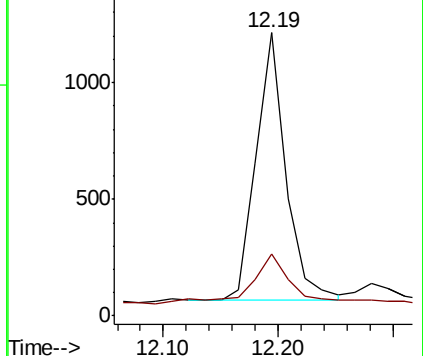

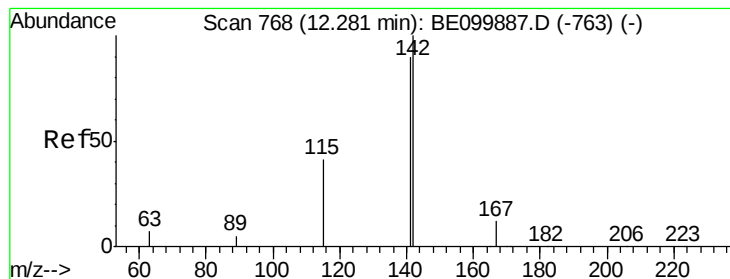

#12

2-Methylnaphthalene

Concen: 0.027 ng

RT: 12.27 min Scan# 767

Delta R.T. -0.01 min

Lab File: BE100029.D

Acq: 14 Jun 2019 18:45

Instrument :

BNA_E

ClientSampleId :

BP-DUP06-20190609


Tot Ion:142 Resp: 152

Ion Ratio Lower Upper

142 100

141 110.4 72.3 108.5#

115 135.8 36.4 54.6#



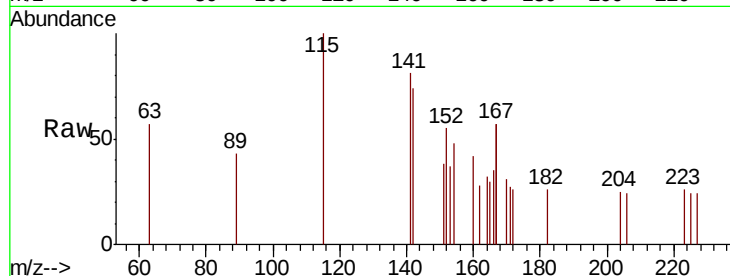


Abundance

Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

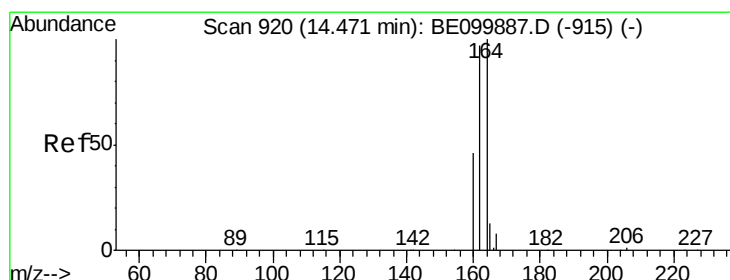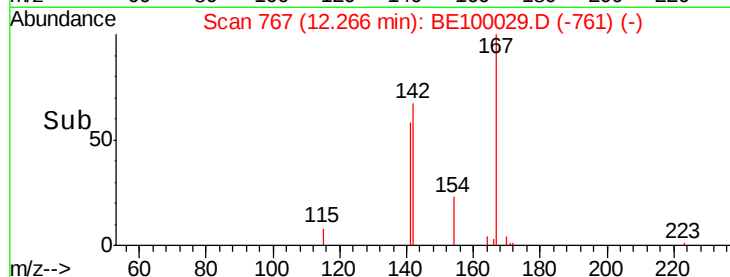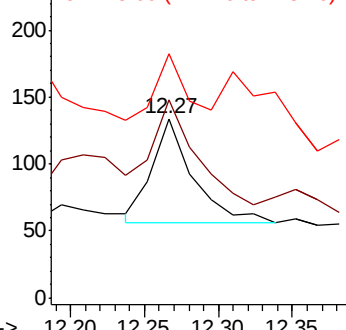

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.46 min Scan# 919

Delta R.T. -0.01 min

Lab File: BE100029.D

Acq: 14 Jun 2019 18:45


Tgt Ion:164 Resp: 2580

Ion Ratio Lower Upper

164 100

162 96.8 77.8 116.8

160 58.2 38.2 57.4#


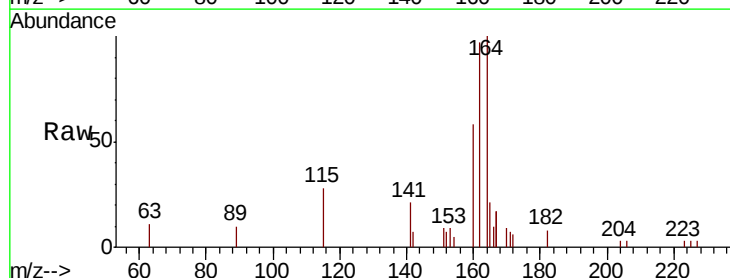



Abundance

Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

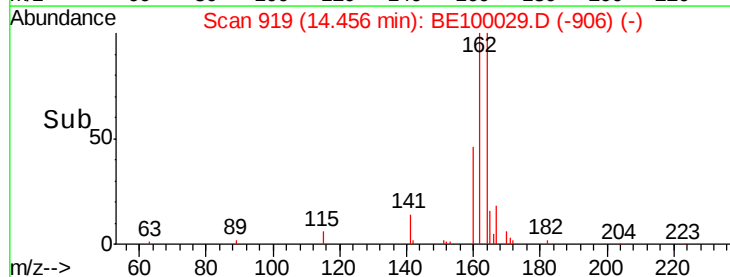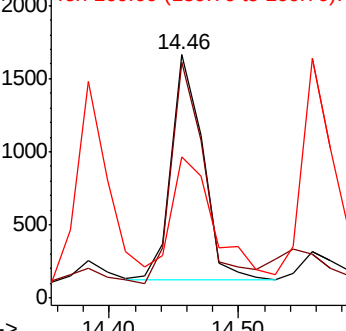

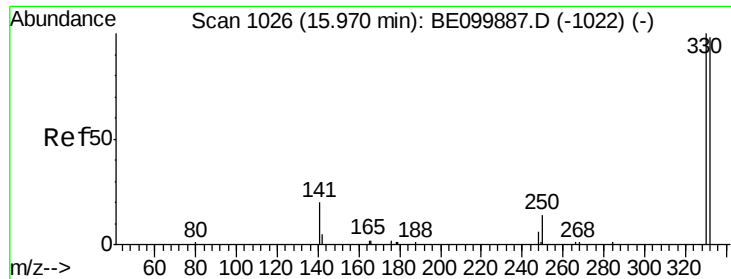

#14

2,4,6-Tribromophenol

Concen: 0.432 ng

RT: 15.96 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BE100029.D

Acq: 14 Jun 2019 18:45

Instrument :

BNA_E

ClientSampleId :

BP-DUP06-20190609


Tot Ion:330 Resp: 823

Ion Ratio Lower Upper

330 100

332 99.0 76.7 115.1




141 0.0 21.0 31.6#



Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

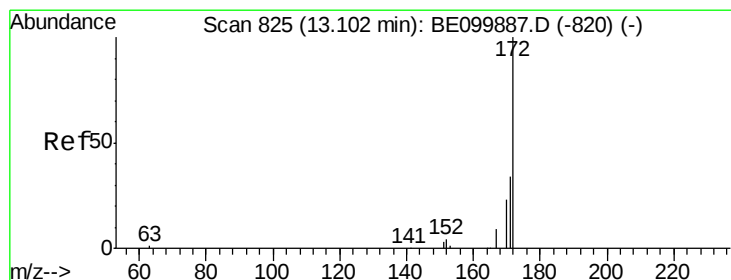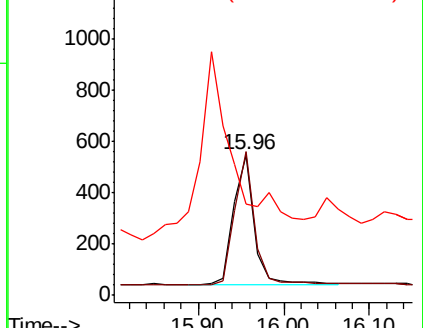

#15

2-Fluorobiphenyl

Concen: 0.475 ng

RT: 13.07 min Scan# 823

Delta R.T. -0.03 min

Lab File: BE100029.D

Acq: 14 Jun 2019 18:45


Tgt Ion:172 Resp: 4645

Ion Ratio Lower Upper

172 100

171 36.9 29.2 43.8



170 27.7 21.2 31.8




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E




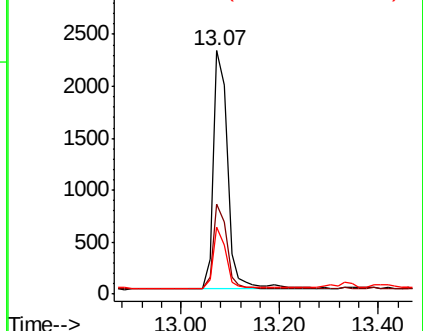


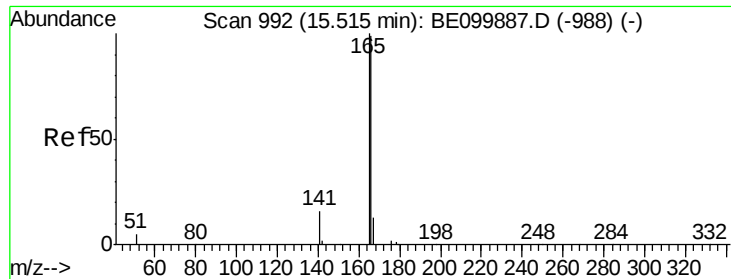

#18
Fluorene
 Concen: 0.050 ng
 RT: 15.50 min Scan# 991
 Delta R.T. -0.01 min
 Lab File: BE100029.D
 Acq: 14 Jun 2019 18:45




Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP06-20190609


Tot Ion:166 Resp: 528
 Ion Ratio Lower Upper
 166 100
 165 97.0 81.8 122.8
 167 58.0 11.2 16.8#

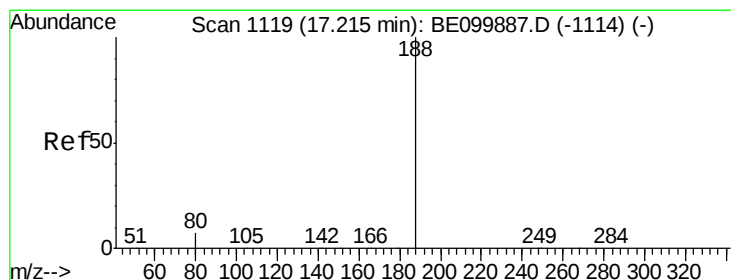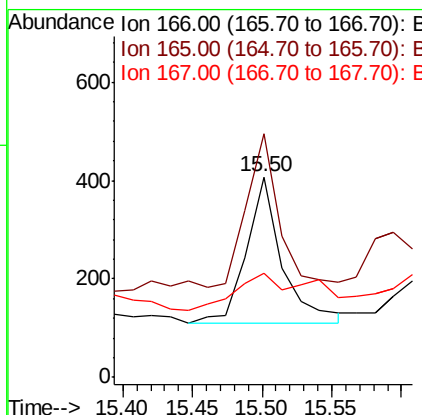

#19
Phenanthrene-d10
 Concen: 0.400 ng
 RT: 17.20 min Scan# 1118
 Delta R.T. -0.01 min
 Lab File: BE100029.D
 Acq: 14 Jun 2019 18:45

Tgt Ion:188 Resp: 7273
 Ion Ratio Lower Upper
 188 100
 94 0.0 0.0 0.0
 80 16.6 6.4 9.6#

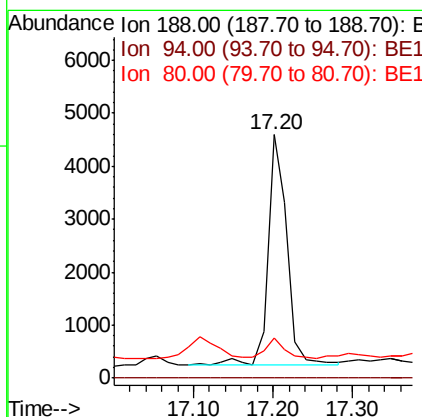







#22
 Pentachlorophenol
 Concen: 0.337 ng
 RT: 16.87 min Scan# 1093
 Delta R.T. -0.04 min
 Lab File: BE100029.D
 Acq: 14 Jun 2019 18:45

Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP06-20190609

Tot Ion:266 Resp: 76
 Ion Ratio Lower Upper
 266 100
 264 83.5 62.2 93.2
 268 88.6 65.5 98.3

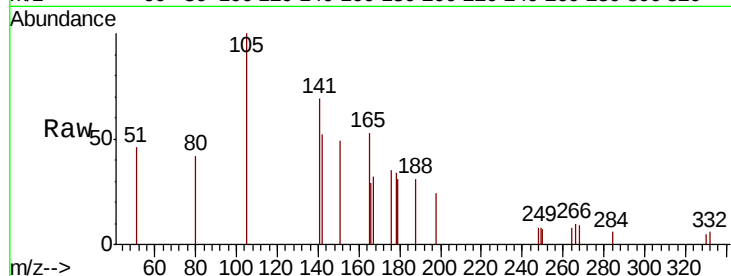


Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E


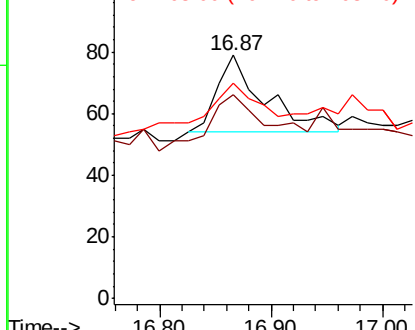



#25
 Fluoranthene-d10
 Concen: 0.393 ng
 RT: 19.24 min Scan# 1388
 Delta R.T. -0.01 min
 Lab File: BE100029.D
 Acq: 14 Jun 2019 18:45

Tgt Ion:212 Resp: 41686
 Ion Ratio Lower Upper
 212 100
 106 1.8 1.4 2.2
 104 1.1 0.9 1.3



Abundance Ion 212.00 (211.70 to 212.70): E
 Ion 106.00 (105.70 to 106.70): E
 Ion 104.00 (103.70 to 104.70): E




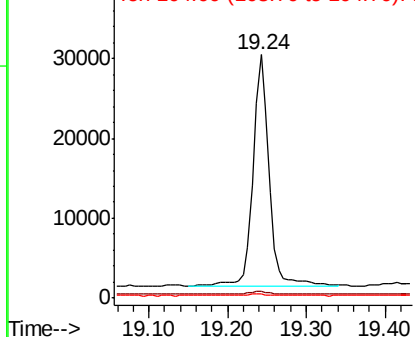




#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.39 min Scan# 1631
 Delta R.T. -0.01 min
 Lab File: BE100029.D
 Acq: 14 Jun 2019 18:45




Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP06-20190609


Tot Ion:240 Resp: 8982
 Ion Ratio Lower Upper
 240 100
 120 10.0 3.8 5.6#
 236 31.0 22.0 33.0

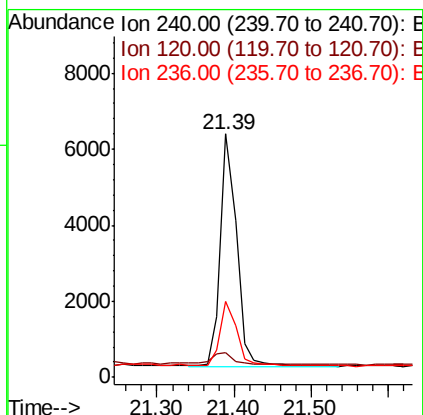

#29
 Terphenyl-d14
 Concen: 0.630 ng
 RT: 19.84 min Scan# 1492
 Delta R.T. -0.01 min
 Lab File: BE100029.D
 Acq: 14 Jun 2019 18:45

Tgt Ion:244 Resp: 10179
 Ion Ratio Lower Upper
 244 100
 212 44.2 25.7 38.5#
 122 9.5 5.5 8.3#



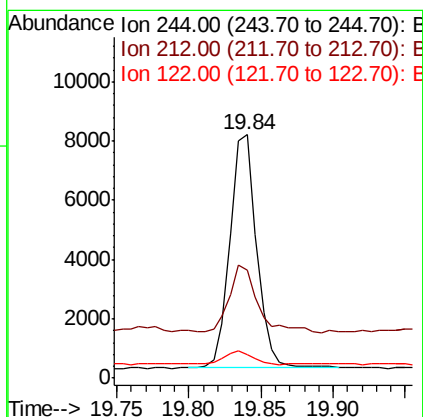



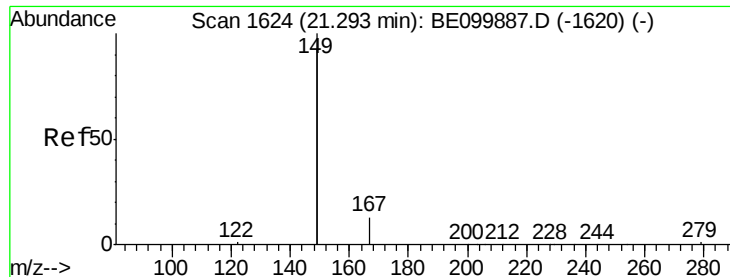

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.049 ng
 RT: 21.29 min Scan# 1623
 Delta R.T. -0.00 min
 Lab File: BE100029.D
 Acq: 14 Jun 2019 18:45

Instrument :
 BNA_E
 ClientSampleId :
 BP-DUP06-20190609

Tot Ion:149 Resp: 1871
 Ion Ratio Lower Upper
 149 100
 167 16.8 5.9 8.9#
 279 0.0 1.2 1.8#

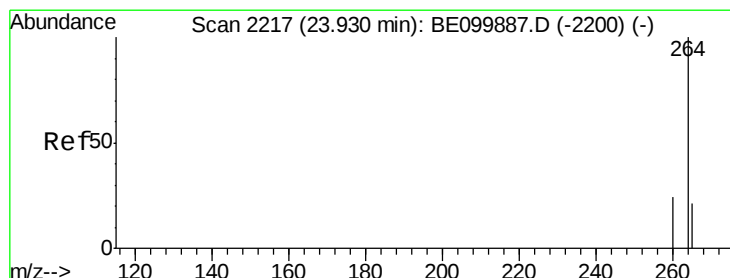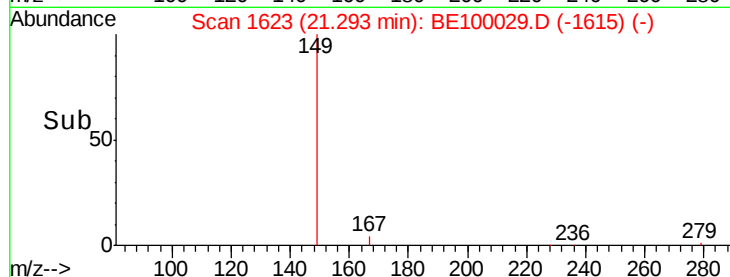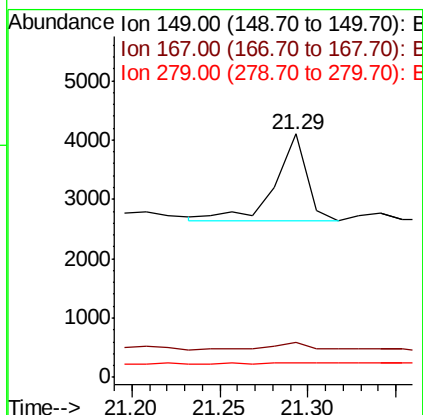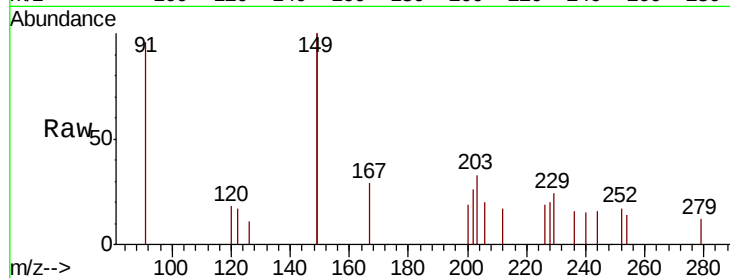

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.92 min Scan# 2213
 Delta R.T. -0.01 min
 Lab File: BE100029.D
 Acq: 14 Jun 2019 18:45

Tgt Ion:264 Resp: 10284
 Ion Ratio Lower Upper
 264 100
 260 26.2 20.2 30.2
 265 35.3 22.0 33.0#

