


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061419\
 Data File : BE100011.D
 Acq On : 14 Jun 2019 7:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 10 14:57:20 2019

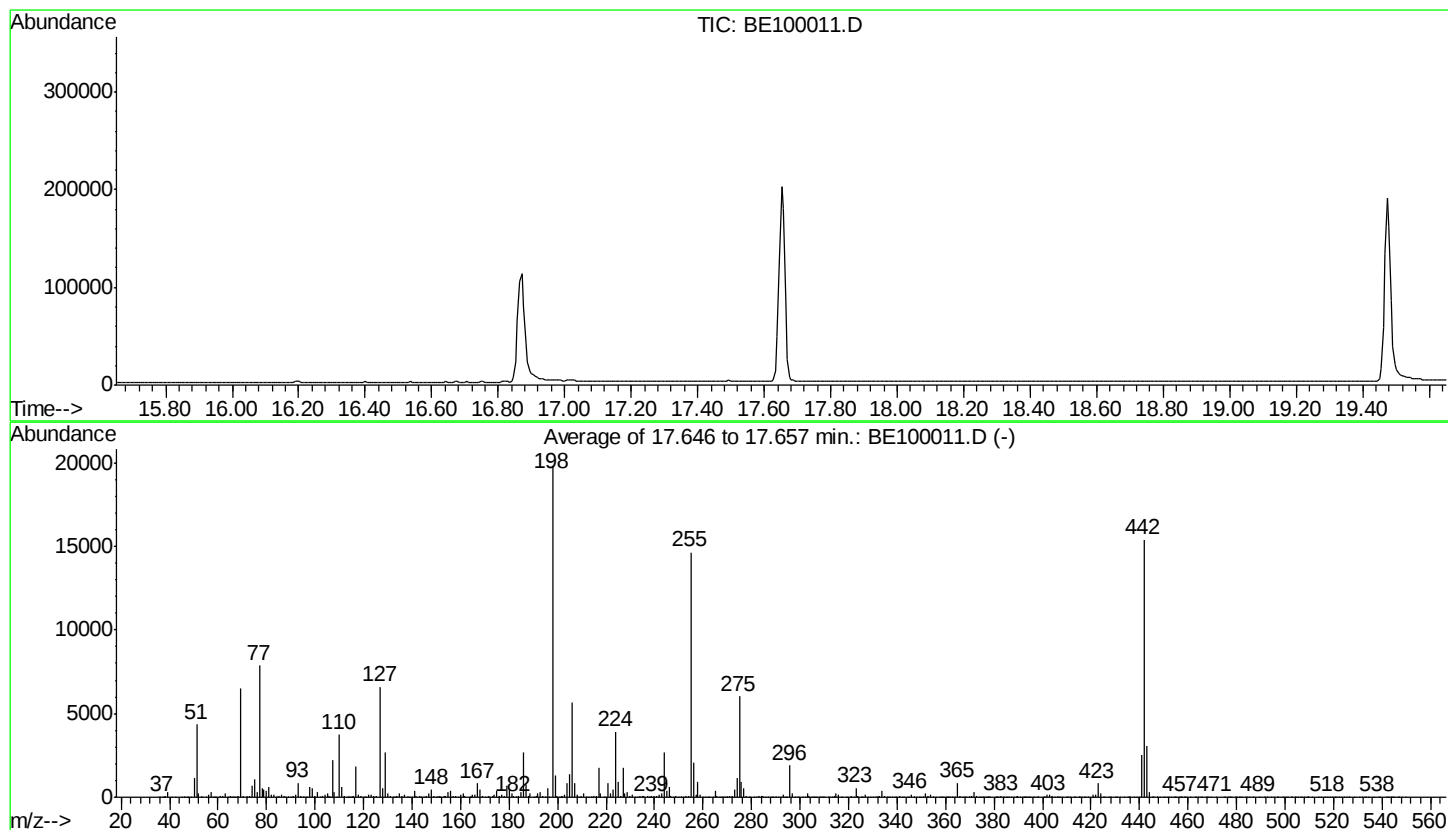

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.8	4329	PASS
68	69	0.00	2	1.8	115	PASS
69	198	0.00	100	32.8	6494	PASS
70	69	0.00	2	0.6	41	PASS
127	198	10	80	33.2	6584	PASS
197	198	0.00	2	0.2	33	PASS
198	198	100	100	100.0	19815	PASS
199	198	5	9	6.6	1312	PASS
275	198	10	60	30.5	6037	PASS
365	198	1	100	4.3	860	PASS
441	198	0.01	100	12.8	2542	PASS
442	198	50	100	77.7	15396	PASS
443	442	15	24	20.1	3090	PASS