


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061419\
 Data File : BE100026.D
 Acq On : 14 Jun 2019 16:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 10 14:57:20 2019

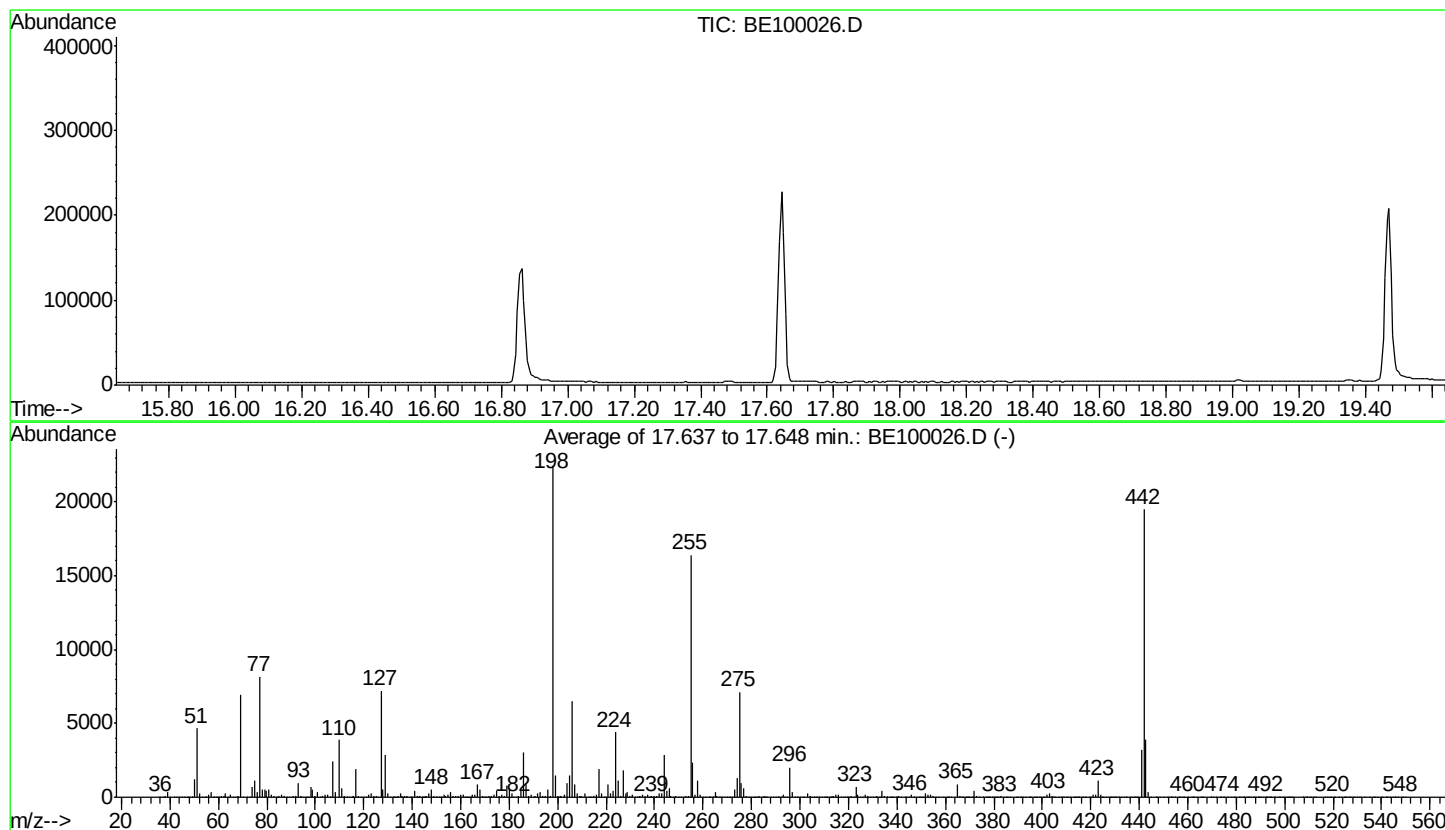

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.8	4666	PASS
68	69	0.00	2	1.6	111	PASS
69	198	0.00	100	30.9	6931	PASS
70	69	0.00	2	0.4	26	PASS
127	198	10	80	32.1	7207	PASS
197	198	0.00	2	0.3	57	PASS
198	198	100	100	100.0	22450	PASS
199	198	5	9	6.7	1505	PASS
275	198	10	60	31.7	7113	PASS
365	198	1	100	3.9	869	PASS
441	198	0.01	100	14.4	3222	PASS
442	198	50	100	86.8	19489	PASS
443	442	15	24	20.2	3942	PASS