


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061419\
Data File : BE100045.D
Acq On : 15 Jun 2019 5:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 10 14:57:20 2019

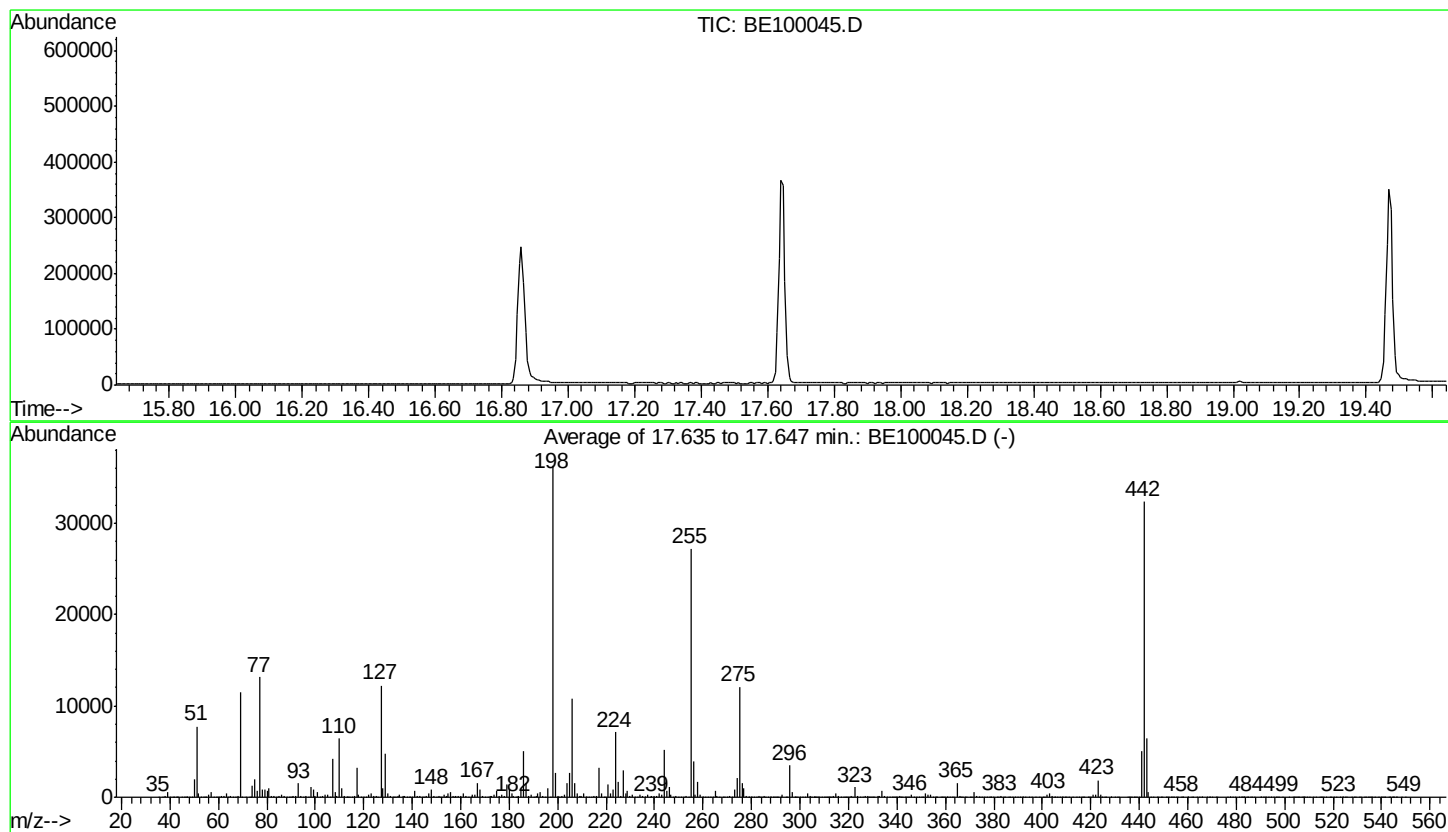

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	7762	PASS
68	69	0.00	2	1.4	156	PASS
69	198	0.00	100	31.8	11555	PASS
70	69	0.00	2	0.5	62	PASS
127	198	10	80	33.8	12271	PASS
197	198	0.00	2	0.2	63	PASS
198	198	100	100	100.0	36334	PASS
199	198	5	9	7.2	2631	PASS
275	198	10	60	33.3	12085	PASS
365	198	1	100	4.3	1561	PASS
441	198	0.01	100	14.1	5107	PASS
442	198	50	100	89.1	32390	PASS
443	442	15	24	19.8	6429	PASS